

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050719\
 Data File : BN005506.D
 Acq On : 07 May 2019 03:22
 Operator : JU/SJ
 Sample : K2403-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5124

Manual Integrations
 APPROVED

mohammad
 5/8/2019 12:01:07 AM

Quant Time: May 07 16:21:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 07 07:04:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1751	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	6890	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	4681	0.40	ng/ul	-0.02
10) Phenanthrene-d10	16.98	188	11299m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.22	240	11435m	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	9112m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.95	152	3963	0.37	ng/ul	-0.04
14) Fluoranthene-d10	19.03	212	11836m	0.33	ng/ul	-0.01
Target Compounds						
3) Naphthalene	10.40	128	3057	0.168	ng/ul	Ovalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050719\
Data File : BN005506.D
Acq On : 07 May 2019 03:22
Operator : JU/SJ
Sample : K2403-07
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A5124

Manual Integrations
APPROVED

mohammad
5/8/2019 12:01:07 AM

Quant Time: May 07 16:21:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 07 07:04:57 2019
Response via : Initial Calibration

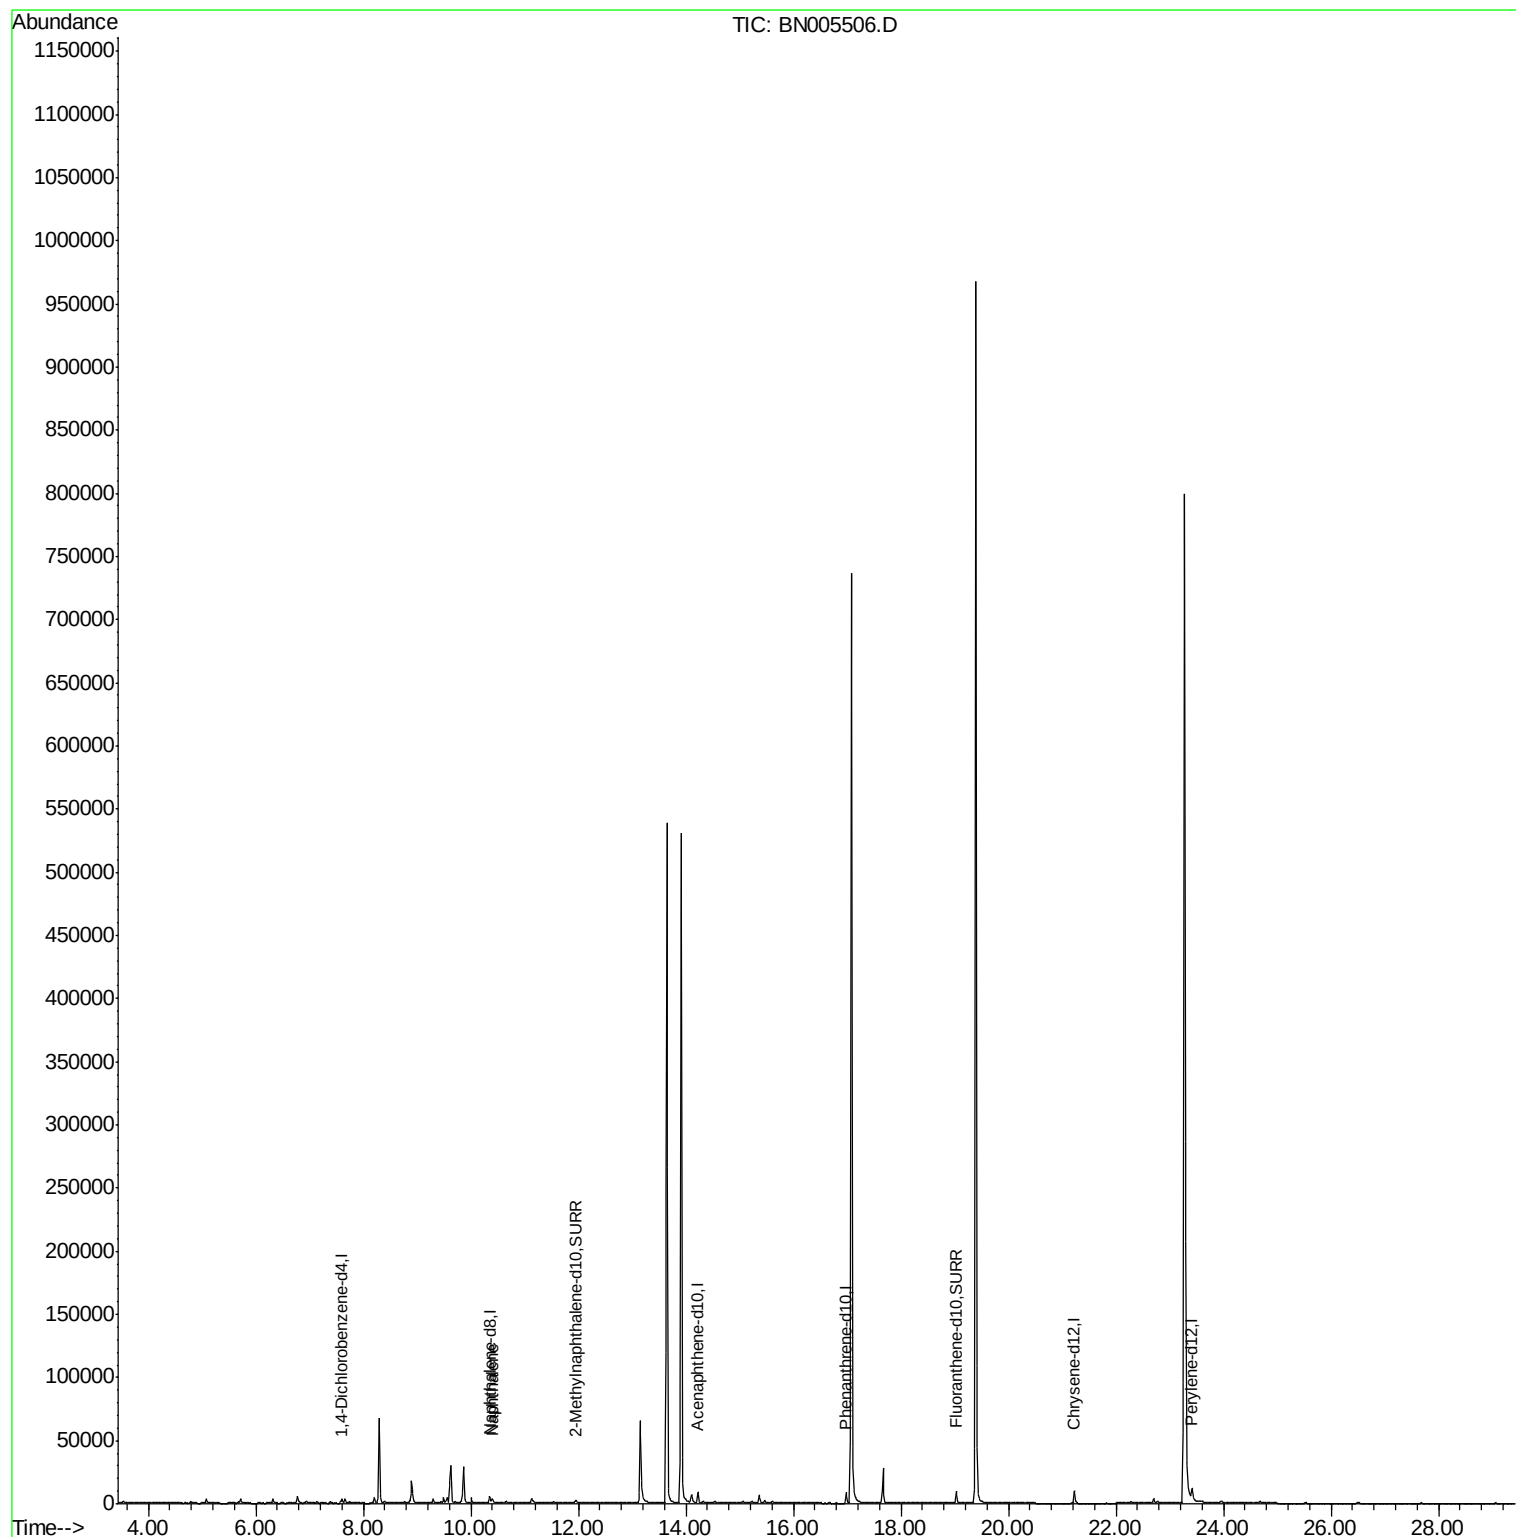

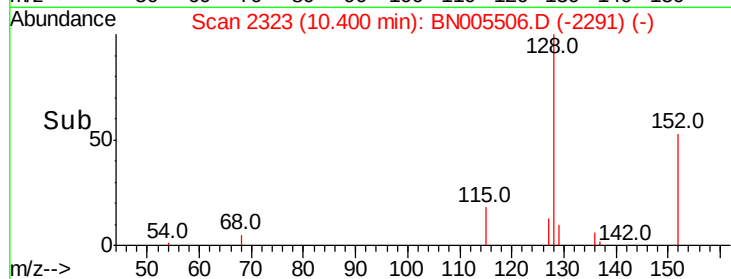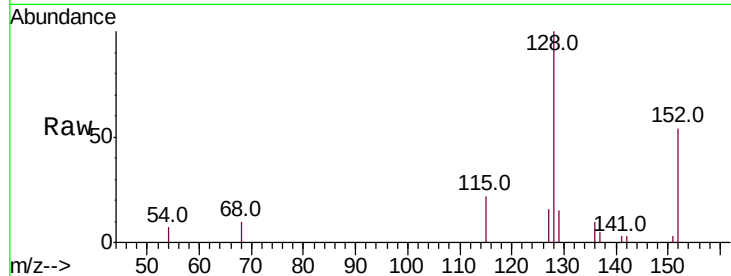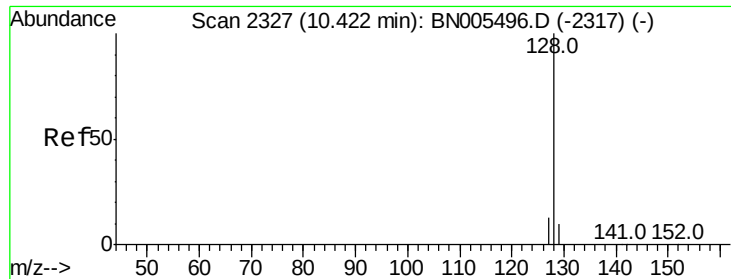

#3

Naphthalene

Concen: 0.168 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN005506.D

Acq: 07 May 2019 03:22

Instrument :

BNA_N

ClientSampleId :

A5124

Tot Ion:	128	Resp:	3057
Ion Ratio	Lower	Upper	
128	100		
129	15.1	10.2	15.2
127	15.7	11.8	17.8

Manual Integrations
APPROVED

mohammad
5/8/2019 12:01:07 AM

