

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050720\
 Data File : BN010696.D
 Acq On : 07 May 2020 19:06
 Operator : CG/JU
 Sample : PB128669BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 07 19:36:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 07 12:59:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	364230	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	1569060	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1030879	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	2215929	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	2015564	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	2071092	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	12725	1.83	ng/uL	0.00
5) Phenol-d5	6.77	99	216571	7.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	523777	36.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	670134	27.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	432401	17.83	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	415327	34.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	437199	32.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	770983	29.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	66699	2.20	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	2952535	38.60	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	3463785	36.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	67074	4.50	ng/ul	0.00
58) Fluorene-d10	15.20	176	2629421	38.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	414248	35.79	ng/ul	0.00
71) Anthracene-d10	17.05	188	4209258	41.01	ng/ul	0.00
79) Pyrene-d10	19.36	212	4571908	40.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	4316997	40.19	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	177591	2.236	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050720\
Data File : BN010696.D
Acq On : 07 May 2020 19:06
Operator : CG/JU
Sample : PB128669BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 07 19:36:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 07 12:59:30 2020
Response via : Initial Calibration

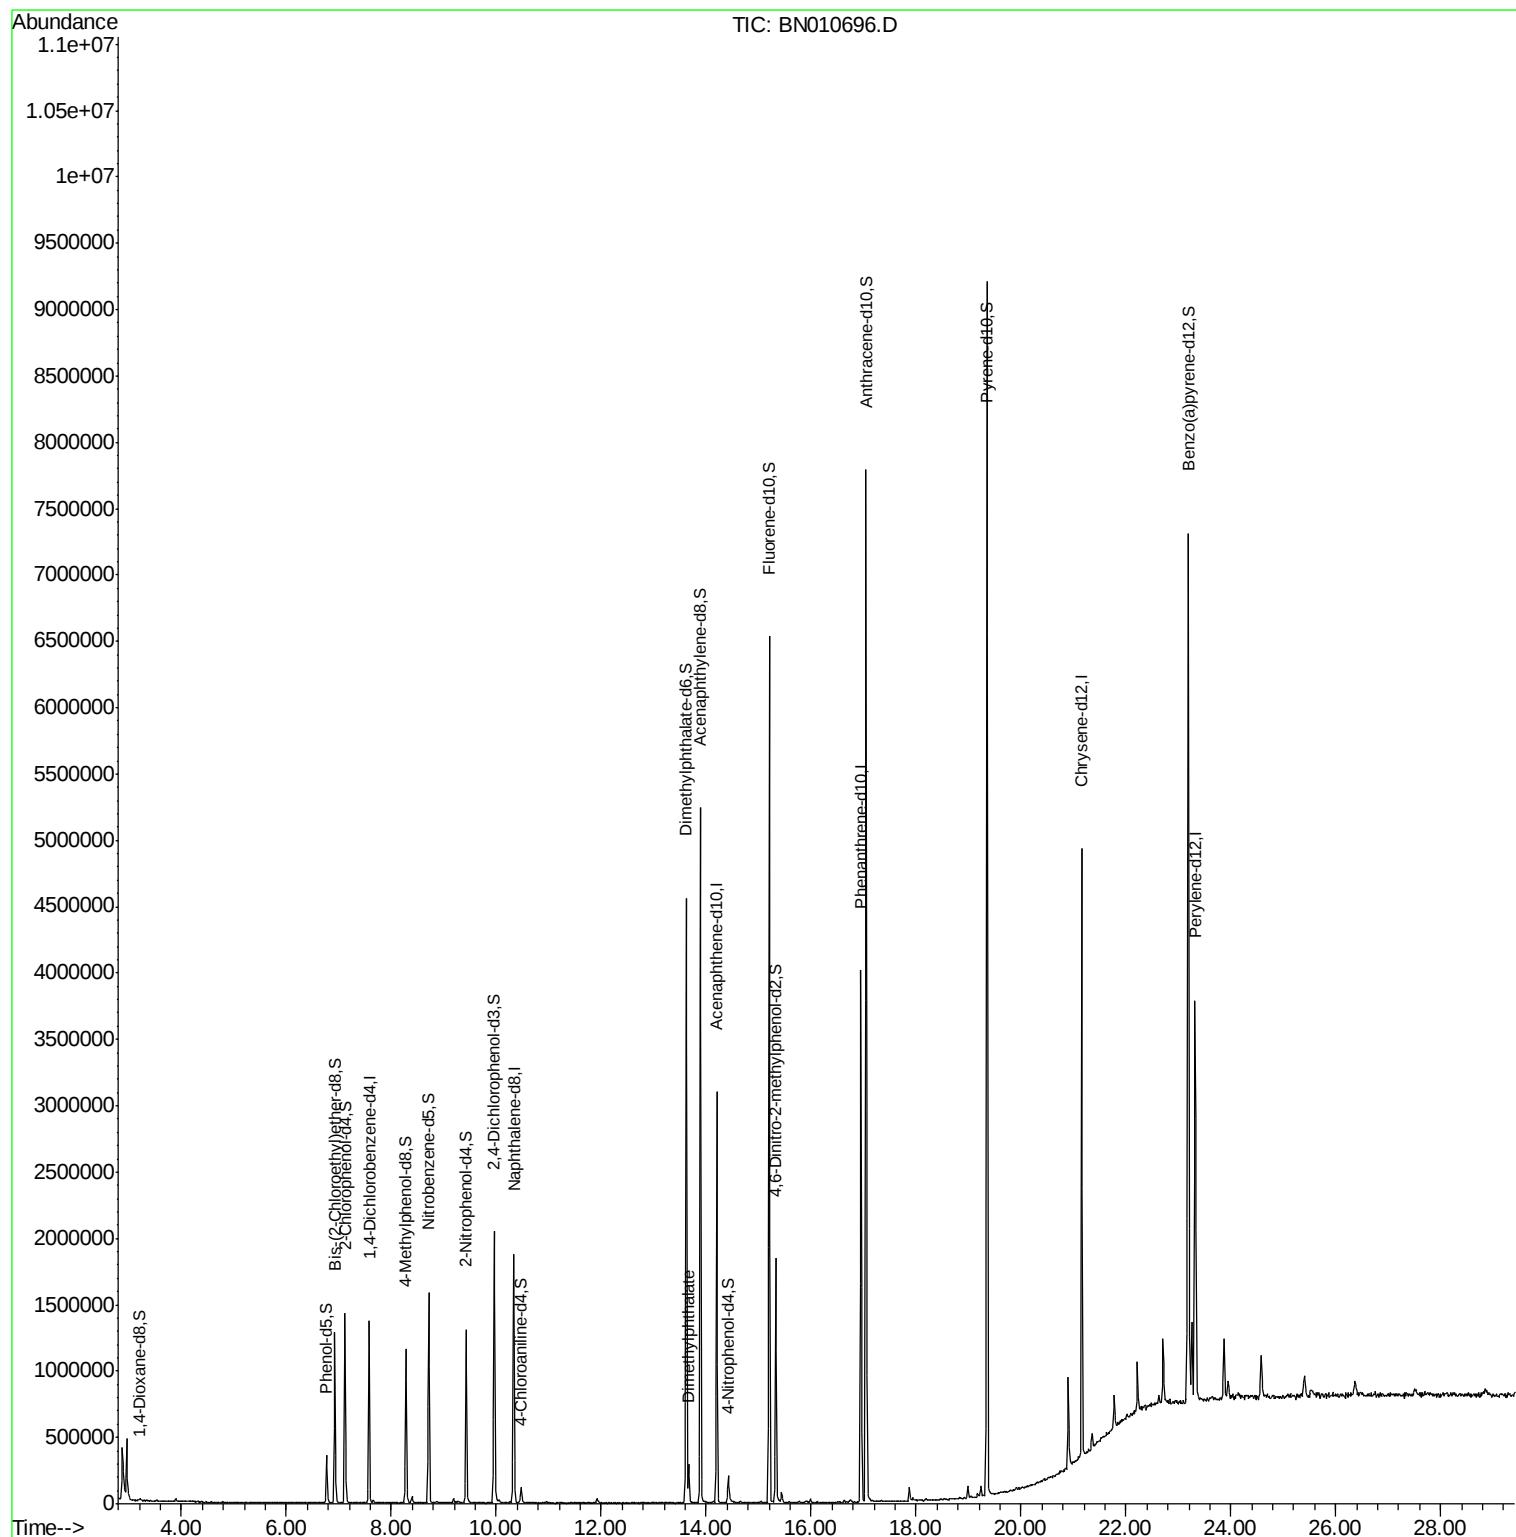

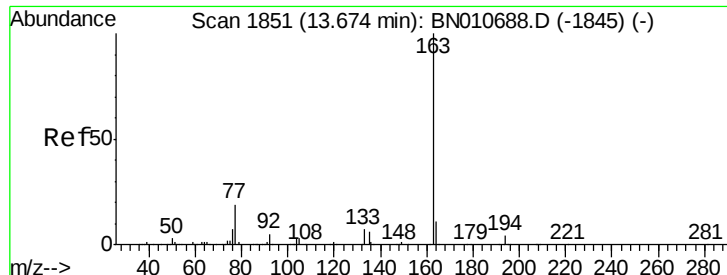

#45

Dimethylphthalate

Concen: 2.236 ng/ul

RT: 13.67 min Scan# 1850

Delta R.T. -0.01 min

Lab File: BN010696.D

Acq: 07 May 2020 19:06

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 177591

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.8 8.0 12.0

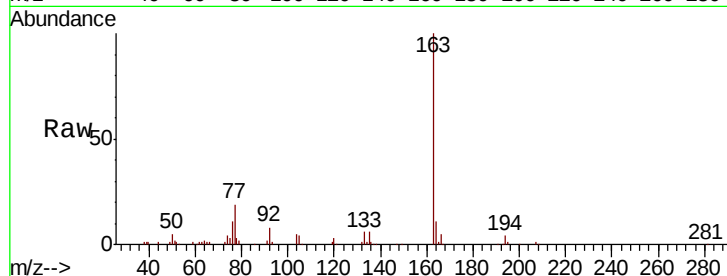

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

