

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050819\
 Data File : BN005541.D
 Acq On : 08 May 2019 20:33
 Operator : JU/SJ
 Sample : PB119645BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 09 02:33:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 07 05:36:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	272495	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1198593	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	776195	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	1864994	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	1728167	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	1560276	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	33904	6.01	ng/uL	0.00
5) Phenol-d5	6.77	99	671098	31.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	393320	29.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	559911	34.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	568132	33.96	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	304035	41.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	346680	46.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	587346	34.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	837985	47.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	2180502	38.70	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	2651860	38.32	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	314747	35.38	ng/ul	0.00
57) Fluorene-d10	15.22	176	1881345	39.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	304974	36.36	ng/ul	0.00
70) Anthracene-d10	17.07	188	3164825	40.48	ng/ul	0.00
78) Pyrene-d10	19.39	212	3583480	40.53	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	2722655	39.93	ng/ul	0.00

Target Compounds


				Ovalue		
15) N-Nitroso-di-n-propylamine	8.29	70	14374	1.004	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050819\
Data File : BN005541.D
Acq On : 08 May 2019 20:33
Operator : JU/SJ
Sample : PB119645BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 09 02:33:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 07 05:36:07 2019
Response via : Initial Calibration

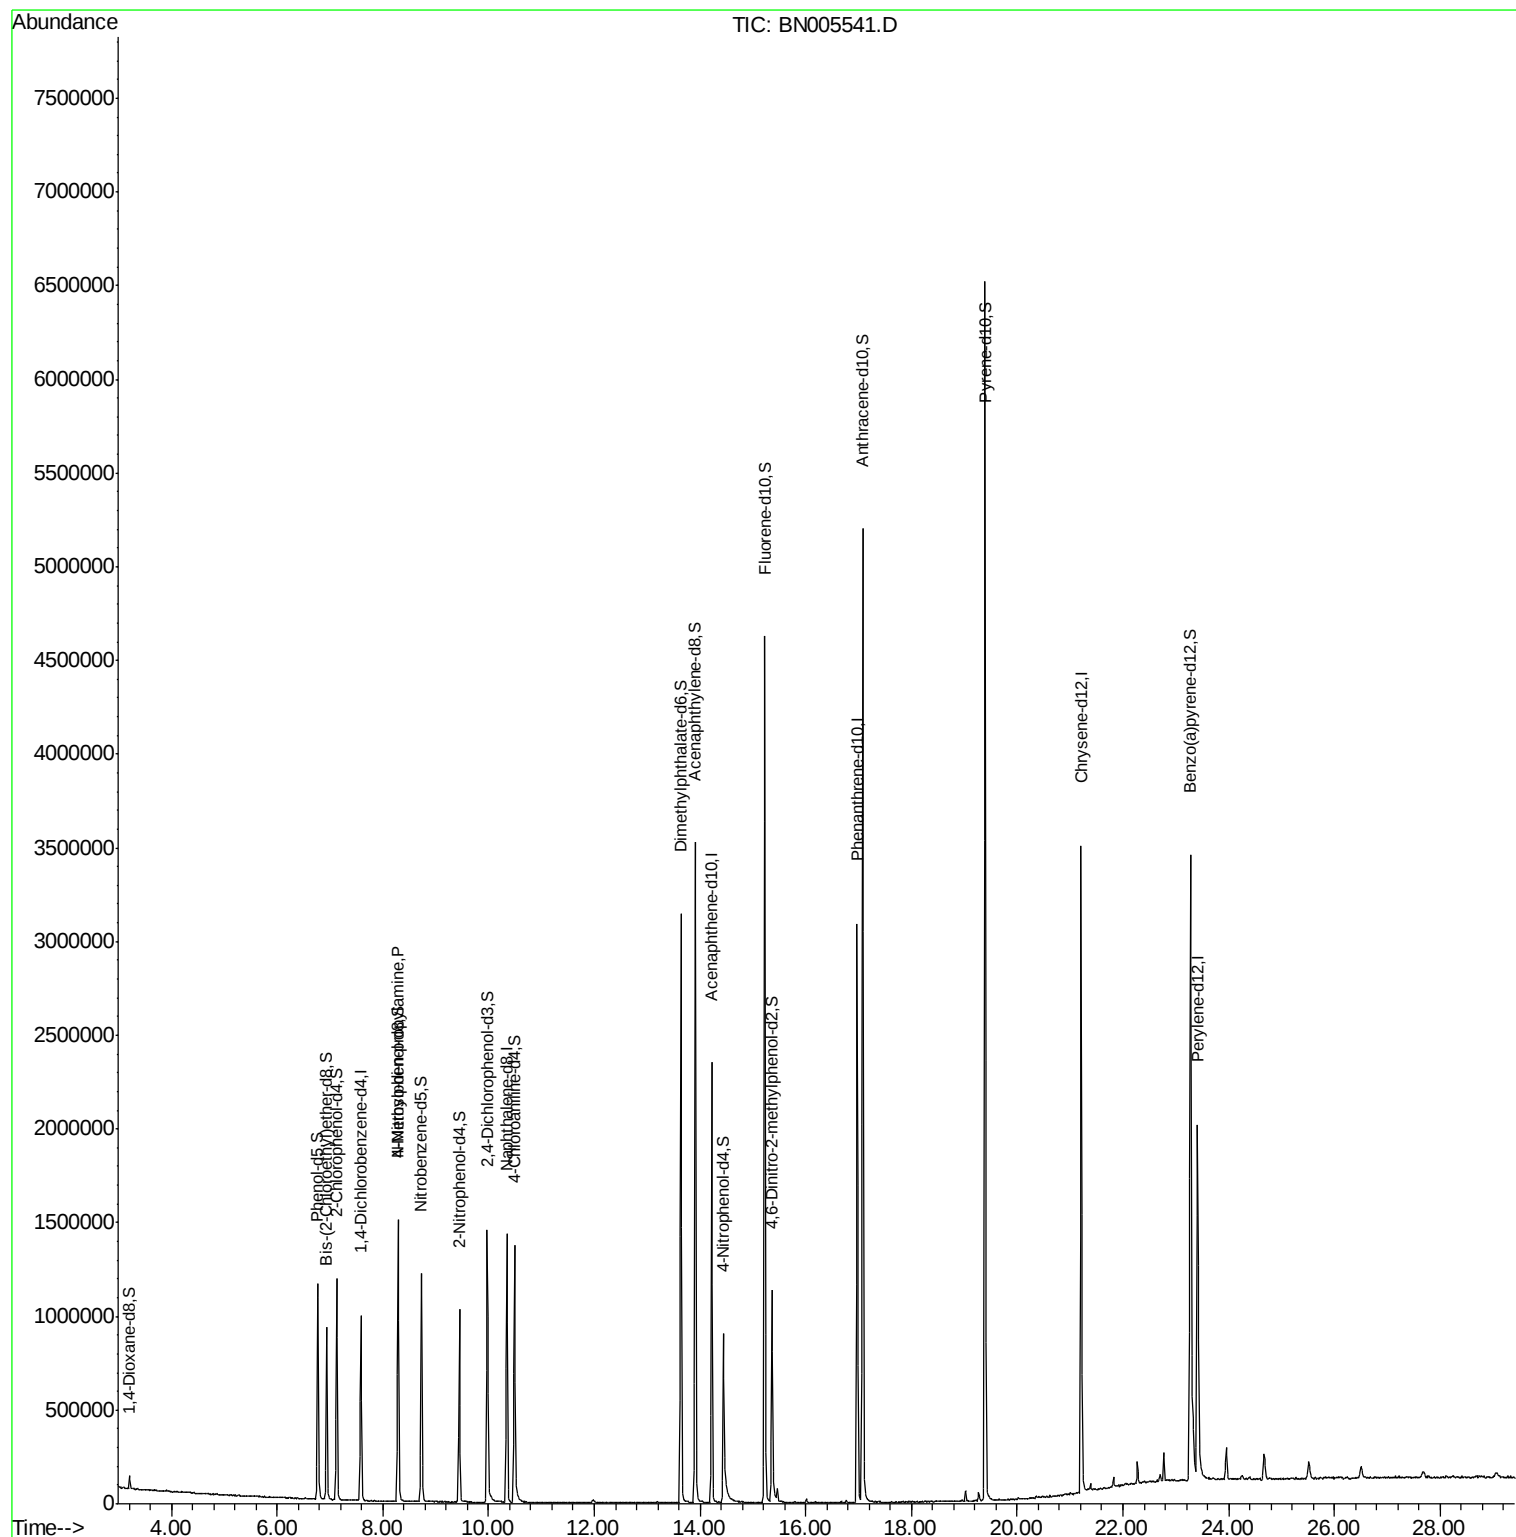

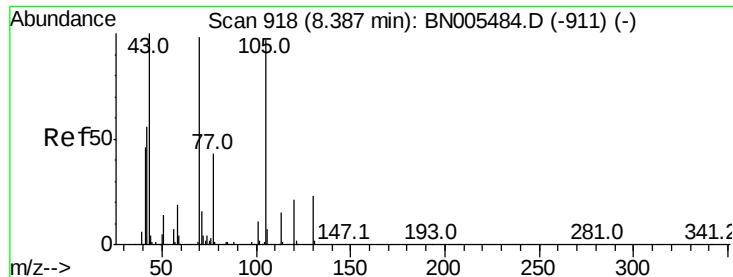

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.004 ng/ul
 RT: 8.29 min Scan# 901
 Delta R.T. -0.10 min
 Lab File: BN005541.D
 Acq: 08 May 2019 20:33

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 14374
 Ion Ratio Lower Upper
 70 100
 42 340.3 53.8 80.8#
 101 0.0 7.7 11.5#
 130 0.0 15.0 22.4#

