

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050819\
 Data File : BN005549.D
 Acq On : 09 May 2019 01:12
 Operator : JU/SJ
 Sample : K2604-10 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 09 02:35:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 07 05:36:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	344866	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1497350	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	918623	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2022978	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	1377654	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	1484212	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	1876	0.26	ng/uL	0.00
5) Phenol-d5	6.78	99	47647	1.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	29295	1.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	41408	2.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	40006	1.89	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	22167	2.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	21356	2.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	39517	1.85	ng/ul	0.02
29) 4-Chloroaniline-d4	10.51	131	31151	1.41	ng/ul	0.02
43) Dimethylphthalate-d6	13.64	166	155173	2.33	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	189222	2.31	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	983	0.09	ng/ul	0.00
57) Fluorene-d10	15.22	176	137840	2.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	3909	0.43	ng/ul	0.02
70) Anthracene-d10	17.08	188	203242	2.40	ng/ul	0.00
78) Pyrene-d10	19.39	212	197298	2.80	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	149531	2.31	ng/ul	0.00

Target Compounds


					Ovalue	
34) 2-Methylnaphthalene	12.02	142	62692	1.230	ng/ul	96
47) Acenaphthylene	13.94	152	1891380	23.498	ng/ul	99
49) Acenaphthene	14.29	153	212718	3.871	ng/ul	99
58) Fluorene	15.28	166	1236388	20.028	ng/ul	98
60) 4-Nitroaniline	15.28	138	14848	1.117	ng/ul#	11
69) Phenanthrene	17.03	178	7869097	79.871	ng/ul	99
71) Anthracene	17.12	178	3438726	34.262	ng/ul	99
76) Fluoranthene	19.06	202	9024394	82.581	ng/ul	97
79) Pyrene	19.43	202	12655033	142.668	ng/ul	97
82) Benzo(a)anthracene	21.25	228	3507475	40.925	ng/ul	94
84) Chrysene	21.25	228	3507978	44.102	ng/ul	97
87) Benzo(b)fluoranthene	22.77	252	2633530	31.565	ng/ul	98
88) Benzo(k)fluoranthene	22.77	252	2633530	33.050	ng/ul	99
90) Benzo(a)pyrene	23.23	252	1603870	20.452	ng/ul	99
91) Indeno(1,2,3-cd)pyrene	25.60	276	1247777	14.391	ng/ul#	94
92) Dibenzo(a,h)anthracene	25.59	278	205002	2.786	ng/ul#	82
93) Benzo(g,h,i)perylene	26.27	276	1238851	17.280	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050819\
Data File : BN005549.D
Acq On : 09 May 2019 01:12
Operator : JU/SJ
Sample : K2604-10 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 09 02:35:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 07 05:36:07 2019
Response via : Initial Calibration




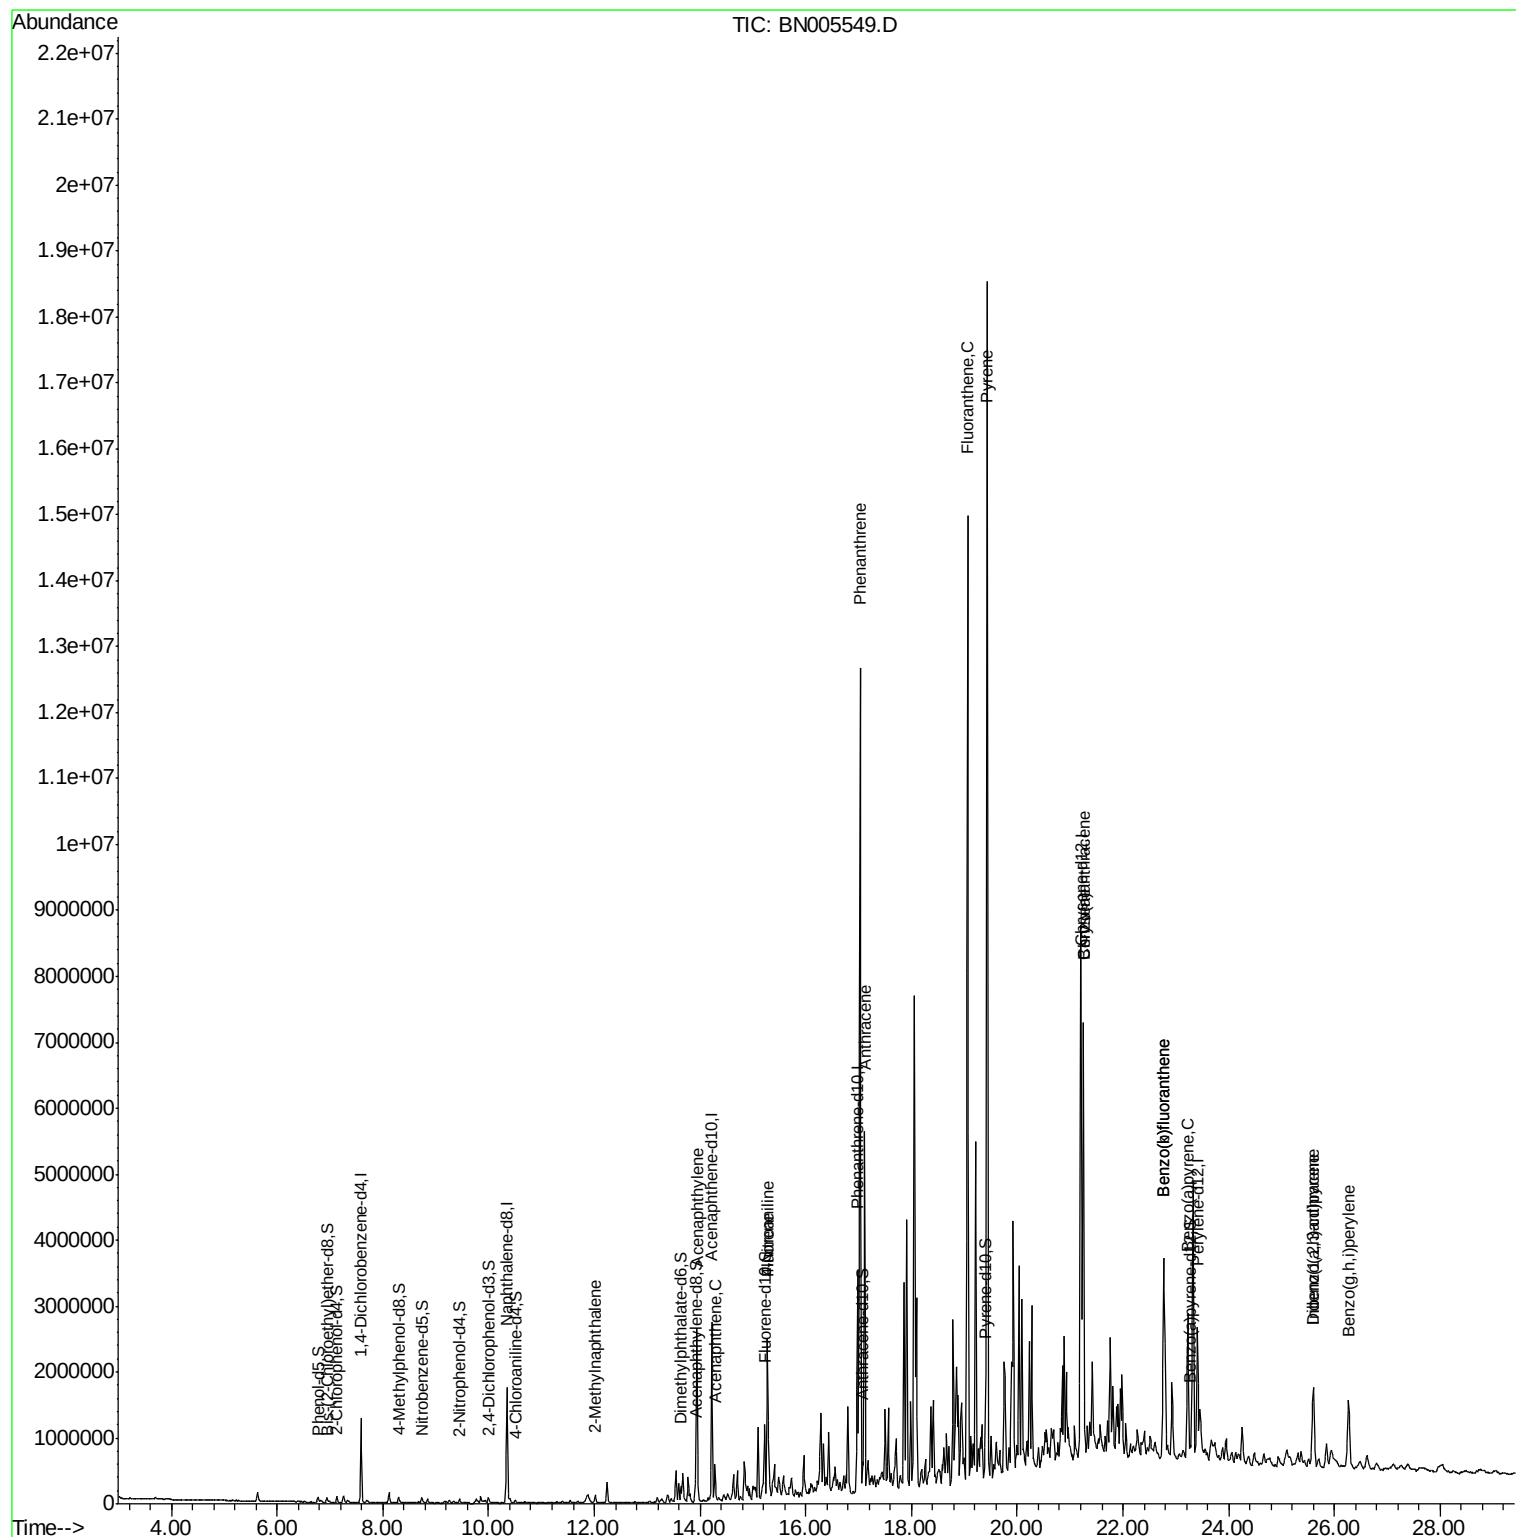


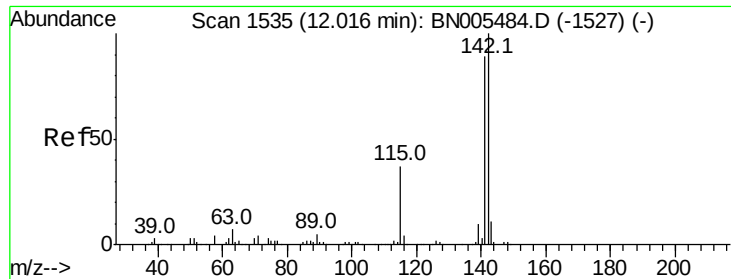

#34
2-Methylnaphthalene
Concen: 1.230 ng/ul
RT: 12.02 min Scan# 1535
Delta R.T. -0.00 min
Lab File: BN005549.D
Acq: 09 May 2019 01:12




Instrument :
BNA_N
ClientSampleId :


Tot Ion:142 Resp: 62692
Ion Ratio Lower Upper
142 100
141 86.6 72.0 108.0

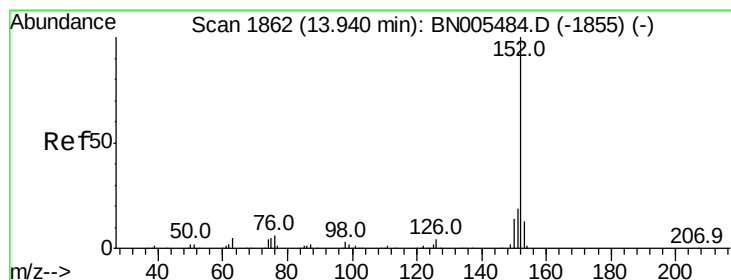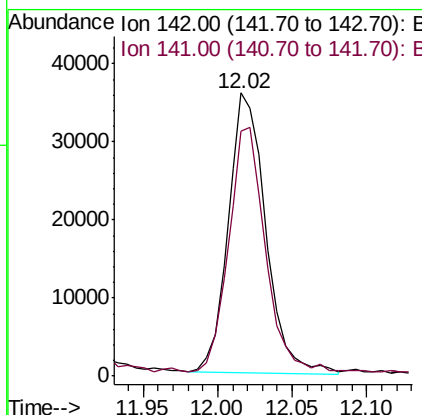

#47
Acenaphthylene
Concen: 23.498 ng/ul
RT: 13.94 min Scan# 1862
Delta R.T. -0.00 min
Lab File: BN005549.D
Acq: 09 May 2019 01:12

Tgt Ion:152 Resp: 1891380
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.8
153 13.2 9.8 14.8

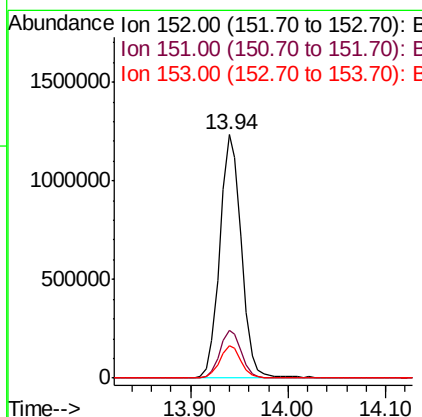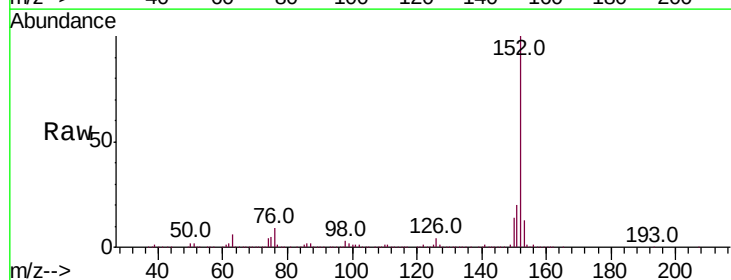



#49

Acenaphthene

Concen: 3.871 ng/ul

RT: 14.29 min Scan# 1921

Delta R.T. -0.00 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12

Instrument :

BNA_N

ClientSampleId :


Tot Ion:153 Resp: 212718

Ion Ratio Lower Upper

153 100

152 47.1 37.4 56.0




154 89.7 71.2 106.8

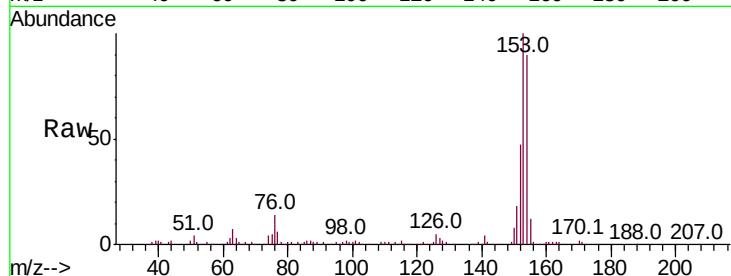

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

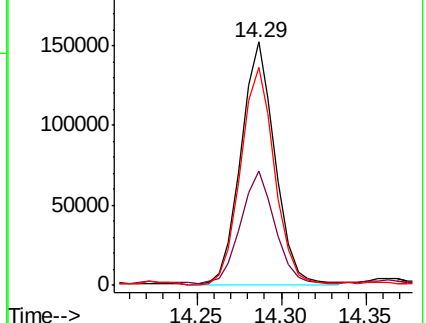

#58

Fluorene

Concen: 20.028 ng/ul

RT: 15.28 min Scan# 2090

Delta R.T. -0.00 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12


Tgt Ion:166 Resp: 1236388

Ion Ratio Lower Upper

166 100

165 98.1 80.0 120.0



167 13.5 10.7 16.1




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E



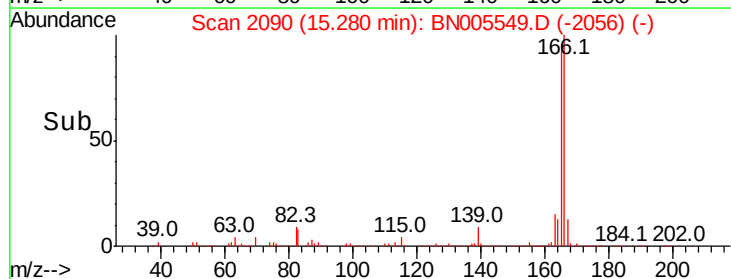
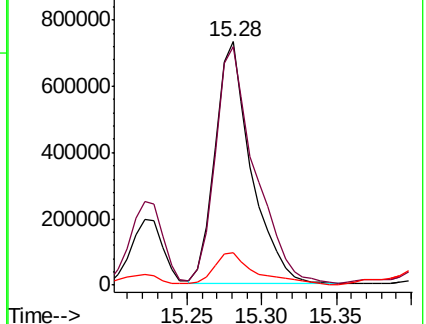




#60
4-Nitroaniline
Concen: 1.117 ng/ul
RT: 15.28 min Scan# 2090
Delta R.T. -0.02 min
Lab File: BN005549.D
Acq: 09 May 2019 01:12




Instrument :
BNA_N
ClientSampled :


Tot Ion:138 Resp: 14848
Ion Ratio Lower Upper
138 100
92 0.0 45.3 67.9#
108 0.0 73.2 109.8#

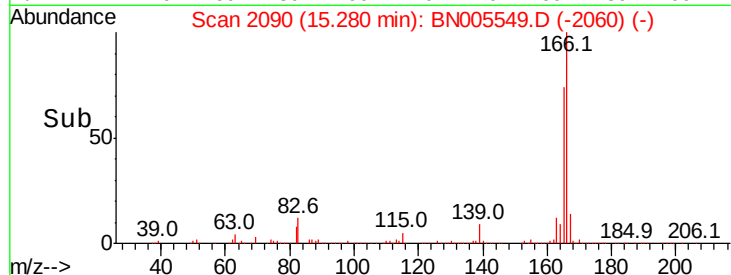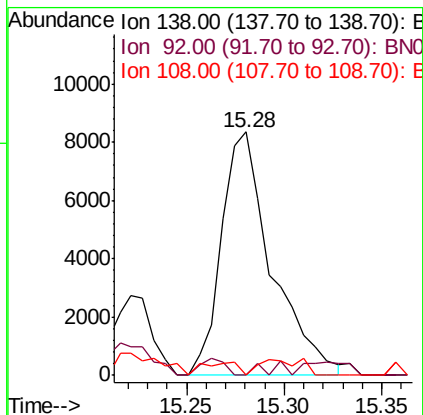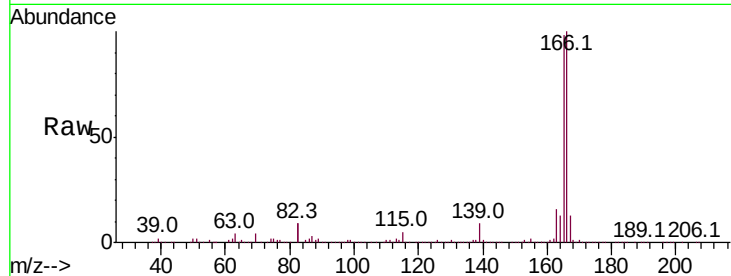

#69
Phenanthrene
Concen: 79.871 ng/ul
RT: 17.03 min Scan# 2387
Delta R.T. 0.01 min
Lab File: BN005549.D
Acq: 09 May 2019 01:12

Tgt Ion:178 Resp: 7869097
Ion Ratio Lower Upper
178 100
179 16.0 12.2 18.4
176 19.5 15.1 22.7

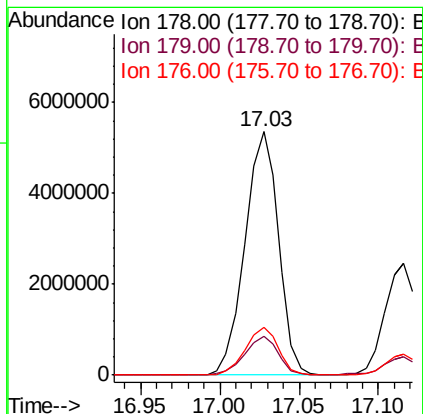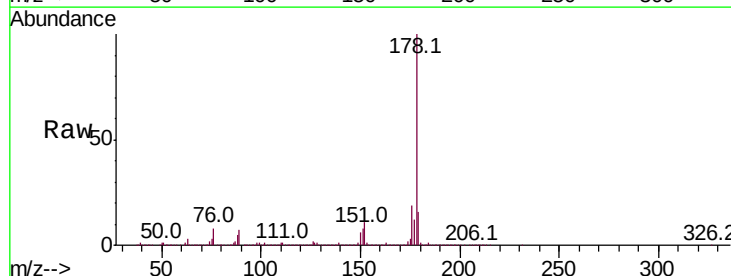


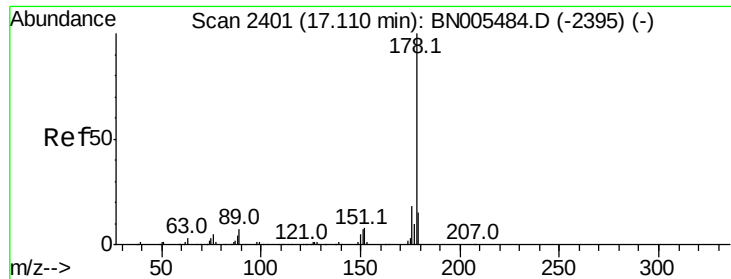




#71
 Anthracene
 Concen: 34.262 ng/ul
 RT: 17.12 min Scan# 2402
 Delta R.T. 0.01 min
 Lab File: BN005549.D
 Acq: 09 May 2019 01:12

Instrument :
 BNA_N
 ClientSampled :

Tot Ion:178 Resp: 3438726
 Ion Ratio Lower Upper
 178 100
 179 15.8 12.3 18.5
 176 18.3 15.1 22.7

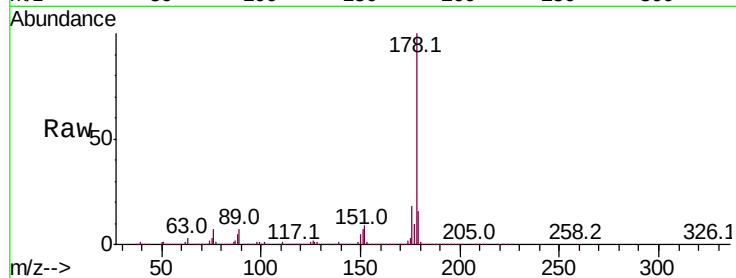


Abundance Ion 178.00 (177.70 to 178.70): E
 6000000 Ion 179.00 (178.70 to 179.70): E
 5000000 Ion 176.00 (175.70 to 176.70): E

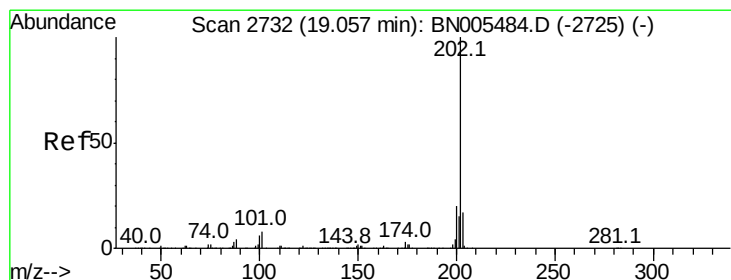
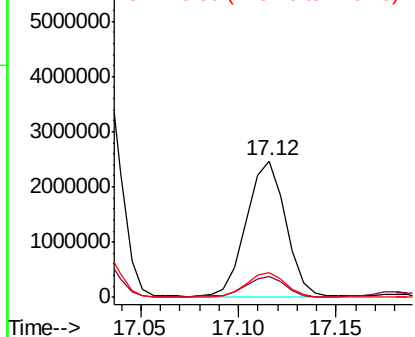



#76
 Fluoranthene
 Concen: 82.581 ng/ul
 RT: 19.06 min Scan# 2733
 Delta R.T. 0.01 min
 Lab File: BN005549.D
 Acq: 09 May 2019 01:12

Tgt Ion:202 Resp: 9024394
 Ion Ratio Lower Upper
 202 100
 101 9.5 8.6 12.8
 100 7.1 6.3 9.5



Abundance Ion 202.00 (201.70 to 202.70): E
 8000000 Ion 101.00 (100.70 to 101.70): E
 6000000 Ion 100.00 (99.70 to 100.70): B

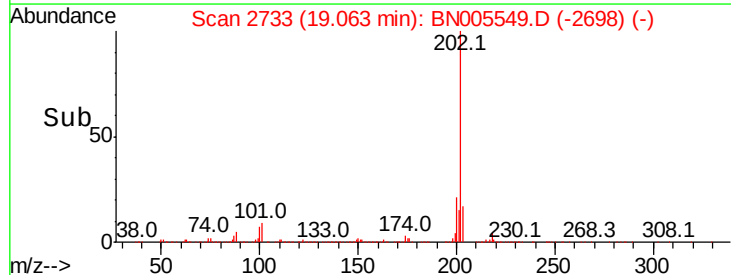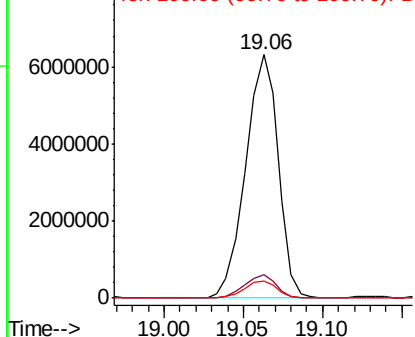

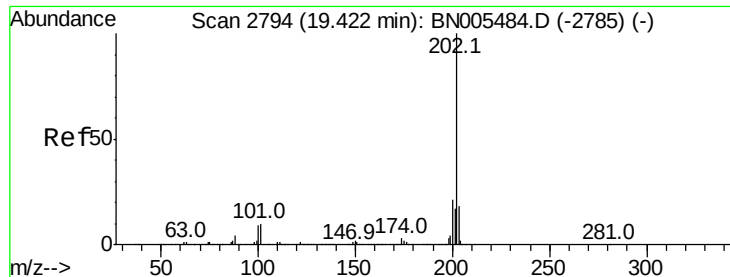

#79

Pvrene

Concen: 142.668 ng/ul

RT: 19.43 min Scan# 2796

Delta R.T. 0.01 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12

Instrument :

BNA_N

ClientSampled :


Tot Ion:202 Resp:12655033

Ion Ratio Lower Upper

202 100

101 11.5 10.3 15.5




100 9.3 7.9 11.9

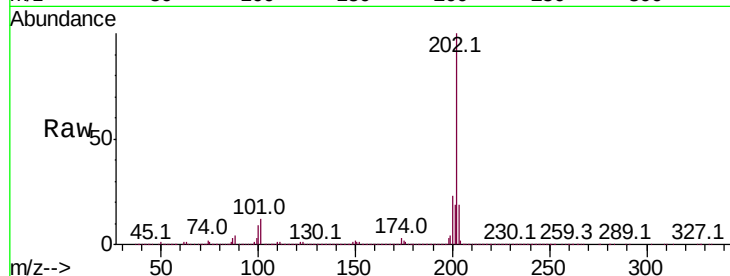

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

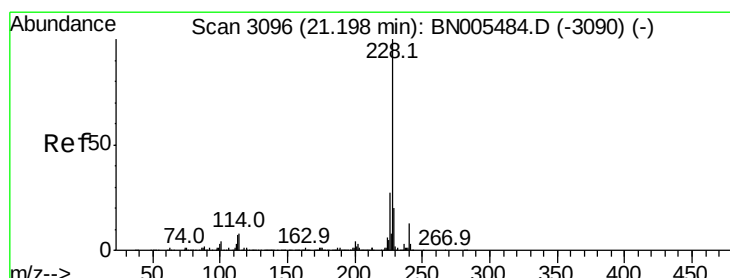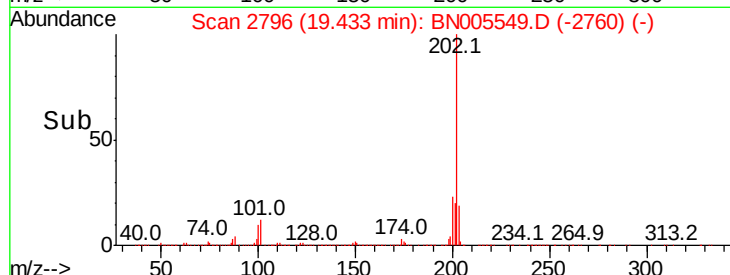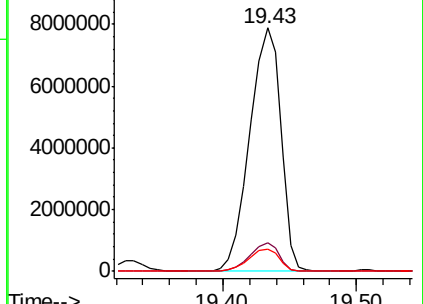

#82

Benzo(a)anthracene

Concen: 40.925 ng/ul

RT: 21.25 min Scan# 3105

Delta R.T. 0.05 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12


Tgt Ion:228 Resp: 3507475

Ion Ratio Lower Upper

228 100

229 20.7 15.8 23.6



226 31.2 21.4 32.2

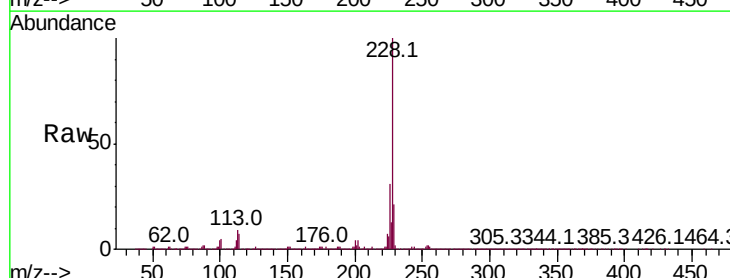


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

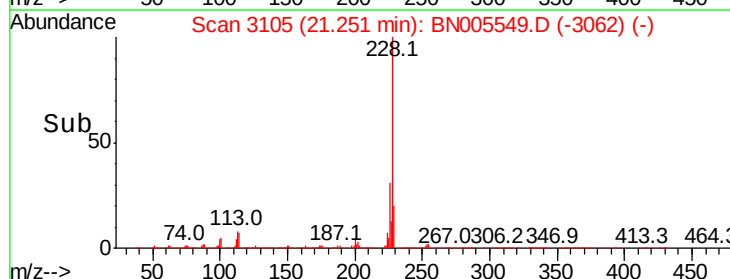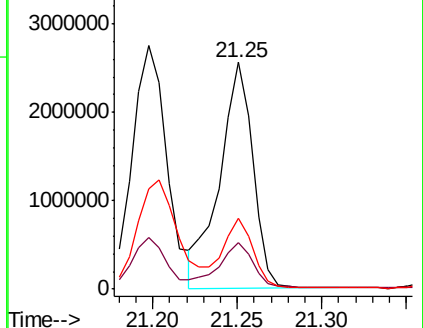

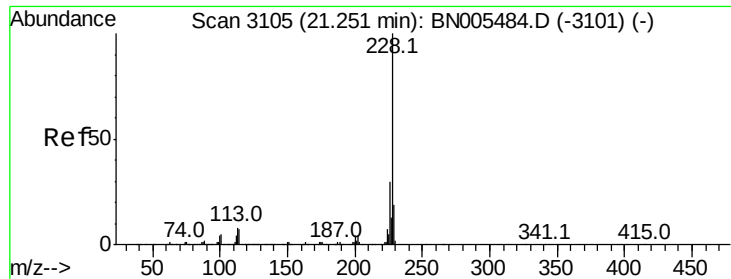

#84

Chrysene

Concen: 44.102 ng/ul

RT: 21.25 min Scan# 3105

Delta R.T. -0.00 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12


Instrument :

BNA_N

ClientSampleId :

Tot Ion:228 Resp: 3507978

Ion	Ratio	Lower	Upper
228	100		
226	31.2	24.0	36.0
229	20.7	15.4	23.0



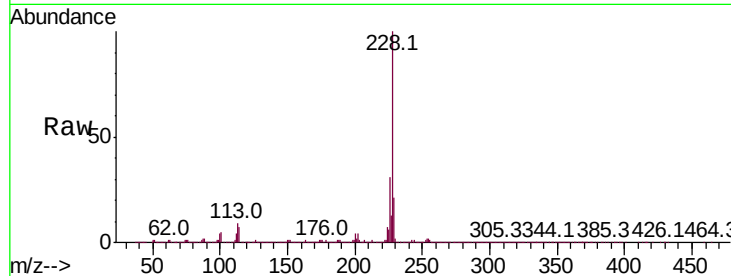


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

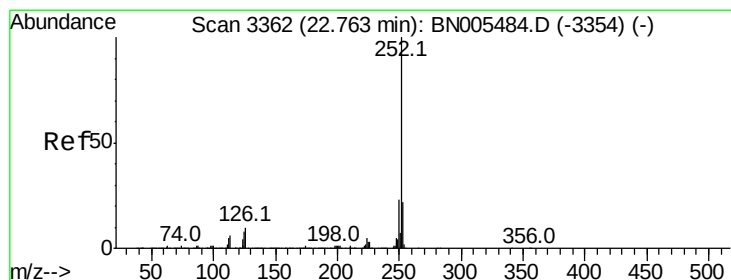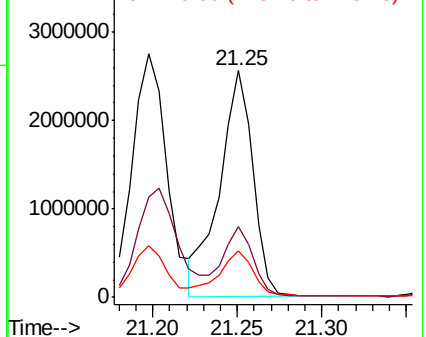

#87

Benzo(b)fluoranthene

Concen: 31.565 ng/ul

RT: 22.77 min Scan# 3363


Delta R.T. 0.01 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12

Tgt Ion:252 Resp: 2633530

Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.7	26.5
125	9.1	8.4	12.6






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

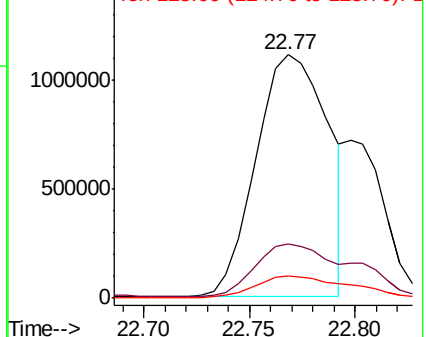



#88

Benzo(k)fluoranthene

Concen: 33.050 ng/ul

RT: 22.77 min Scan# 3363

Delta R.T. -0.04 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12

Instrument :

BNA_N

ClientSampled :


Tot Ion:252 Resp: 2633530

Ion Ratio Lower Upper

252 100

253 22.3 17.4 26.0




125 9.1 7.5 11.3



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

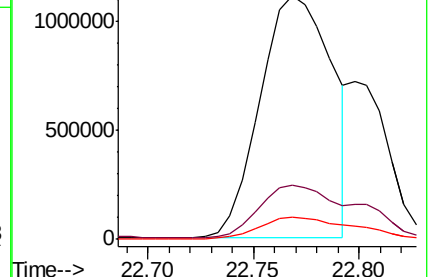

#90

Benzo(a)pyrene

Concen: 20.452 ng/ul

RT: 23.23 min Scan# 3441

Delta R.T. -0.10 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12


Tgt Ion:252 Resp: 1603870

Ion Ratio Lower Upper

252 100

253 22.1 17.3 25.9



125 10.8 8.6 13.0




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

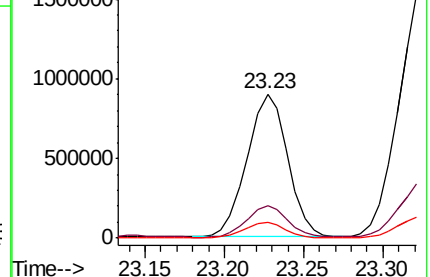




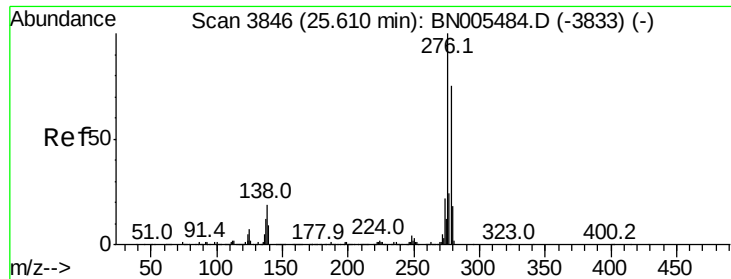


#91

Indeno(1,2,3-cd)pyrene
Concen: 14.391 ng/ul
RT: 25.60 min Scan# 3844
Delta R.T. -0.01 min
Lab File: BN005549.D
Acq: 09 May 2019 01:12

Instrument :
BNA_N
ClientSampleId :




Tot Ion:276 Resp: 1247777
Ion Ratio Lower Upper
276 100
138 16.6 17.9 26.9#
277 24.3 19.7 29.5

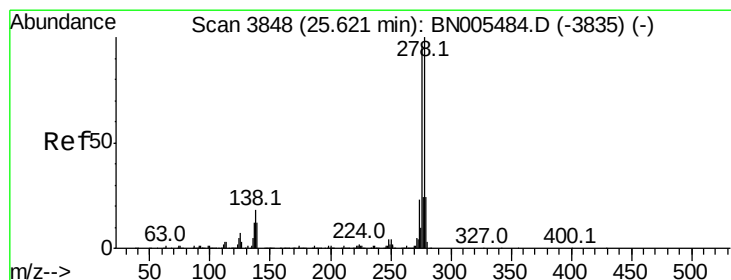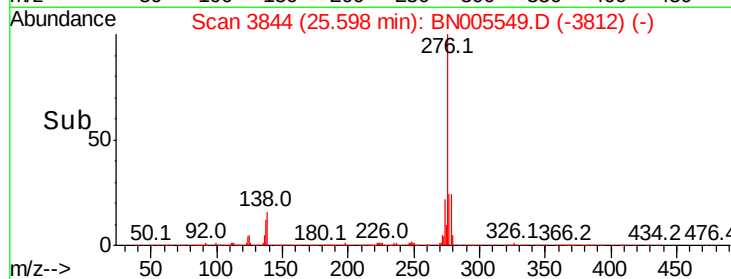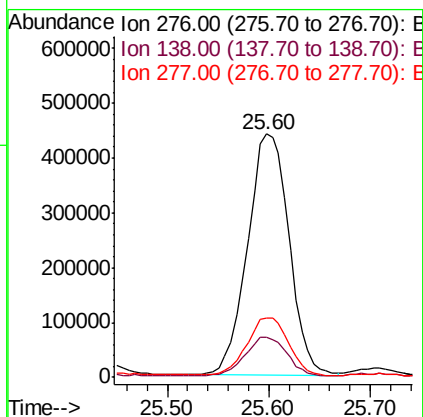


#92

Dibenzo(a,h)anthracene
Concen: 2.786 ng/ul
RT: 25.59 min Scan# 3843
Delta R.T. -0.03 min
Lab File: BN005549.D
Acq: 09 May 2019 01:12

Tgt Ion:278 Resp: 205002
Ion Ratio Lower Upper
278 100
139 0.0 13.1 19.7#
279 22.3 19.4 29.0

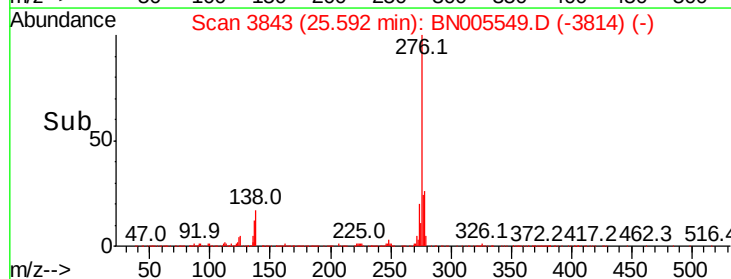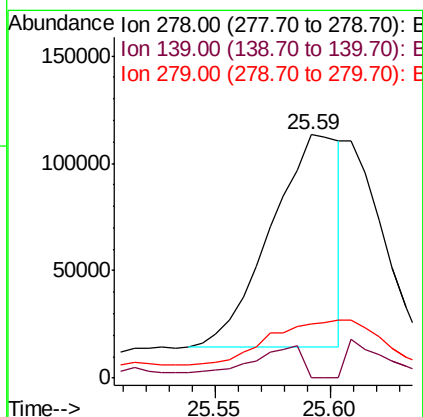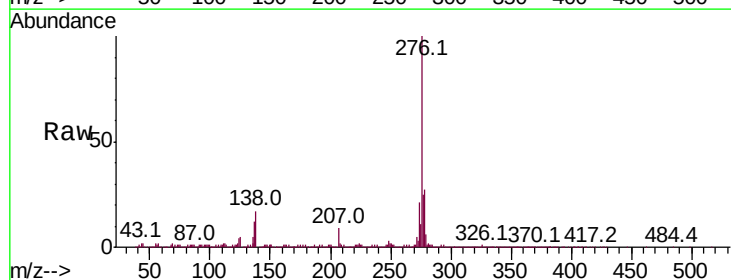



#93

Benzo(a,h,i)perylene

Concen: 17.280 ng/ul

RT: 26.27 min Scan# 3958

Delta R.T. -0.01 min

Lab File: BN005549.D

Acq: 09 May 2019 01:12

Instrument :

BNA_N

ClientSampleId :

Tot Ion:276 Resp: 1238851

Ion Ratio Lower Upper

276 100

138 16.3 16.7 25.1#

277 24.5 18.2 27.2

