

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050819\
 Data File : BN005534.D
 Acq On : 08 May 2019 15:56
 Operator : JU/SJ
 Sample : K2606-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5145

Quant Time: May 08 17:19:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 07 05:36:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	263866	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1150807	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	753046	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	1790346	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	1650880	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	1472892	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	24614	4.50	ng/uL	0.00
5) Phenol-d5	6.77	99	605392	29.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	347711	26.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	493873	31.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	530733	32.76	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	276159	38.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	321905	44.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	565512	34.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	789460	46.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	2155933	39.44	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	2604322	38.79	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	345769	40.06	ng/ul	0.00
57) Fluorene-d10	15.22	176	1855030	40.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	300466	37.31	ng/ul	0.00
70) Anthracene-d10	17.08	188	3084990	41.10	ng/ul	0.00
78) Pyrene-d10	19.39	212	3477426	41.18	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	2715076	42.18	ng/ul	0.00
Target Compounds						
6) Phenol	6.80	94	32645	1.531	ng/ul#	88
44) Dimethylphthalate	13.69	163	603126	11.073	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050819\
Data File : BN005534.D
Acq On : 08 May 2019 15:56
Operator : JU/SJ
Sample : K2606-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5145

Quant Time: May 08 17:19:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 07 05:36:07 2019
Response via : Initial Calibration

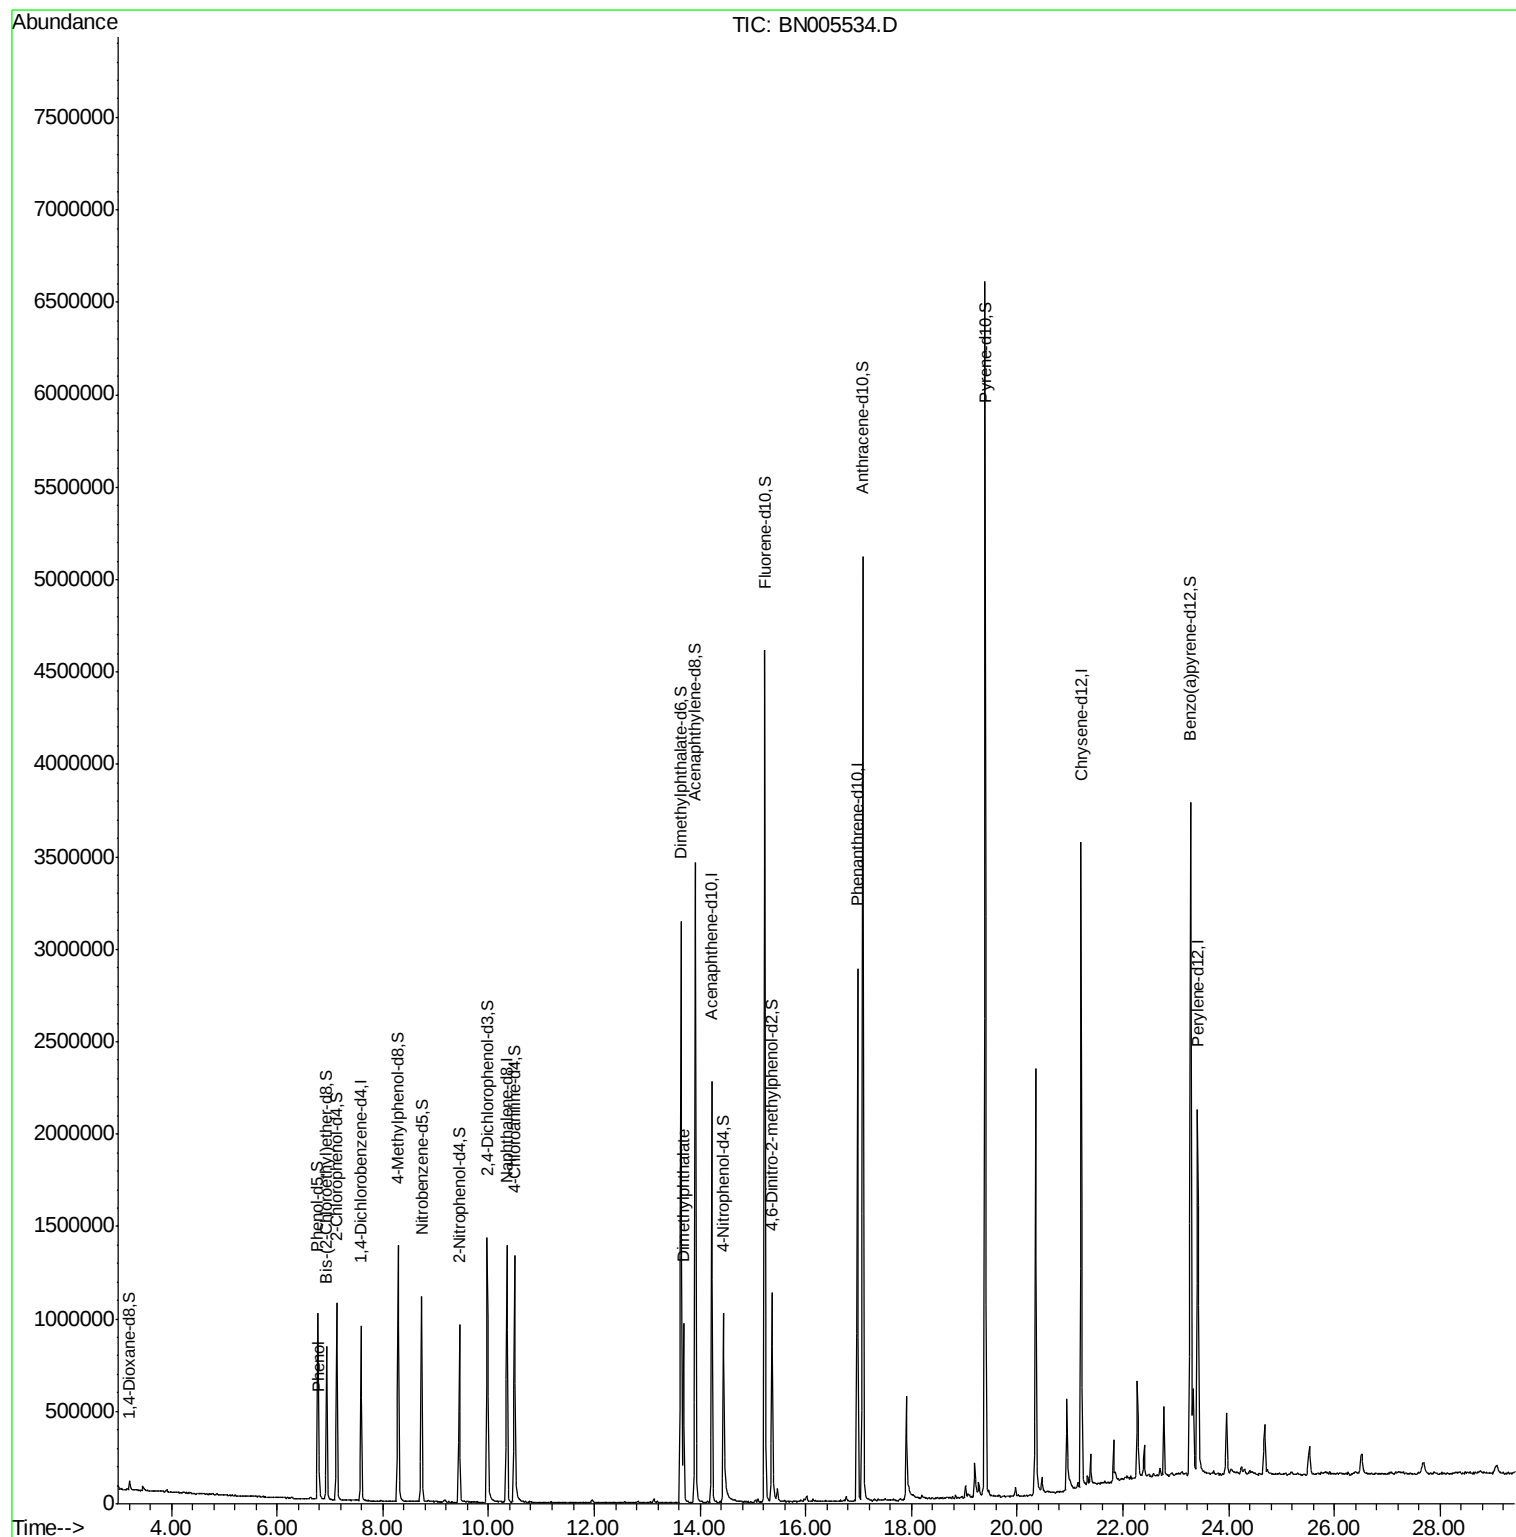

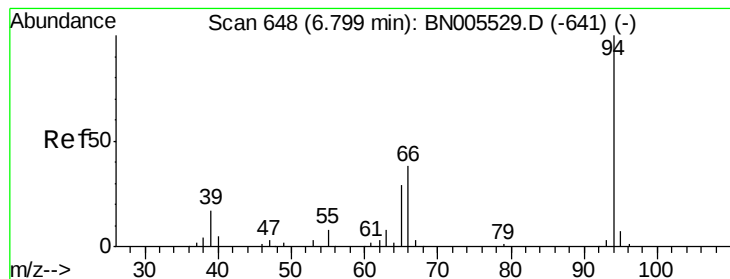





#6

Phenol

Concen: 1.531 ng/ul
 RT: 6.80 min Scan# 648
 Delta R.T. -0.00 min
 Lab File: BN005534.D
 Acq: 08 May 2019 15:56

Instrument :
 BNA_N
 ClientSampleId :
 A5145

Tot Ion: 94 Resp: 32645
 Ion Ratio Lower Upper
 94 100
 65 33.0 24.2 36.4
 66 53.2 33.8 50.6#

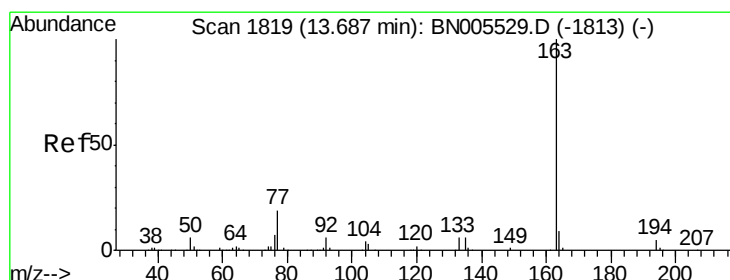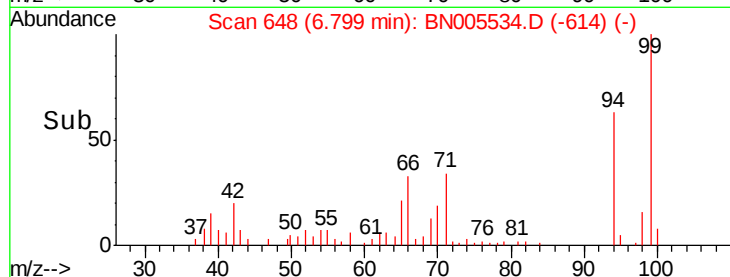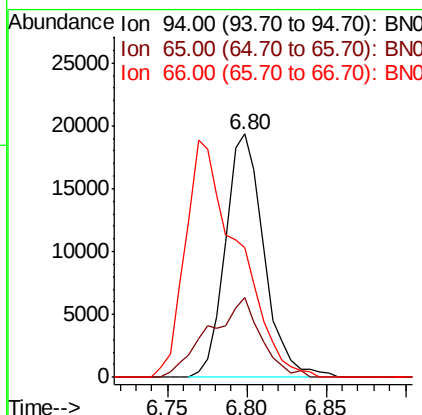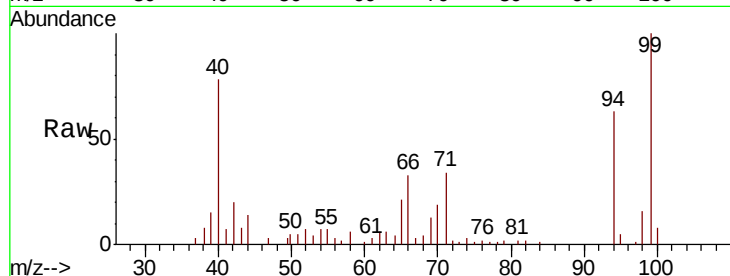

#44

Dimethylphthalate

Concen: 11.073 ng/ul
 RT: 13.69 min Scan# 1819
 Delta R.T. -0.00 min
 Lab File: BN005534.D
 Acq: 08 May 2019 15:56

Tgt Ion:163 Resp: 603126
 Ion Ratio Lower Upper
 163 100
 194 4.4 3.4 5.0
 164 10.2 8.1 12.1

