

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050819\
 Data File : BN005537.D
 Acq On : 08 May 2019 17:40
 Operator : JU/SJ
 Sample : K2602-04DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFH59DL

Manual Integrations
 APPROVED

Sohil
 5/9/2019 2:35:24 PM

Quant Time: May 08 18:16:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 07 05:36:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	258130	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1131433	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	735260	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	1788134	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	1756189	20.00	ng/ul	0.00
85) Perylene-d12	23.41	264	1530926	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	809	0.15	ng/uL	0.00
5) Phenol-d5	6.78	99	24112m	1.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	14599	1.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	20602	1.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	18986	1.20	ng/ul	0.01
19) Nitrobenzene-d5	8.75	128	10774	1.55	ng/ul	0.01
22) 2-Nitrophenol-d4	9.46	143	10764	1.52	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.01	165	22893m	1.41	ng/ul	0.03
29) 4-Chloroaniline-d4	10.53	131	23725m	1.42	ng/ul	0.04
43) Dimethylphthalate-d6	13.65	166	94623	1.77	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	116239	1.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	7011m	0.83	ng/ul	0.06
57) Fluorene-d10	15.23	176	92573	2.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	2515	0.31	ng/ul	0.03
70) Anthracene-d10	17.08	188	157772	2.10	ng/ul	0.00
78) Pyrene-d10	19.39	212	175126	1.95	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	121497	1.82	ng/ul	0.00

Target Compounds

				Ovalue	
83) Bis(2-ethylhexyl)phthalate	21.14	149	2562885	37.178	ng/ul# 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050819\
Data File : BN005537.D
Acq On : 08 May 2019 17:40
Operator : JU/SJ
Sample : K2602-04DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BFH59DL

Manual Integrations
APPROVED

Sohil
5/9/2019 2:35:24 PM

Quant Time: May 08 18:16:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 07 05:36:07 2019
Response via : Initial Calibration

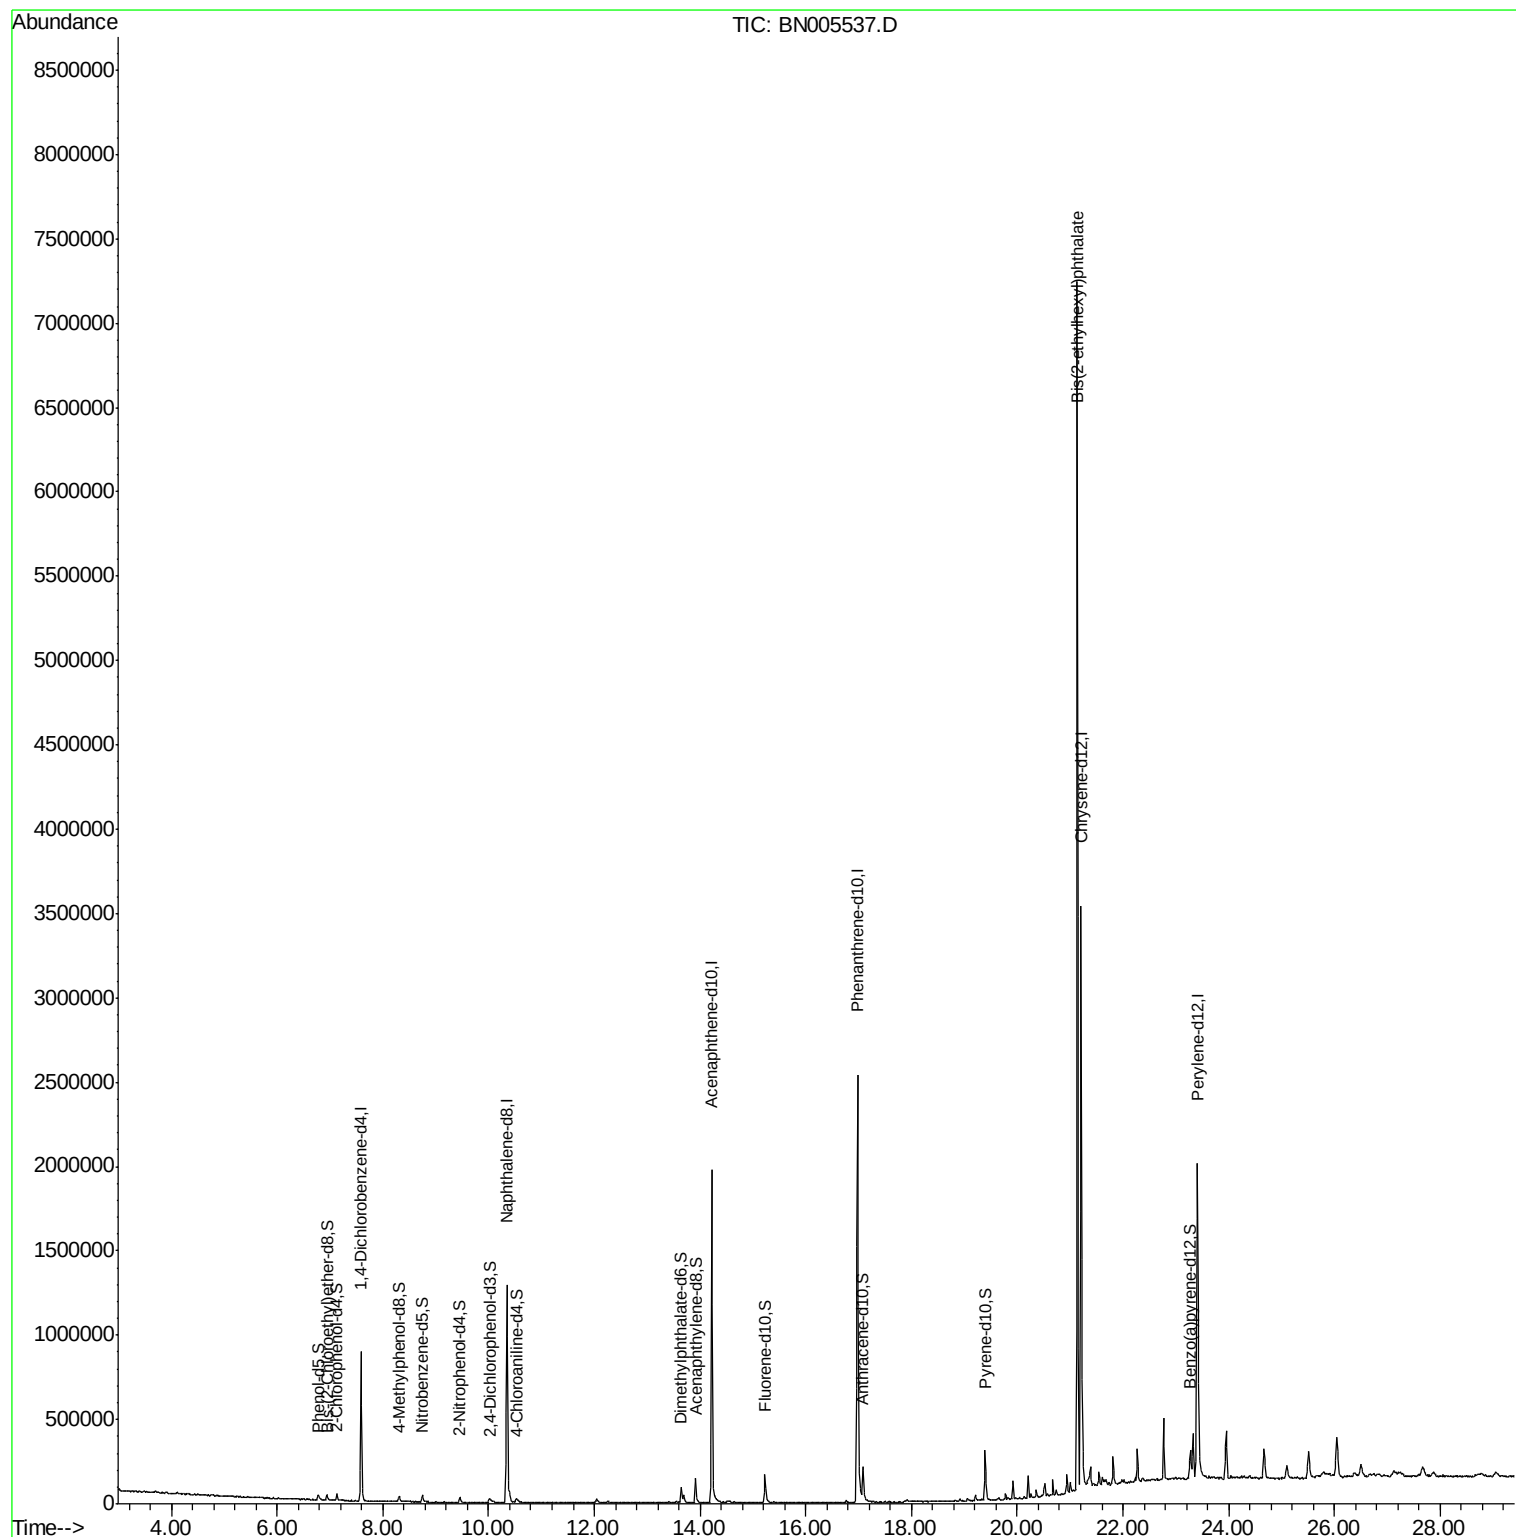

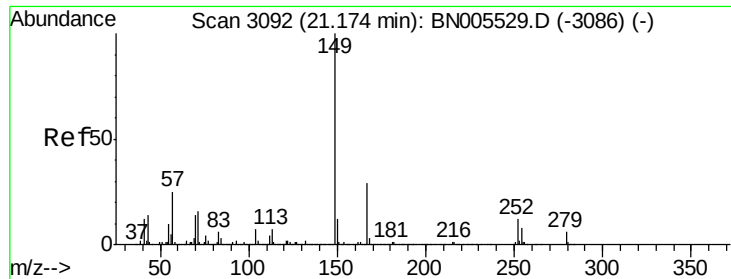

#83

Bis(2-ethylhexyl)phthalate

Concen: 37.178 ng/ul

RT: 21.14 min Scan# 3087

Delta R.T. -0.01 min

Lab File: BN005537.D

Acq: 08 May 2019 17:40

Instrument :

BNA_N

ClientSampleId :

BFH59DL

Tot Ion:149 Resp: 2562885

Ion Ratio Lower Upper

149 100

167 30.3 22.3 33.5

279 5.7 3.3 4.9#

Manual Integrations

APPROVED

Sohil

5/9/2019 2:35:24 PM

