

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050819\
 Data File : BN005553.D
 Acq On : 09 May 2019 03:31
 Operator : JU/SJ
 Sample : K2602-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFH48

Manual Integrations
 APPROVED

Sohil
 5/9/2019 2:35:38 PM

Quant Time: May 09 07:01:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 07 05:36:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	308172	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1331016	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	845932	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	1936100m	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1363340	20.00	ng/ul	-0.01
85) Perylene-d12	23.40	264	1237235	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	18908	2.96	ng/uL	0.00
5) Phenol-d5	6.78	99	461595	19.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	274473	18.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	392747	21.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	382290	20.21	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	209138	25.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	233120	28.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	409774	21.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	471180	24.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	1418041	23.09	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	1708545	22.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	195758	20.19	ng/ul	0.00
57) Fluorene-d10	15.22	176	1216272	23.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	102709m	11.79	ng/ul	0.00
70) Anthracene-d10	17.07	188	1812463	22.33	ng/ul	0.00
78) Pyrene-d10	19.39	212	1963151	28.15	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	1289506	23.85	ng/ul	-0.01

Target Compounds				Ovalue
44) Dimethylphthalate	13.69	163	455836	7.450 ng/ul 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050819\
Data File : BN005553.D
Acq On : 09 May 2019 03:31
Operator : JU/SJ
Sample : K2602-01
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BFH48

Manual Integrations
APPROVED

Sohil
5/9/2019 2:35:38 PM

Quant Time: May 09 07:01:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 07 05:36:07 2019
Response via : Initial Calibration

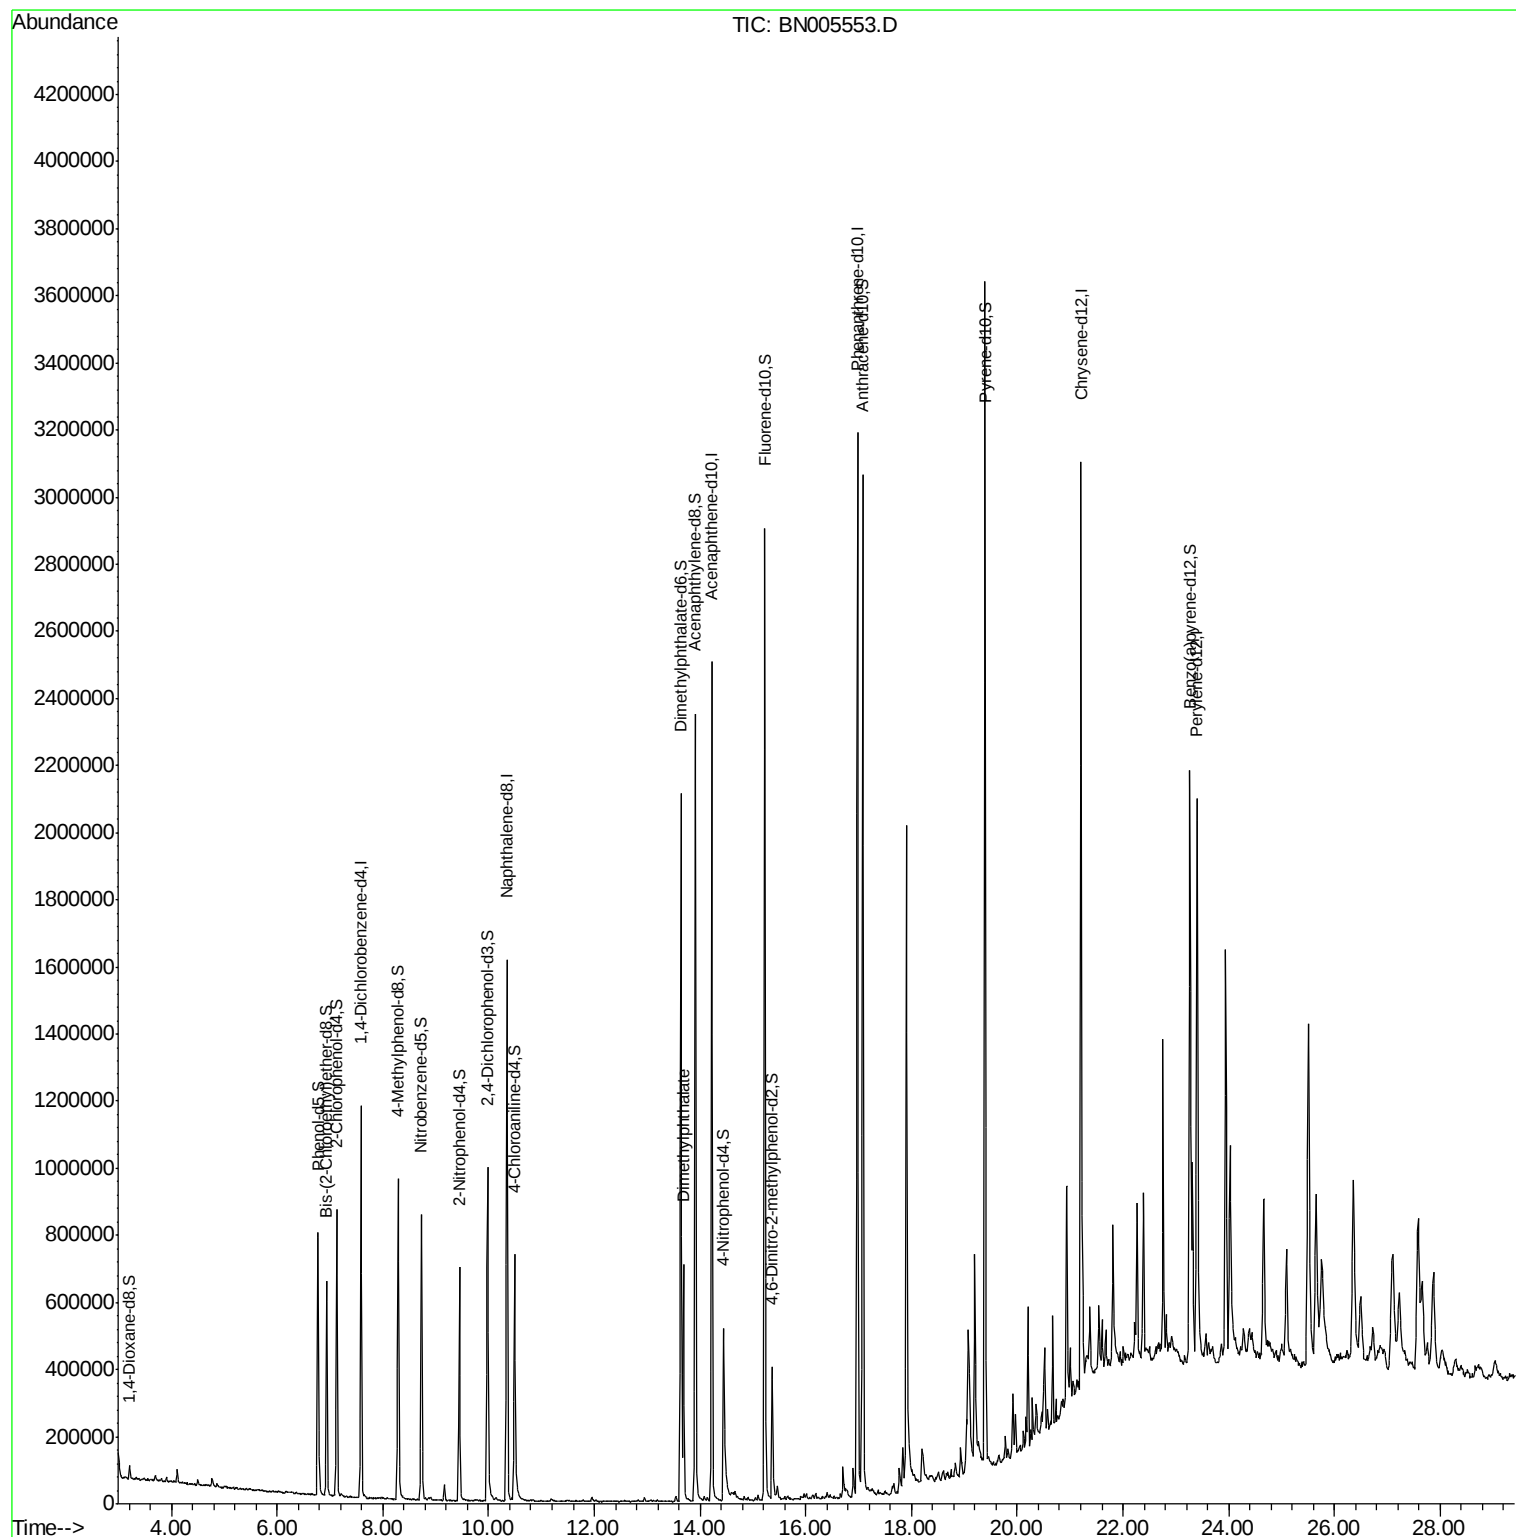

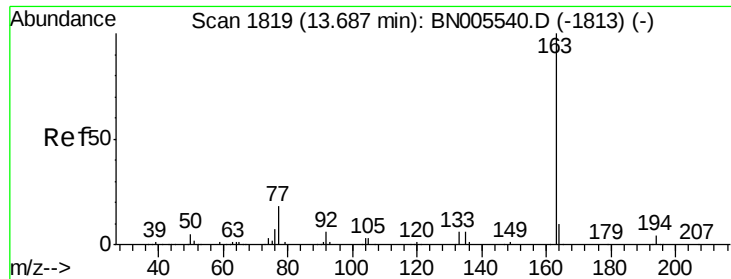

#44
 Dimethylphthalate
 Concen: 7.450 ng/ul
 RT: 13.69 min Scan# 1819
 Delta R.T. -0.00 min
 Lab File: BN005553.D
 Acq: 09 May 2019 03:31

Instrument :
 BNA_N
 ClientSampleId :
 BFH48

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.6	3.4	5.0
164	8.9	8.1	12.1

Manual Integrations
 APPROVED

Sohil
 5/9/2019 2:35:38 PM

