

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050919\
 Data File : BN005562.D
 Acq On : 09 May 2019 12:23
 Operator : JU/SJ
 Sample : K2606-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5146

Quant Time: May 09 13:49:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 09 12:49:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	193827	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	851395	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.22	164	559271	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	1345633	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	1118097	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	986372	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	18477	4.60	ng/uL	0.00
5) Phenol-d5	6.76	99	471320	30.96	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.93	67	276011	29.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	381207	32.72	ng/ul	-0.01
13) 4-Methylphenol-d8	8.28	113	440941	37.05	ng/ul	-0.01
19) Nitrobenzene-d5	8.72	128	227998	43.51	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.44	143	261620	49.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	463887	38.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	665726	53.01	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	1882948	46.38	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	2250790	45.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	291107	45.41	ng/ul	0.00
57) Fluorene-d10	15.22	176	1646077	48.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	231753	38.29	ng/ul	0.00
70) Anthracene-d10	17.07	188	2800619	49.65	ng/ul	0.00
78) Pyrene-d10	19.39	212	3073138	53.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	2225165	51.62	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.79	94	30452	1.945	ng/ul	99
44) Dimethylphthalate	13.69	163	538376	13.309	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050919\
Data File : BN005562.D
Acq On : 09 May 2019 12:23
Operator : JU/SJ
Sample : K2606-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5146

Quant Time: May 09 13:49:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 09 12:49:39 2019
Response via : Initial Calibration

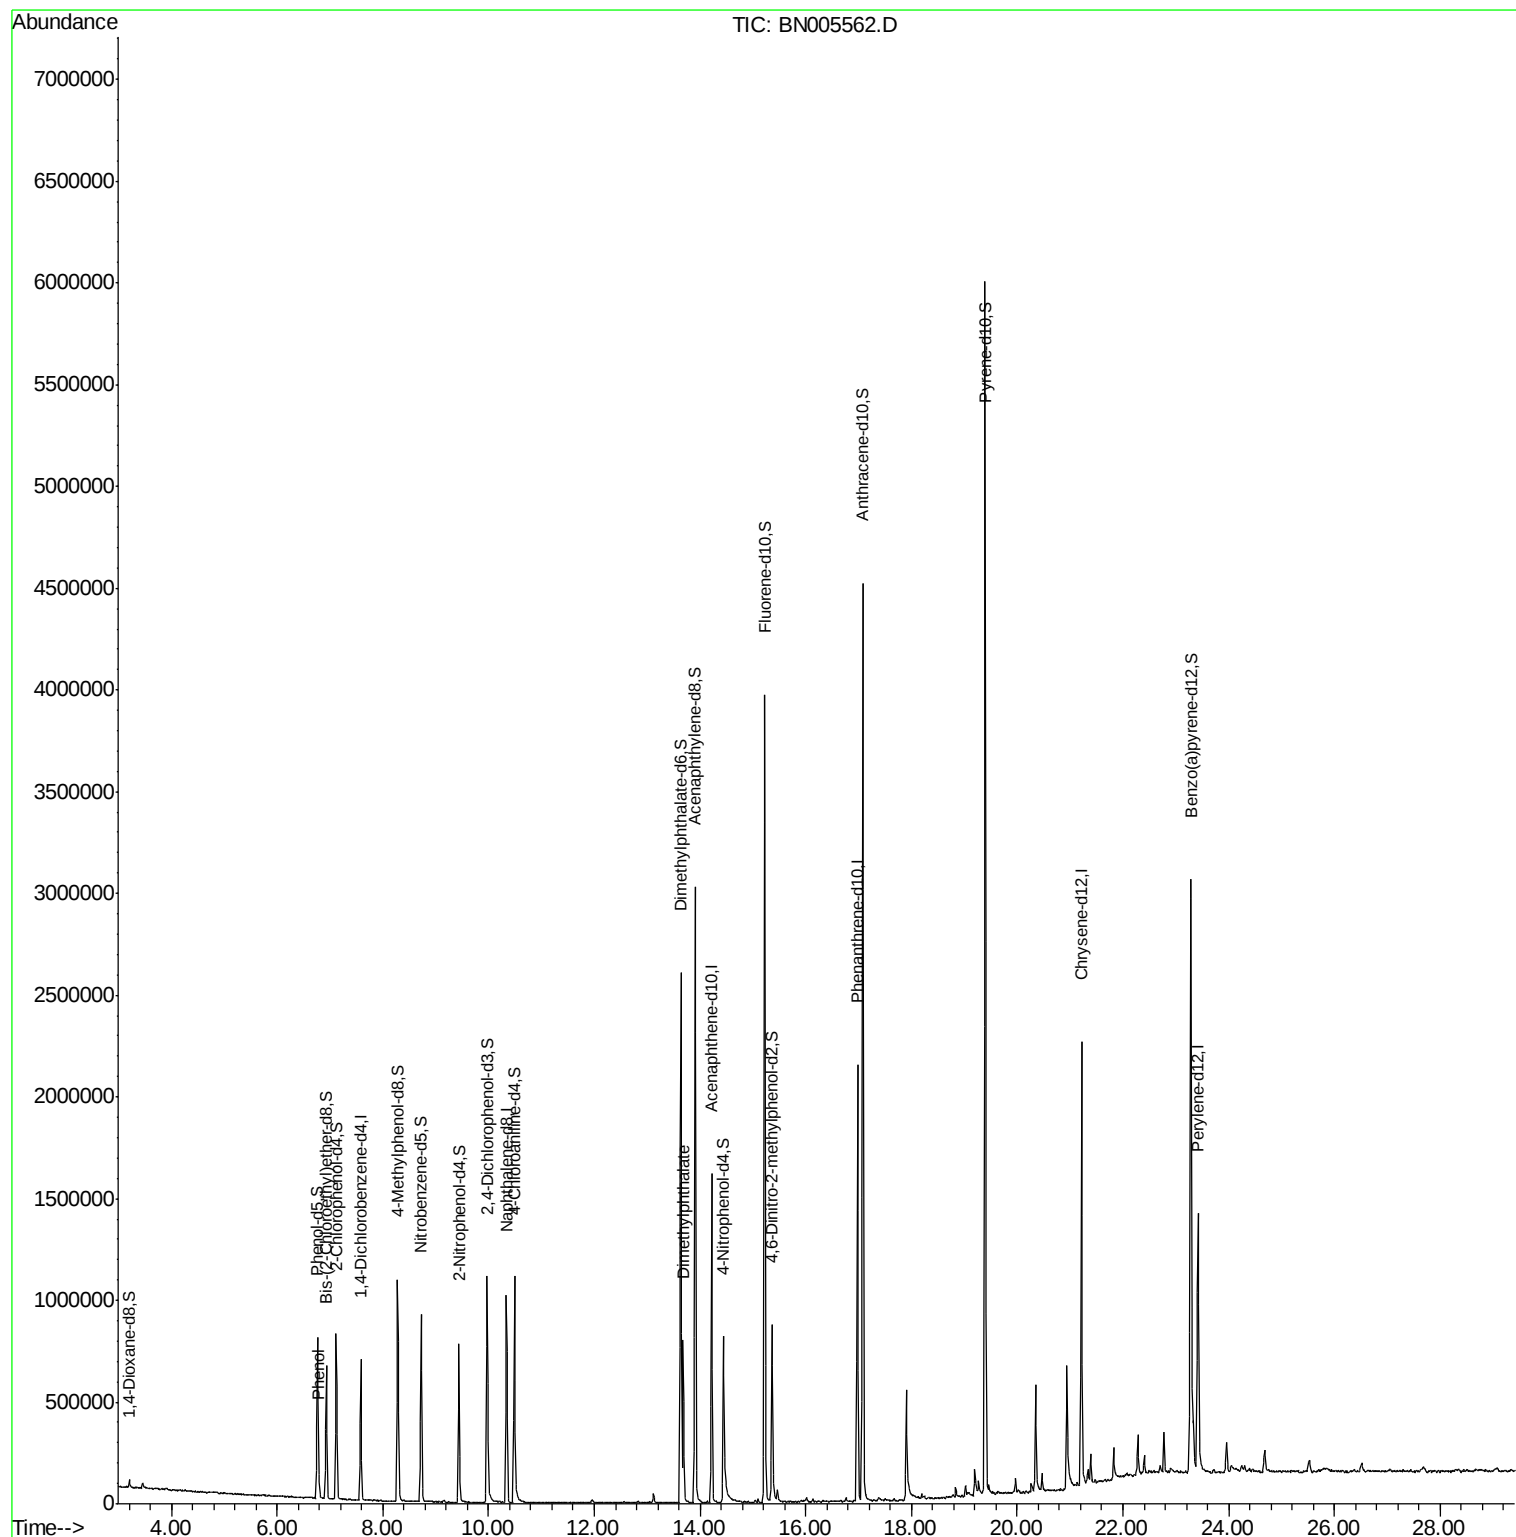

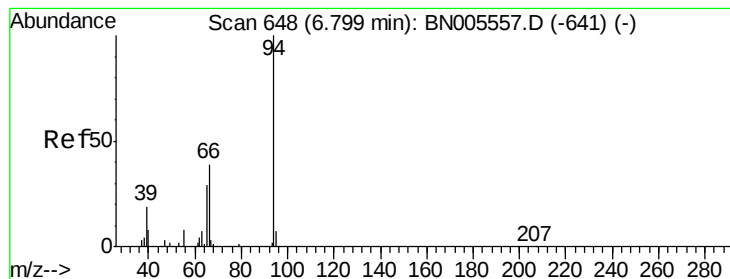





#6

Phenol

Concen: 1.945 ng/ul
 RT: 6.79 min Scan# 647
 Delta R.T. -0.01 min
 Lab File: BN005562.D
 Acq: 09 May 2019 12:23

Instrument :
 BNA_N
 ClientSampleId :
 A5146

Tot Ion	Ratio	Lower	Upper
94	100		
65	28.9	24.2	36.4
66	42.2	33.8	50.6

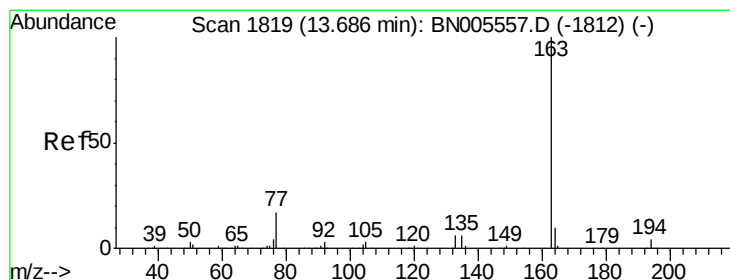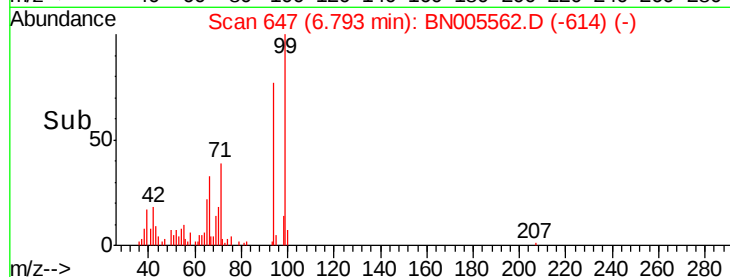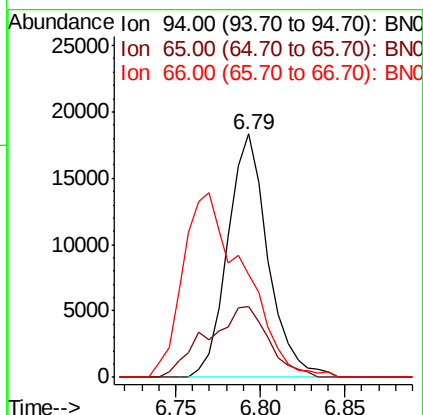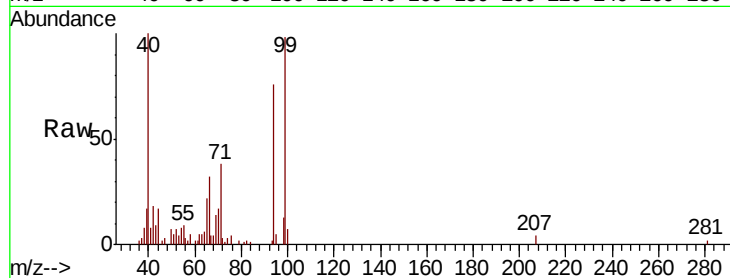

#44

Dimethylphthalate

Concen: 13.309 ng/ul
 RT: 13.69 min Scan# 1819
 Delta R.T. 0.00 min
 Lab File: BN005562.D
 Acq: 09 May 2019 12:23

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.4	5.0
164	9.8	8.1	12.1

