

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050924\
 Data File : BN031450.D
 Acq On : 09 May 2024 19:05
 Operator : MA/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: May 10 01:59:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 10 01:50:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.718	152	9983	0.400	ng	0.00
7) Naphthalene-d8	10.496	136	33212	0.400	ng	0.00
13) Acenaphthene-d10	14.349	164	20437	0.400	ng	0.00
19) Phenanthrene-d10	17.091	188	47232	0.400	ng	0.00
29) Chrysene-d12	21.274	240	40947	0.400	ng	0.00
35) Perylene-d12	23.519	264	45034	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.299	112	47058	2.012	ng	0.00
5) Phenol-d6	6.873	99	64007	2.305	ng	0.00
8) Nitrobenzene-d5	8.862	82	39304	1.348	ng	0.00
11) 2-Methylnaphthalene-d10	12.092	152	89843	1.828	ng	0.00
14) 2,4,6-Tribromophenol	15.837	330	13042	1.435	ng	0.00
15) 2-Fluorobiphenyl	12.981	172	132369	1.751	ng	0.00
27) Fluoranthene-d10	19.124	212	217673	1.703	ng	0.00
31) Terphenyl-d14	19.732	244	165194	1.589	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.248	88	20188	1.694	ng	# 85
3) n-Nitrosodimethylamine	3.551	42	20451	1.720	ng	97
6) bis(2-Chloroethyl)ether	7.148	93	56187	2.164	ng	99
9) Naphthalene	10.549	128	154007	1.659	ng	96
10) Hexachlorobutadiene	10.837	225	26754	1.381	ng	# 99
12) 2-Methylnaphthalene	12.168	142	104971	1.840	ng	99
16) Acenaphthylene	14.071	152	172012	1.919	ng	100
17) Acenaphthene	14.413	154	108320	1.763	ng	99
18) Fluorene	15.397	166	142037	1.786	ng	100
20) 4,6-Dinitro-2-methylph...	15.472	198	6690	0.886	ng	# 29
21) 4-Bromophenyl-phenylether	16.296	248	46390	1.702	ng	95
22) Hexachlorobenzene	16.396	284	46565	1.492	ng	99
23) Atrazine	16.569	200	42126	1.970	ng	97
24) Pentachlorophenol	16.731	266	17805	1.389	ng	98
25) Phenanthrene	17.128	178	220469	1.627	ng	100
26) Anthracene	17.227	178	218330	1.916	ng	100
28) Fluoranthene	19.151	202	266781	1.612	ng	100
30) Pyrene	19.514	202	277391	1.680	ng	100
32) Benzo(a)anthracene	21.256	228	266825	1.887	ng	99
33) Chrysene	21.310	228	251651	1.708	ng	99
34) Bis(2-ethylhexyl)phtha...	21.220	149	148503	1.988	ng	100
36) Indeno(1,2,3-cd)pyrene	25.788	276	299470	1.646	ng	98
37) Benzo(b)fluoranthene	22.844	252	271878	1.539	ng	97
38) Benzo(k)fluoranthene	22.888	252	259183	1.496	ng	96
39) Benzo(a)pyrene	23.420	252	236118	1.593	ng	97
40) Dibenzo(a,h)anthracene	25.814	278	237107	1.654	ng	97
41) Benzo(g,h,i)perylene	26.481	276	254724	1.751	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050924\
Data File : BN031450.D
Acq On : 09 May 2024 19:05
Operator : MA/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Quant Time: May 10 01:59:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 01:50:23 2024
Response via : Initial Calibration

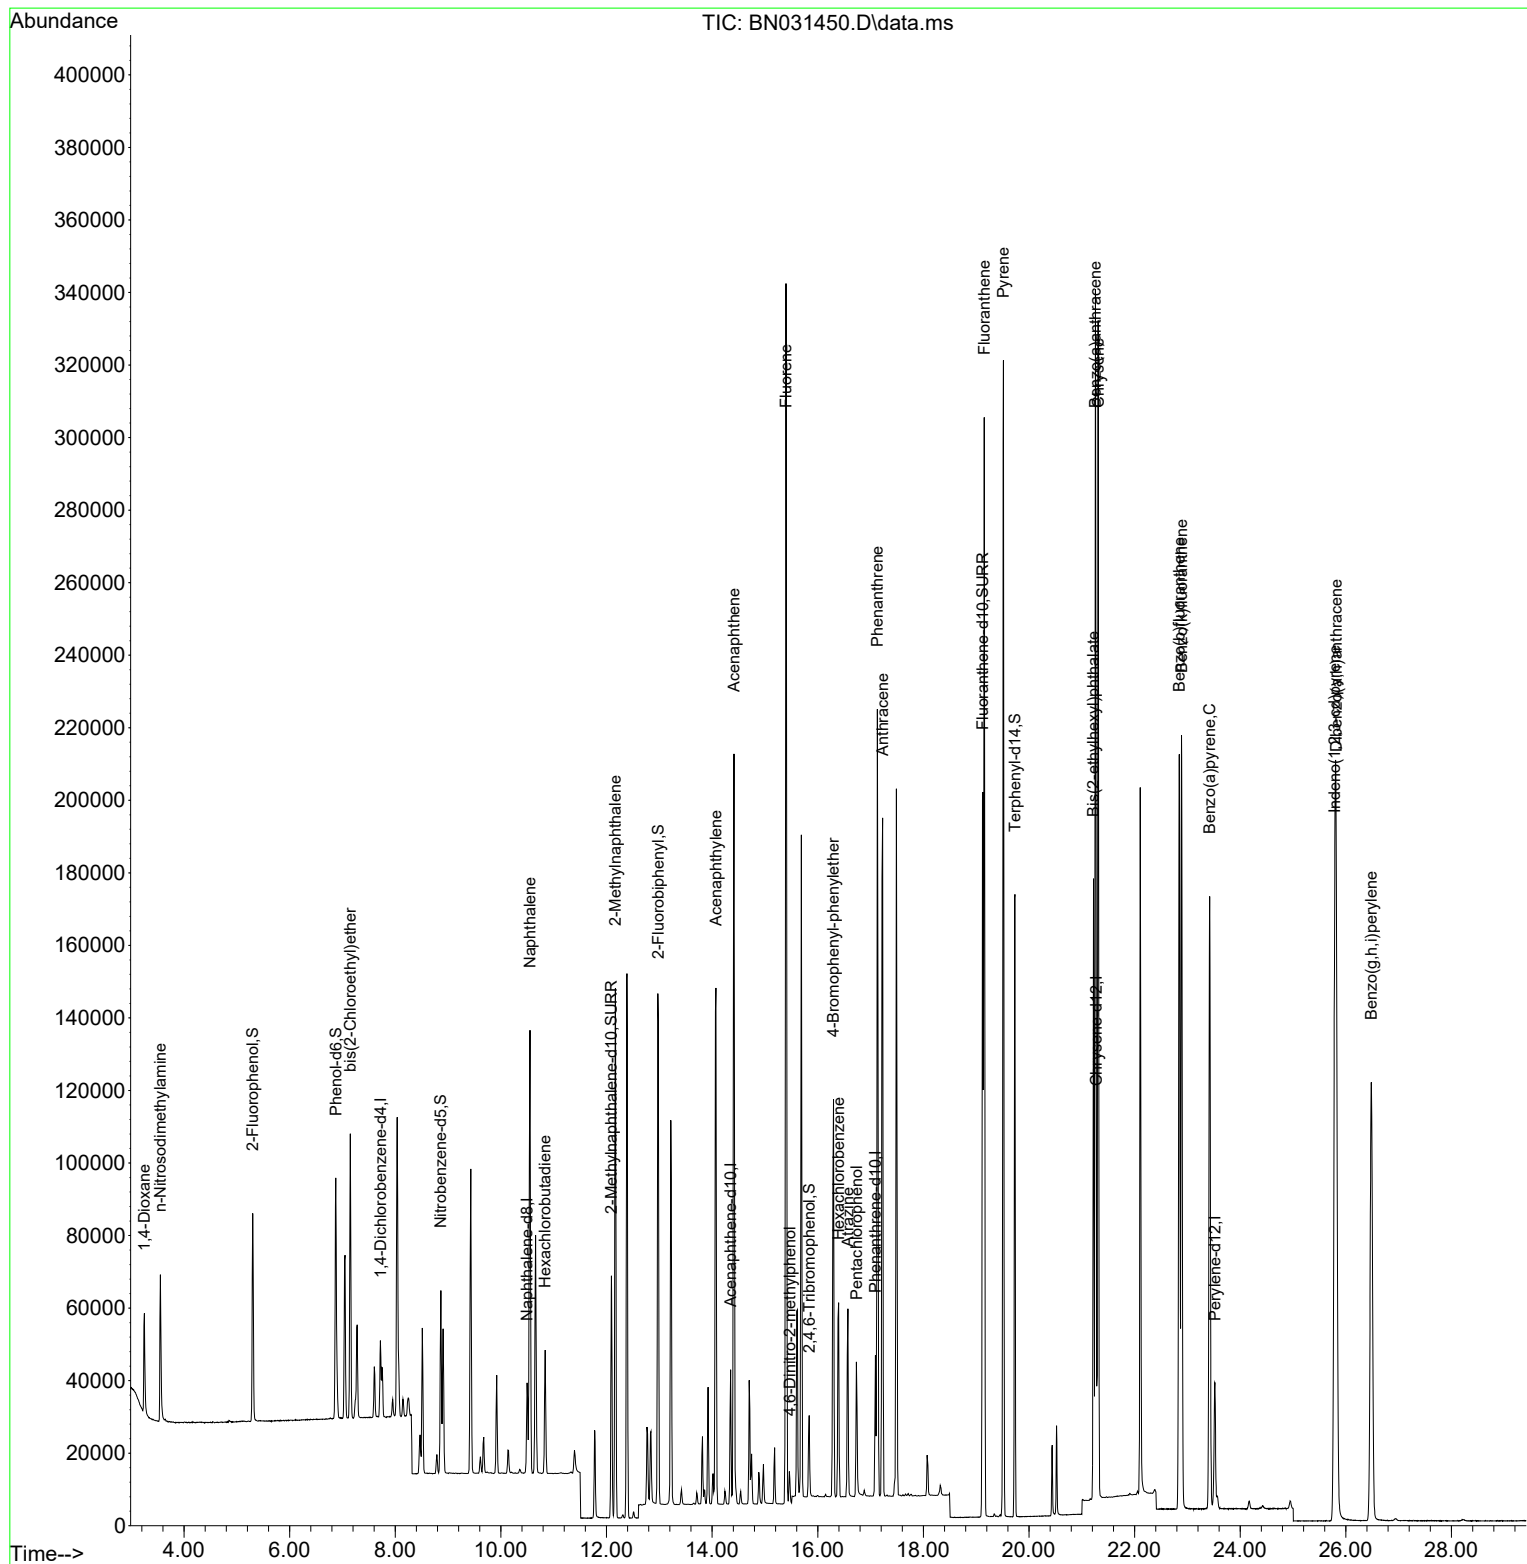






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.718 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6







Tgt Ion:152 Resp: 9983
Ion Ratio Lower Upper
152 100
150 149.3 119.3 178.9
115 67.4 54.8 82.2

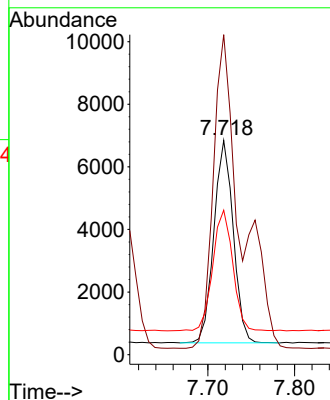

#2
1,4-Dioxane
Concen: 1.694 ng
RT: 3.248 min Scan# 37
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion: 88 Resp: 20188
Ion Ratio Lower Upper
88 100
43 25.6 39.0 58.6#
58 67.0 54.9 82.3


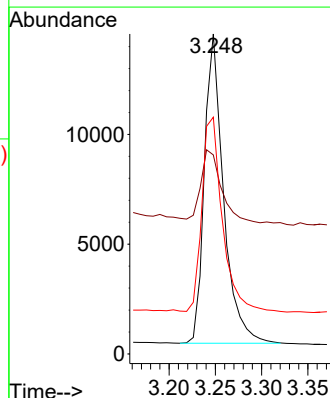






#3
n-Nitrosodimethylamine
Concen: 1.720 ng
RT: 3.551 min Scan# 74
Delta R.T. -0.007 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 20451
Ion Ratio Lower Upper
42 100
74 154.7 126.4 189.6
44 7.1 6.9 10.3

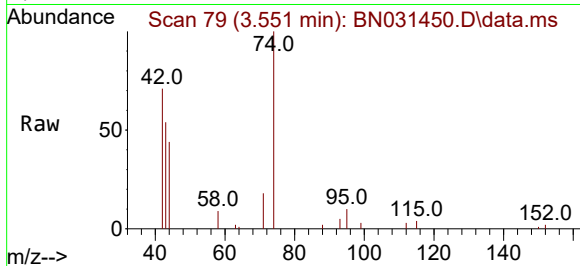

#4
2-Fluorophenol
Concen: 2.012 ng
RT: 5.299 min Scan# 321
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion: 112 Resp: 47058
Ion Ratio Lower Upper
112 100
64 54.7 44.0 66.0
63 27.8 22.2 33.4




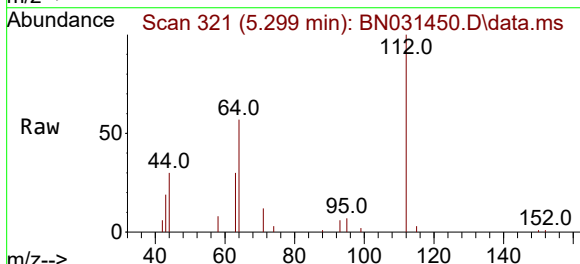




#5
Phenol-d6
Concen: 2.305 ng
RT: 6.873 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 64007
Ion Ratio Lower Upper
99 100
42 15.9 13.5 20.3
71 31.5 26.1 39.1

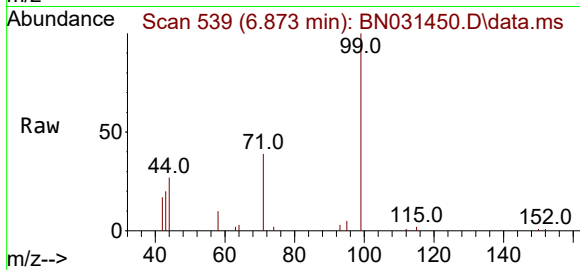

#6
bis(2-Chloroethyl)ether
Concen: 2.164 ng
RT: 7.148 min Scan# 577
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion: 93 Resp: 56187
Ion Ratio Lower Upper
93 100
63 71.2 56.6 85.0
95 32.4 27.3 40.9


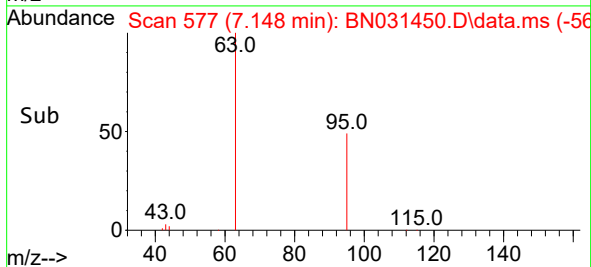

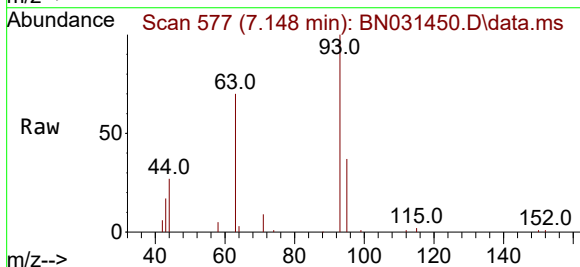




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.496 min Scan# 94
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	33212
Ion	Ratio	Lower	Upper
136	100		
137	12.3	10.1	15.1
54	12.2	10.5	15.7
68	12.7	11.1	16.7



#8
Nitrobenzene-d5
Concen: 1.348 ng
RT: 8.862 min Scan# 790
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:	82	Resp:	39304
Ion	Ratio	Lower	Upper
82	100		
128	39.8	29.0	43.6
54	45.1	37.2	55.8









#9
Naphthalene
Concen: 1.659 ng
RT: 10.549 min Scan# 94
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 154007
Ion Ratio Lower Upper
128 100
129 11.2 10.2 15.4
127 13.2 11.7 17.5



#10
Hexachlorobutadiene
Concen: 1.381 ng
RT: 10.837 min Scan# 975
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:225 Resp: 26754
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 50.7 76.1









#11
2-Methylnaphthalene-d10
Concen: 1.828 ng
RT: 12.092 min Scan# 1151
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 89843
Ion Ratio Lower Upper
152 100
151 20.3 16.6 25.0



#12
2-Methylnaphthalene
Concen: 1.840 ng
RT: 12.168 min Scan# 1212
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:142 Resp: 104971
Ion Ratio Lower Upper
142 100
141 88.9 71.0 106.6
115 35.1 30.2 45.2









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.349 min Scan# 14
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 20437
Ion Ratio Lower Upper
164 100
162 104.4 81.2 121.8
160 47.5 37.0 55.6

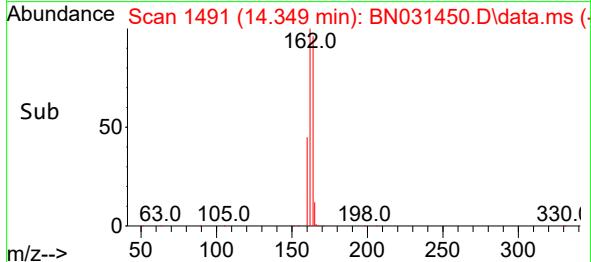

#14
2,4,6-Tribromophenol
Concen: 1.435 ng
RT: 15.837 min Scan# 1626
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:330 Resp: 13042
Ion Ratio Lower Upper
330 100
332 96.2 76.6 114.8
141 44.4 37.0 55.4


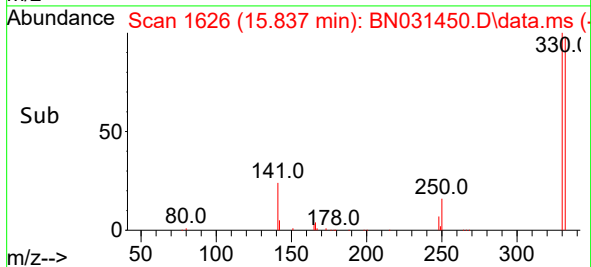

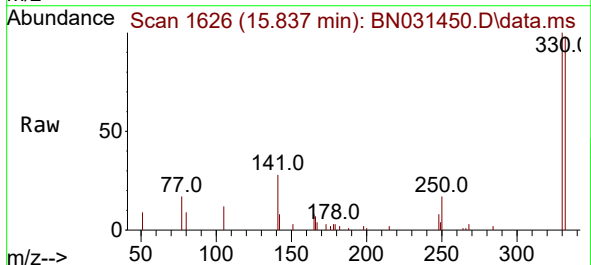




#15
2-Fluorobiphenyl
Concen: 1.751 ng
RT: 12.981 min Scan# 1363
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 132369
Ion Ratio Lower Upper
172 100
171 33.9 27.8 41.8
170 21.8 18.3 27.5



#16
Acenaphthylene
Concen: 1.919 ng
RT: 14.071 min Scan# 1465
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:152 Resp: 172012
Ion Ratio Lower Upper
152 100
151 19.5 15.7 23.5
153 13.0 10.5 15.7




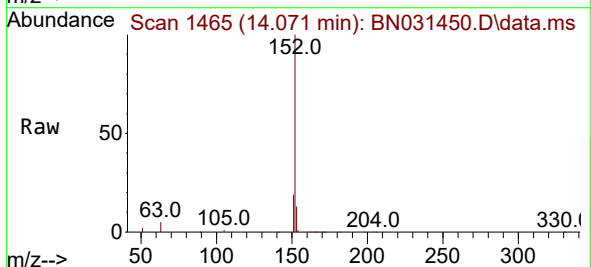




#17
Acenaphthene
Concen: 1.763 ng
RT: 14.413 min Scan# 1484
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 108320
Ion Ratio Lower Upper
154 100
153 110.9 89.1 133.7
152 52.8 42.6 64.0

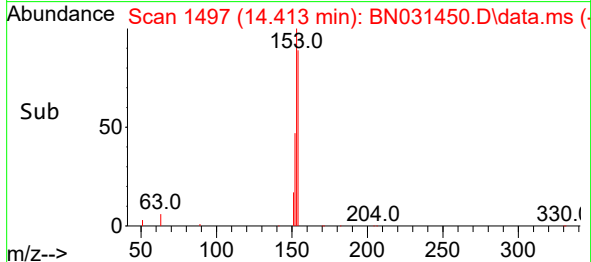

#18
Fluorene
Concen: 1.786 ng
RT: 15.397 min Scan# 1589
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:166 Resp: 142037
Ion Ratio Lower Upper
166 100
165 97.5 78.2 117.2
167 13.4 10.8 16.2


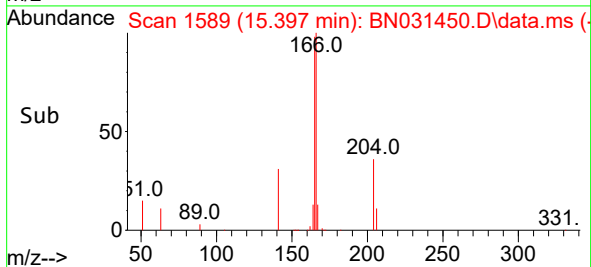

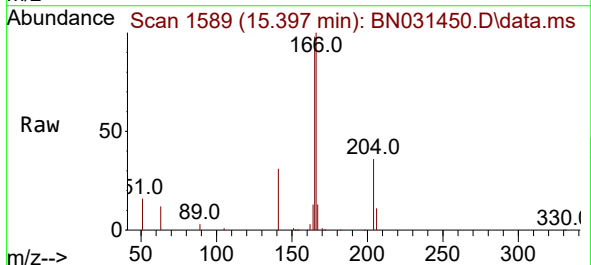




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.091 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 47232
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.4 9.6 14.4

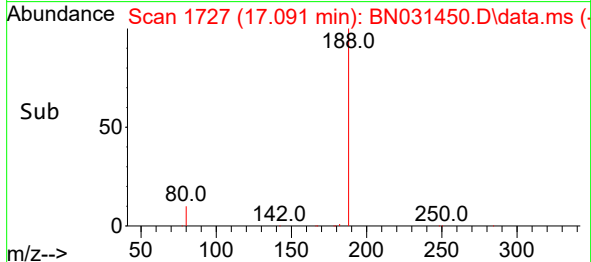

#20
4,6-Dinitro-2-methylphenol
Concen: 0.886 ng
RT: 15.472 min Scan# 1596
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:198 Resp: 6690
Ion Ratio Lower Upper
198 100
51 36.5 78.3 117.5#
105 49.2 117.2 175.8#


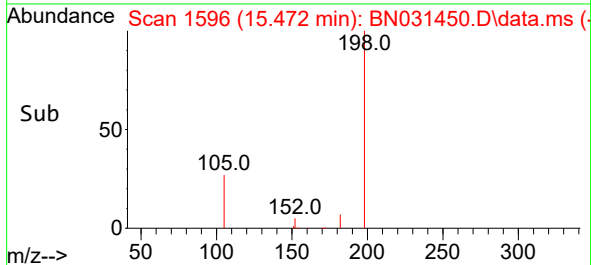

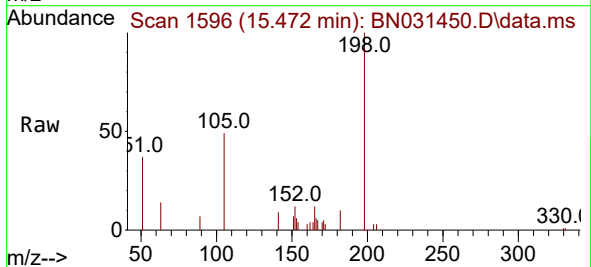


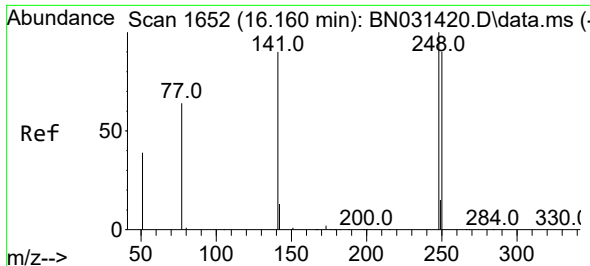

#21
4-Bromophenyl-phenylether
Concen: 1.702 ng
RT: 16.296 min Scan# 1663
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 46390
Ion Ratio Lower Upper
248 100
250 99.8 77.9 116.9
141 47.1 43.4 65.2

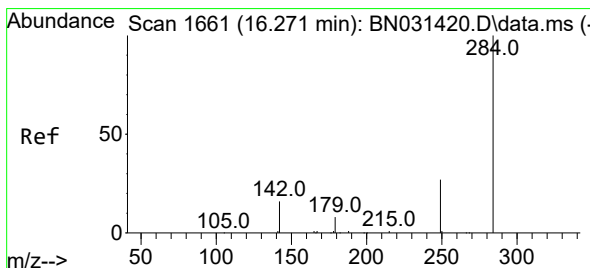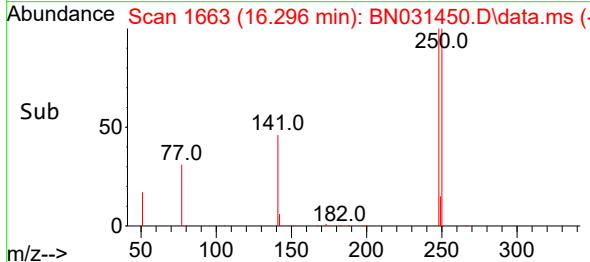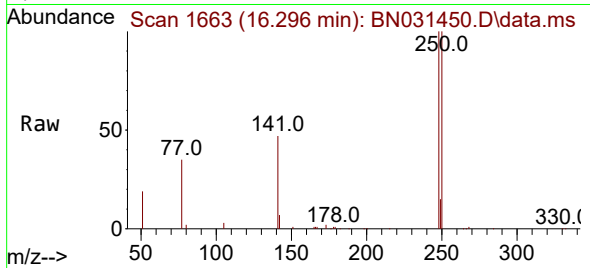

#22
Hexachlorobenzene
Concen: 1.492 ng
RT: 16.396 min Scan# 1671
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:284 Resp: 46565
Ion Ratio Lower Upper
284 100
142 38.5 31.0 46.6
249 31.0 25.5 38.3

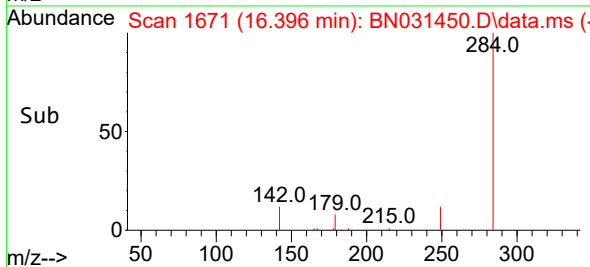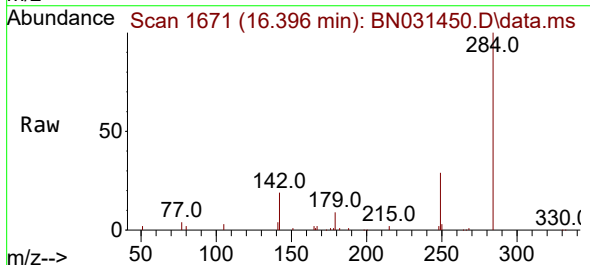



#23

Atrazine

Concen: 1.970 ng

RT: 16.569 min Scan# 1685

Delta R.T. -0.000 min

Lab File: BN031450.D

Acq: 09 May 2024 19:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:200 Resp: 42126

Ion Ratio Lower Upper

200 100

173 22.4 19.6 29.4

215 48.2 39.8 59.8

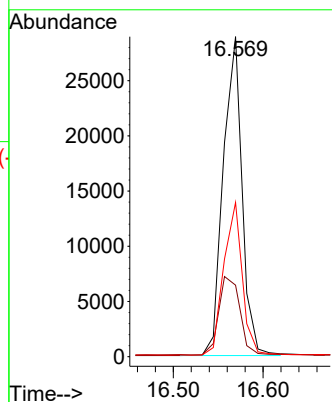

#24

Pentachlorophenol

Concen: 1.389 ng

RT: 16.731 min Scan# 1698

Delta R.T. -0.000 min

Lab File: BN031450.D

Acq: 09 May 2024 19:05




Tgt Ion:266 Resp: 17805


Ion Ratio Lower Upper

266 100

264 62.8 50.6 75.8

268 63.4 49.0 73.4







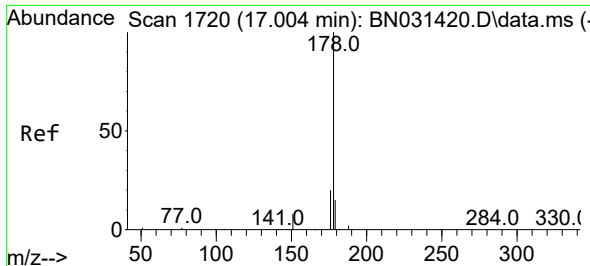

#25
Phenanthrene
Concen: 1.627 ng
RT: 17.128 min Scan# 1730
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 220469
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 15.2 12.3 18.5

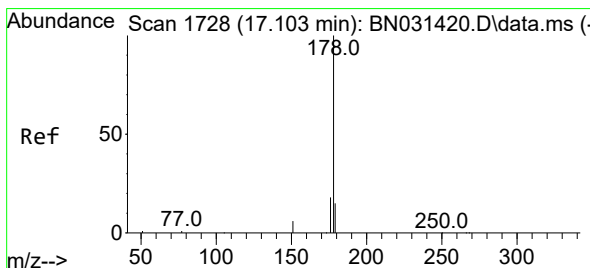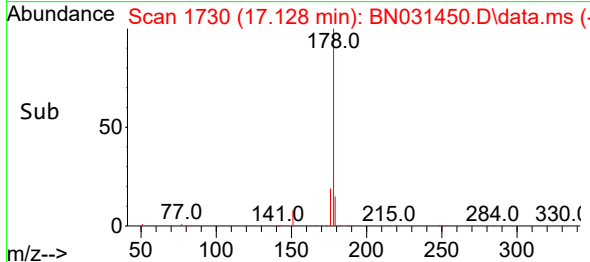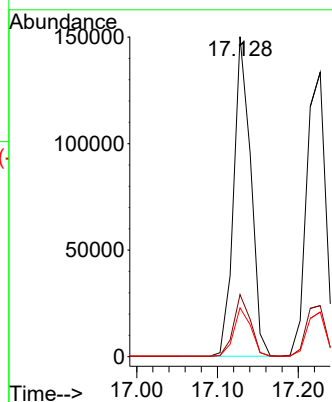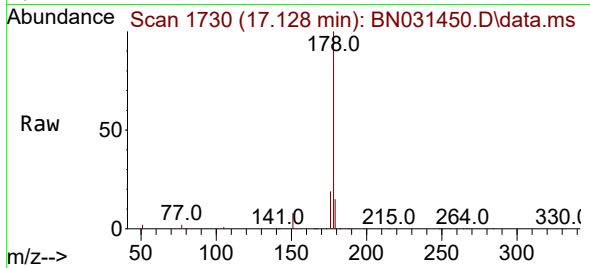

#26
Anthracene
Concen: 1.916 ng
RT: 17.227 min Scan# 1738
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:178 Resp: 218330
Ion Ratio Lower Upper
178 100
176 18.5 14.9 22.3
179 15.3 12.4 18.6


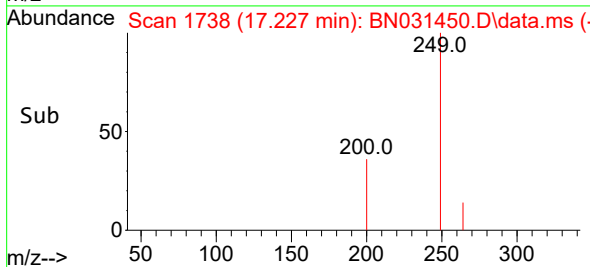

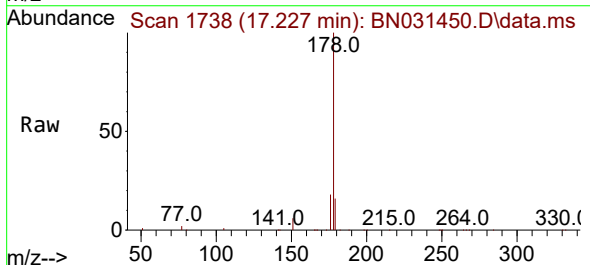




#27
Fluoranthene-d10
Concen: 1.703 ng
RT: 19.124 min Scan# 1974
Delta R.T. 0.005 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 217673
Ion Ratio Lower Upper
212 100
106 15.0 12.0 18.0
104 8.5 6.9 10.3



#28
Fluoranthene
Concen: 1.612 ng
RT: 19.151 min Scan# 1980
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:202 Resp: 266781
Ion Ratio Lower Upper
202 100
101 12.1 9.8 14.6
203 17.3 13.8 20.8



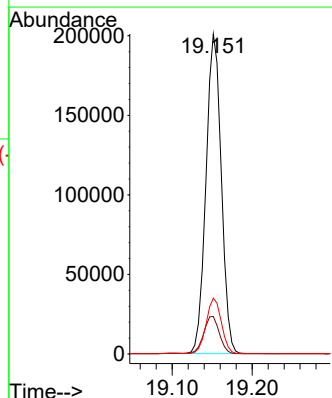



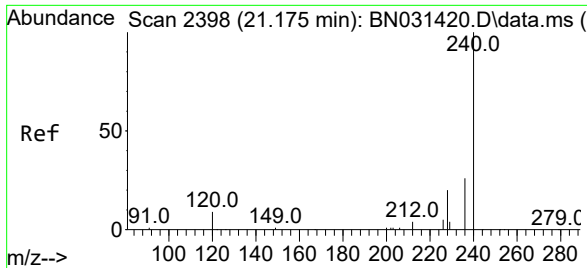

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.274 min Scan# 2409
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:240 Resp: 40947
Ion Ratio Lower Upper
240 100
120 12.2 11.4 17.2
236 27.4 22.2 33.4

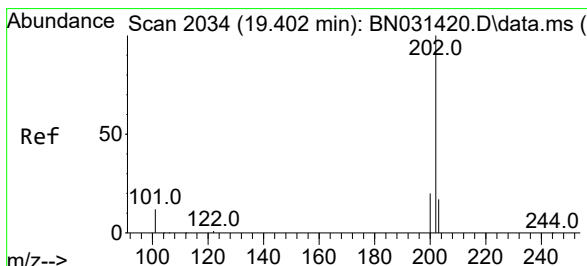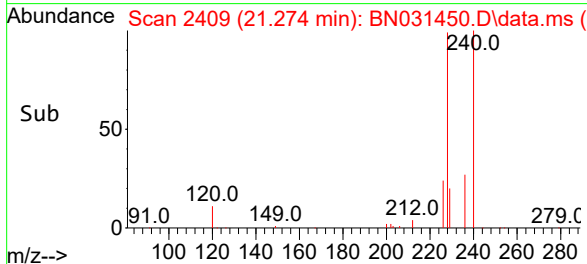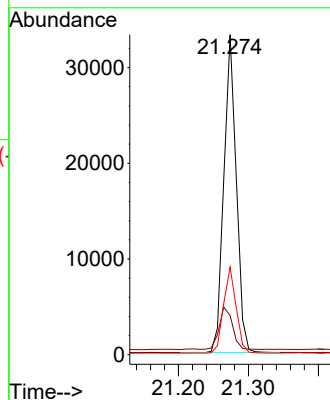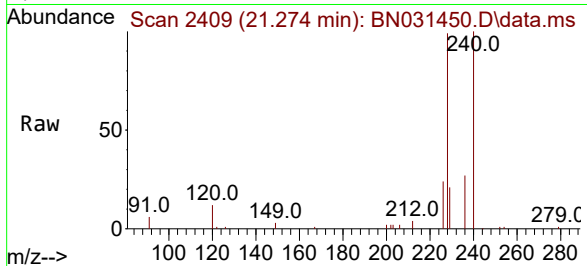

#30
Pyrene
Concen: 1.680 ng
RT: 19.514 min Scan# 2058
Delta R.T. -0.000 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:202 Resp: 277391
Ion Ratio Lower Upper
202 100
200 20.8 16.6 25.0
203 17.9 14.3 21.5

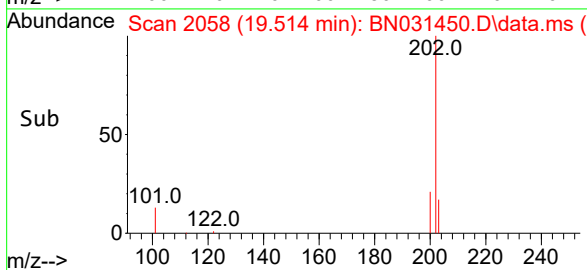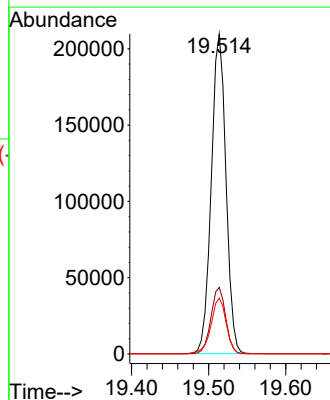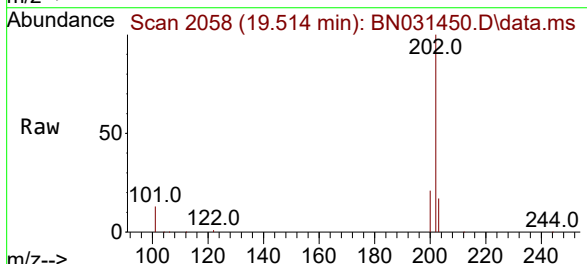



#31

Terphenyl-d14

Concen: 1.589 ng

RT: 19.732 min Scan# 2105

Delta R.T. -0.000 min

Lab File: BN031450.D

Acq: 09 May 2024 19:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:244 Resp: 165194

Ion Ratio Lower Upper

244 100

212 7.9 6.5 9.7

122 13.4 11.4 17.2

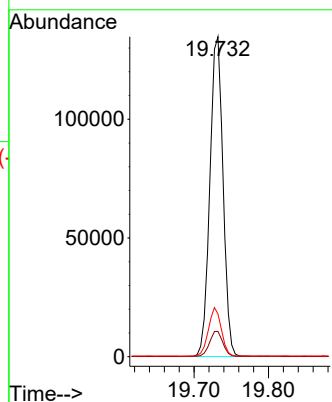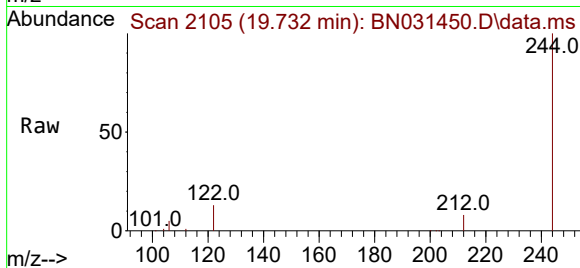

#32

Benzo(a)anthracene

Concen: 1.887 ng

RT: 21.256 min Scan# 2407

Delta R.T. -0.000 min

Lab File: BN031450.D

Acq: 09 May 2024 19:05




Tgt Ion:228 Resp: 266825


Ion Ratio Lower Upper

228 100

226 27.6 22.4 33.6

229 19.2 15.5 23.3

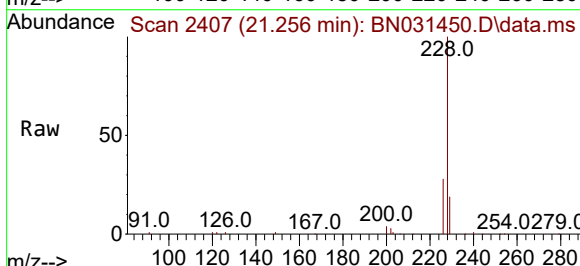

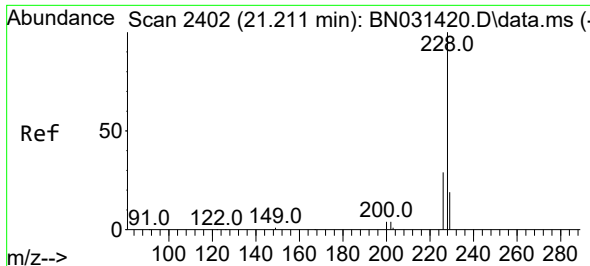

#33

Chrysene

Concen: 1.708 ng

RT: 21.310 min Scan# 2403

Delta R.T. -0.000 min

Lab File: BN031450.D

Acq: 09 May 2024 19:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 251651

Ion Ratio Lower Upper

228 100

226 30.0 24.5 36.7

229 19.7 15.8 23.8

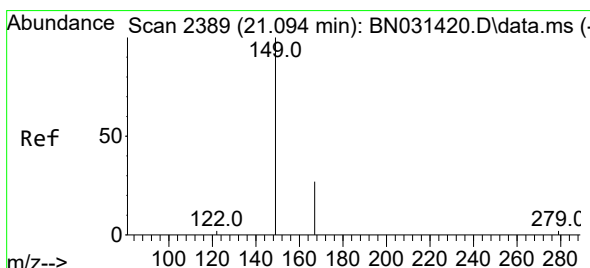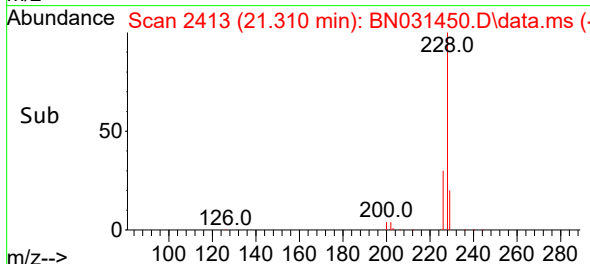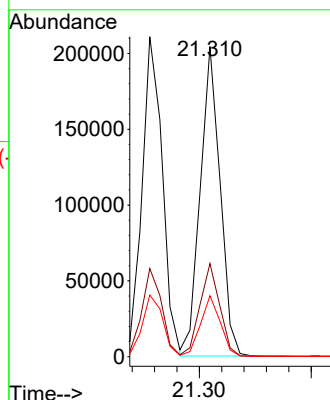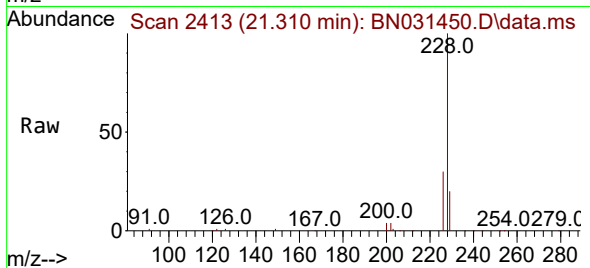

#34

Bis(2-ethylhexyl)phthalate

Concen: 1.988 ng

RT: 21.220 min Scan# 2403

Delta R.T. -0.000 min

Lab File: BN031450.D

Acq: 09 May 2024 19:05




Tgt Ion:149 Resp: 148503


Ion Ratio Lower Upper

149 100

167 27.5 22.1 33.1

279 3.4 2.7 4.1

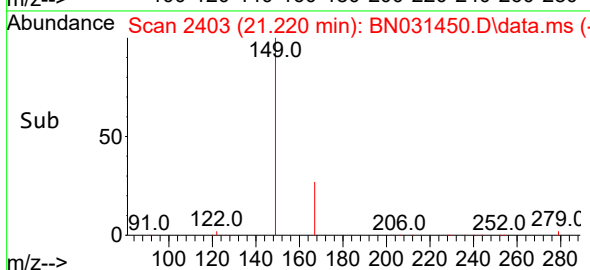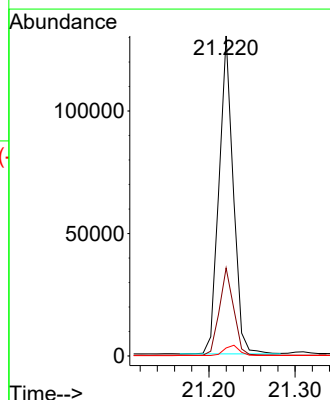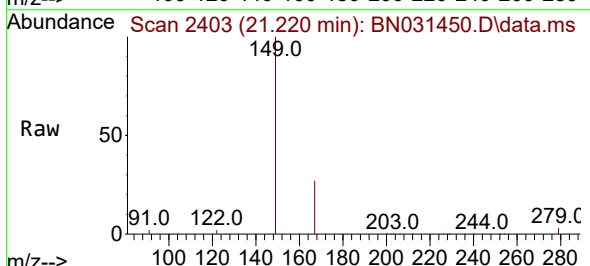



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.519 min Scan# 2915

Delta R.T. -0.000 min

Lab File: BN031450.D


Acq: 09 May 2024 19:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6






Tgt Ion:264 Resp: 45034

Ion Ratio Lower Upper

264 100

260 25.3 20.6 31.0

265 31.5 24.0 36.0

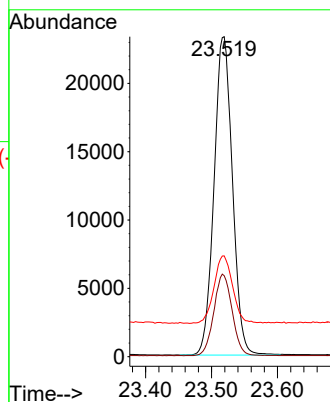

#36

Indeno(1,2,3-cd)pyrene

Concen: 1.646 ng

RT: 25.788 min Scan# 3691

Delta R.T. -0.006 min

Lab File: BN031450.D

Acq: 09 May 2024 19:05




Tgt Ion:276 Resp: 299470


Ion Ratio Lower Upper

276 100

138 27.2 23.0 34.6

277 25.0 19.9 29.9



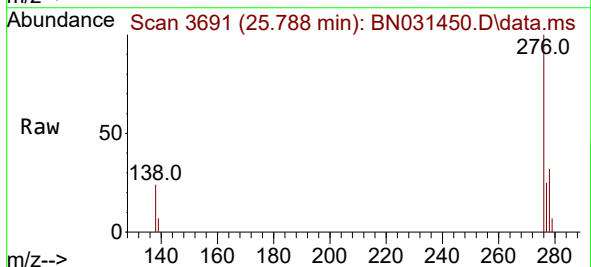
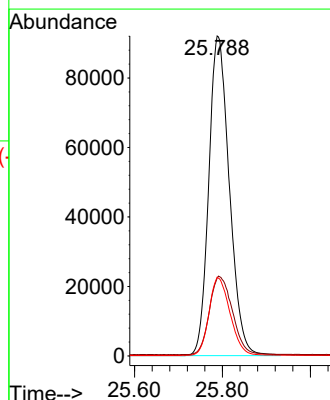




#37
Benzo(b)fluoranthene
Concen: 1.539 ng
RT: 22.844 min Scan# 2684
Delta R.T. -0.003 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 271878
Ion Ratio Lower Upper
252 100
253 22.0 18.2 27.4
125 11.2 10.5 15.7

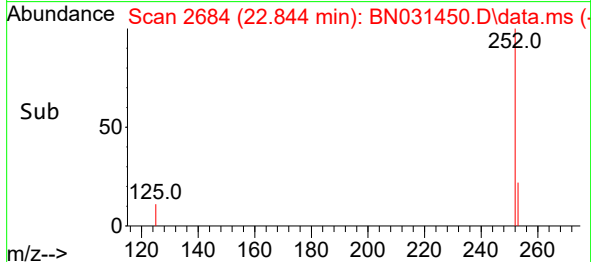

#38
Benzo(k)fluoranthene
Concen: 1.496 ng
RT: 22.888 min Scan# 2699
Delta R.T. -0.003 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Tgt Ion:252 Resp: 259183
Ion Ratio Lower Upper
252 100
253 21.8 18.2 27.2
125 11.2 11.0 16.6


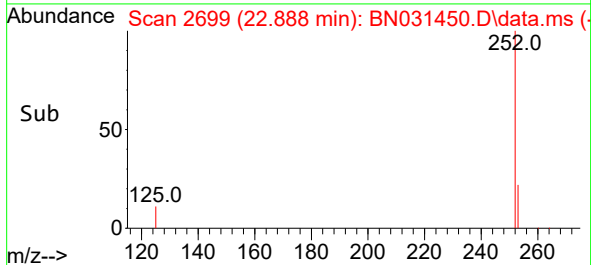

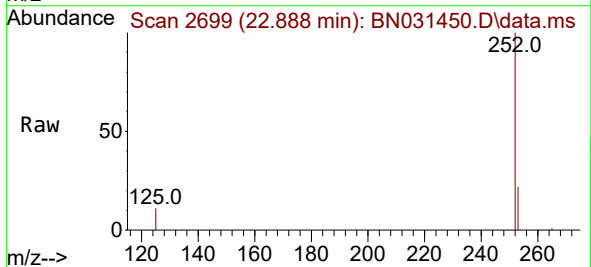




#39
Benzo(a)pyrene
Concen: 1.593 ng
RT: 23.420 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 236118
Ion Ratio Lower Upper
252 100
253 22.1 18.2 27.2
125 12.5 11.9 17.9



#40
Dibenzo(a,h)anthracene
Concen: 1.654 ng
RT: 25.814 min Scan# 3700
Delta R.T. -0.006 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05


Tgt Ion:278 Resp: 237107
Ion Ratio Lower Upper
278 100
139 18.0 15.9 23.9
279 23.6 19.8 29.8

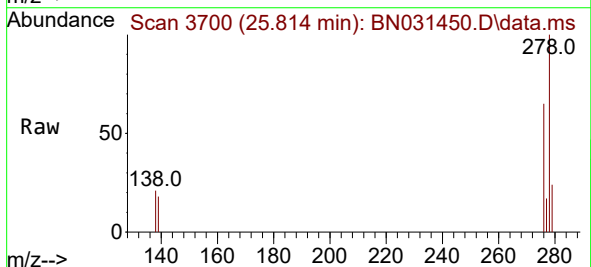

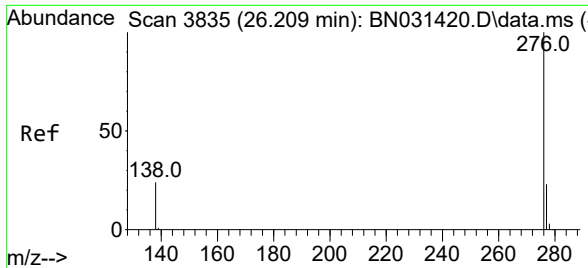

#41
Benzo(g,h,i)perylene
Concen: 1.751 ng
RT: 26.481 min Scan# 3928
Delta R.T. -0.003 min
Lab File: BN031450.D
Acq: 09 May 2024 19:05

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

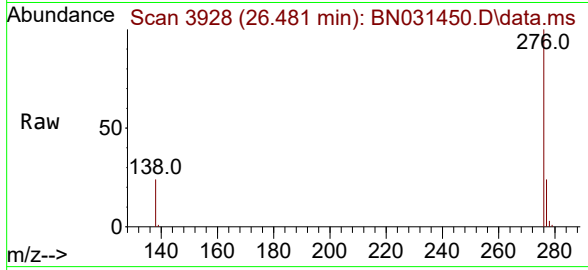

Tgt Ion:276 Resp: 254724
Ion Ratio Lower Upper
276 100
277 23.6 19.4 29.0
138 23.9 20.4 30.6

