
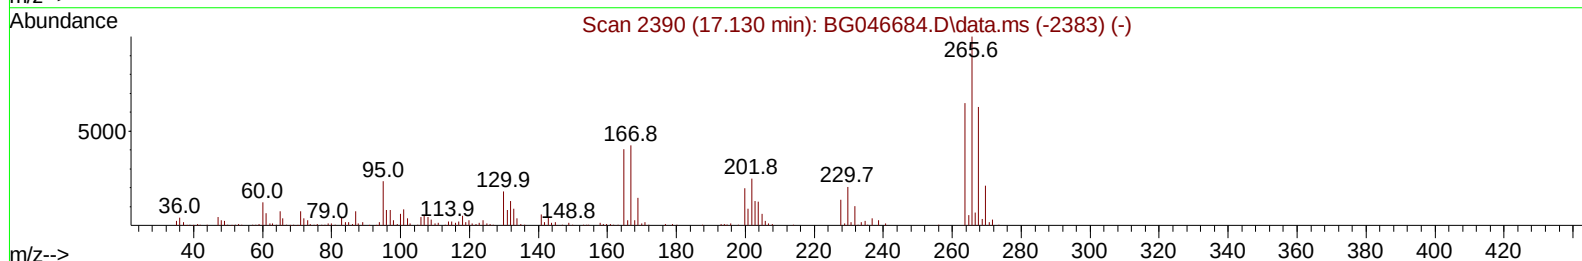
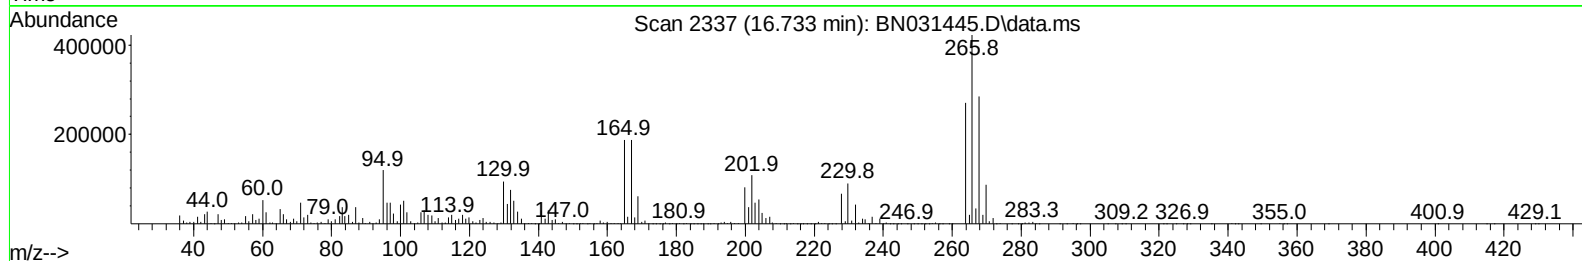


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050924\
Data File : BN031445.D
Acq On : 09 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 03:37:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 03:37:33 2024
Response via : Initial Calibration

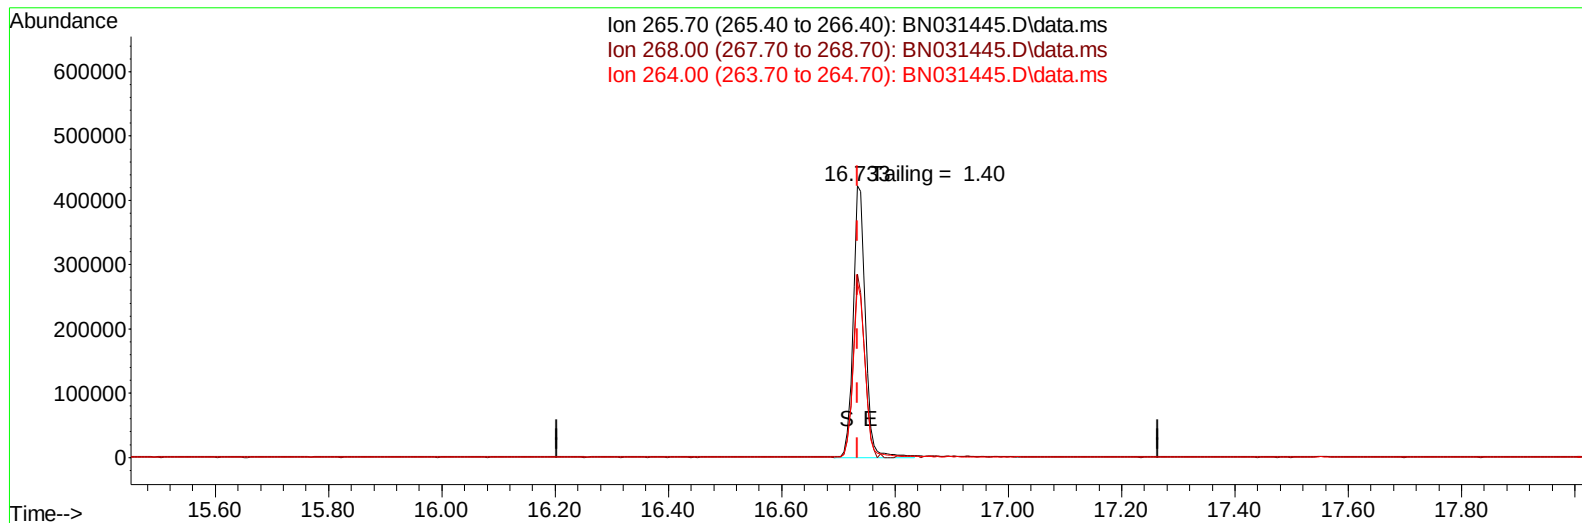




TIC: BN031445.D\data.ms

(70) Pentachlorophenol (C)**16.733min (0.000) 194431.17 ng****response 637804**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.56
264.00	61.60	64.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050924\
Data File : BN031445.D
Acq On : 09 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 03:37:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 03:37:33 2024
Response via : Initial Calibration

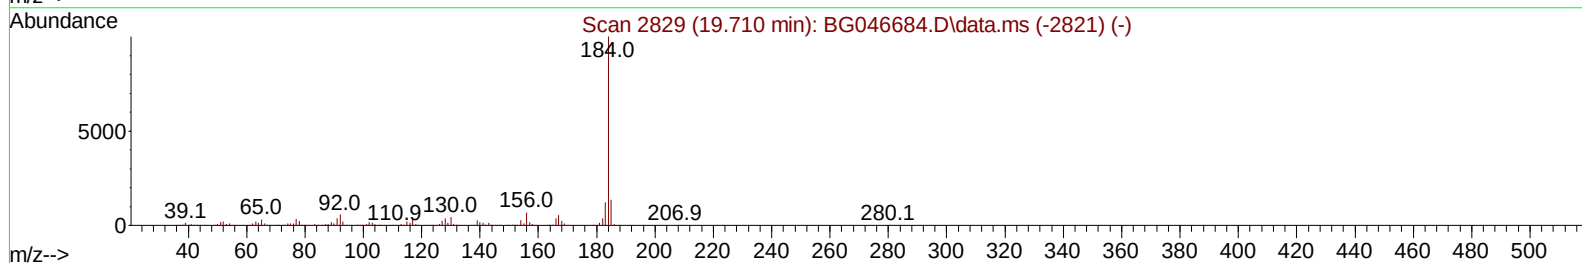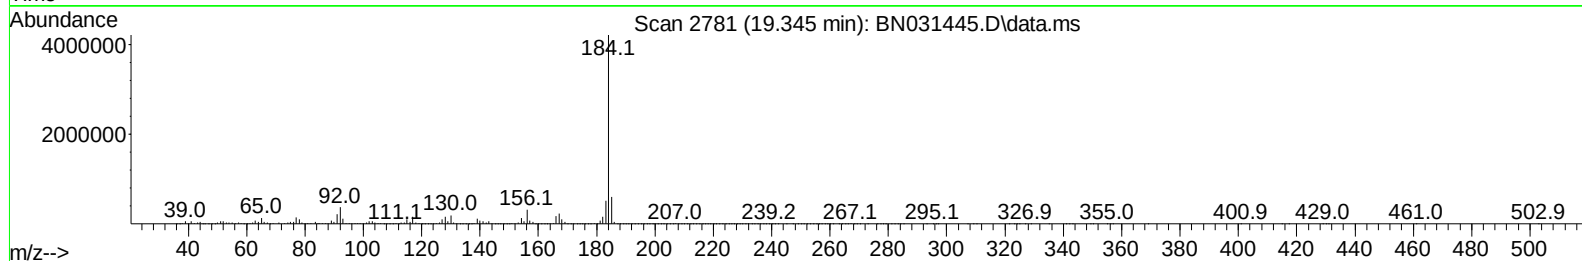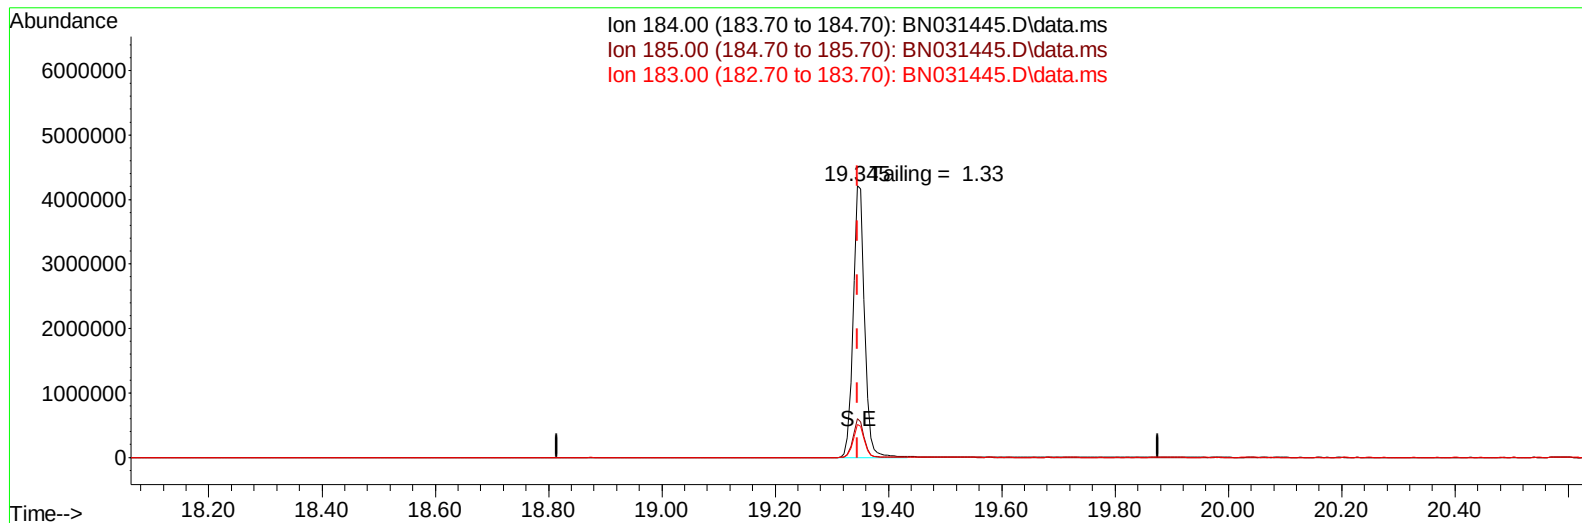

TIC: BN031445.D\data.ms

(77) Benzidine**19.345min (0.000) 220087.80 ng****response 5956605**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.22
183.00	13.20	12.09
0.00	0.00	0.00