
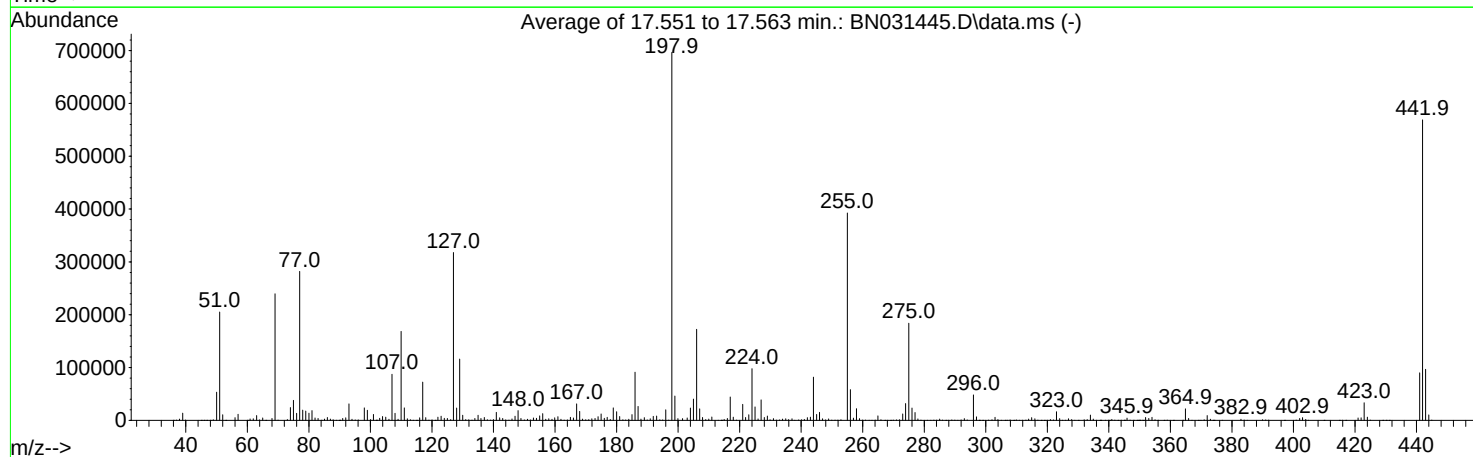


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050924\
Data File : BN031445.D
Acq On : 09 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

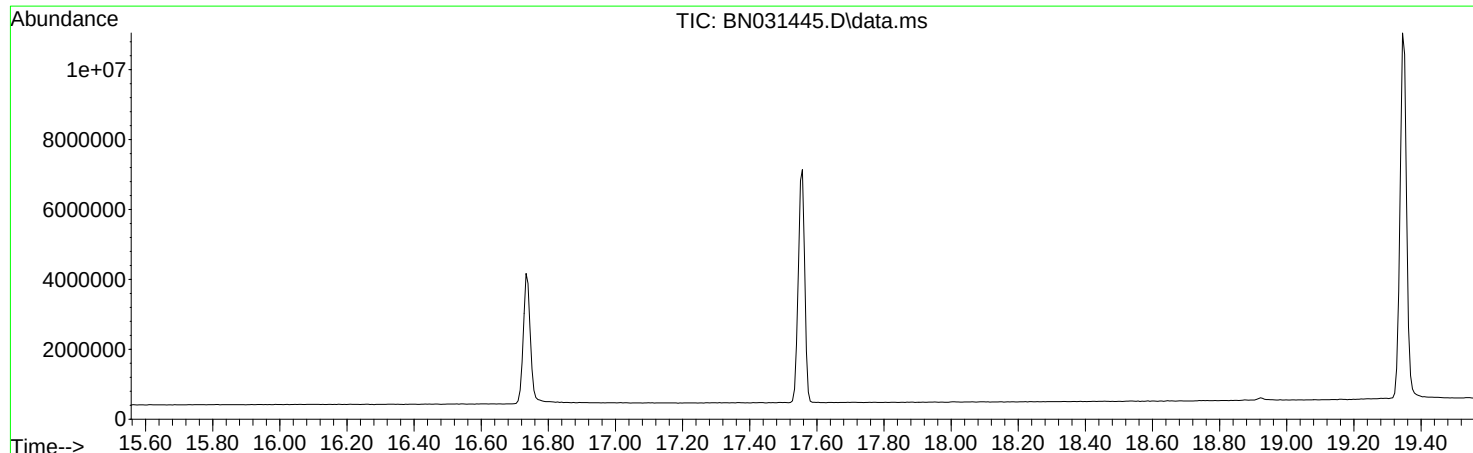




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	205037	PASS
68	69	0.00	2	1.5	3633	PASS
69	198	0.00	100	34.4	239740	PASS
70	69	0.00	2	0.2	572	PASS
127	198	10	80	45.6	317645	PASS
197	198	0.00	2	0.1	741	PASS
198	198	100	100	100.0	696347	PASS
199	198	5	9	6.6	46024	PASS
275	198	10	60	26.4	183829	PASS
365	198	1	100	3.1	21749	PASS
441	198	0.01	100	12.9	89837	PASS
442	442	50	100	100.0	568811	PASS
443	442	15	24	17.0	96757	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050924\
Data File : BN031445.D
Acq On : 09 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 10 03:37:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 03:37:33 2024
Response via : Initial Calibration

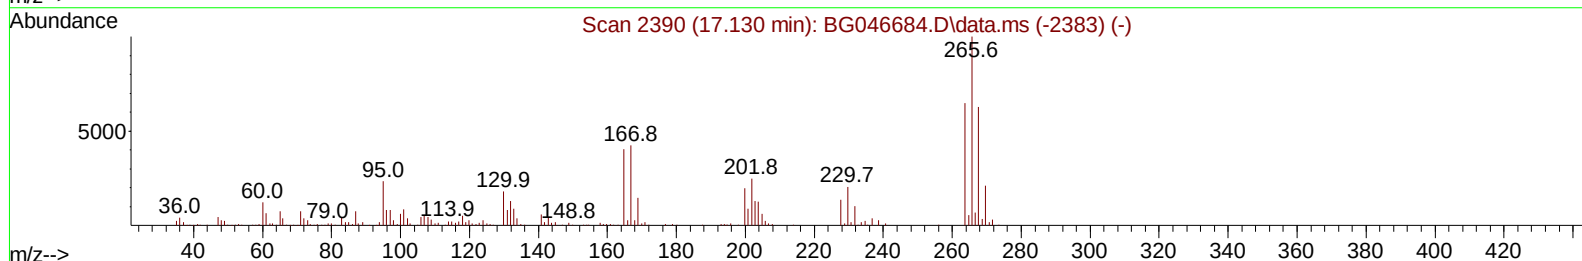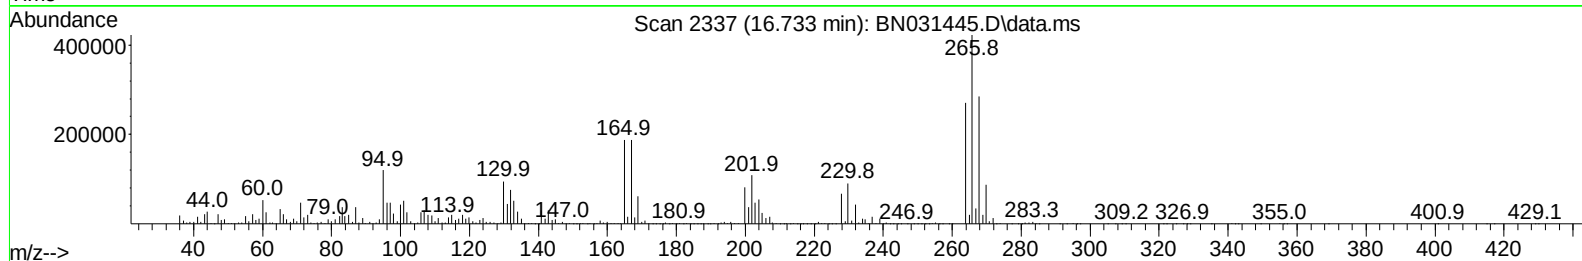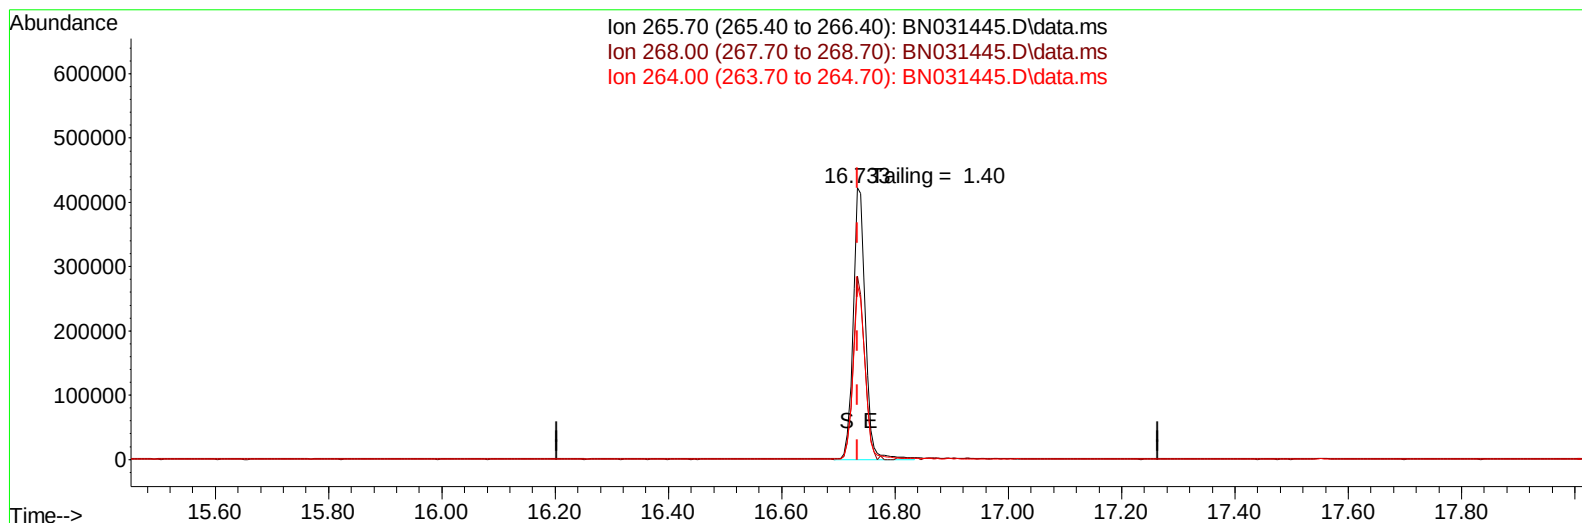

TIC: BN031445.D\data.ms

(70) Pentachlorophenol (C)

16.733min (0.000) 194431.17 ng




response 637804

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.56
264.00	61.60	64.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050924\
Data File : BN031445.D
Acq On : 09 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 10 03:37:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 03:37:33 2024
Response via : Initial Calibration

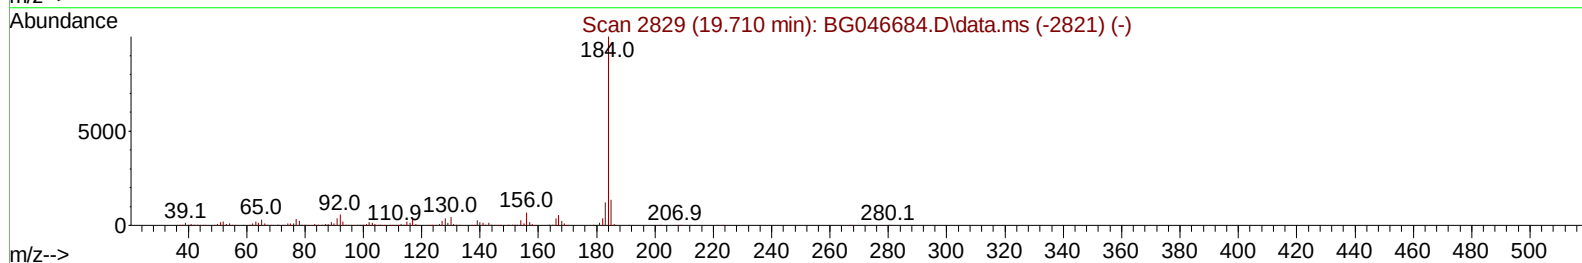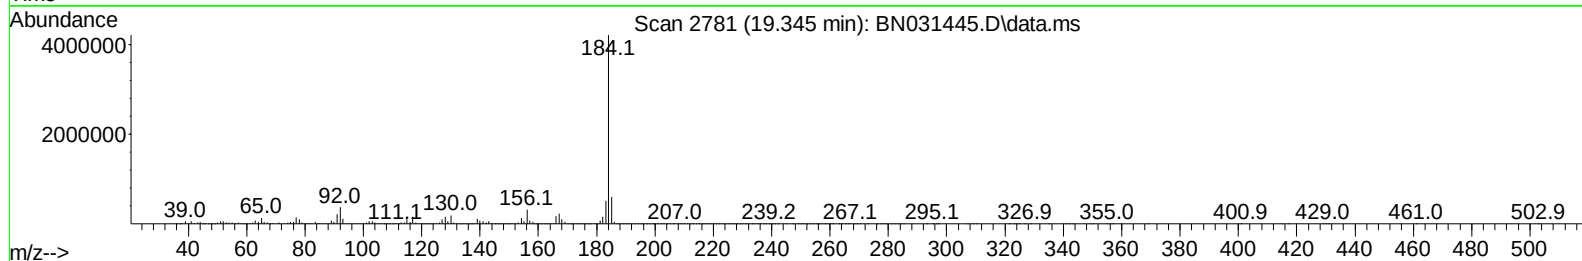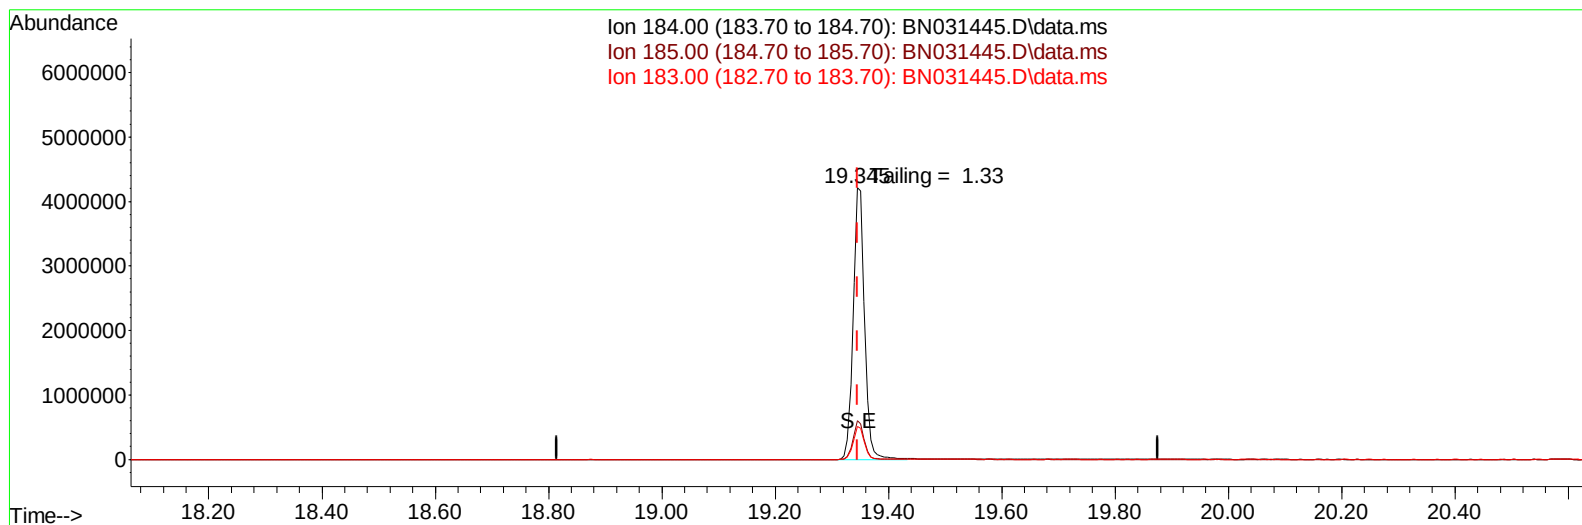

TIC: BN031445.D\data.ms

(77) Benzidine

19.345min (0.000) 220087.80 ng

response 5956605

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.22
183.00	13.20	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/9/2024	BNA_N	<u>BN031445.D</u>
Compound Name	Response	Retention Time
DDT	2290282	20.586
DDD	40211	20.145
DDE	1558	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41769	2332051	1.79

Instrument :
BNA_N
ClientSampleId :
DFTPP