

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051019\
 Data File : BN005602.D
 Acq On : 10 May 2019 23:07
 Operator : JU/SJ
 Sample : K2613-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 11 02:48:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 07 05:36:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	211724	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	874014	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.22	164	524630	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	1192381	20.00	ng/ul	-0.01
77) Chrysene-d12	21.20	240	1047193	20.00	ng/ul	-0.01
85) Perylene-d12	23.40	264	954436	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	12885	2.94	ng/uL	0.00
5) Phenol-d5	6.77	99	341996	20.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	199800	19.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	281526	22.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	296125	22.78	ng/ul	-0.01
19) Nitrobenzene-d5	8.72	128	158032	29.38	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.44	143	180913	33.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	312423	24.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	427045	33.13	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	1055679	27.72	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	1318590	28.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	137097	22.80	ng/ul	0.00
57) Fluorene-d10	15.22	176	902762	28.25	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	123035	22.94	ng/ul	0.00
70) Anthracene-d10	17.07	188	1413433	28.28	ng/ul	-0.01
78) Pyrene-d10	19.39	212	1551682	28.97	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.26	264	1215844	29.15	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	6.79	94	24123	1.410	ng/ul	98
44) Dimethylphthalate	13.68	163	338252	8.914	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051019\
Data File : BN005602.D
Acq On : 10 May 2019 23:07
Operator : JU/SJ
Sample : K2613-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 11 02:48:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 07 05:36:07 2019
Response via : Initial Calibration

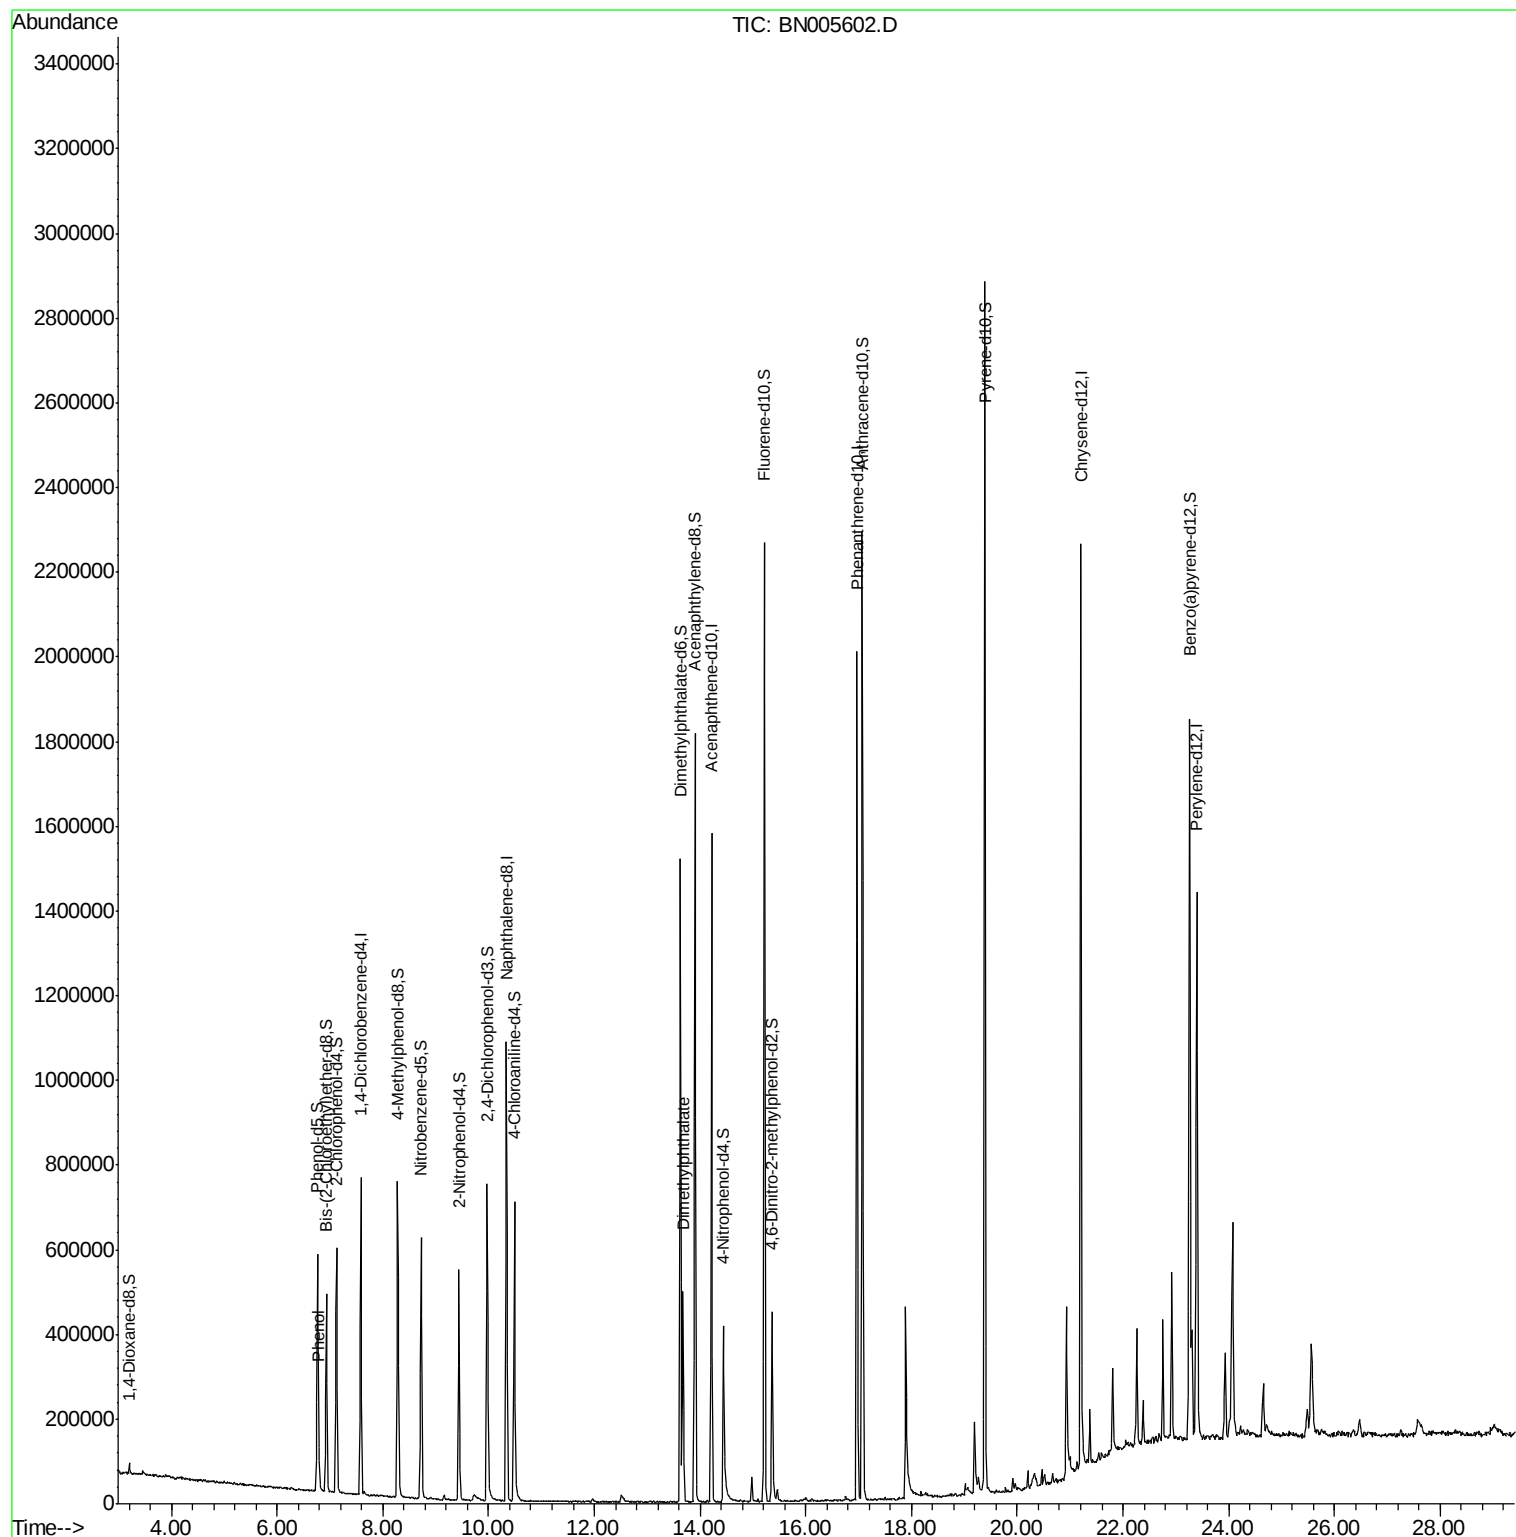

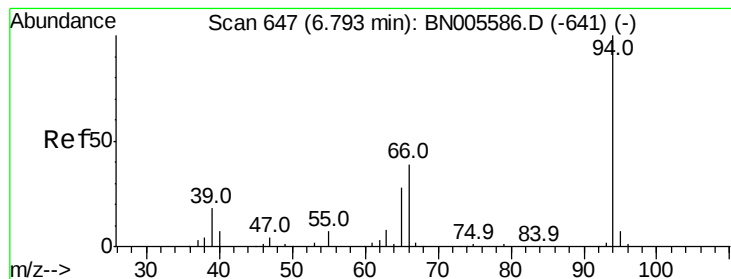





#6

Phenol

Concen: 1.410 ng/ul
 RT: 6.79 min Scan# 647
 Delta R.T. -0.01 min
 Lab File: BN005602.D
 Acq: 10 May 2019 23:07

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 94 Resp: 24123
 Ion Ratio Lower Upper
 94 100
 65 31.4 24.2 36.4
 66 41.0 33.8 50.6

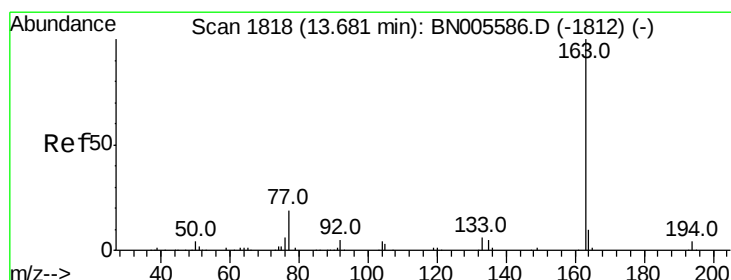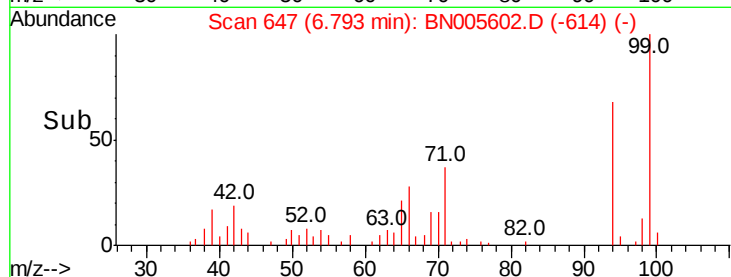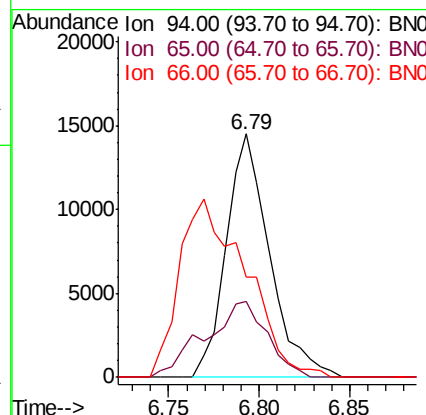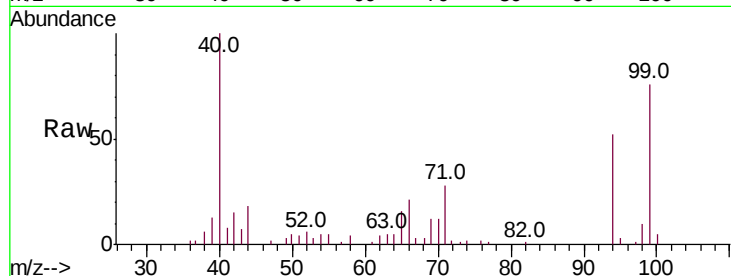

#44

Dimethylphthalate

Concen: 8.914 ng/ul
 RT: 13.68 min Scan# 1818
 Delta R.T. -0.01 min
 Lab File: BN005602.D
 Acq: 10 May 2019 23:07

Tgt Ion: 163 Resp: 338252
 Ion Ratio Lower Upper
 163 100
 194 4.7 3.4 5.0
 164 10.0 8.1 12.1

