

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\
 Data File : BN005630.D
 Acq On : 11 May 2019 17:14
 Operator : JU/SJ
 Sample : PB119423BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK23

Quant Time: May 12 00:39:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun May 12 00:36:09 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2061	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	8124	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	4809	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.08	188	822157	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.22
20) Perylene-d12	23.28	264	626726	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	4116	0.32	ng/ul	0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.22	166	1408	0.070	ng/ul#	Qvalue 16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\
Data File : BN005630.D
Acq On : 11 May 2019 17:14
Operator : JU/SJ
Sample : PB119423BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK23

Quant Time: May 12 00:39:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 12 00:36:09 2019
Response via : Initial Calibration

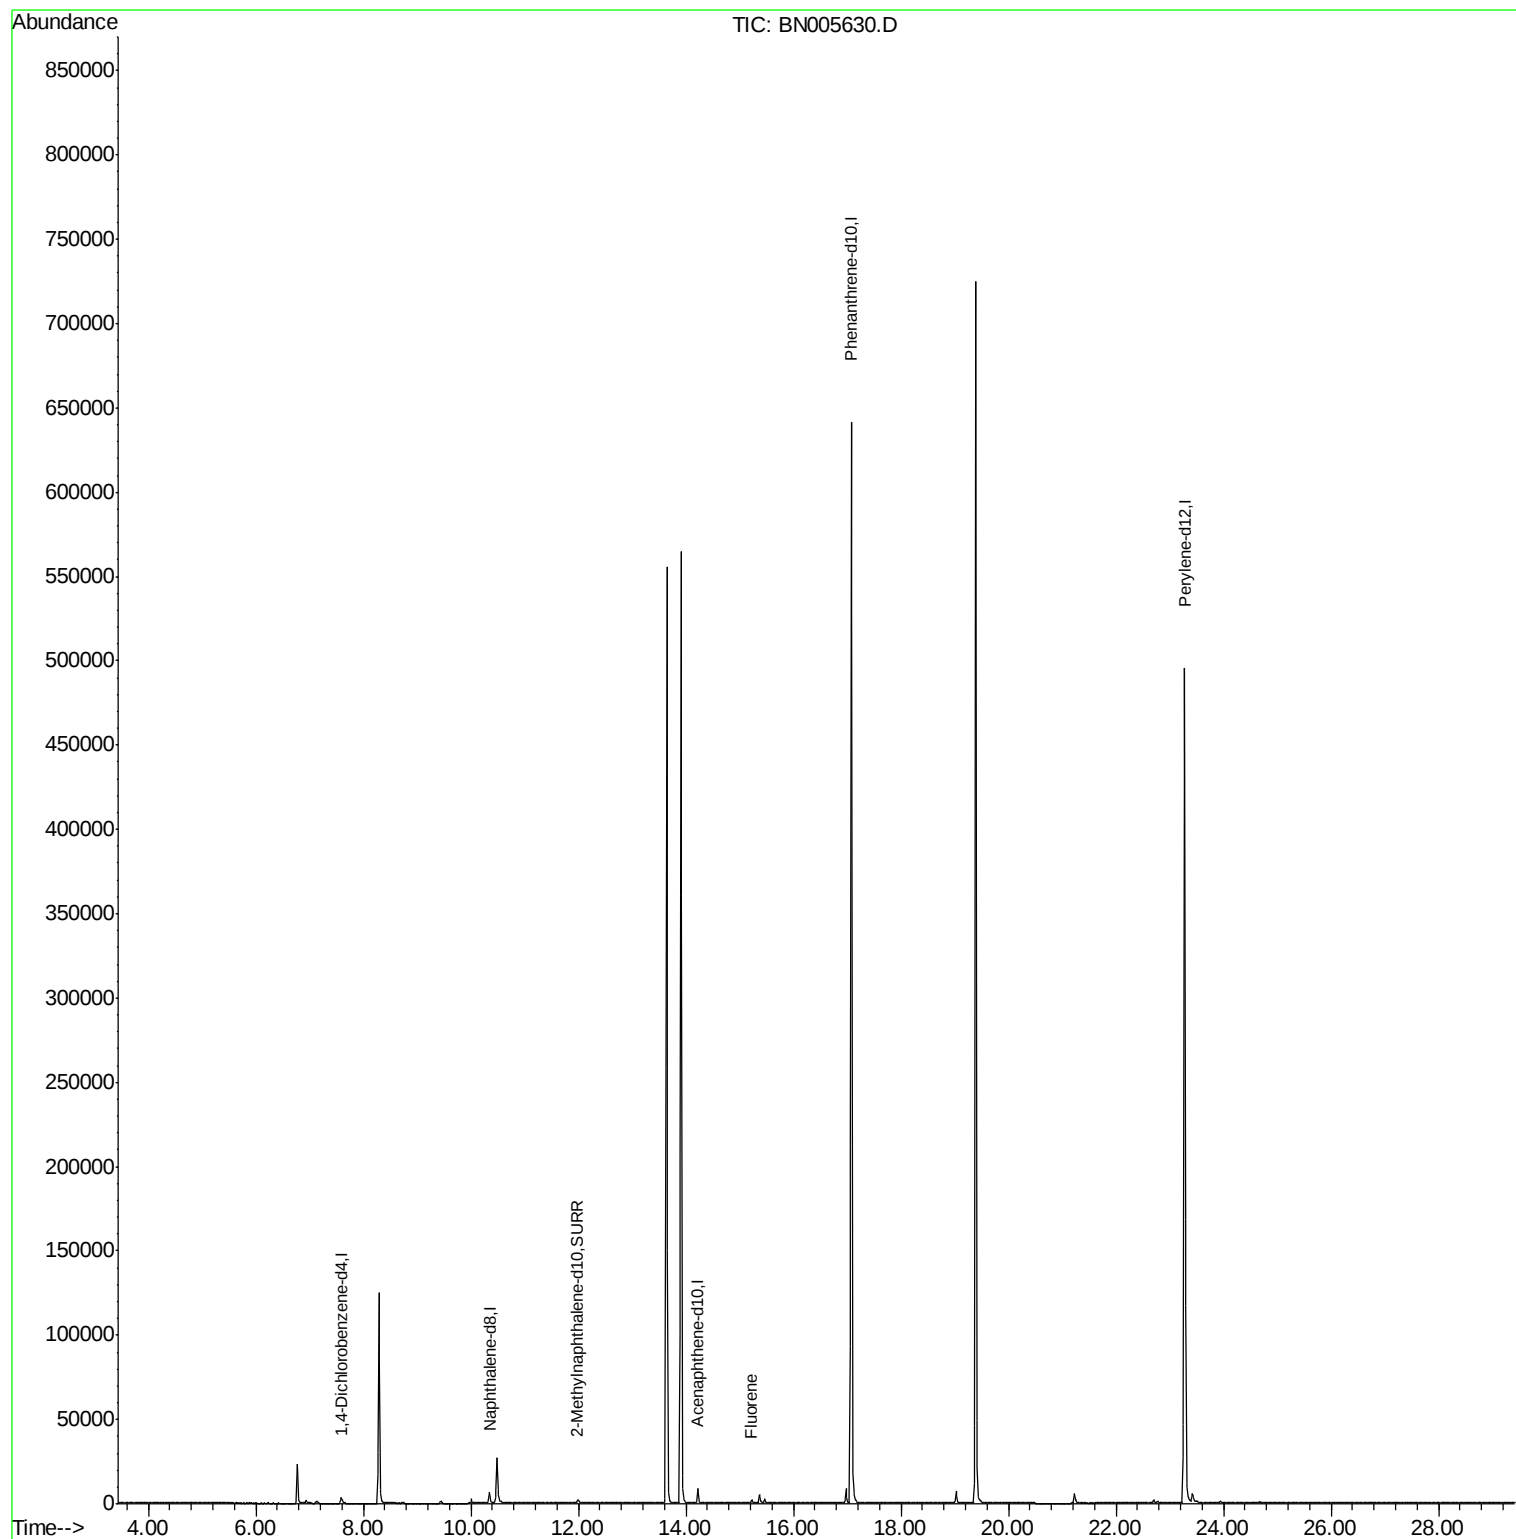

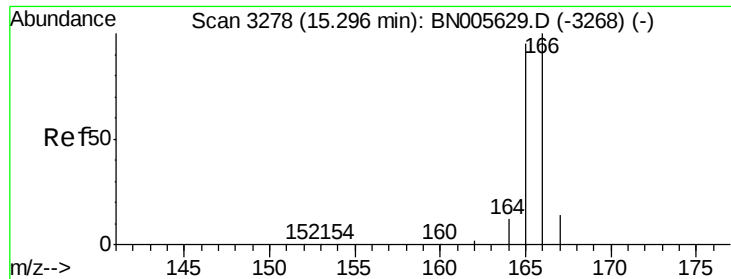

#9

Fluorene

Concen: 0.070 ng/ul

RT: 15.22 min Scan# 3262

Delta R.T. -0.07 min

Lab File: BN005630.D

Acq: 11 May 2019 17:14

Instrument :

BNA_N

ClientSampleId :

SBLK23

Tgt Ion:166 Resp: 1408

Ion Ratio Lower Upper

166 100

165 9.9 78.0 117.0#

167 36.9 12.2 18.4#

