

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:19:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019


Response via : Initial Calibration

Instrument :

BNA_N

Client Sample ID :

A5144

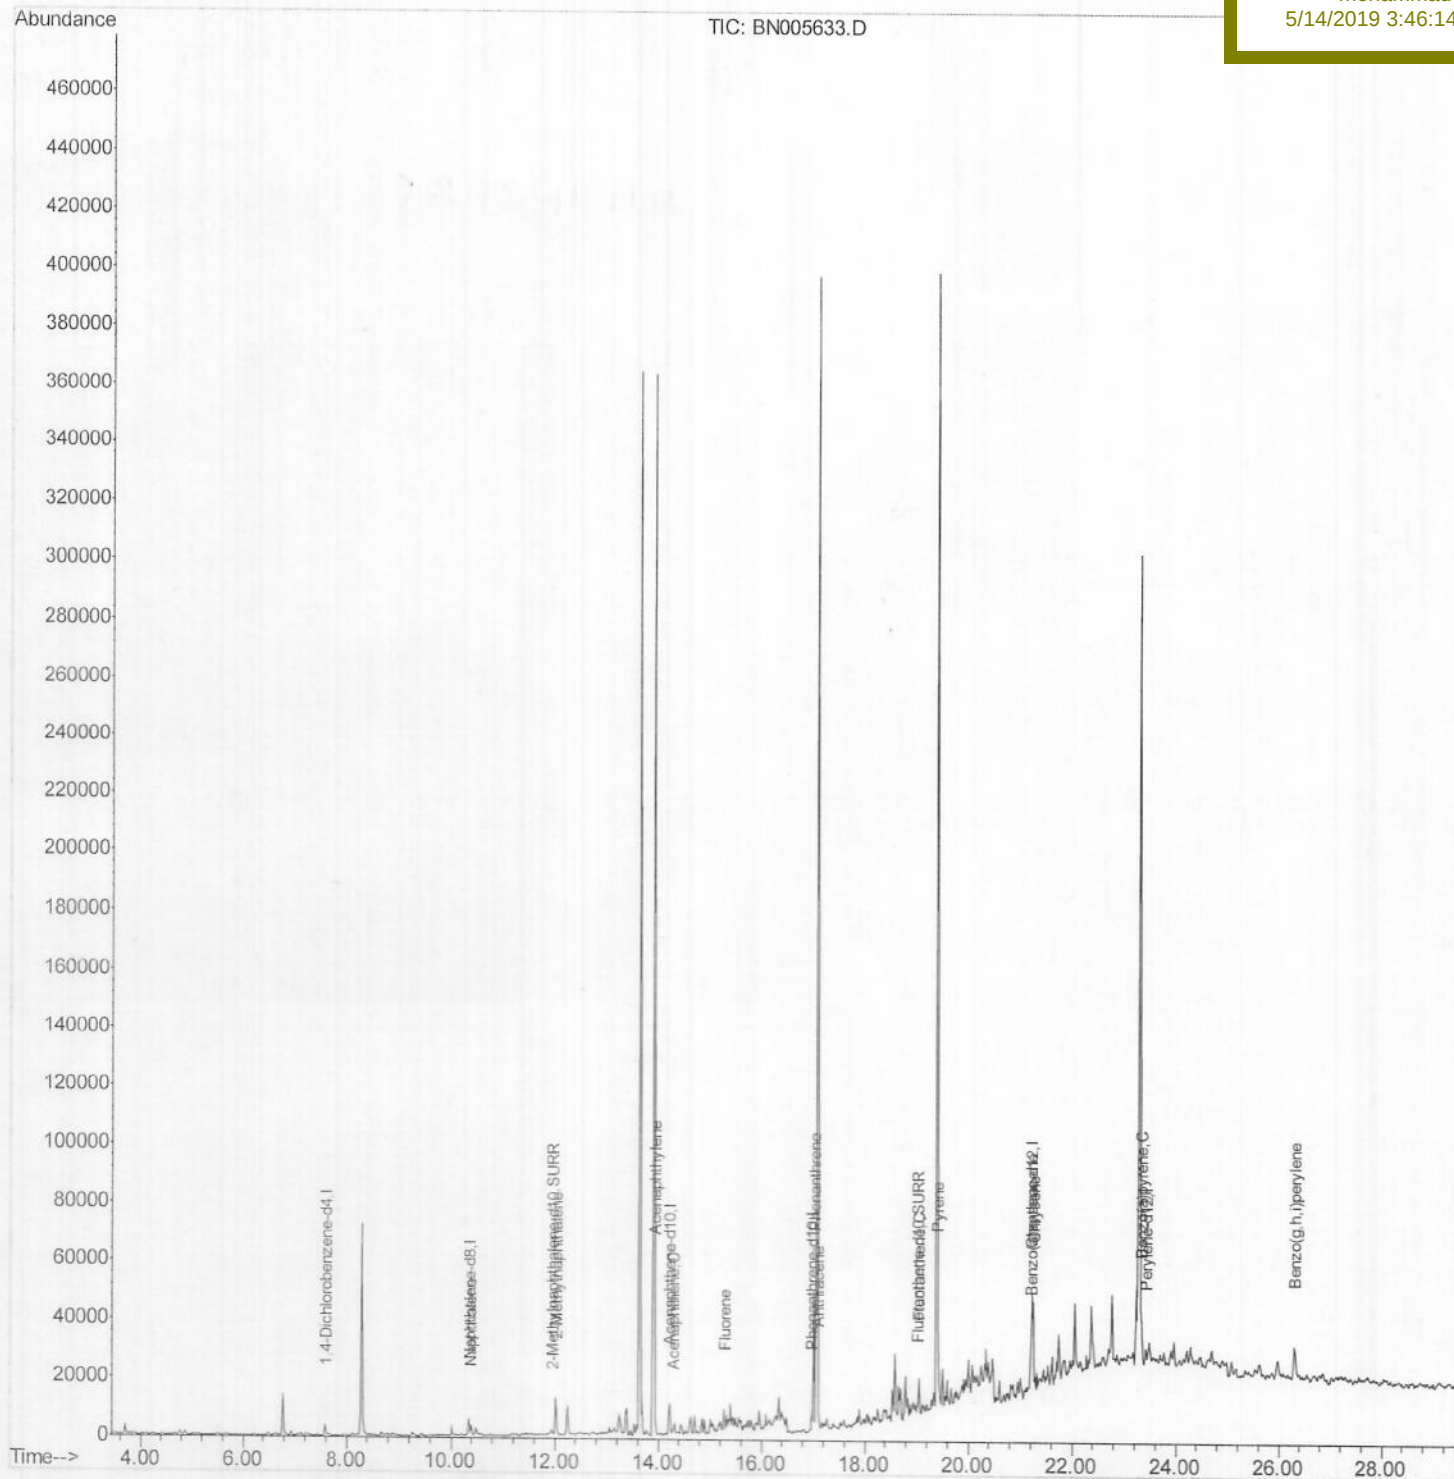Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 00:40:09 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A5144

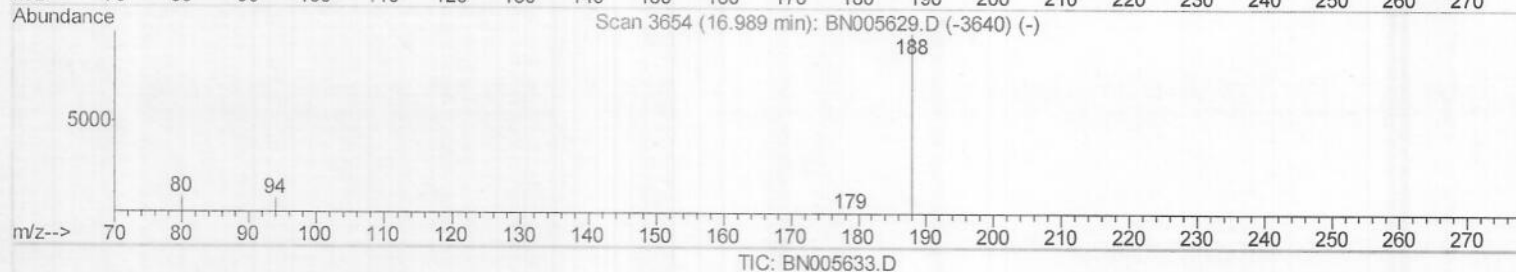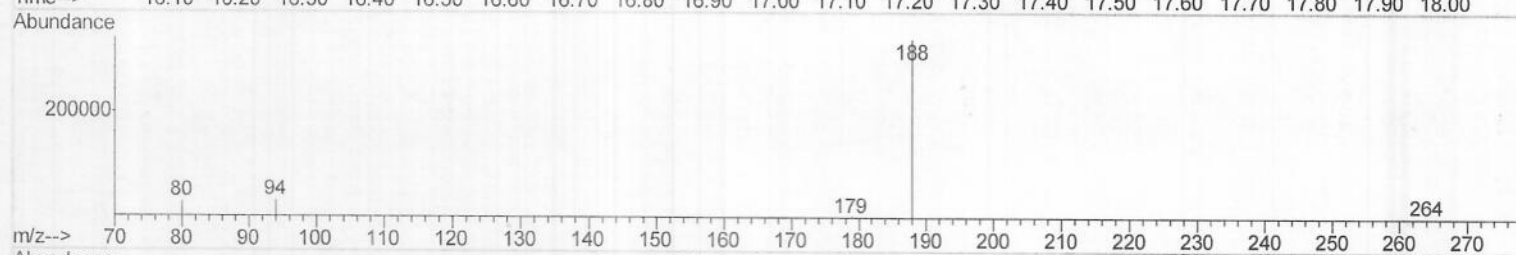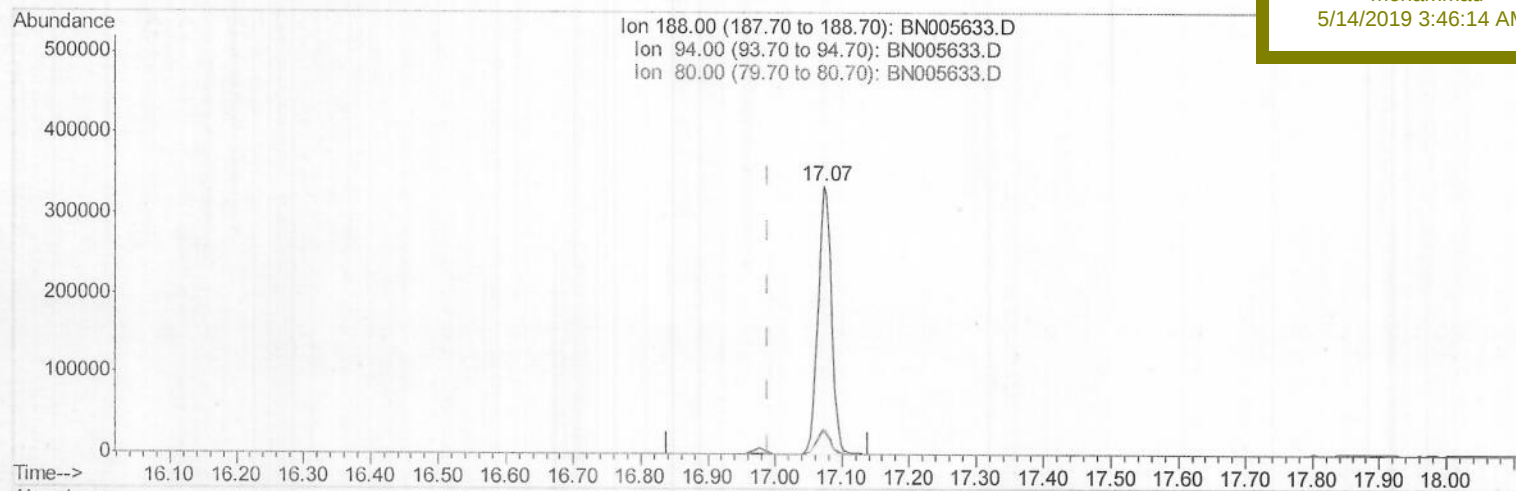Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(10) Phenanthrene-d10 (I)

17.073min (+0.084) 0.40ng/ul

response 471111

Ion	Exp%	Act%
188.00	100	100
94.00	9.40	9.20
80.00	9.80	8.41
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 00:40:09 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A5144

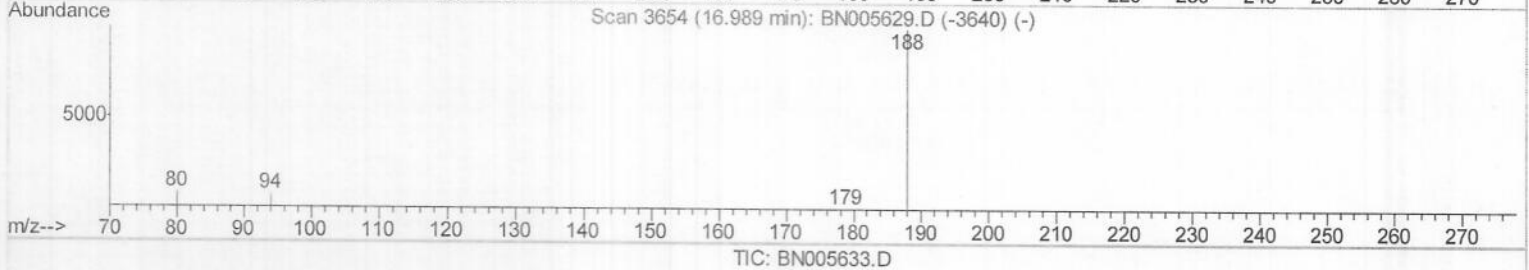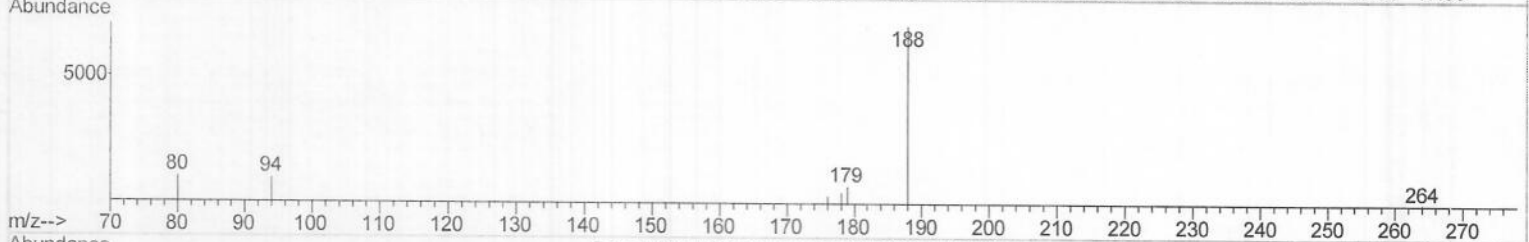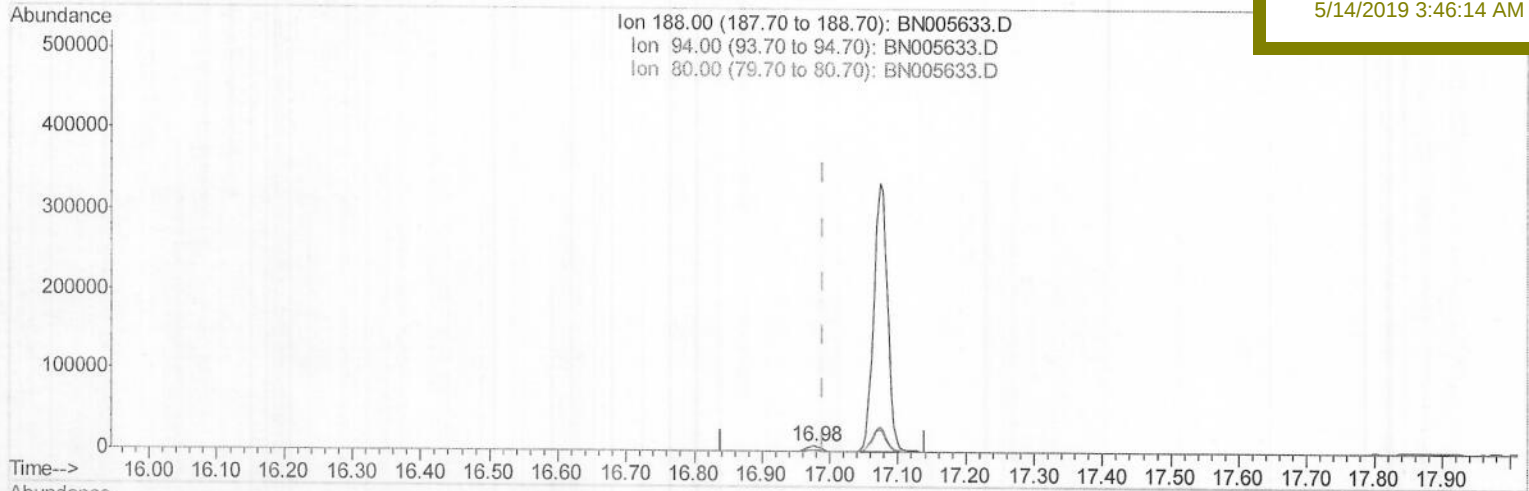Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(10) Phenanthrene-d10 (I)

16.976min (-0.013) 0.40ng/ul m) JU05114119

response 9424

Ion	Exp%	Act%
188.00	100	100
94.00	9.40	14.79#
80.00	9.80	15.36#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

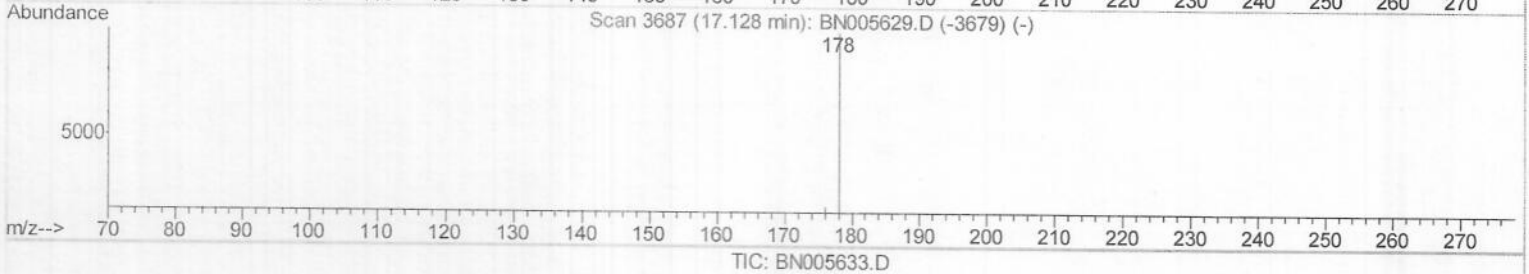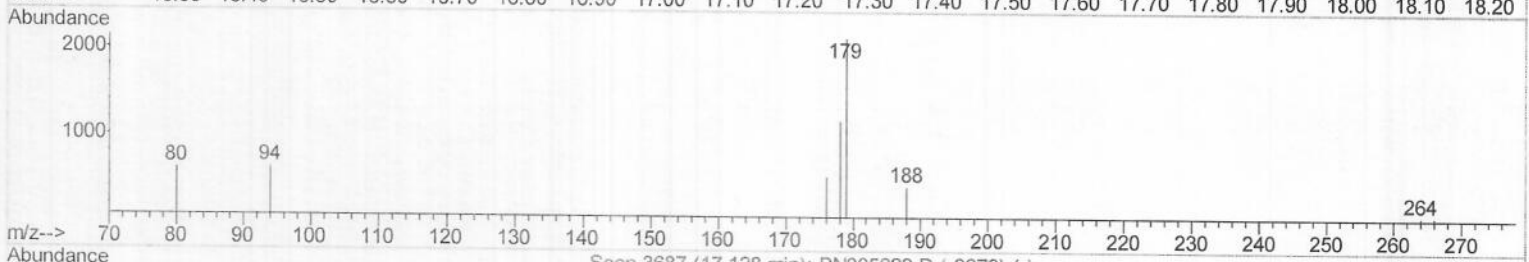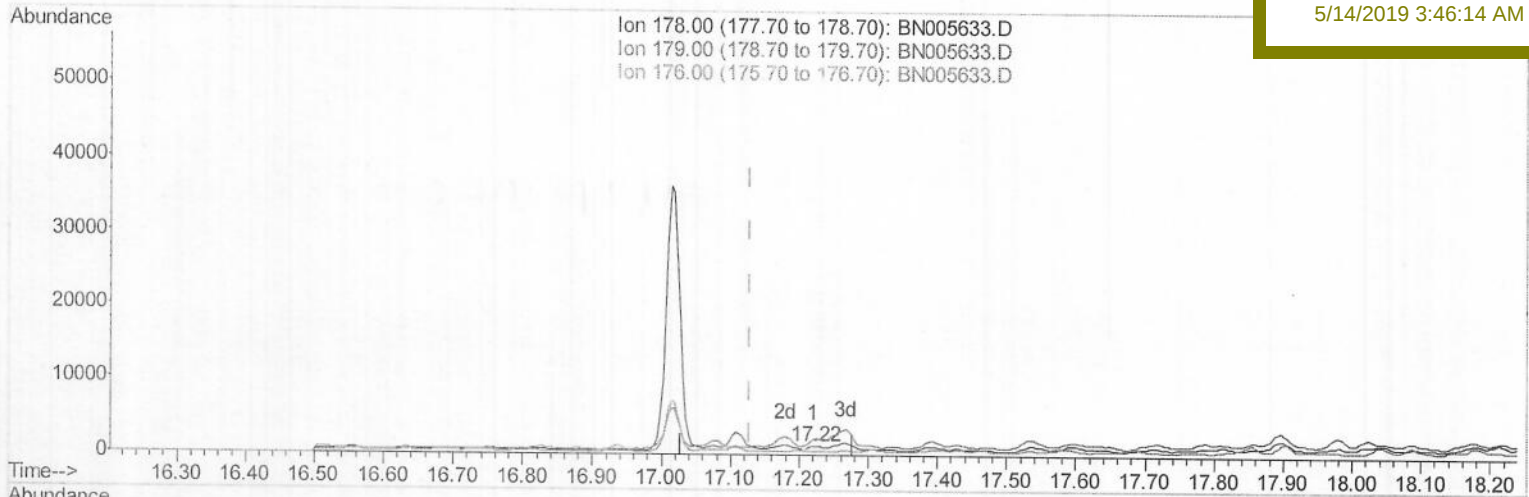

(13) Anthracene

17.221min (+0.093) 0.02ng/ul

response 576

Ion	Exp%	Act%
178.00	100	100
179.00	16.80	180.41#
176.00	18.90	44.68#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

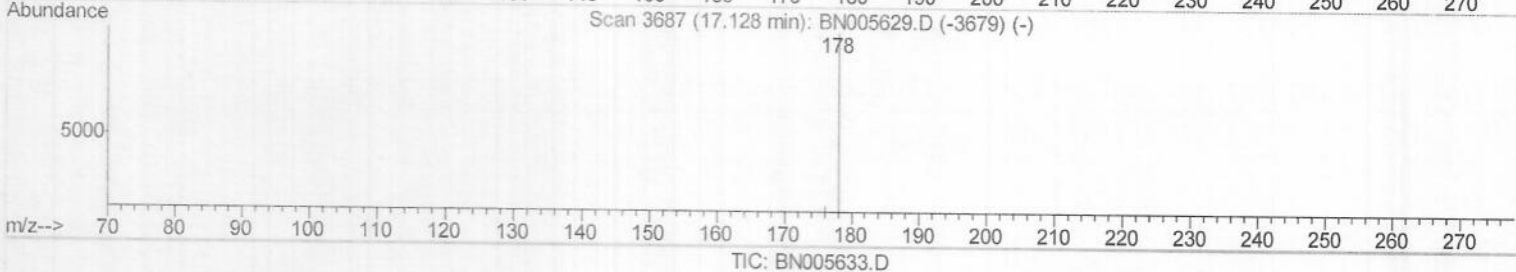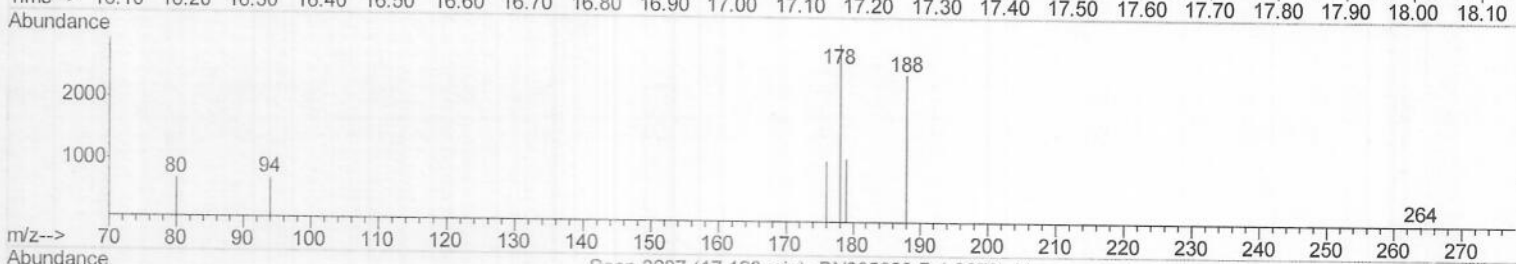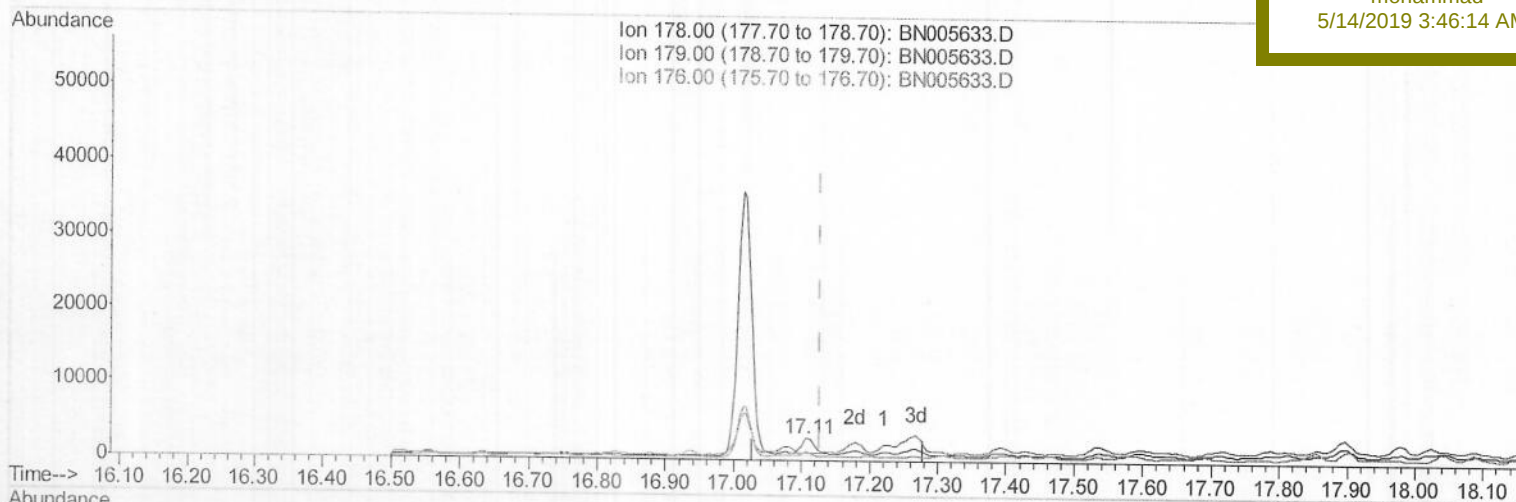

TIC: BN005633.D

(13) Anthracene

17.107min (-0.021) 0.14ng/ul m

JU05/14/19

response 3482

Ion	Exp%	Act%
178.00	100	100
179.00	16.80	36.87#
176.00	18.90	35.78#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A5144

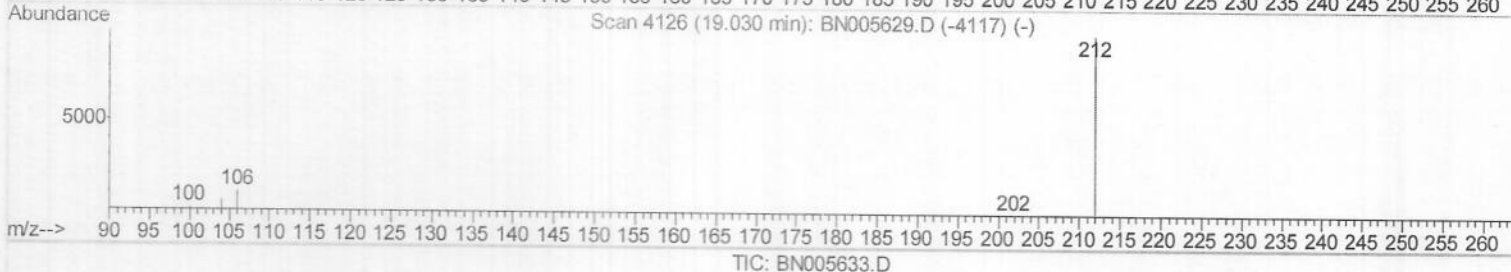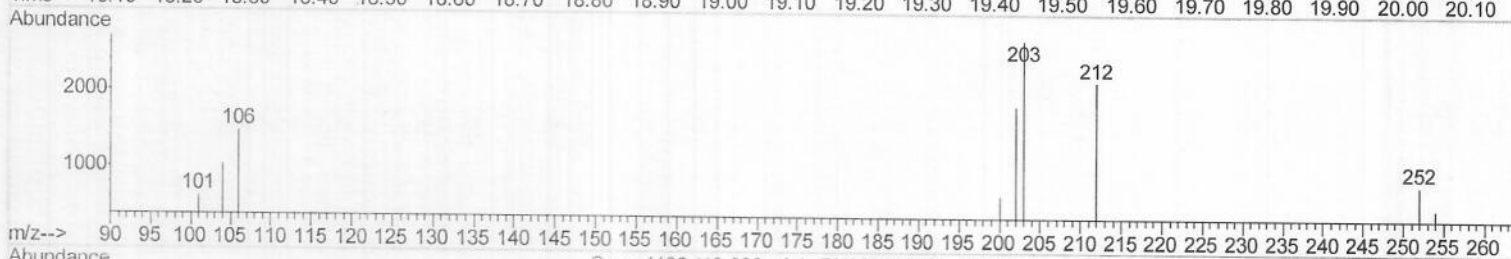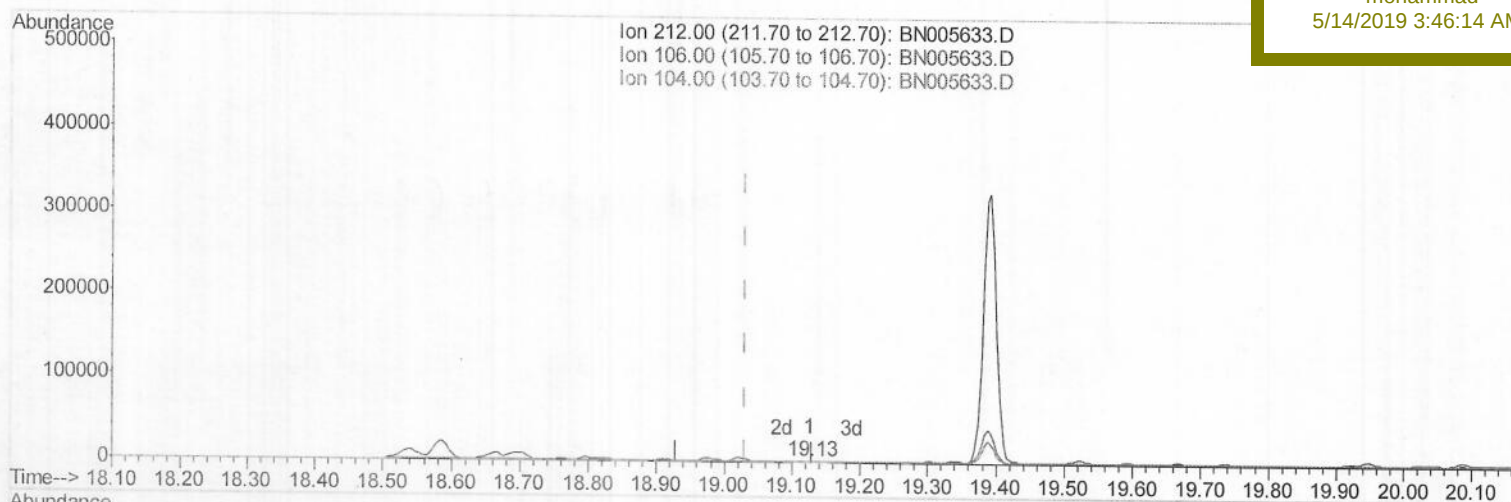Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(14) Fluoranthene-d10 (SURR)

19.127min (+0.098) 0.11ng/ul

response 3372

Ion	Exp%	Act%
212.00	100	100
106.00	10.80	30.13#
104.00	6.20	27.25#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A5144

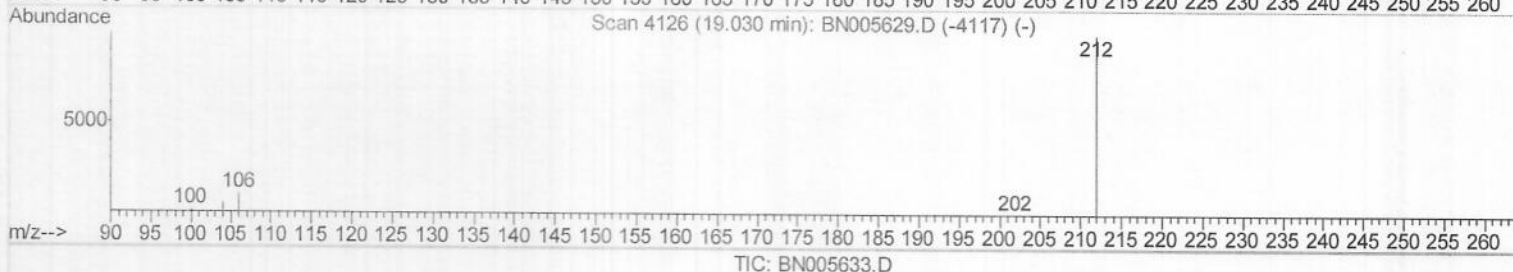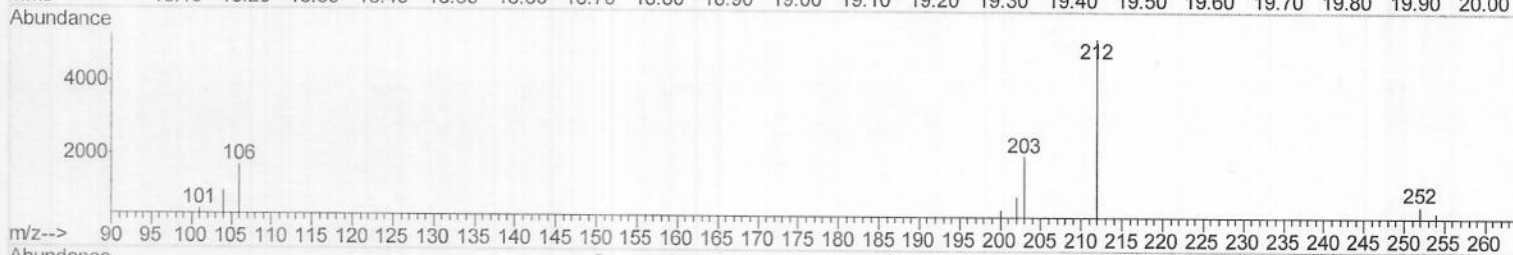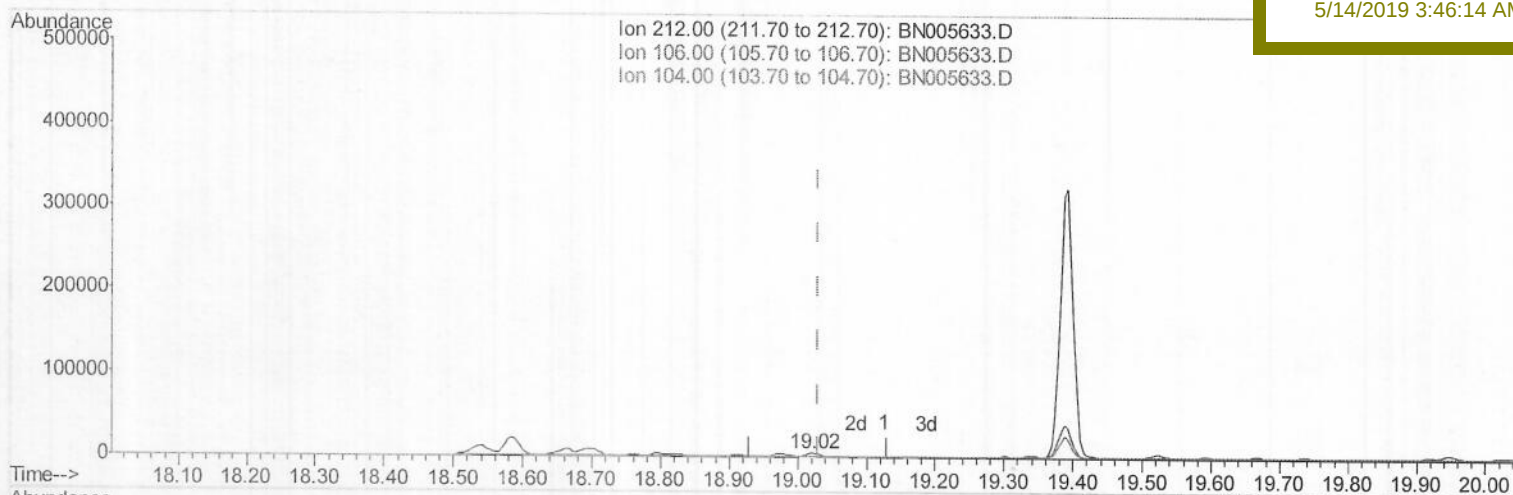Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(14) Fluoranthene-d10 (SURR)

19.020min (-0.009) 0.23ng/ul m > JU0514119

response 6783

Ion	Exp%	Act%
212.00	100	100
106.00	10.80	14.96#
104.00	6.20	13.55#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampled :

A5144

Manual Integrations
APPROVED

mohammad

5/14/2019 3:46:14 AM

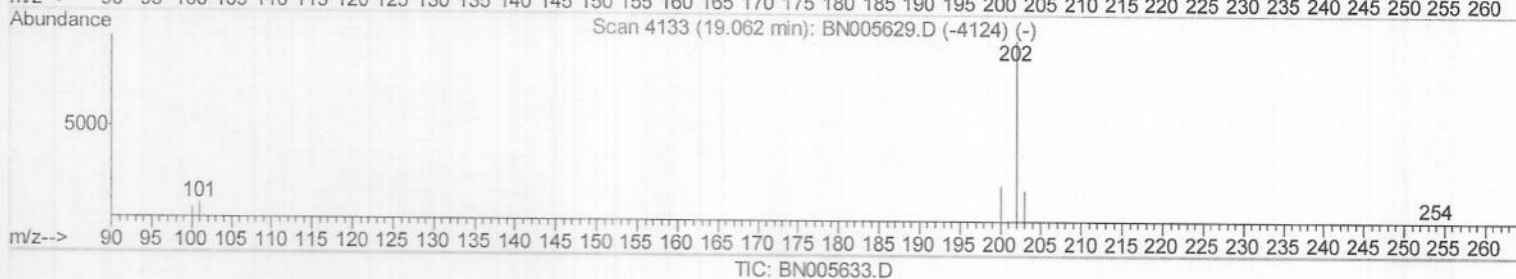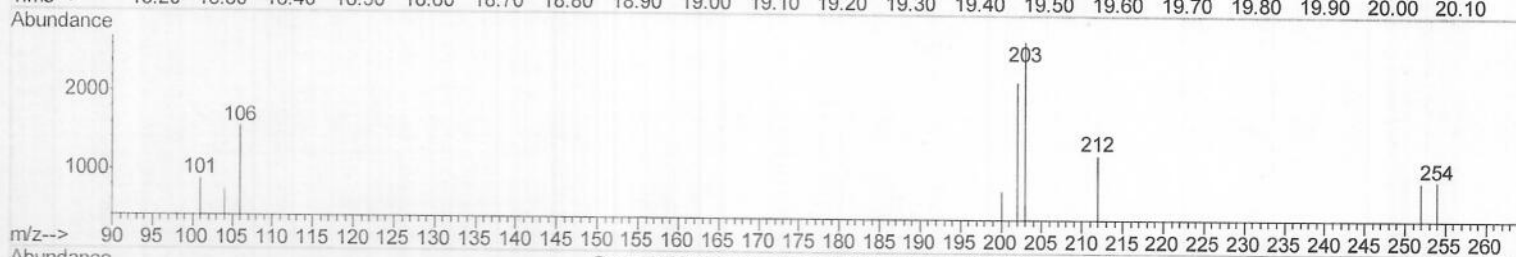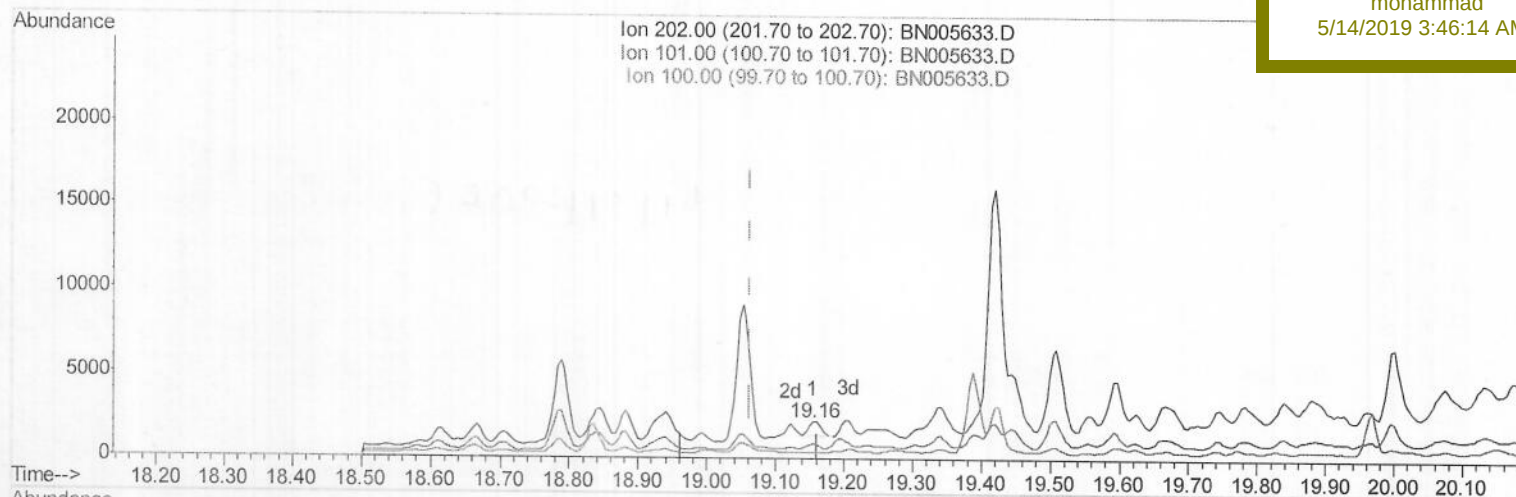

(15) Fluoranthene (C)

19.155min (+0.093) 0.03ng/ul

response 1175

Ion	Exp%	Act%
202.00	100	100
101.00	9.40	39.69#
100.00	7.10	18.14
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

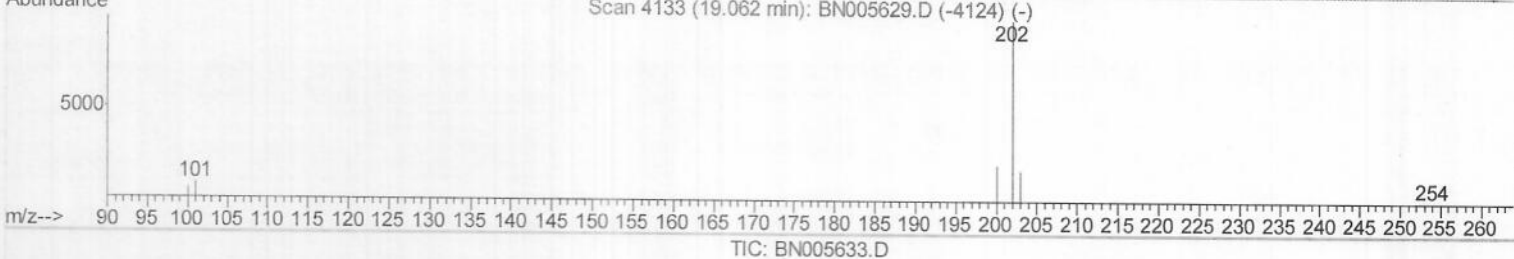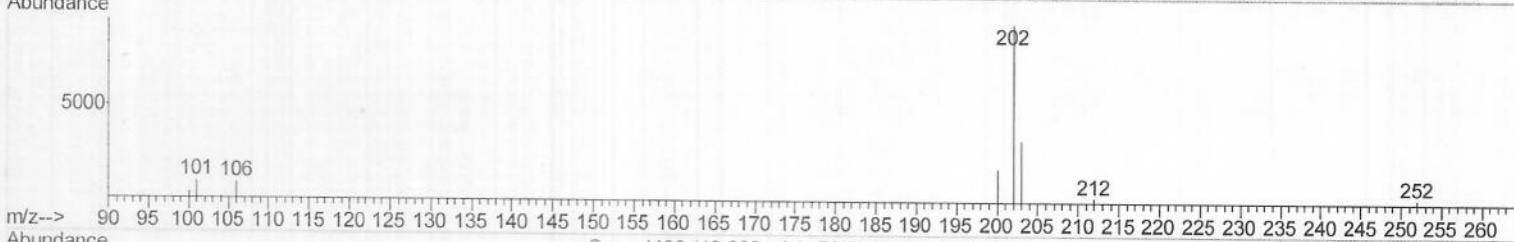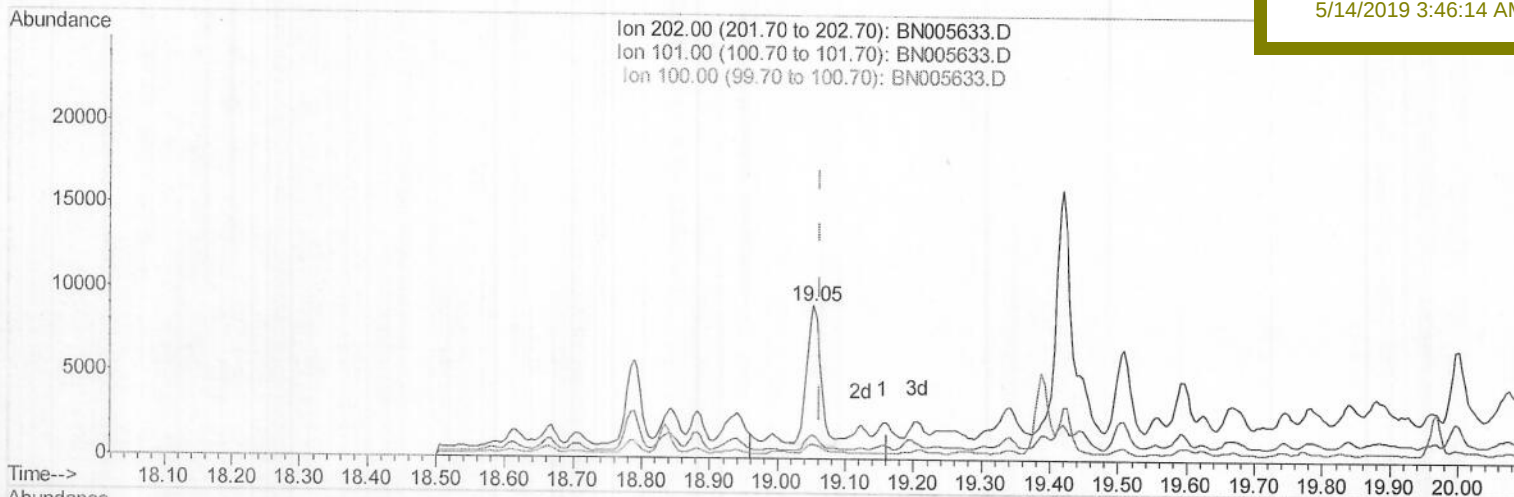

(15) Fluoranthene (C)

19.053min (-0.009) 0.33ng/ul m

JU05114119

response 11658

Ion	Exp%	Act%
202.00	100	100
101.00	9.40	15.53
100.00	7.10	9.81
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

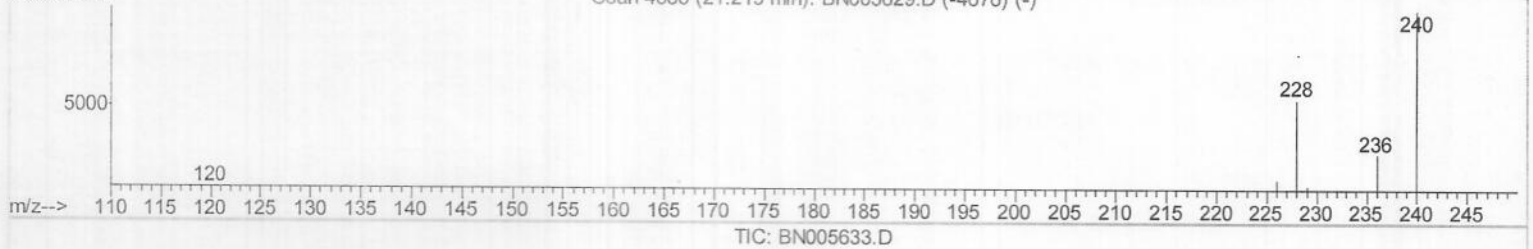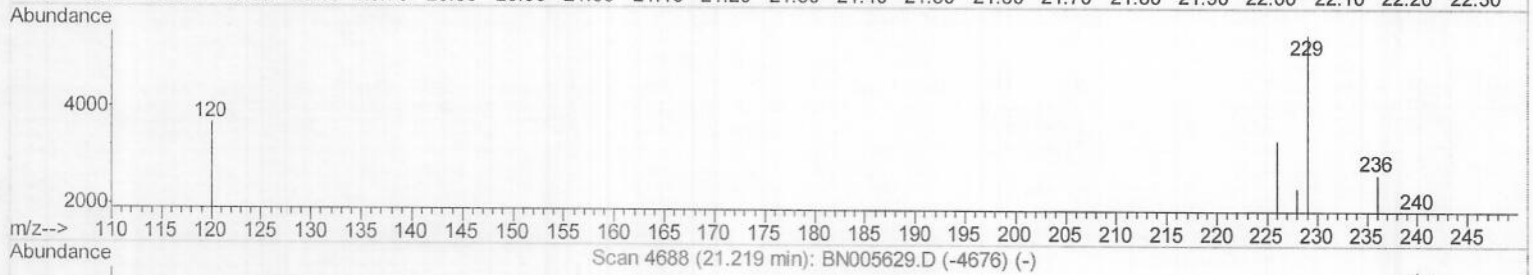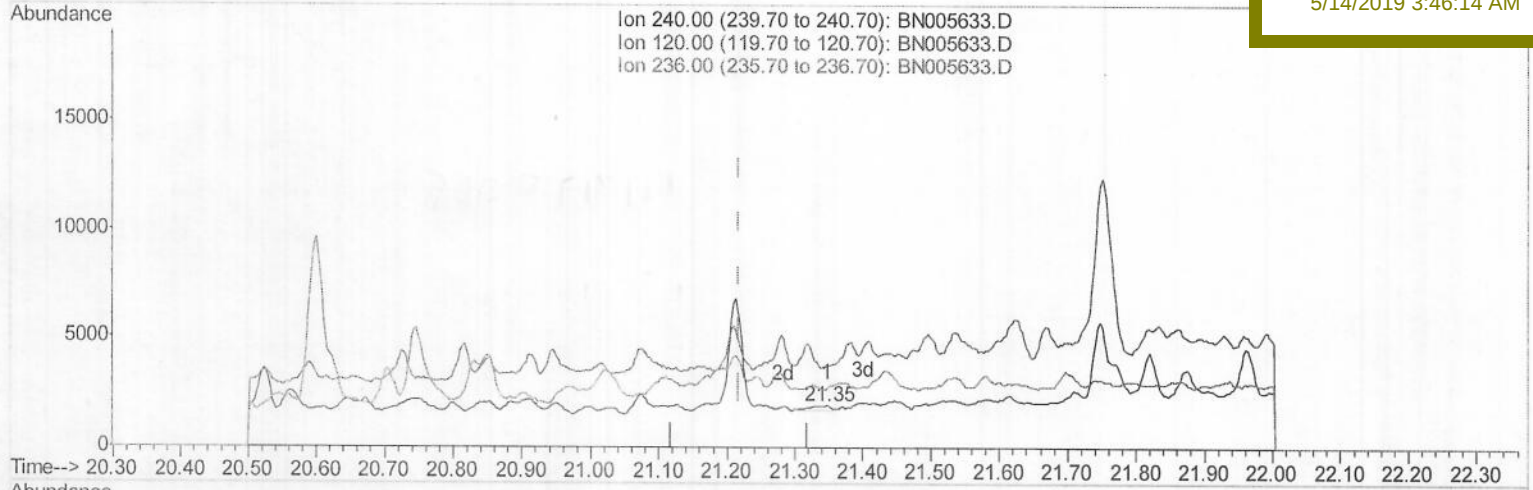

(16) Chrysene-d12 (I)

21.347min (+0.128) 0.40ng/ul

response 534

Ion	Exp%	Act%
240.00	100	100
120.00	11.90	193.98#
236.00	28.00	139.95#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:09:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

A5144

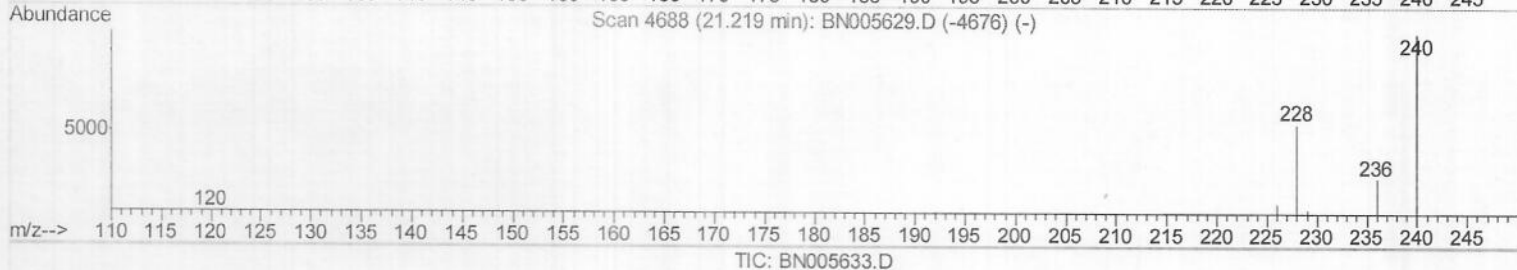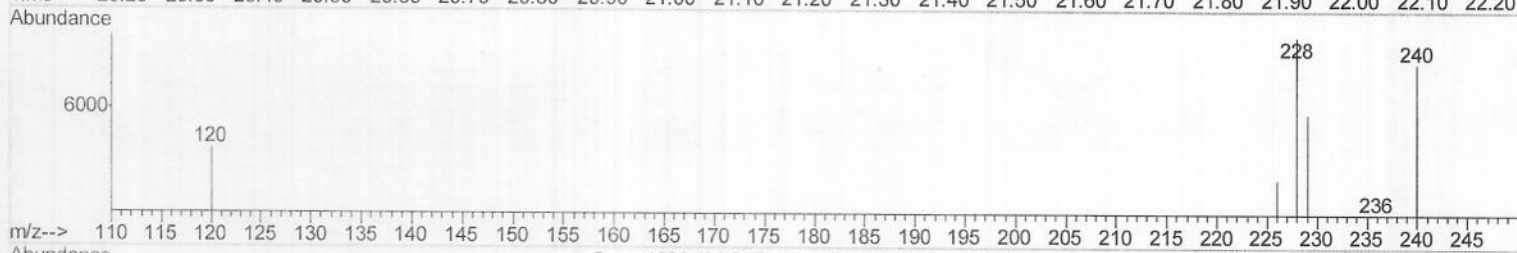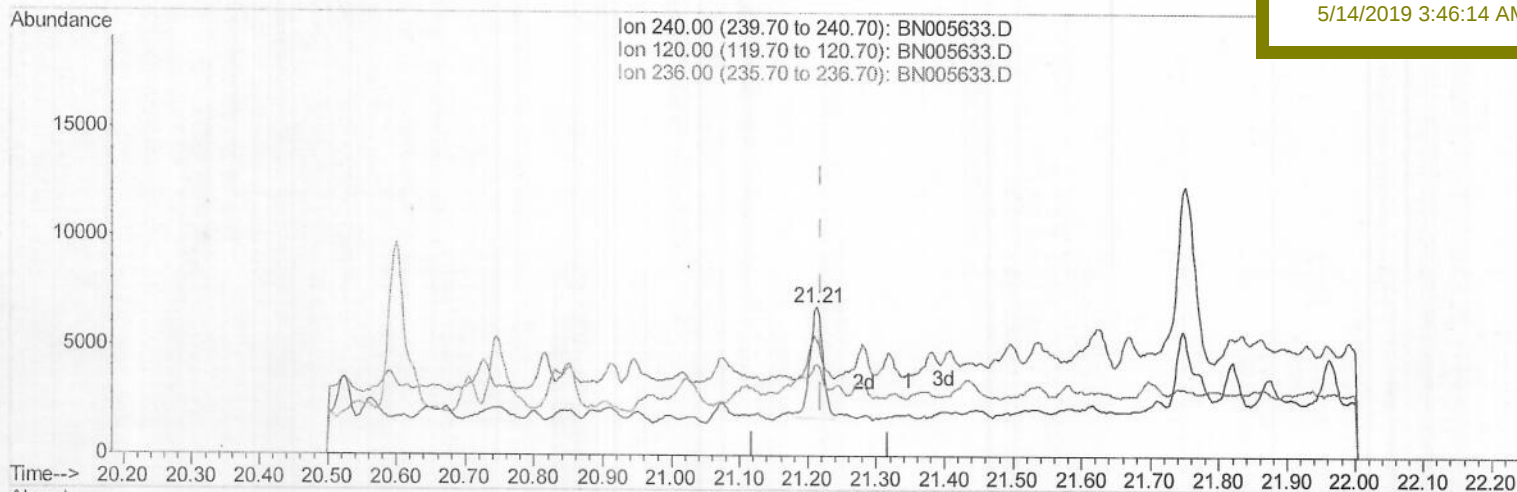Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(16) Chrysene-d12 (I)

21.213min (-0.006) 0.40ng/ul m > JU0514119

response 6817

Ion	Exp%	Act%
240.00	100	100
120.00	11.90	77.92#
236.00	28.00	61.46#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:11:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

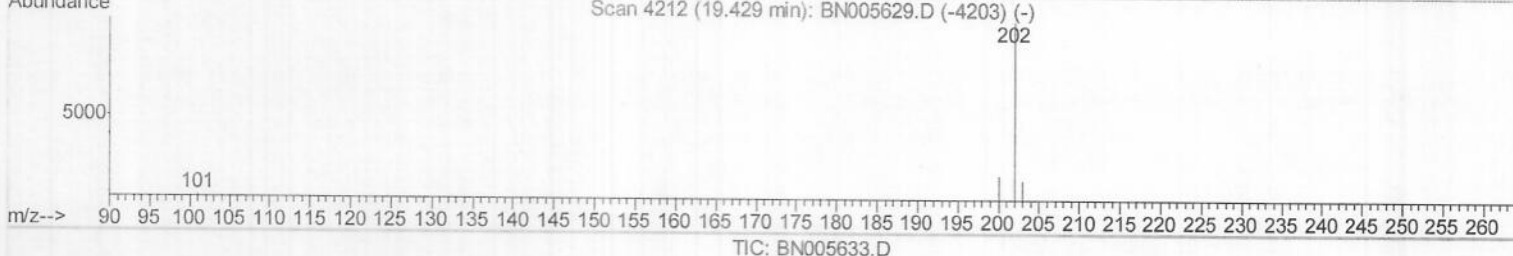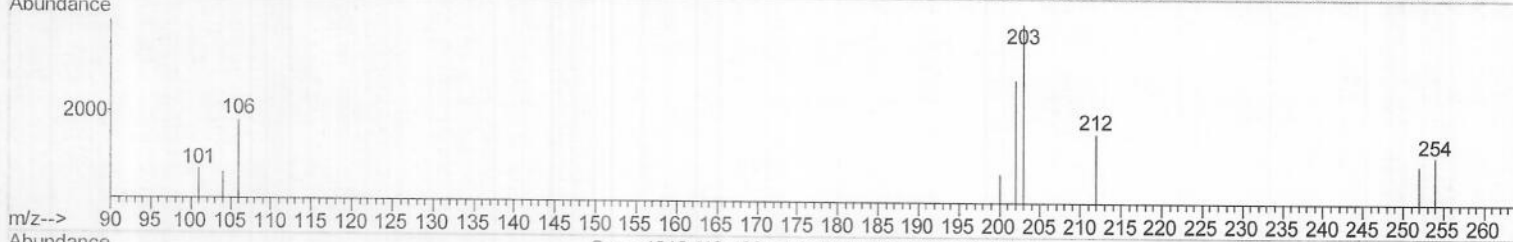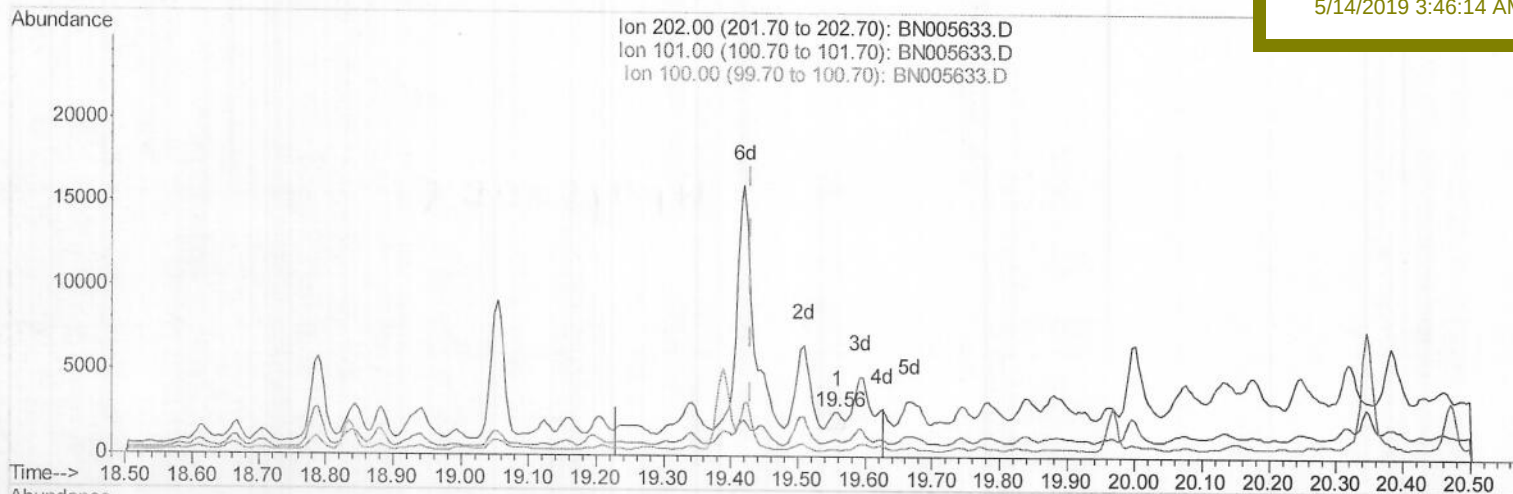

(17) Pyrene

19.560min (+0.130) 0.05ng/ul

response 1157

Ion	Exp%	Act%
202.00	100	100
101.00	10.60	36.53#
100.00	8.60	16.92#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:11:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

A5144

Manual Integrations
APPROVED

mohammad

5/14/2019 3:46:14 AM

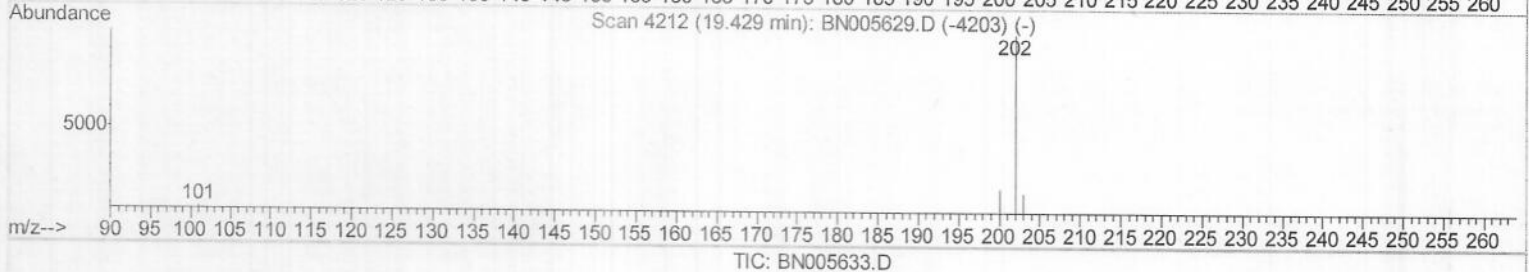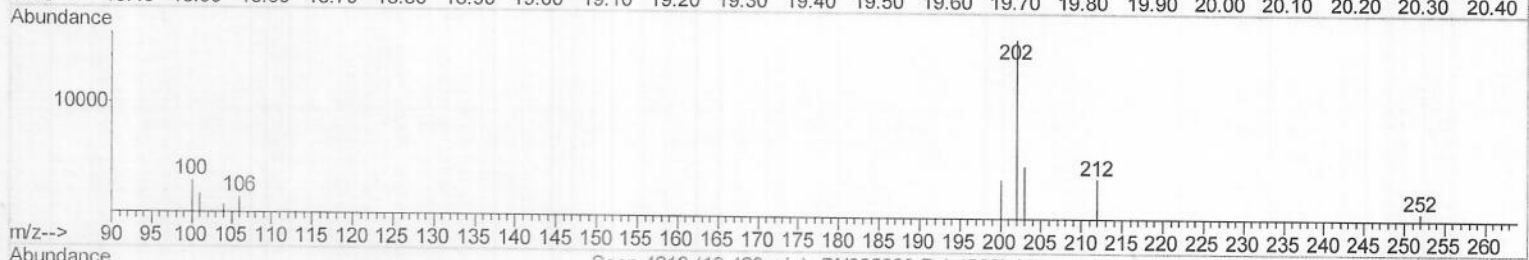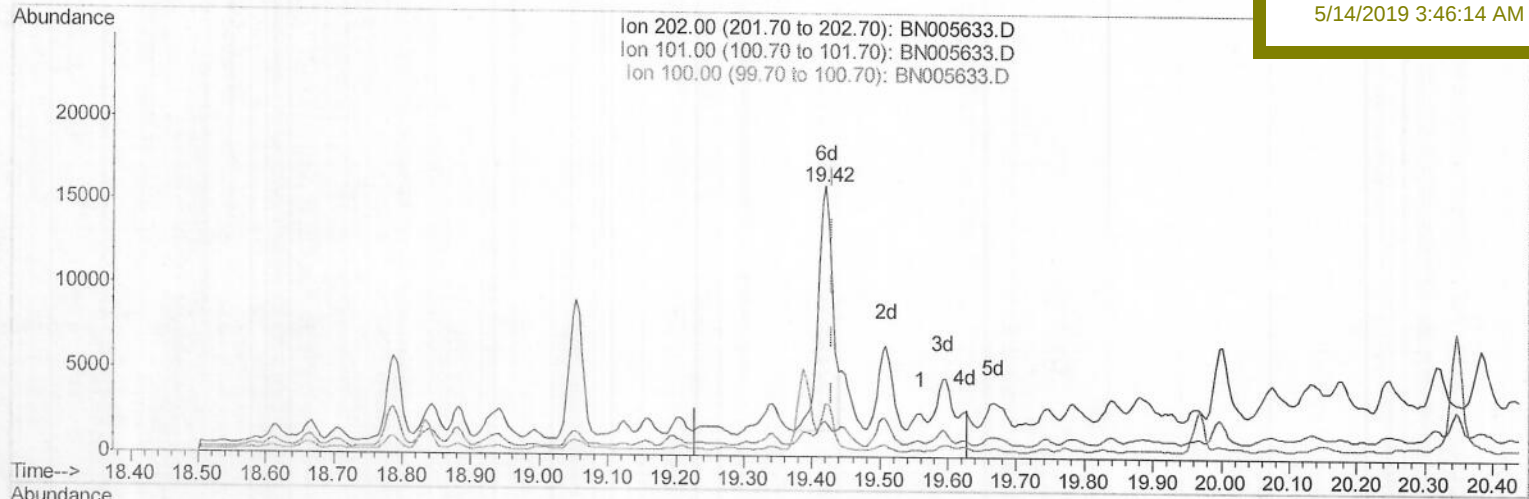

(17) Pyrene

19.420min (-0.009) 0.84ng/ul m >JU05/14/19

response 21130

Ion	Exp%	Act%
202.00	100	100
101.00	10.60	12.98#
100.00	8.60	19.54#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:13:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

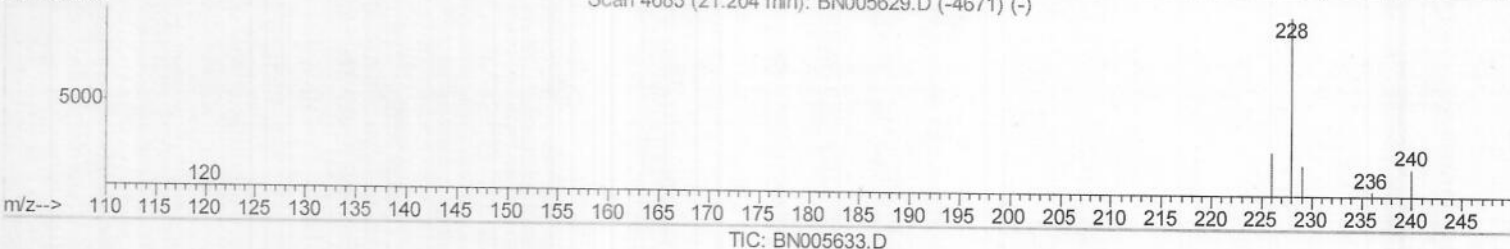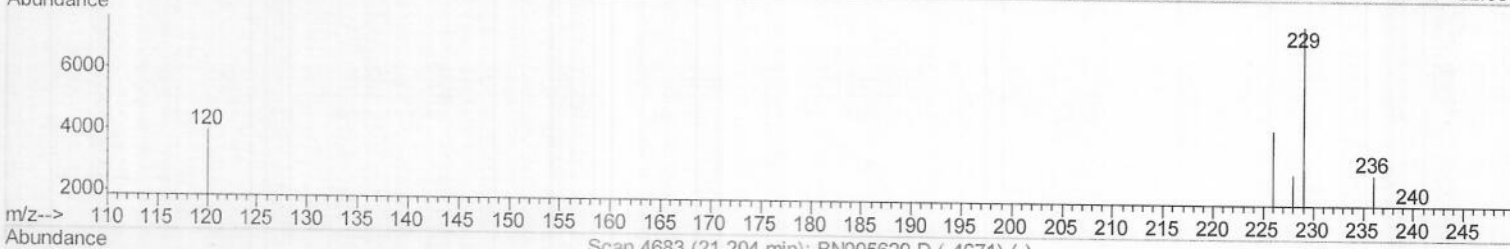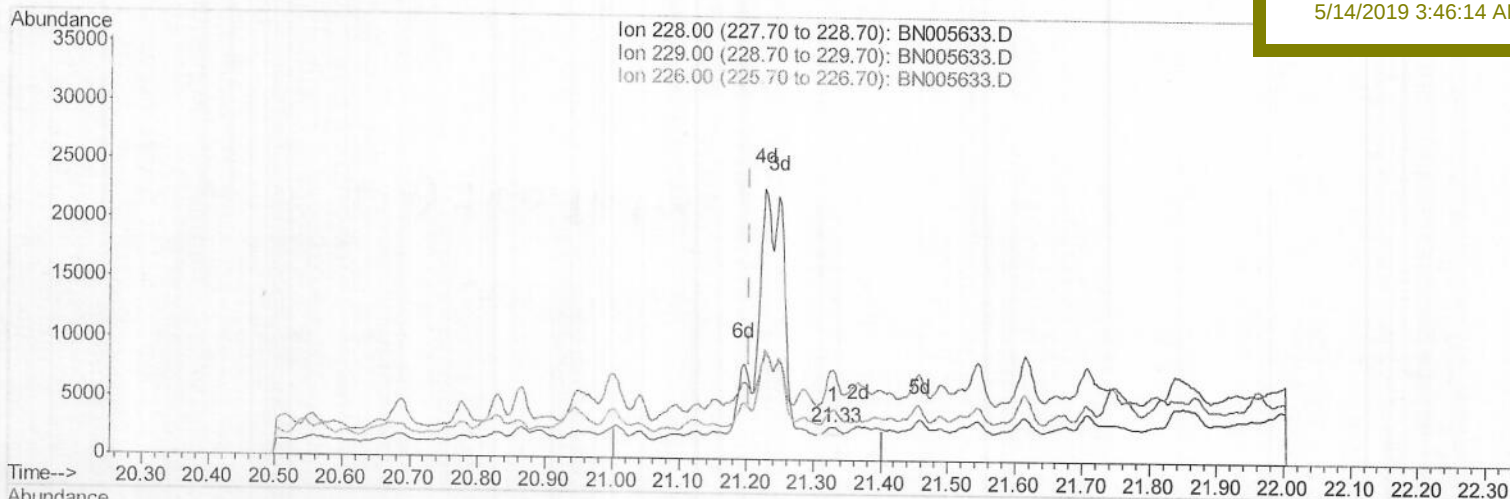

(18) Benzo(a)anthracene

21.330min (+0.126) 0.04ng/ul

response 908

Ion	Exp%	Act%
228.00	100	100
229.00	19.80	272.31#
226.00	27.10	151.12#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:13:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A5144

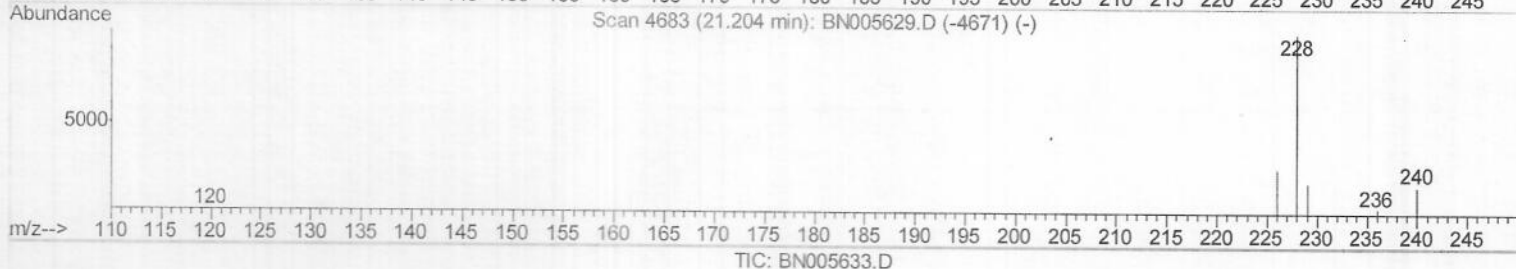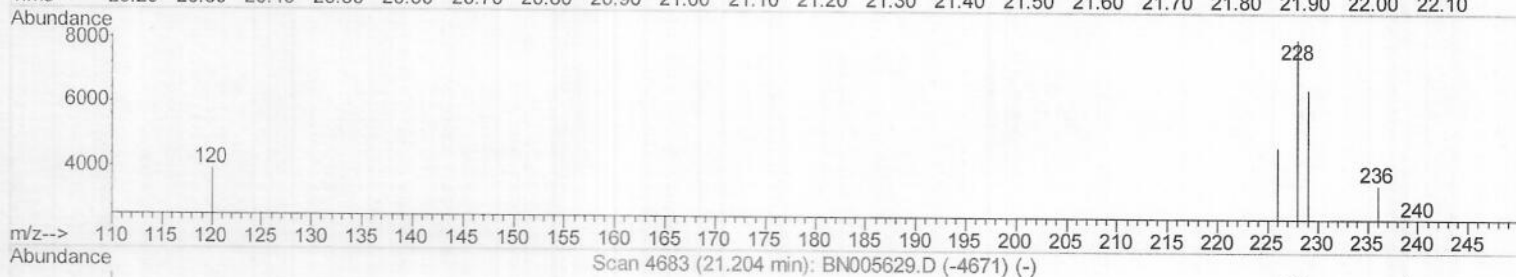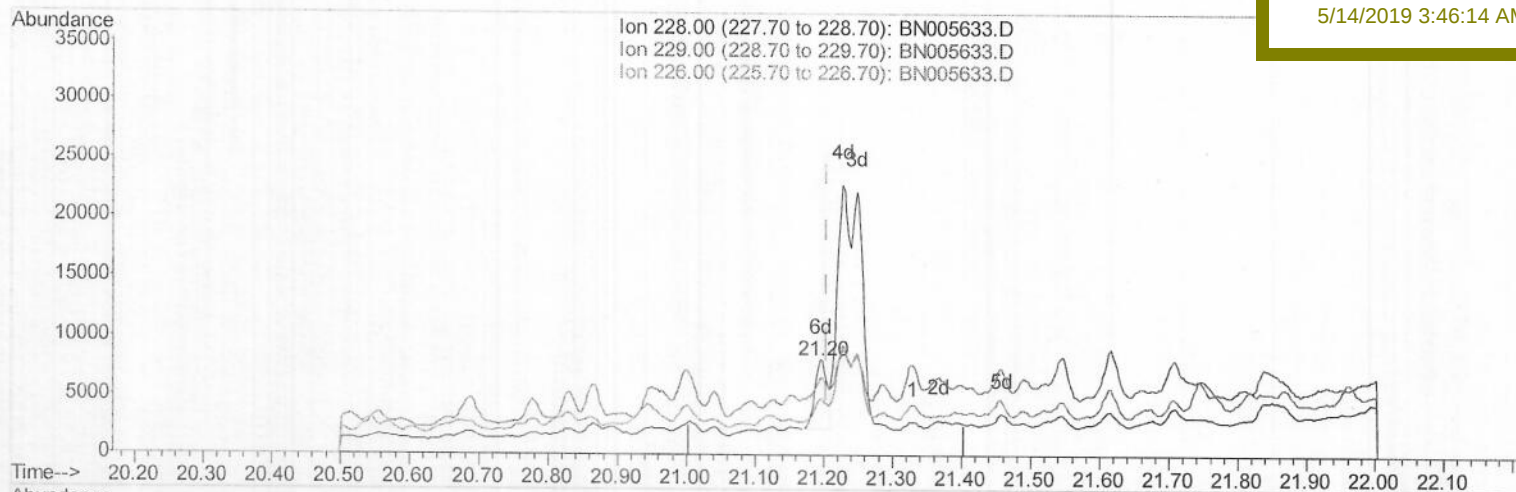Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(18) Benzo(a)anthracene

21.195min (-0.009) 0.33ng/ul m

S J 05/14/19

response 7807

Ion	Exp%	Act%
228.00	100	100
229.00	19.80	80.82#
226.00	27.10	58.66#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:13:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

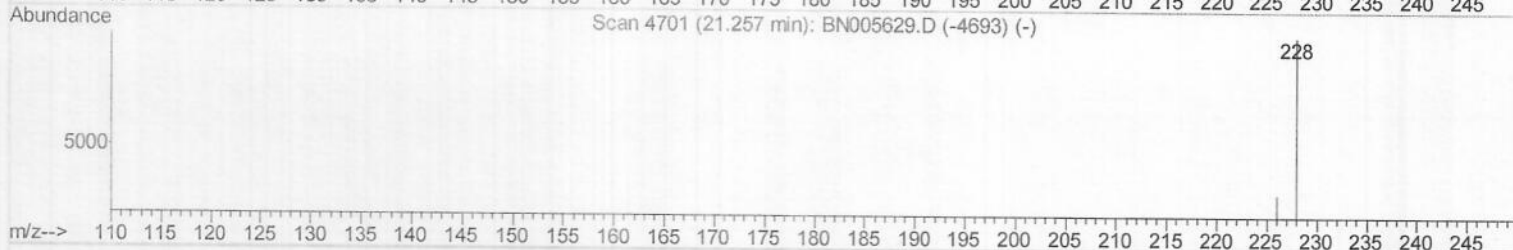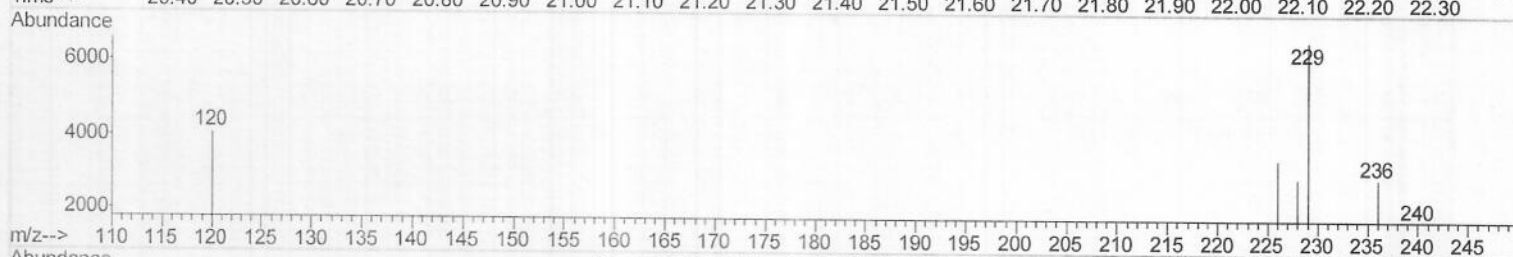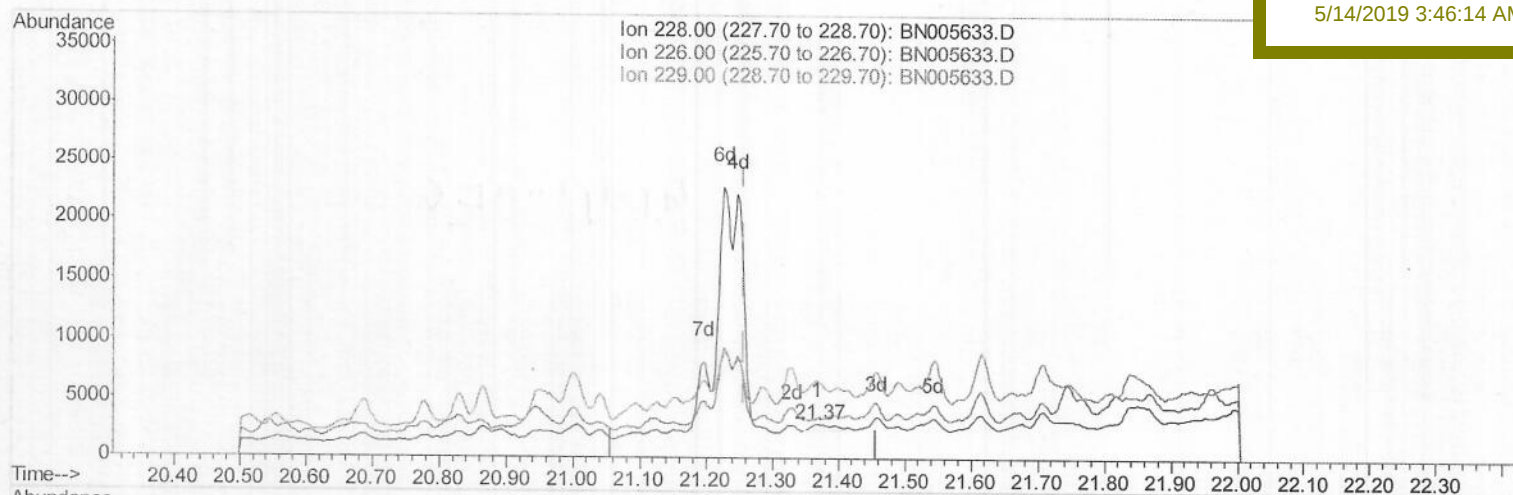

(19) Chrysene

21.368min (+0.111) 0.05ng/ul

response 1565

Ion	Exp%	Act%
228.00	100	100
226.00	29.00	116.05#
229.00	20.00	223.96#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:13:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019


Response via : Initial Calibration

Instrument :

BNA_N

Client Sample ID :

A5144

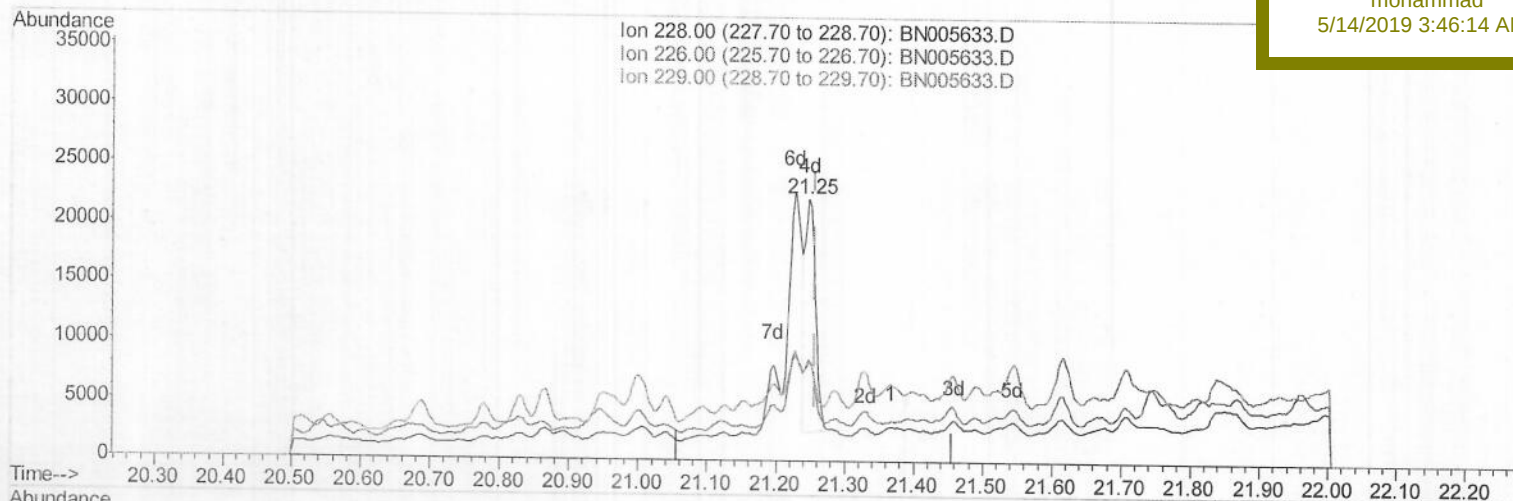Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(19) Chrysene

21.248min (-0.009) 0.71ng/ul m

response 20456

Ion	Exp%	Act%
228.00	100	100
226.00	29.00	38.65#
229.00	20.00	37.79#
0.00	0.00	0.00

JU05/14/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:13:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A5144

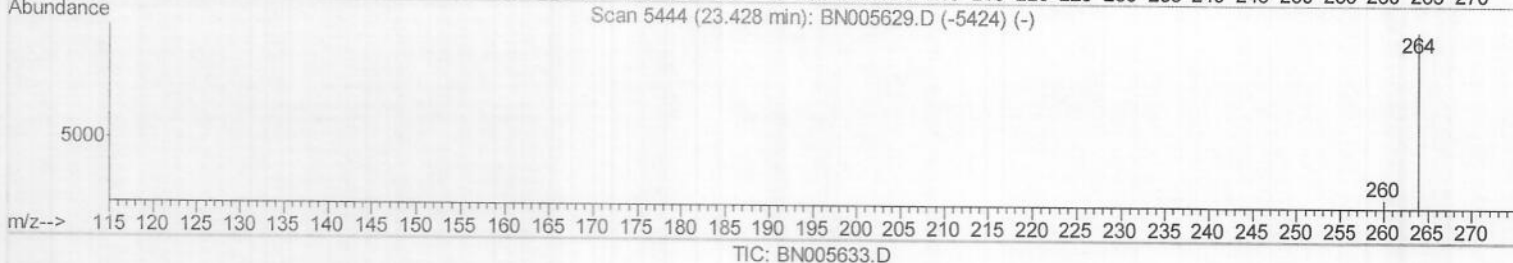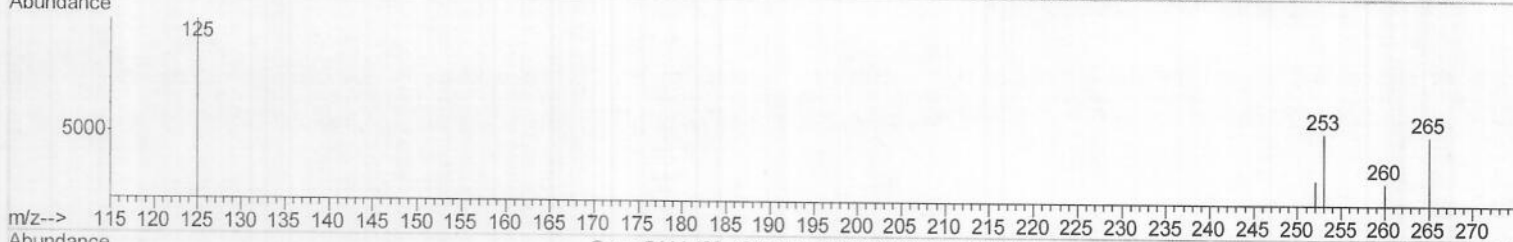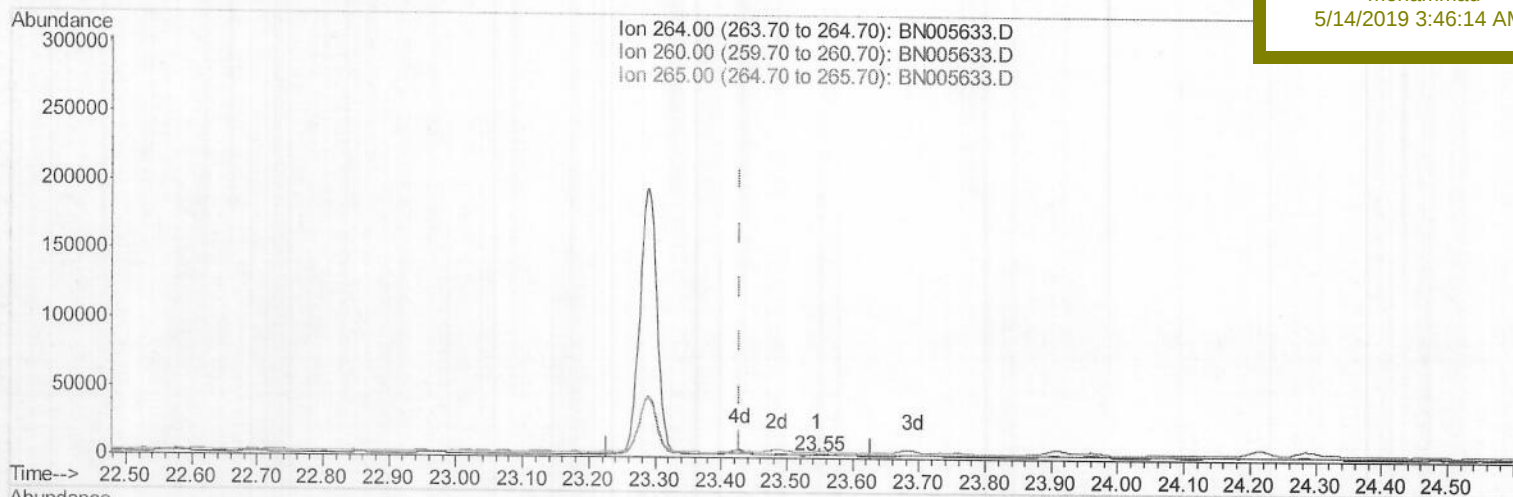Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(20) Perylene-d12 (I)

23.545min (+0.117) 0.40ng/ul

response 397

Ion	Exp%	Act%
264.00	100	100
260.00	25.30	138.45#
265.00	31.70	217.60#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:13:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampled :

A5144

Manual Integrations
APPROVED

mohammad

5/14/2019 3:46:14 AM

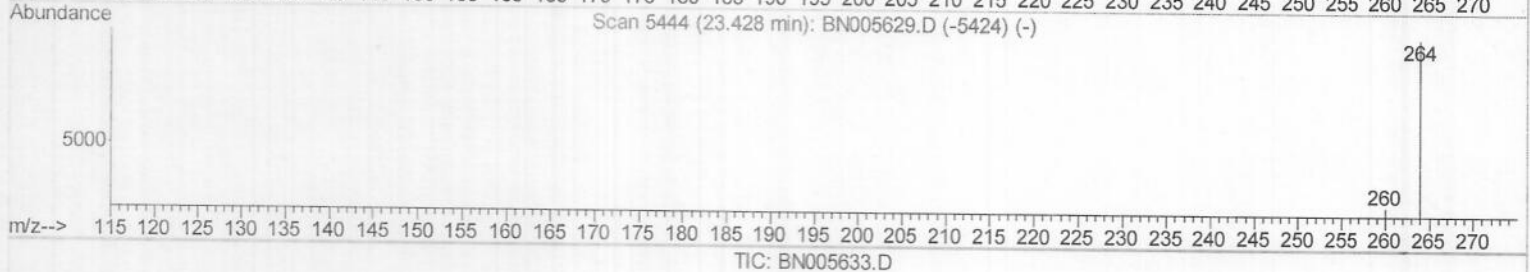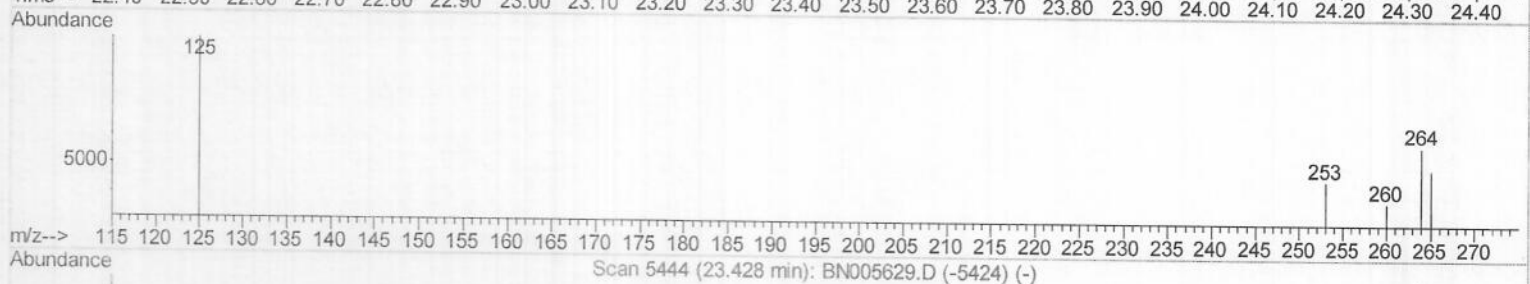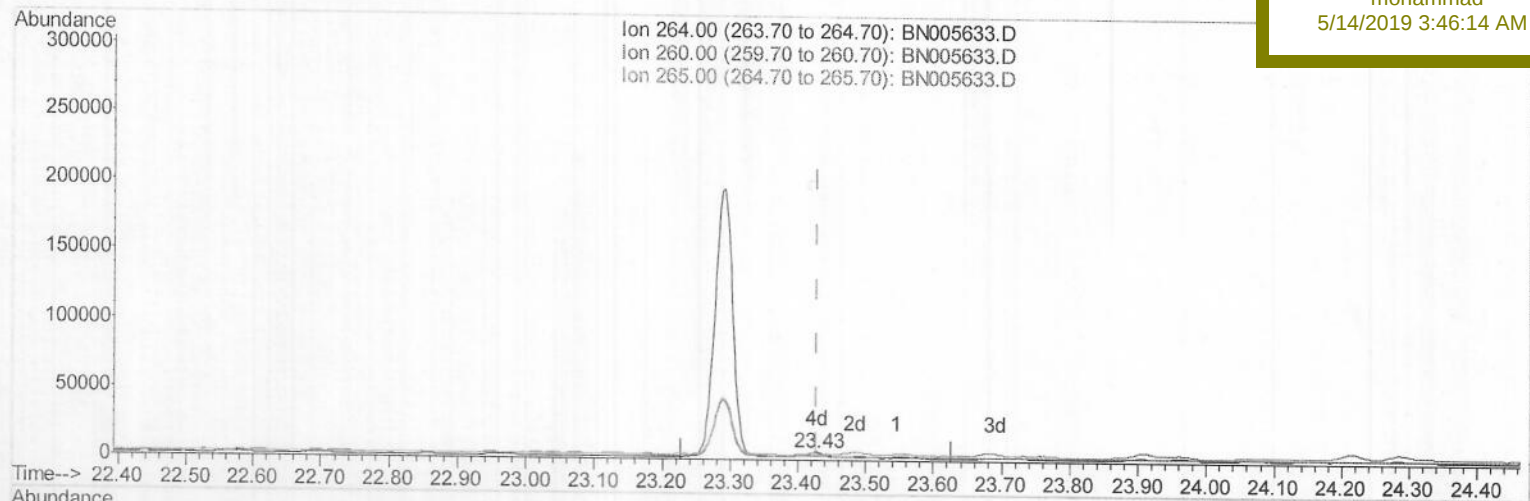

(20) Perylene-d12 (I)

23.428min (-0.000) 0.40ng/ul m

JU05114119

response 6081

Ion	Exp%	Act%
264.00	100	100
260.00	25.30	66.61#
265.00	31.70	86.93#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:17:25 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

A5144

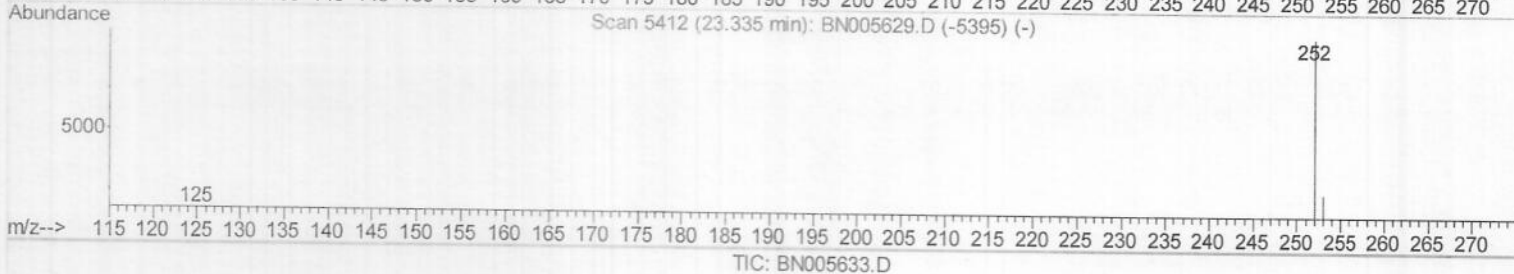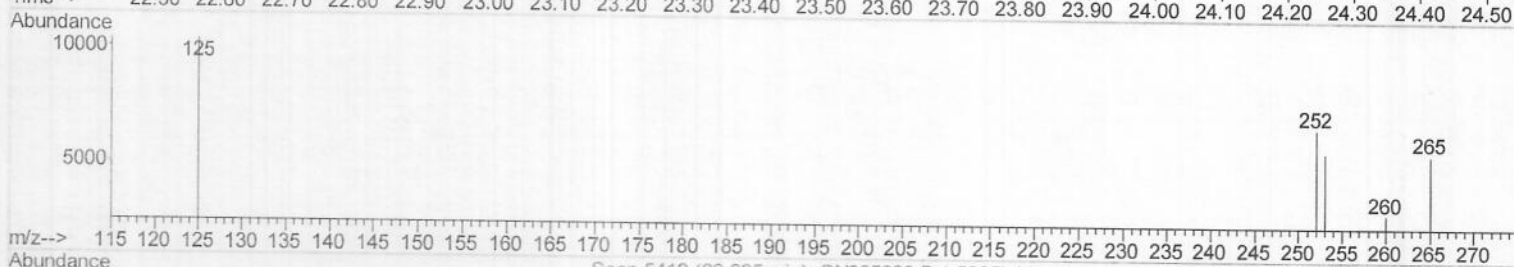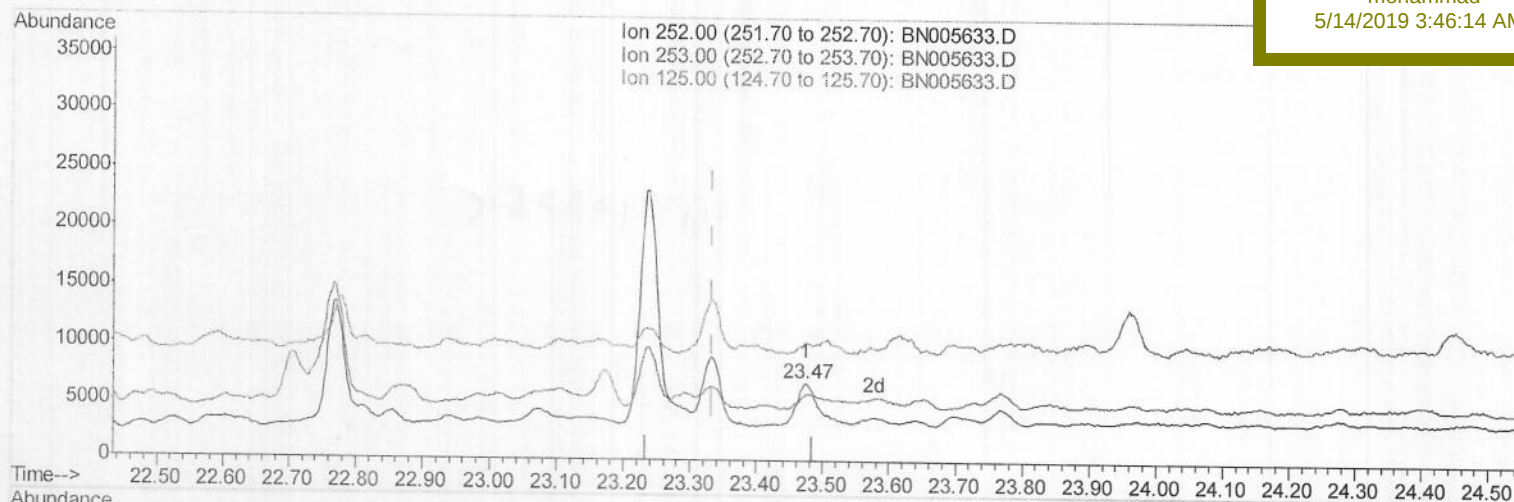Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(23) Benzo(a)pyrene (C)

23.475min (+0.140) 0.42ng/ul

response 8538

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	85.05#
125.00	12.60	152.63#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:17:25 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019




Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

A5144

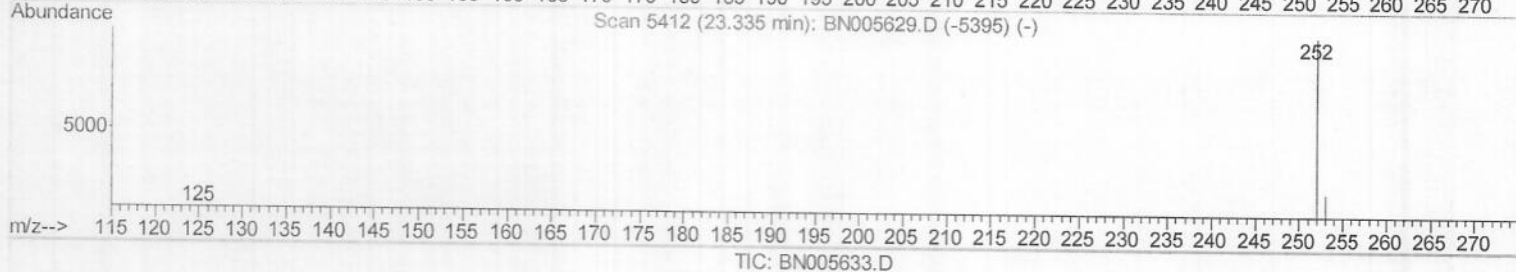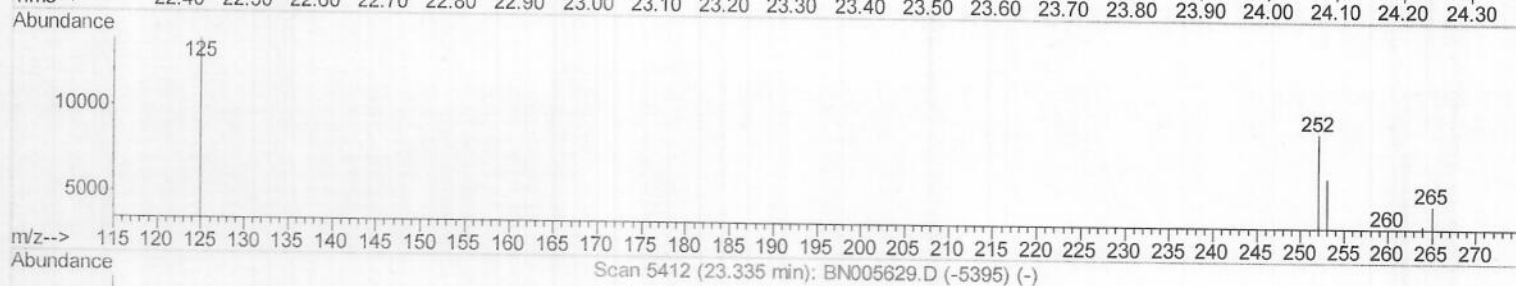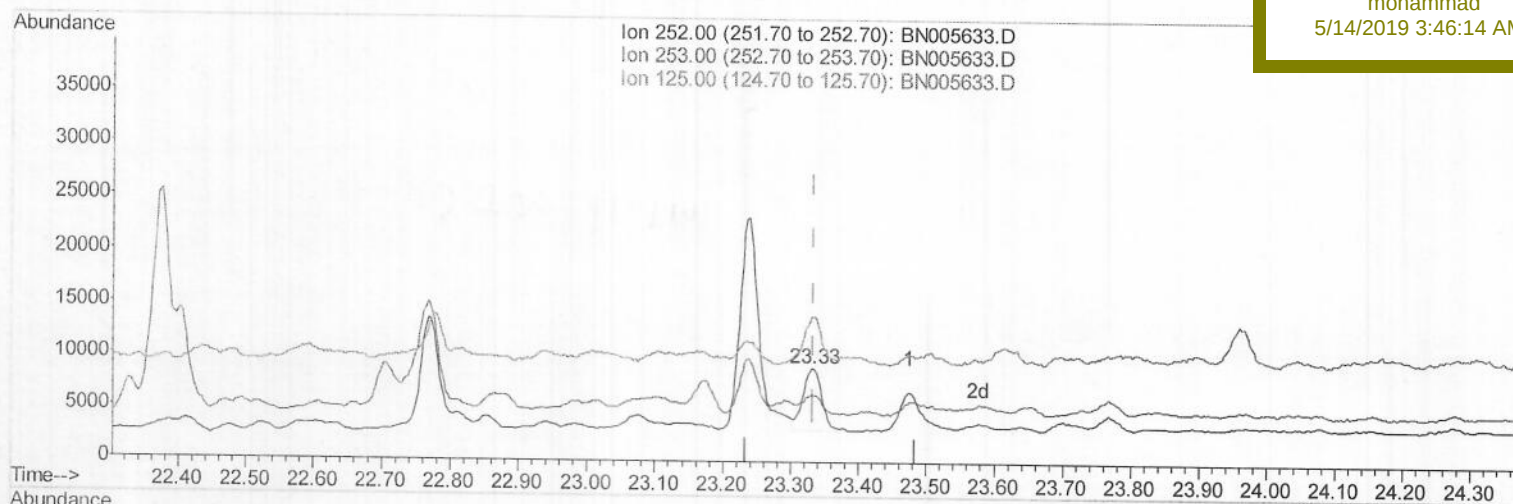Manual Integrations
APPROVEDmohammad
5/14/2019 3:46:14 AM

(23) Benzo(a)pyrene (C)

23.332min (-0.003) 0.55ng/ul m

> JU05/14/19

response 11196

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	71.66#
125.00	12.60	155.16#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051219\

Data File : BN005633.D

Acq On : 11 May 2019 18:58

Operator : JU/SJ

Sample : K2606-10

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 12 01:19:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun May 12 00:36:09 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A5144

Manual Integrations

APPROVED

mohammad

5/14/2019 3:46:14 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1867	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	7514	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	4920	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	9424m)	0.40	ng/ul	-0.01
16) Chrysene-d12	21.21	240	6817m)	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	6081m)	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.95	152	2919	0.25	ng/ul	-0.03
14) Fluoranthene-d10	19.02	212	6783m)	0.23	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.39	128	4609	0.232	ng/ul	98
5) 2-Methylnaphthalene	12.02	142	10051	0.740	ng/ul	99
7) Acenaphthylene	13.94	152	2917	0.118	ng/ul#	65
8) Acenaphthene	14.28	153	1317	0.075	ng/ul#	89
9) Fluorene	15.28	166	2874	0.140	ng/ul#	70
12) Phenanthrene	17.01	178	49996	1.947	ng/ul	98
13) Anthracene	17.11	178	3482m)	0.136	ng/ul	
15) Fluoranthene	19.05	202	11658m)	0.328	ng/ul	
17) Pyrene	19.42	202	21130m)	0.839	ng/ul	
18) Benzo(a)anthracene	21.20	228	7807m)	0.332	ng/ul	
19) Chrysene	21.25	228	20456m)	0.709	ng/ul	
23) Benzo(a)pyrene	23.33	252	11196m)	0.548	ng/ul	
26) Benzo(g,h,i)perylene	26.31	276	23279	1.194	ng/ul#	57

(#)= qualifier out of range (m)= manual integration (+)= signals summed

JU05/14/19