

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
 Data File : BN005648.D
 Acq On : 12 May 2019 17:05
 Operator : JU/SJ
 Sample : PB119502BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5120

Quant Time: May 13 02:10:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 11 23:17:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	87310	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	423918	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	305105	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	776466	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	850580	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	1002816	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	10789	5.97	ng/uL	0.00
5) Phenol-d5	6.78	99	231658	33.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	134570	31.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	195271	37.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	207383	38.69	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	112361	43.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	132670	50.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	202304	33.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	335047	53.58	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	1004818	45.37	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	1116223	41.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	775	0.22	ng/ul	0.13
57) Fluorene-d10	15.22	176	814172	43.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	144156	41.28	ng/ul	0.01
70) Anthracene-d10	17.07	188	1444951	44.39	ng/ul	0.00
78) Pyrene-d10	19.39	212	1754216	40.32	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	1957439	44.66	ng/ul	0.01


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.28	70	4702	1.025	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
Data File : BN005648.D
Acq On : 12 May 2019 17:05
Operator : JU/SJ
Sample : PB119502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5120

Quant Time: May 13 02:10:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 11 23:17:30 2019
Response via : Initial Calibration

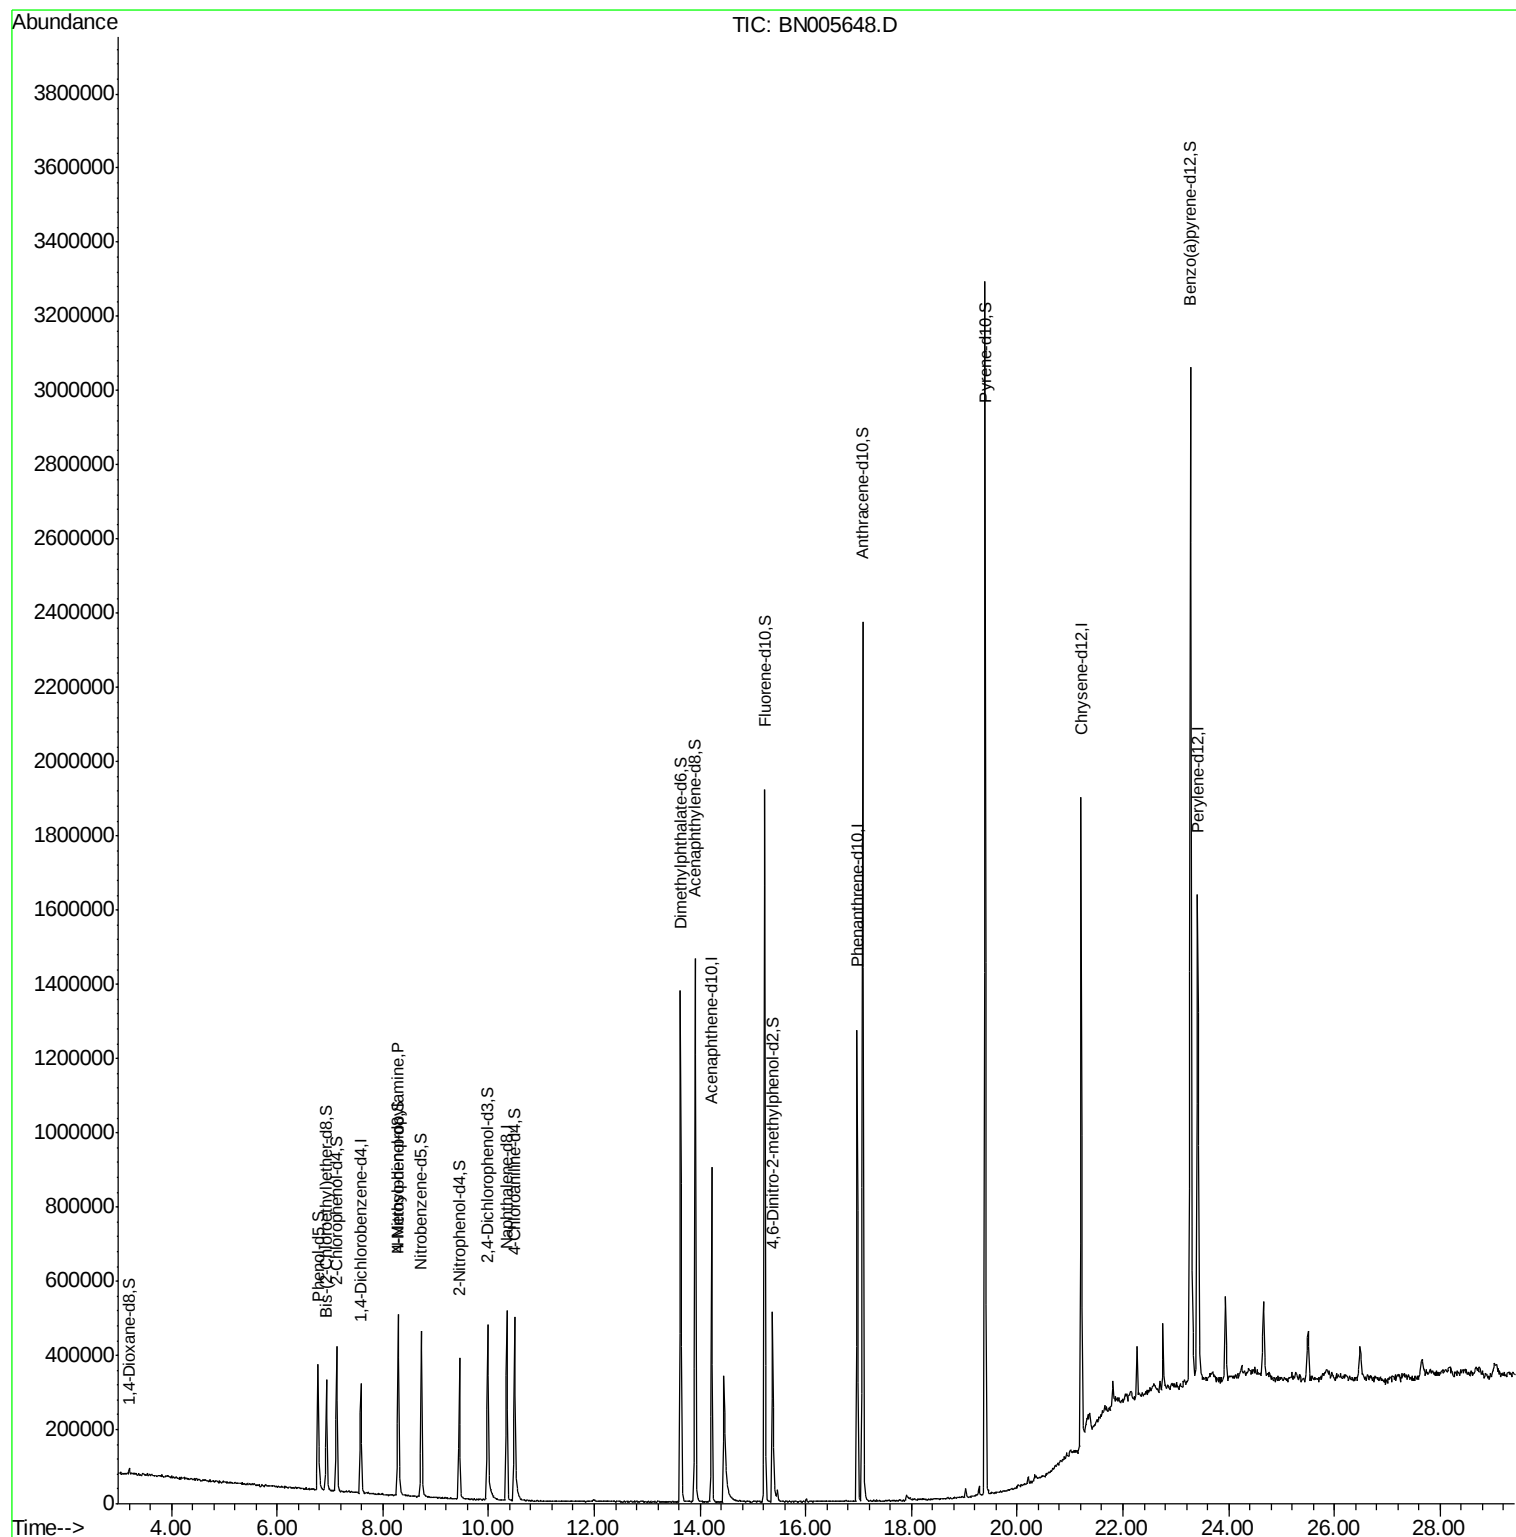

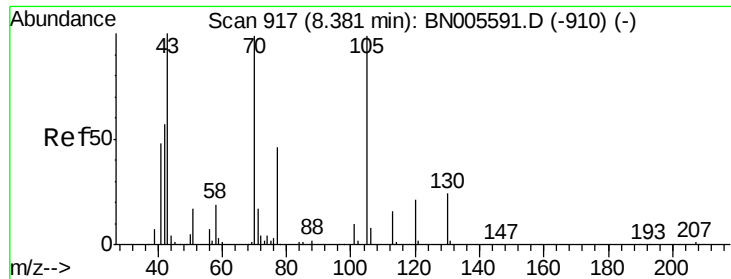

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.025 ng/ul
 RT: 8.28 min Scan# 900
 Delta R.T. -0.10 min
 Lab File: BN005648.D
 Acq: 12 May 2019 17:05

Instrument :
 BNA_N
 ClientSampleId :
 A5120

Tgt Ion:	70	Resp:	4702
Ion	Ratio	Lower	Upper
70	100		
42	321.2	53.8	80.8#
101	0.0	7.7	11.5#
130	0.0	15.0	22.4#

