

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
Quantitation Report (Not Reviewed)

Data File : BN005653.D
Acq On : 13 May 2019 15:41
Operator : JU/SJ
Sample : PB119474BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK74

Quant Time: May 14 05:27:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 05:24:26 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	988	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	4249	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	2890	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.08	188	629860	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.29	264	733216	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	2385	0.36	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.22	166	912	0.076	ng/ul#	Qvalue 17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN005653.D
Acq On : 13 May 2019 15:41
Operator : JU/SJ
Sample : PB119474BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK74

Quant Time: May 14 05:27:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 05:24:26 2019
Response via : Initial Calibration

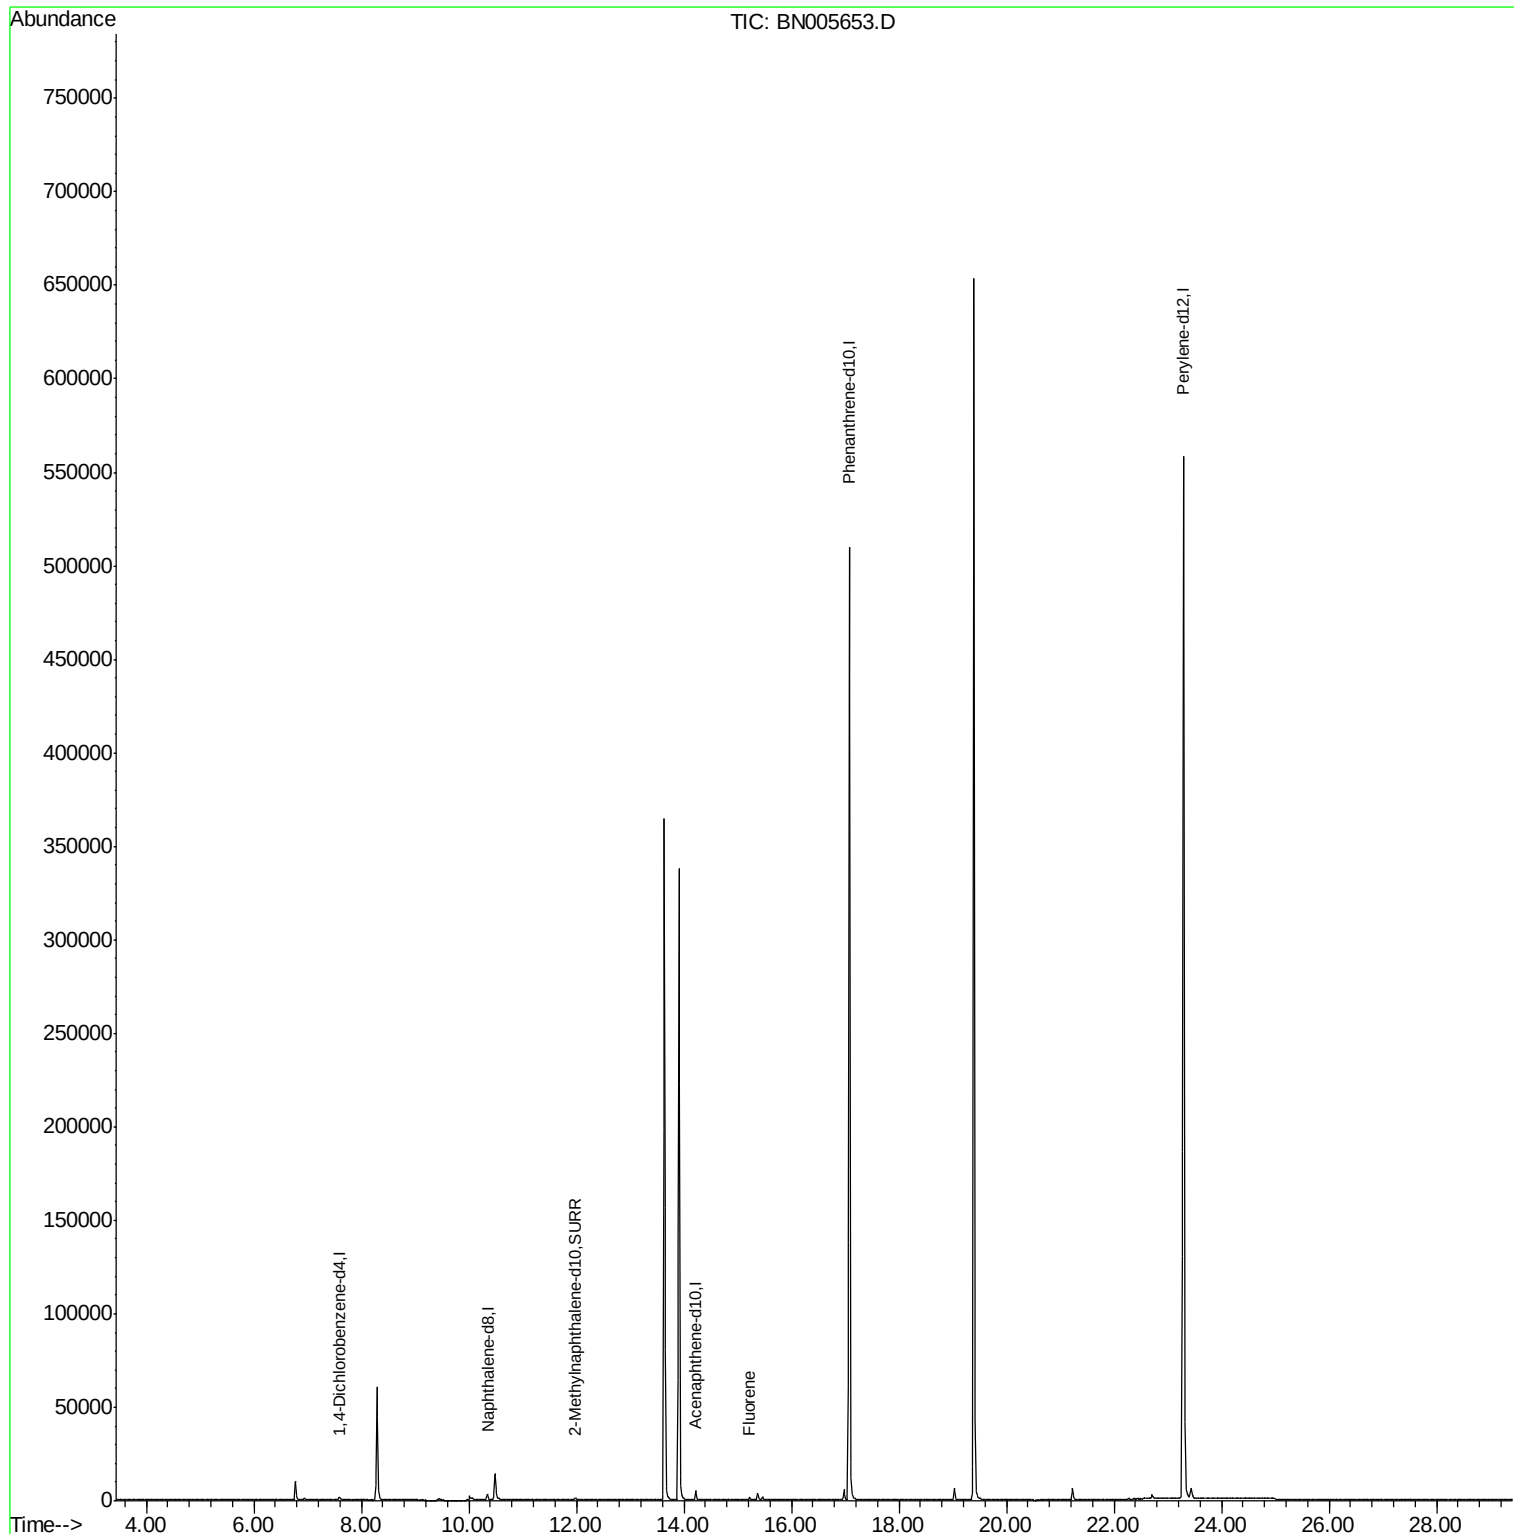

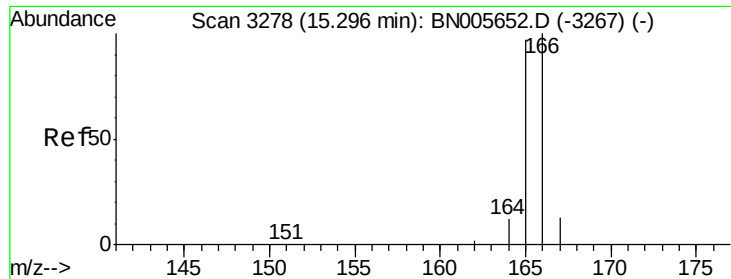

#9

Fluorene

Concen: 0.076 ng/ul

RT: 15.22 min Scan# 3262

Delta R.T. -0.07 min

Lab File: BN005653.D

Acq: 13 May 2019 15:41

Instrument :

BNA_N

ClientSampleId :

SBLK74


Tgt Ion:166 Resp: 912

Ion Ratio Lower Upper

166 100

165 11.1 78.0 117.0#

167 37.5 12.2 18.4#

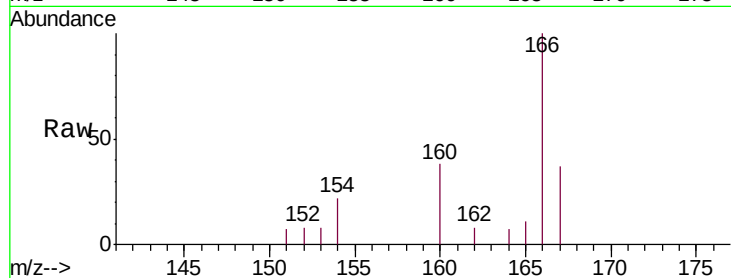

Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

