

Data File : BN005655.D
Acq On : 13 May 2019 16:49
Operator : JU/SJ
Sample : K2690-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5150

Quant Time: May 14 05:27:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 05:24:26 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1190	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	5073	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.22	164	3281	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	8414	0.40	ng/ul	-0.01
16) Chrysene-d12	21.23	240	8108	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	9641	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	663	0.08	ng/ul	0.02
14) Fluoranthene-d10	19.03	212	2219	0.08	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.30	252	753	0.023	ng/ul#	Qvalue 13

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN005655.D

Acq On : 13 May 2019 16:49

Operator : JU/SJ

Sample : K2690-04

Misc :

ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5150


Quant Time: May 14 05:27:38 2019


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue May 14 05:24:26 2019

Response via : Initial Calibration

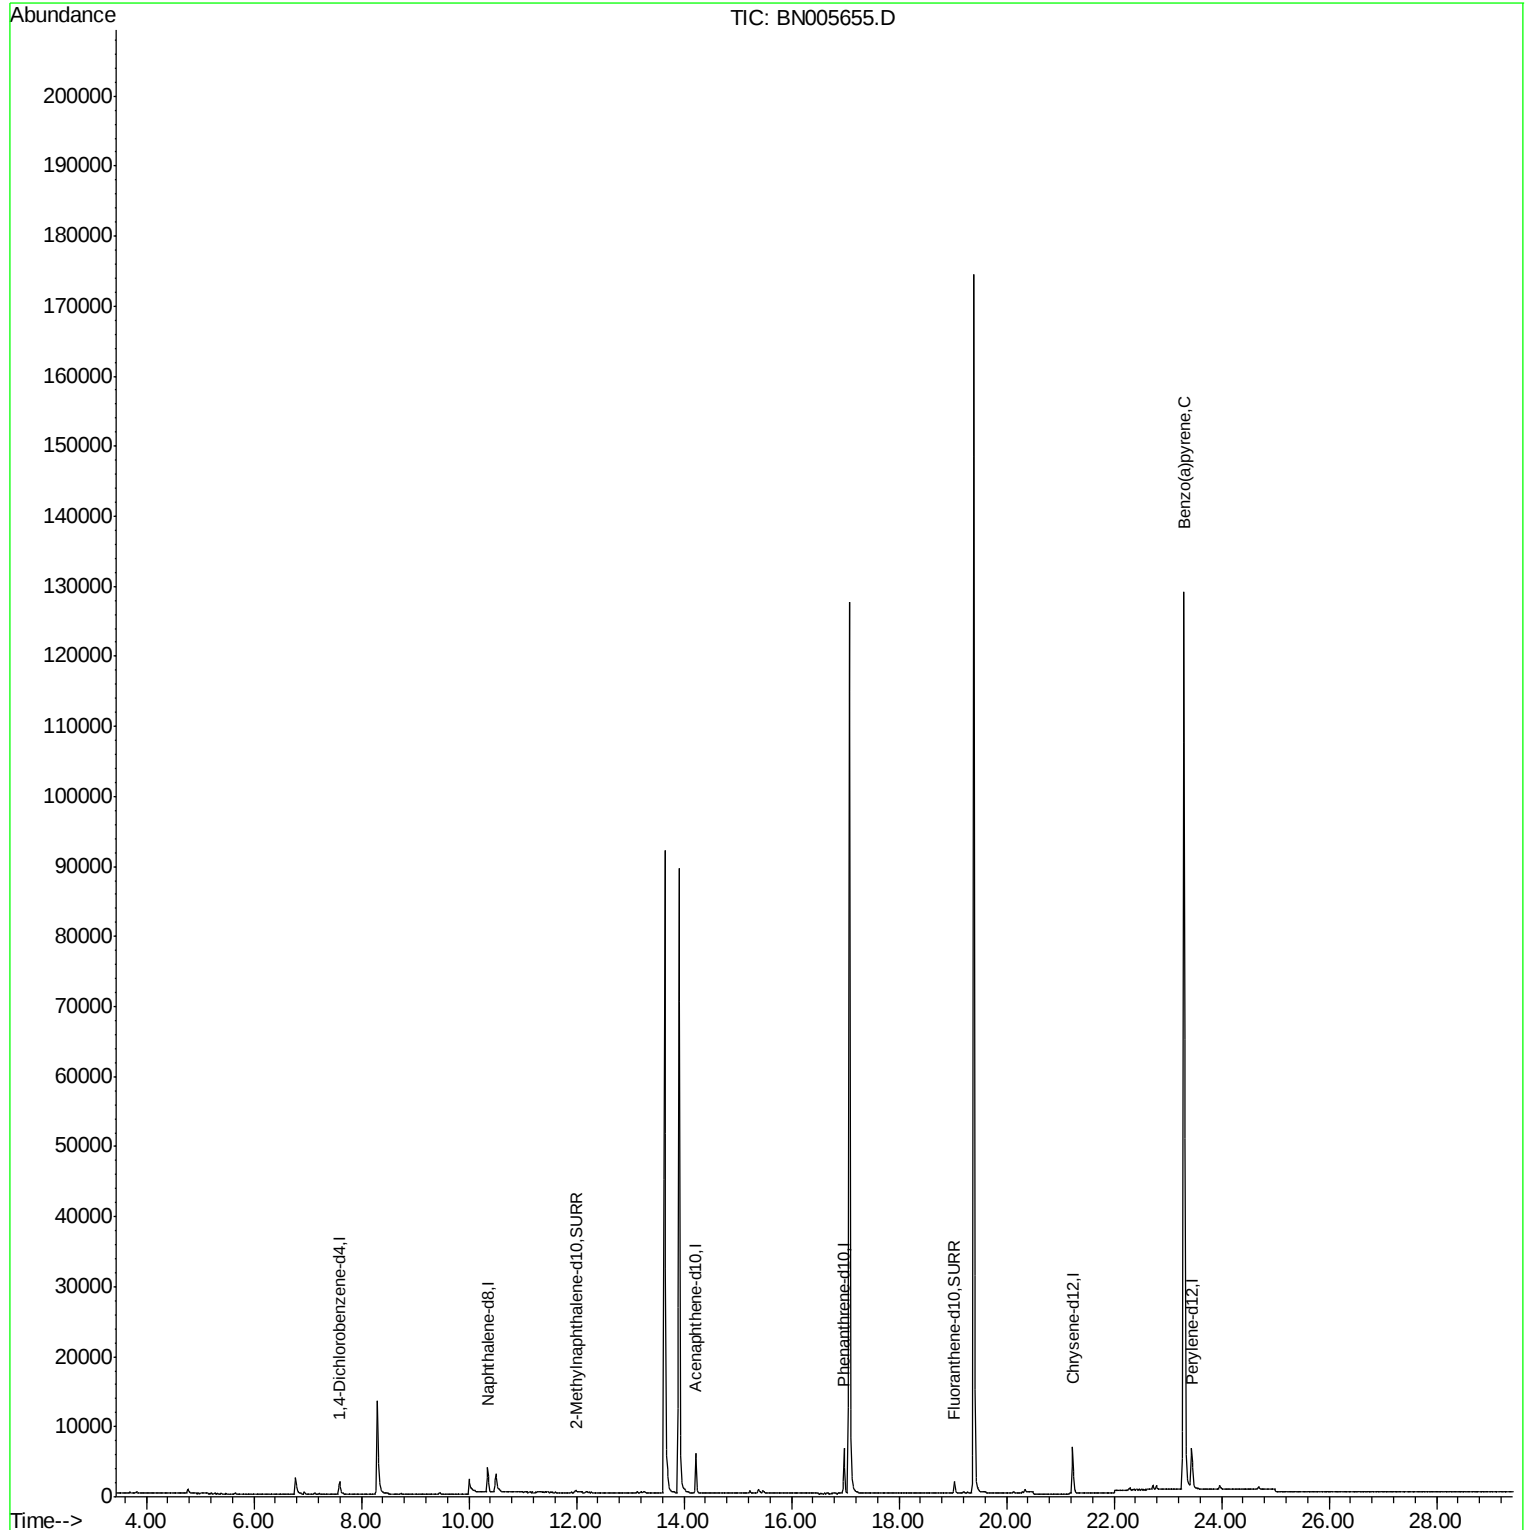

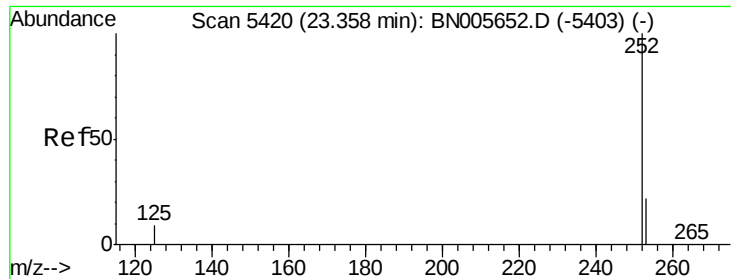

#23

Benzo(a)pyrene

Concen: 0.023 ng/ul

RT: 23.30 min Scan# 5400

Delta R.T. -0.06 min

Lab File: BN005655.D

Acq: 13 May 2019 16:49

Instrument :

BNA_N

ClientSampleId :

A5150

Tgt Ion: 252 Resp: 753

Ion Ratio Lower Upper

252 100

253 62.4 19.6 29.4#

125 54.8 10.1 15.1#

