

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
Quantitation Report (Not Reviewed)

Data File : BN005660.D
Acq On : 13 May 2019 19:42
Operator : JU/SJ
Sample : K2690-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5156

Quant Time: May 14 05:28:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 05:24:26 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1353	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.34	136	5674	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	3846	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.08	188	837870	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.31	264	862630	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	3851	0.43	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.39	128	320	0.021	ng/ul#	Qvalue 57




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN005660.D
Acq On : 13 May 2019 19:42
Operator : JU/SJ
Sample : K2690-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5156

Quant Time: May 14 05:28:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 05:24:26 2019
Response via : Initial Calibration

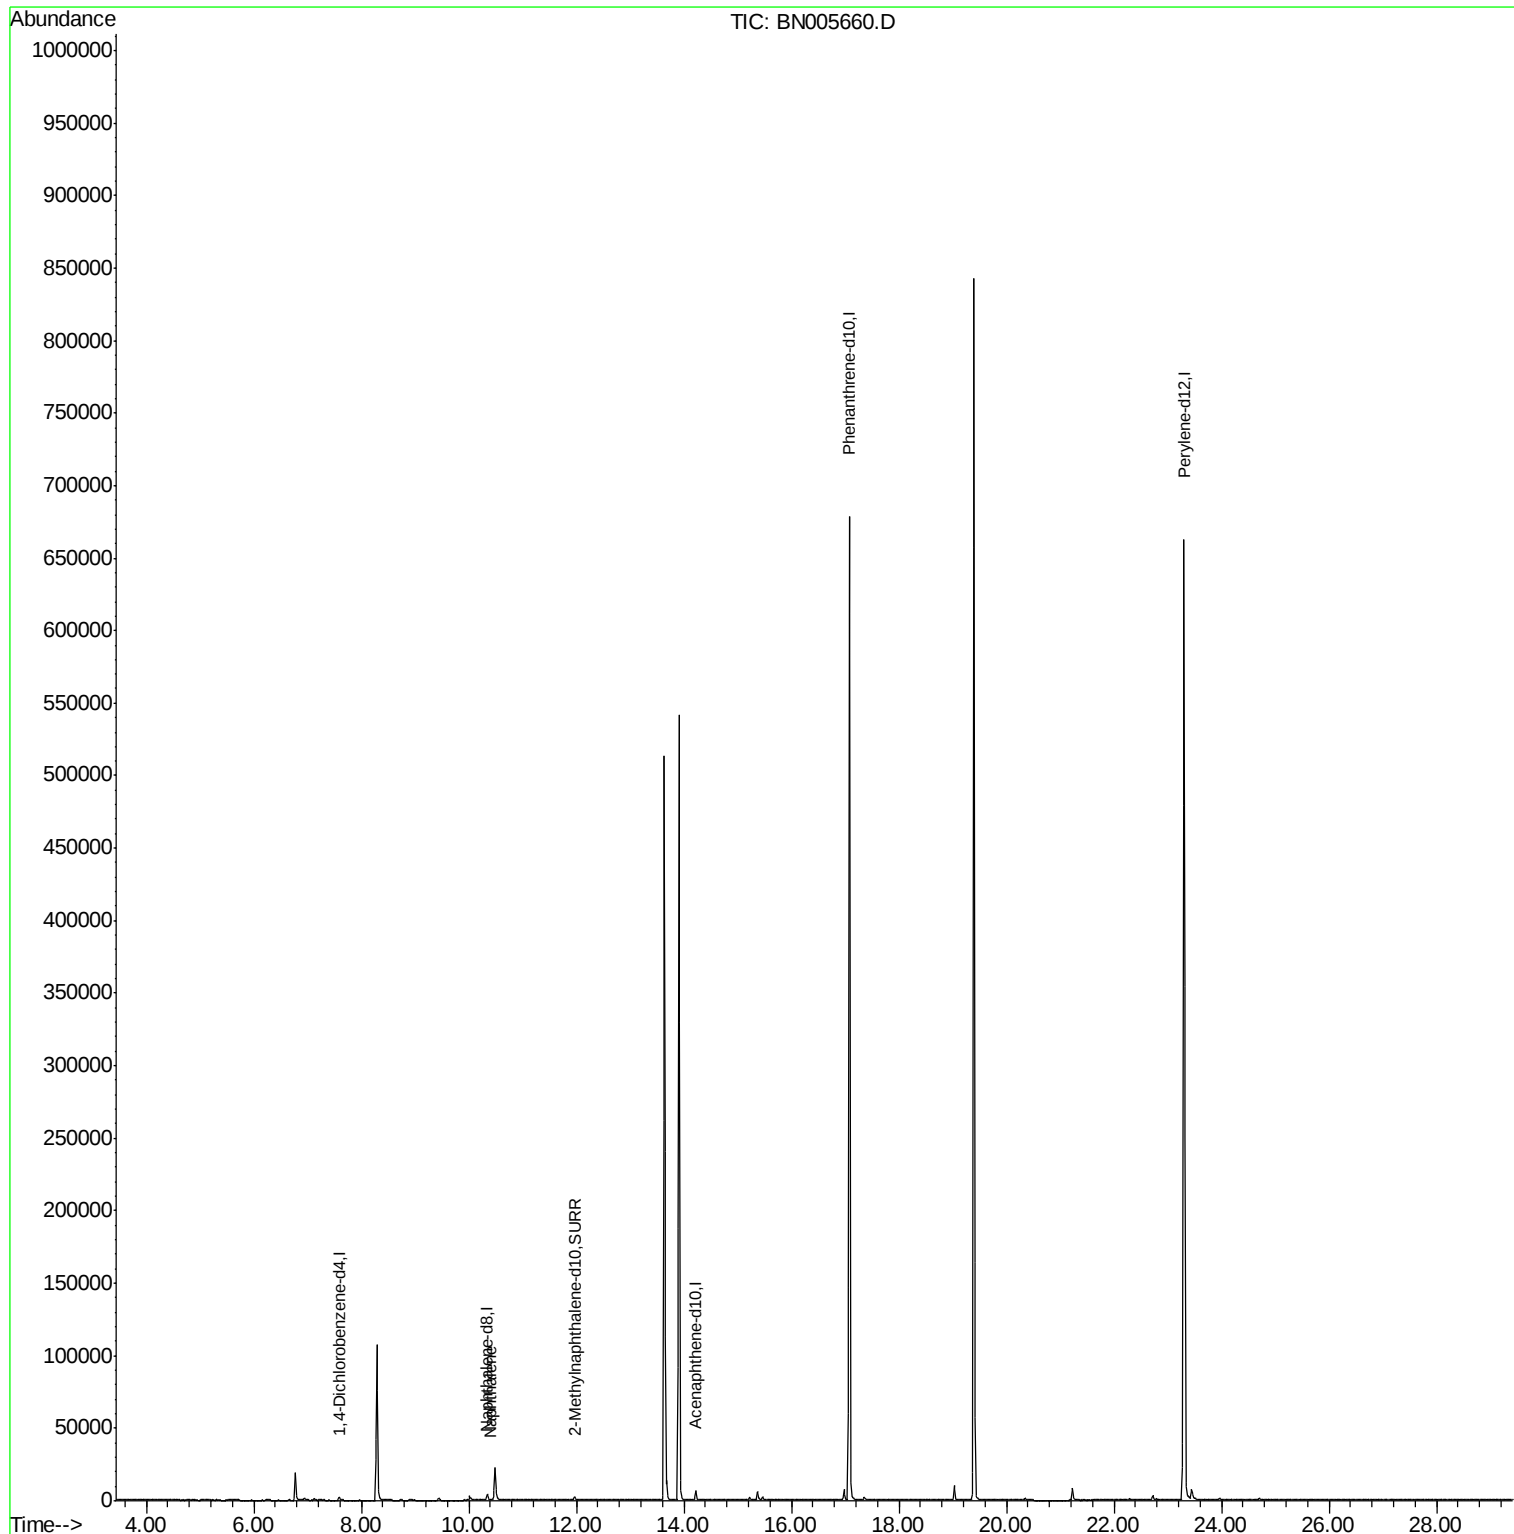

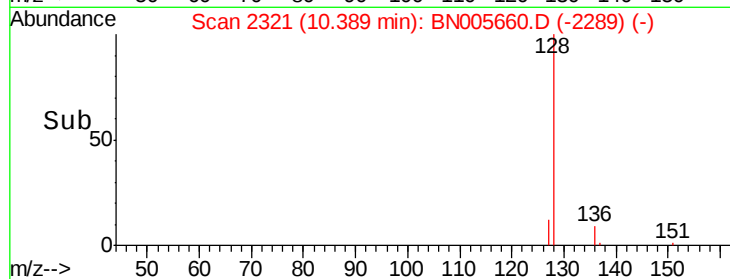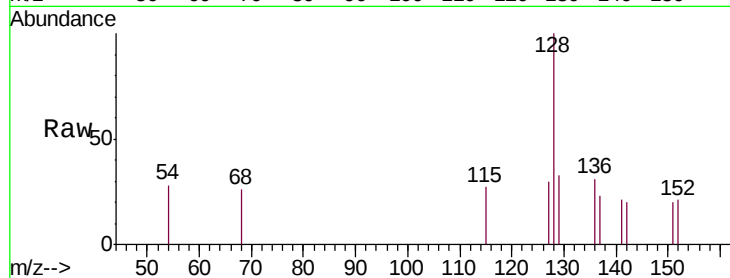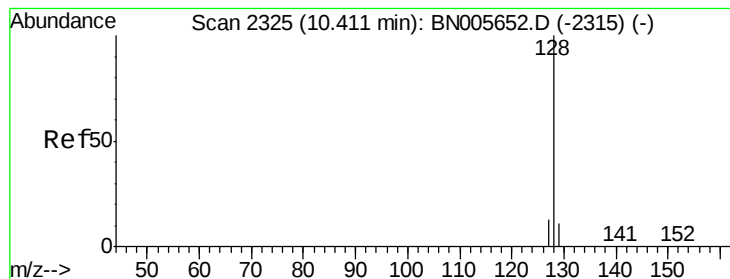

#3

Naphthalene

Concen: 0.021 ng/ul

RT: 10.39 min Scan# 2321

Delta R.T. -0.02 min

Lab File: BN005660.D

Acq: 13 May 2019 19:42

Instrument :

BNA_N

ClientSampleId :

A5156

Tgt Ion:128 Resp: 320

Ion Ratio Lower Upper

128 100

129 32.7 10.2 15.2#

127 30.2 11.8 17.8#

