

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
 Data File : BN005664.D
 Acq On : 13 May 2019 21:59
 Operator : JU/SJ
 Sample : K2690-25
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5169

Manual Integrations
 APPROVED

mohammad
 5/16/2019 11:35:13 AM

Quant Time: May 14 07:00:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 14 05:24:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1315	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.34	136	5433	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	3842	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	9076m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.22	240	8708m	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	6894m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.95	152	3629	0.43	ng/ul	-0.02
14) Fluoranthene-d10	19.03	212	11236m	0.39	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.39	128	2057	0.143	ng/ul#	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
Data File : BN005664.D
Acq On : 13 May 2019 21:59
Operator : JU/SJ
Sample : K2690-25
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A5169

Manual Integrations
APPROVED

mohammad
5/16/2019 11:35:13 AM

Quant Time: May 14 07:00:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 05:24:26 2019
Response via : Initial Calibration

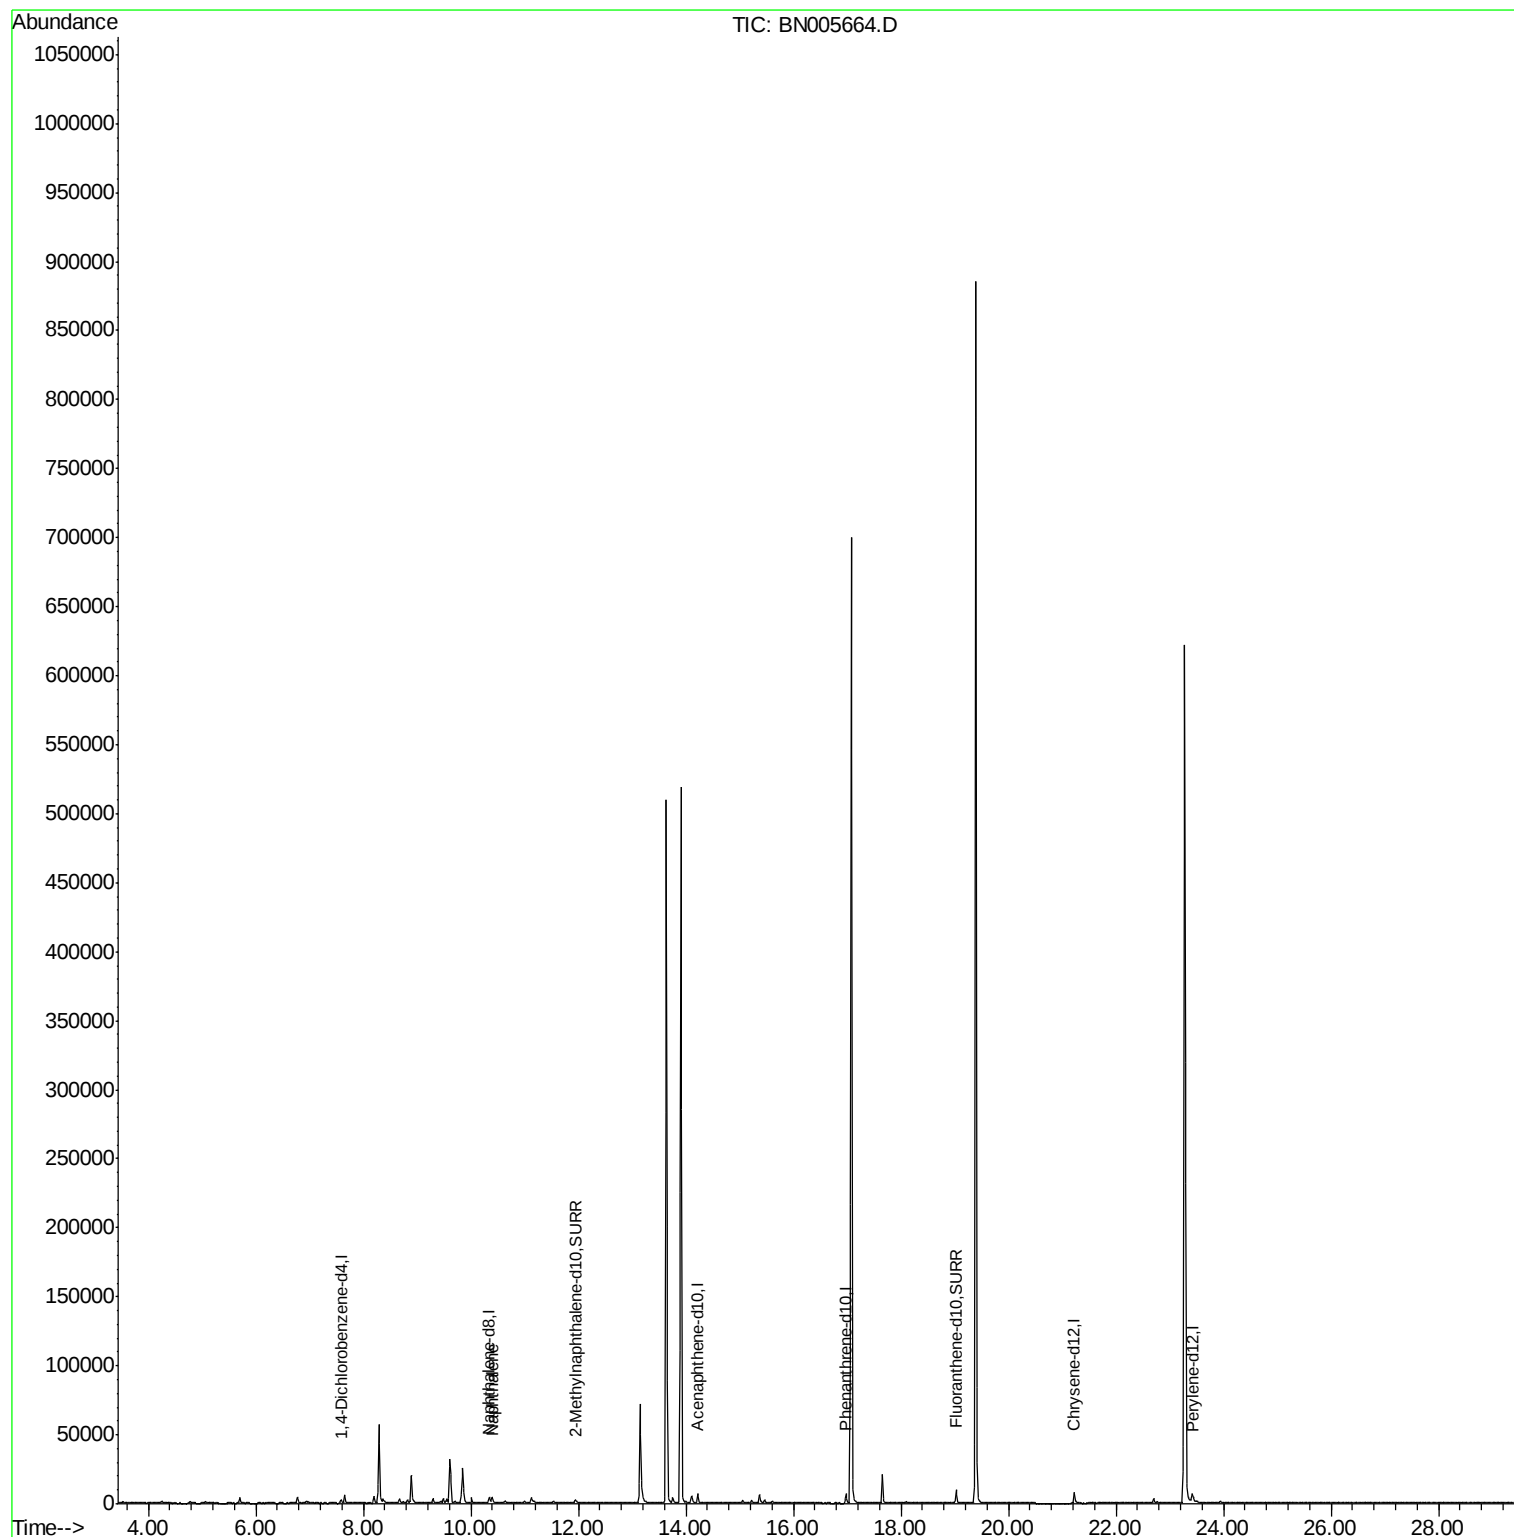

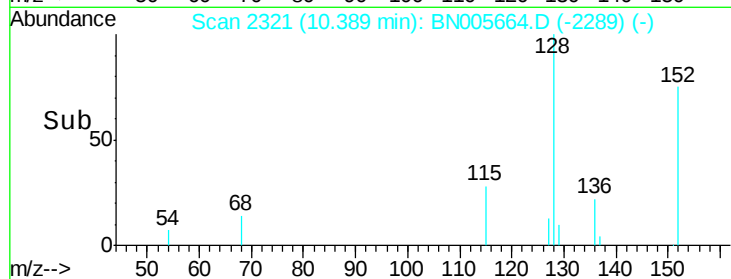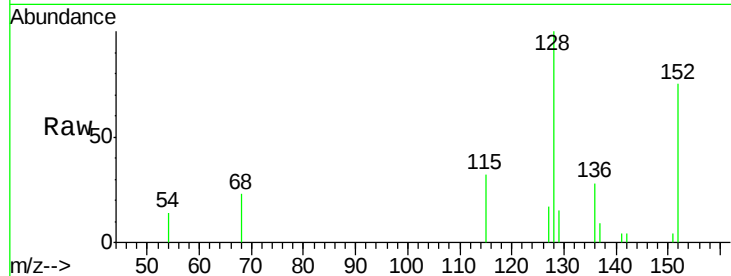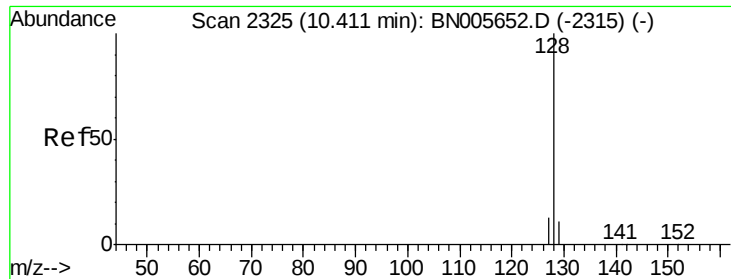

#3

Naphthalene

Concen: 0.143 ng/ul

RT: 10.39 min Scan# 2321

Delta R.T. -0.02 min

Lab File: BN005664.D

Acq: 13 May 2019 21:59

Tgt Ion:	128	Resp:	2057
Ion Ratio	Lower	Upper	
128	100		
129	15.4	10.2	15.2#
127	16.9	11.8	17.8

Instrument :

BNA_N

ClientSampleId :

A5169

Manual Integrations
APPROVED

mohammad
5/16/2019 11:35:13 AM

