

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
 Data File : BN005684.D
 Acq On : 14 May 2019 10:06
 Operator : JU/SJ
 Sample : K2692-27
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5189

Manual Integrations
 APPROVED

mohammad
 5/16/2019 11:36:22 AM

Quant Time: May 14 16:25:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 14 07:15:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1074	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.35	136	4606	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.22	164	3175	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	7747m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.22	240	7936m	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	6711m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	3101	0.43	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	9298m	0.38	ng/ul	0.00
Target Compounds						
5) 2-Methylnaphthalene	12.04	142	388	0.047	ng/ul	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051319\
Data File : BN005684.D
Acq On : 14 May 2019 10:06
Operator : JU/SJ
Sample : K2692-27
Misc :
ALS Vial : 37 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A5189

Manual Integrations
APPROVED

mohammad
5/16/2019 11:36:22 AM

Quant Time: May 14 16:25:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 07:15:06 2019
Response via : Initial Calibration

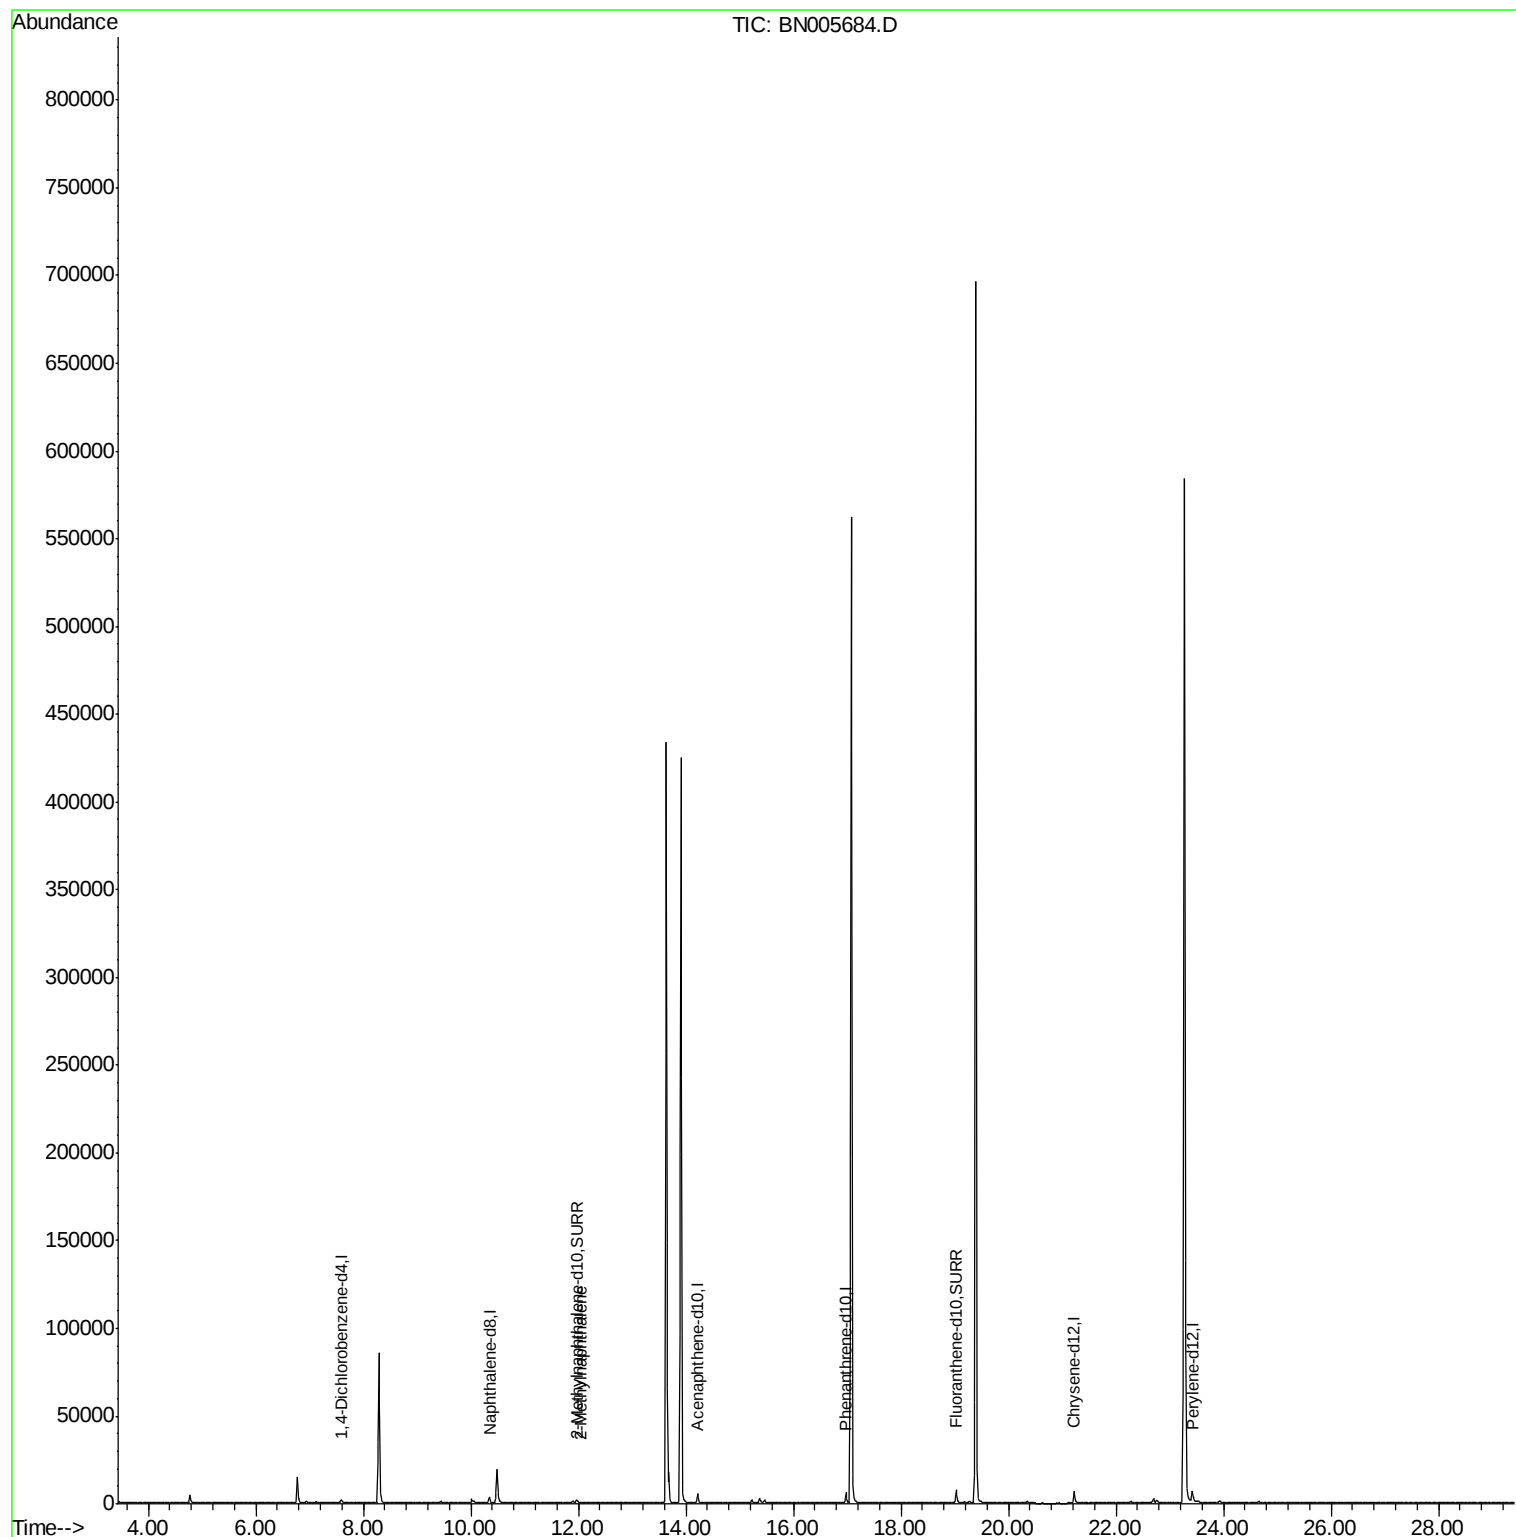

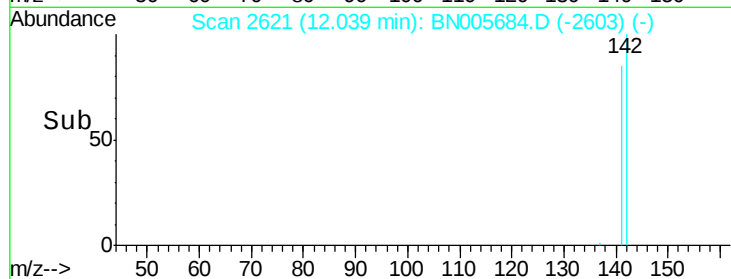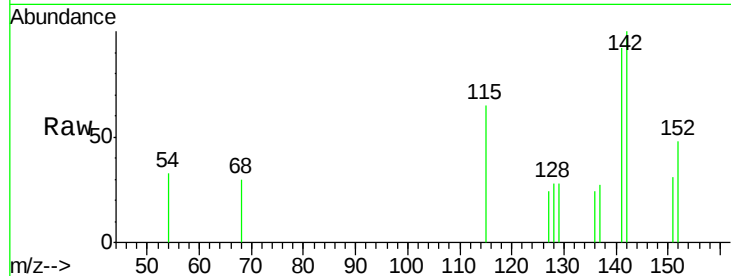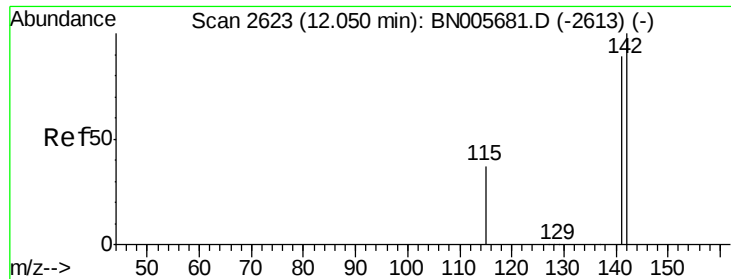

#5

2-Methylnaphthalene

Concen: 0.047 ng/ul

RT: 12.04 min Scan# 2621

Delta R.T. -0.00 min

Lab File: BN005684.D

Acq: 14 May 2019 10:06

Tgt Ion: 142 Resp: 388

Ion Ratio Lower Upper

142 100

141 81.4 72.2 108.2

Instrument :

BNA_N

ClientSampleId :

A5189

Manual Integrations

APPROVED

mohammad

5/16/2019 11:36:22 AM

