

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051320\
 Data File : BN010704.D
 Acq On : 13 May 2020 11:57
 Operator : CG/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Manual Integrations
 APPROVED

mohammad
 5/14/2020 9:19:24 AM

Quant Time: May 13 13:29:18 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed May 13 13:23:01 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3353	0.40	ng	0.00
7) Naphthalene-d8	10.33	136	12757	0.40	ng	0.00
13) Acenaphthene-d10	14.20	164	7810	0.40	ng	0.00
19) Phenanthrene-d10	16.95	188	16347	0.40	ng	0.00
27) Chrysene-d12	21.15	240	13729	0.40	ng	0.00
34) Perylene-d12	23.32	264	12813	0.40	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.22	112	4968	0.68	ng	0.00
5) Phenol-d6	6.77	99	6051	0.63	ng	0.00
8) Nitrobenzene-d5	8.71	82	6843	0.77	ng	0.00
11) 2-Methylnaphthalene-d10	11.93	152	16020	0.76	ng	0.00
14) 2,4,6-Tribromophenol	15.71	330	2083	0.57	ng	0.00
15) 2-Fluorobiphenyl	12.82	172	22672	0.80	ng	0.00
25) Fluoranthene-d10	18.99	212	33111	0.67	ng	0.00
29) Terphenyl-d14	19.60	244	24867	0.79	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.23	88	2274	0.92	ng	99
3) n-Nitrosodimethylamine	3.55	42	1246	0.78	ng	# 97
6) bis(2-Chloroethyl)ether	7.02	93	6213	0.75	ng	95
9) Naphthalene	10.38	128	24613	0.78	ng	98
10) Hexachlorobutadiene	10.68	225	5661	0.74	ng	# 100
12) 2-Methylnaphthalene	12.00	142	17427	0.77	ng	98
16) Acenaphthylene	13.91	152	24016	0.71	ng	100
17) Acenaphthene	14.26	154	16462	0.76	ng	99
18) Fluorene	15.25	166	21410	0.75	ng	100
20) 4-Bromophenyl-phenylether	16.16	248	6895	0.76	ng	# 89
21) Hexachlorobenzene	16.26	284	8286	0.80	ng	100
22) Pentachlorophenol	16.61	266	2337	0.57	ng	99
23) Phenanthrene	16.99	178	33482	0.76	ng	100
24) Anthracene	17.08	178	27752	0.69	ng	99
26) Fluoranthene	19.02	202	37797	0.69	ng	99
28) Pyrene	19.38	202	36605	0.79	ng	100
30) Benzo(a)anthracene	21.14	228	29709	0.66	ng	99
31) Chrysene	21.19	228	34621	0.78	ng	98
32) Bis(2-ethylhexyl)phthalate	21.09	149	12499	0.54	ng	99
33) Indeno(1,2,3-cd)pyrene	25.46	276	31166	0.79	ng	99
35) Benzo(b)fluoranthene	22.68	252	31881m	0.76	ng	
36) Benzo(k)fluoranthene	22.72	252	34635	0.82	ng	# 93
37) Benzo(a)pyrene	23.22	252	27802	0.74	ng	# 88
38) Dibenzo(a,h)anthracene	25.47	278	23963	0.70	ng	93
39) Benzo(g,h,i)perylene	26.10	276	27183	0.79	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051320\
Data File : BN010704.D
Acq On : 13 May 2020 11:57
Operator : CG/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Manual Integrations
APPROVED

mohammad
5/14/2020 9:19:24 AM

Quant Time: May 13 13:29:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 13:23:01 2020
Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 0.40 ng

RT: 7.58 min Scan# 590

Delta R.T. 0.00 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Instrument :

BNA_N


ClientSampleId :

SSTDICC0.8




Tgt Ion:	152	Resp:	3353
Ion Ratio	Lower	Upper	
152	100		
150	146.6	119.4	179.0
115	55.8	45.9	68.9

Manual Integrations
APPROVED

mohammad
5/14/2020 9:19:24 AM



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E



#2

1,4-Dioxane

Concen: 0.92 ng


RT: 3.23 min Scan# 50

Delta R.T. -0.01 min



Lab File: BN010704.D


Acq: 13 May 2020 11:57

Tgt Ion:	88	Resp:	2274
Ion Ratio	Lower	Upper	
88	100		
58	47.8	39.0	58.6
43	16.5	13.1	19.7



Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC





#3





n-Nitrosodimethylamine
Concen: 0.78 ng
RT: 3.55 min Scan# 90
Delta R.T. -0.02 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion	Ratio	Lower	Upper
42	100		
74	186.6	146.2	219.2
44	5.7	3.0	4.4#

Manual Integrations
APPROVED




mohammad
5/14/2020 9:19:24 AM






#4

2-Fluorophenol
Concen: 0.68 ng
RT: 5.22 min Scan# 297
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
112	100		
64	46.2	36.2	54.4
63	24.1	19.8	29.8



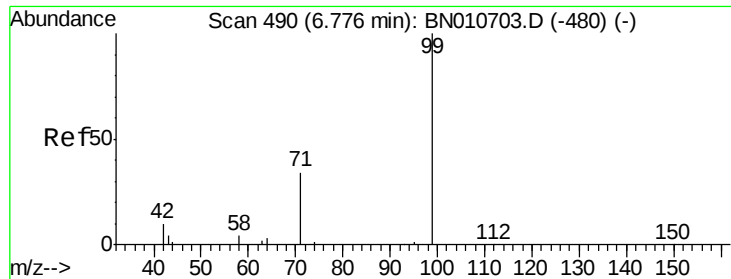





#5
Phenol-d6
Concen: 0.63 ng
RT: 6.77 min Scan# 489
Delta R.T. -0.01 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
99	100		
42	13.4	9.8	14.8
71	35.0	28.6	42.8

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#6
bis(2-Chloroethyl)ether
Concen: 0.75 ng
RT: 7.02 min Scan# 520
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
93	100		
63	58.0	43.1	64.7
95	32.7	24.6	37.0





#7

Naphthalene-d8

Concen: 0.40 ng

RT: 10.33 min Scan# 840

Delta R.T. 0.00 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Instrument :

BNA_N





ClientSampleId :

SSTDIC0.8

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.2	13.8
54	4.2	3.6	5.4
68	4.9	4.1	6.1

Manual Integrations
APPROVED

mohammad
5/14/2020 9:19:24 AM



#8

Nitrobenzene-d5

Concen: 0.77 ng




RT: 8.71 min Scan# 712


Delta R.T. 0.00 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
82	100		
128	37.9	29.0	43.4
54	34.0	29.3	43.9









#9
Naphthalene
Concen: 0.78 ng
RT: 10.38 min Scan# 844
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.1	9.3	13.9
127	13.1	11.0	16.6




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#10
Hexachlorobutadiene
Concen: 0.74 ng
RT: 10.68 min Scan# 868
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.3	50.7	76.1





#11

2-Methylnaphthalene-d10

Concen: 0.76 ng

RT: 11.93 min Scan# 1027

Delta R.T. 0.00 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Instrument :

BNA_N

ClientSampled :

SSTDICC0.8

Tgt Ion:152 Resp: 16020

Ion Ratio Lower Upper

152 100





151 19.1 15.0 22.6

Manual Integrations

APPROVED

mohammad

5/14/2020 9:19:24 AM



#12

2-Methylnaphthalene

Concen: 0.77 ng

RT: 12.00 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57




Tgt Ion:142 Resp: 17427


Ion Ratio Lower Upper

142 100

141 87.9 71.7 107.5

115 35.8 29.8 44.6









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.20 min Scan# 1310
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.7	81.1	121.7
160	45.9	37.9	56.9




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#14
2,4,6-Tribromophenol
Concen: 0.57 ng
RT: 15.71 min Scan# 1445
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	34.9	28.8	43.2









#15
2-Fluorobiphenyl
Concen: 0.80 ng
RT: 12.82 min Scan# 1186
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.6	28.6	42.8
170	22.5	19.8	29.8




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#16
Acenaphthylene
Concen: 0.71 ng
RT: 13.91 min Scan# 1284
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.7	15.6	23.4
153	13.1	10.4	15.6









#17
Acenaphthene
Concen: 0.76 ng
RT: 14.26 min Scan# 1315
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion	Ratio	Lower	Upper
154	100		
153	115.2	91.5	137.3
152	57.2	45.6	68.4




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#18
Fluorene
Concen: 0.75 ng
RT: 15.25 min Scan# 1404
Delta R.T. -0.01 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
166	100		
165	97.7	77.9	116.9
167	13.6	11.0	16.4









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.95 min Scan# 1561
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion	Ratio	Resp Lower	Resp Upper
188	100		
94	0.0	0.0	0.0
80	6.1	6.3	9.5#




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#20
4-Bromophenyl-phenylether
Concen: 0.76 ng
RT: 16.16 min Scan# 1486
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Resp Lower	Resp Upper
248	100		
250	100.5	77.4	116.0
141	49.0	53.1	79.7#





#21

Hexachlorobenzene

Concen: 0.80 ng

RT: 16.26 min Scan# 1496

Delta R.T. 0.00 min

Lab File: BN010704.D


Acq: 13 May 2020 11:57

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.8



Tgt Ion: 284 Resp: 8286

Ion Ratio Lower Upper




284 100

142 34.9 28.2 42.2

249 33.0 26.4 39.6

Manual Integrations
APPROVED

mohammad
5/14/2020 9:19:24 AM



#22

Pentachlorophenol

Concen: 0.57 ng

RT: 16.61 min Scan# 1529

Delta R.T. -0.01 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57




Tgt Ion: 266 Resp: 2337


Ion Ratio Lower Upper

266 100

264 65.4 51.1 76.7

268 65.7 52.1 78.1





#23

Phenanthrene

Concen: 0.76 ng

RT: 16.99 min Scan# 1564

Delta R.T. -0.01 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Instrument :

BNA_N





ClientSampled :

SSTDICC0.8

Tgt Ion:	178	Resp:	33482
Ion Ratio	Lower	Upper	
178	100		
176	18.8	14.9	22.3
179	15.5	12.2	18.4

Manual Integrations
APPROVED

mohammad
5/14/2020 9:19:24 AM



#24

Anthracene

Concen: 0.69 ng




RT: 17.08 min Scan# 1573


Delta R.T. -0.01 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Tgt Ion:	178	Resp:	27752
Ion Ratio	Lower	Upper	
178	100		
176	17.9	14.7	22.1
179	15.1	12.3	18.5





#25

Fluoranthene-d10

Concen: 0.67 ng

RT: 18.99 min Scan# 1858

Delta R.T. 0.00 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Instrument :

BNA_N





ClientSampleId :

SSTDICC0.8

Tgt Ion:	212	Resp:	33111
Ion Ratio	Lower	Upper	
212	100		
106	9.9	8.2	12.2
104	5.7	4.7	7.1

Manual Integrations
APPROVED

mohammad
5/14/2020 9:19:24 AM



#26

Fluoranthene

Concen: 0.69 ng




RT: 19.02 min Scan# 1864


Delta R.T. -0.00 min

Lab File: BN010704.D

Acq: 13 May 2020 11:57

Tgt Ion:	202	Resp:	37797
Ion Ratio	Lower	Upper	
202	100		
101	8.7	6.7	10.1
203	17.0	13.4	20.0









#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.15 min Scan# 2171
Delta R.T. 0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.2	9.5	14.3#
236	27.3	22.5	33.7




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#28
Pyrene
Concen: 0.79 ng
RT: 19.38 min Scan# 1937
Delta R.T. -0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.4	16.2	24.4
203	17.4	14.1	21.1









#29
 Terphenyl-d14
 Concen: 0.79 ng
 RT: 19.60 min Scan# 1981
 Delta R.T. -0.00 min
 Lab File: BN010704.D
 Acq: 13 May 2020 11:57

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion	Ratio	Resp	Lower	Upper
244	100	24867		
212	8.1	6.8	10.2	
122	9.9	8.1	12.1	




Manual Integrations
 APPROVED


mohammad
 5/14/2020 9:19:24 AM



#30
 Benzo(a)anthracene
 Concen: 0.66 ng
 RT: 21.14 min Scan# 2170
 Delta R.T. 0.00 min
 Lab File: BN010704.D
 Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	29709		
226	26.0	21.3	31.9	
229	20.0	16.0	24.0	









#31
 Chrysene
 Concen: 0.78 ng
 RT: 21.19 min Scan# 2174
 Delta R.T. -0.01 min
 Lab File: BN010704.D
 Acq: 13 May 2020 11:57

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.5	23.4	35.0
229	19.2	16.1	24.1




Manual Integrations
 APPROVED


mohammad
 5/14/2020 9:19:24 AM



#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.54 ng
 RT: 21.09 min Scan# 2165
 Delta R.T. 0.00 min
 Lab File: BN010704.D
 Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
149	100		
167	28.4	22.5	33.7
279	4.8	4.1	6.1









#33
Indeno(1,2,3-cd)pyrene
Concen: 0.79 ng
RT: 25.46 min Scan# 3180
Delta R.T. -0.01 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampled :
SSTDIC0.8

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.6	15.1	22.7
277	24.7	19.4	29.0




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#34
Perylene-d12
Concen: 0.40 ng
RT: 23.32 min Scan# 2555
Delta R.T. -0.01 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.6	29.4
265	77.0	70.1	105.1









#35
Benzo(b)fluoranthene
Concen: 0.76 ng m
RT: 22.68 min Scan# 2368
Delta R.T. -0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.0	22.0	33.0
125	10.3	10.8	16.2




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#36
Benzo(k)fluoranthene
Concen: 0.82 ng
RT: 22.72 min Scan# 2380
Delta R.T. -0.01 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.0	21.9	32.9
125	11.1	11.1	16.7









#37
Benzo(a)pyrene
Concen: 0.74 ng
RT: 23.22 min Scan# 2528
Delta R.T. -0.01 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.6	24.8	37.2
125	13.1	15.8	23.6




Manual Integrations
APPROVED


mohammad
5/14/2020 9:19:24 AM



#38
Dibenzo(a,h)anthracene
Concen: 0.70 ng
RT: 25.47 min Scan# 3185
Delta R.T. -0.00 min
Lab File: BN010704.D
Acq: 13 May 2020 11:57

Tgt Ion	Ratio	Lower	Upper
278	100		
139	14.6	13.0	19.4
279	27.0	25.1	37.7





#39

Benzo(g,h,i)perylene

Concen: 0.79 ng

RT: 26.10 min Scan# 3368

Delta R.T. -0.00 min

Lab File: BN010704.D


Acq: 13 May 2020 11:57

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.8



Tgt Ion	Ratio	Lower	Upper
276	100		
277	25.0	20.6	30.8
138	18.8	16.0	24.0

Manual Integrations
APPROVED

mohammad
5/14/2020 9:19:24 AM

