
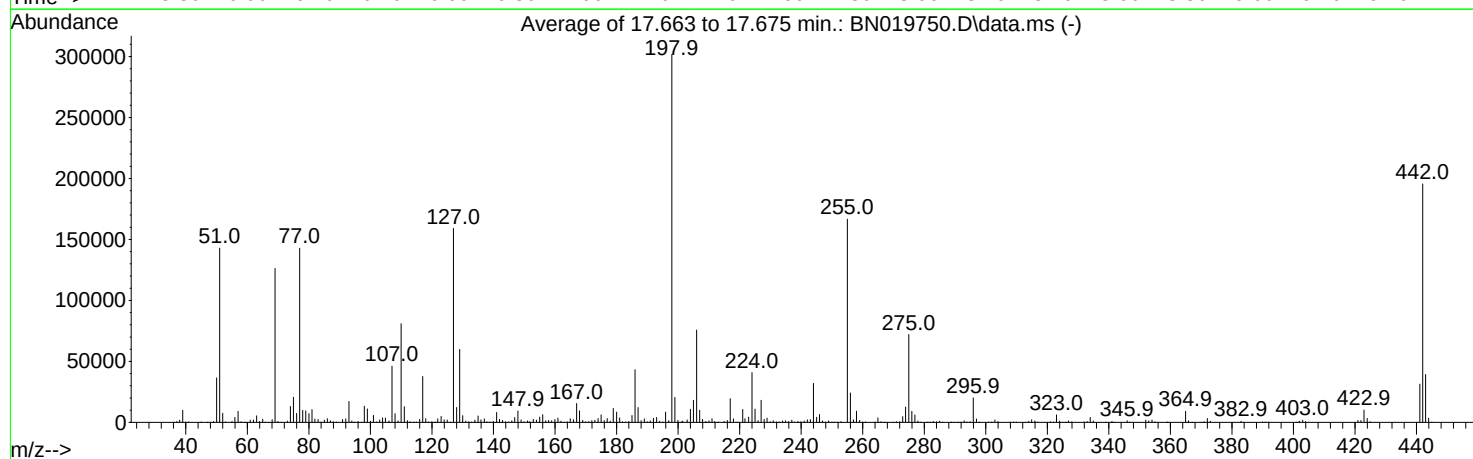


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
 Data File : BN019750.D
 Acq On : 12 May 2022 15:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 18 07:42:52 2022

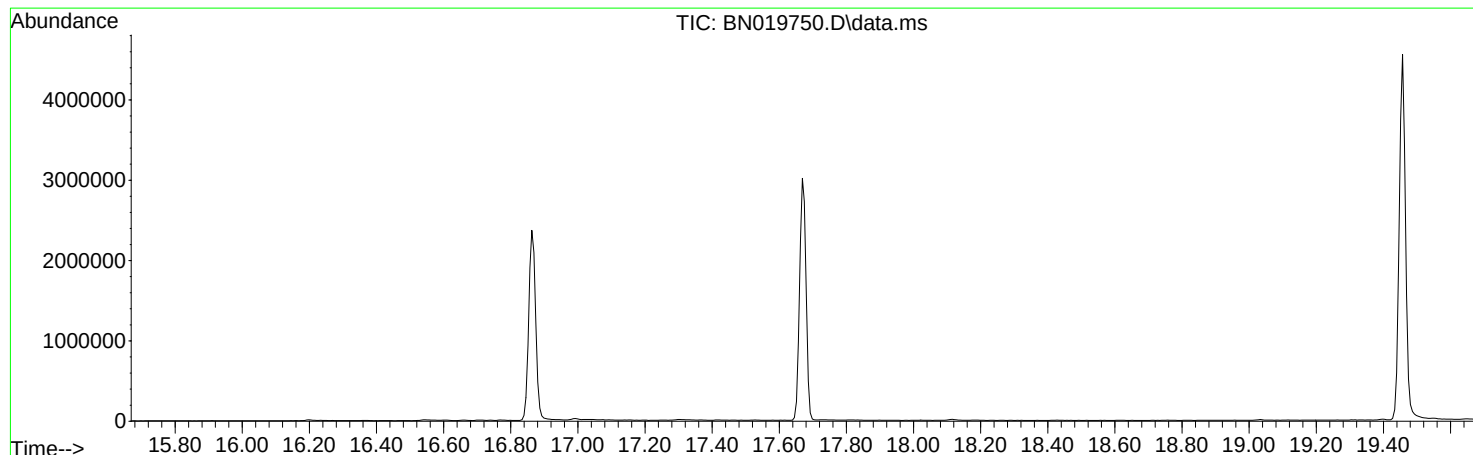

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	142939	PASS
68	69	0.00	2	1.8	2289	PASS
69	198	0.00	100	41.9	126302	PASS
70	69	0.00	2	0.6	738	PASS
127	198	10	80	52.7	158997	PASS
197	198	0.00	2	0.5	1470	PASS
198	198	100	100	100.0	301653	PASS
199	198	5	9	6.8	20485	PASS
275	198	10	60	23.9	71984	PASS
365	198	1	100	3.0	9065	PASS
441	198	0.01	100	10.4	31387	PASS
442	442	50	100	100.0	195541	PASS
443	442	15	24	20.1	39304	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/13/2022	BNA_N	<u>BN019750.D</u>
Compound Name	Response	Retention Time
DDT	1024081	20.704
DDD	10973	20.257
DDE	60	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11033	1035114	1.07

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
Data File : BN019750.D
Acq On : 12 May 2022 15:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 02:49:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

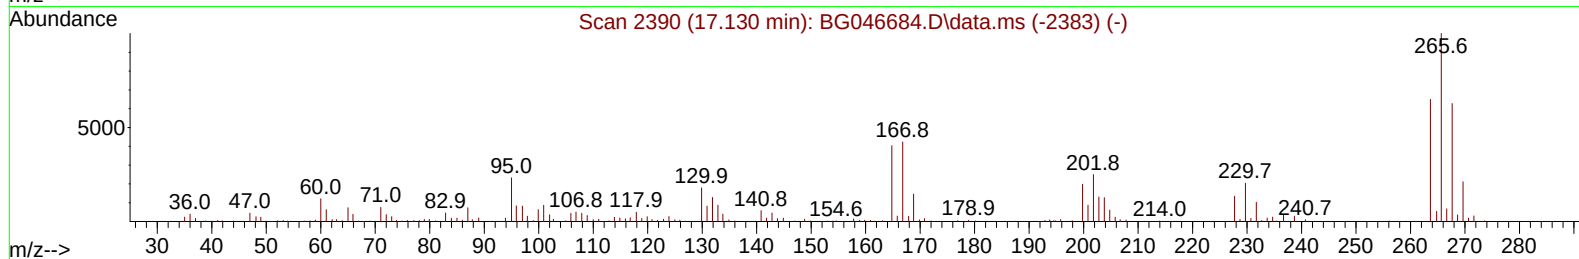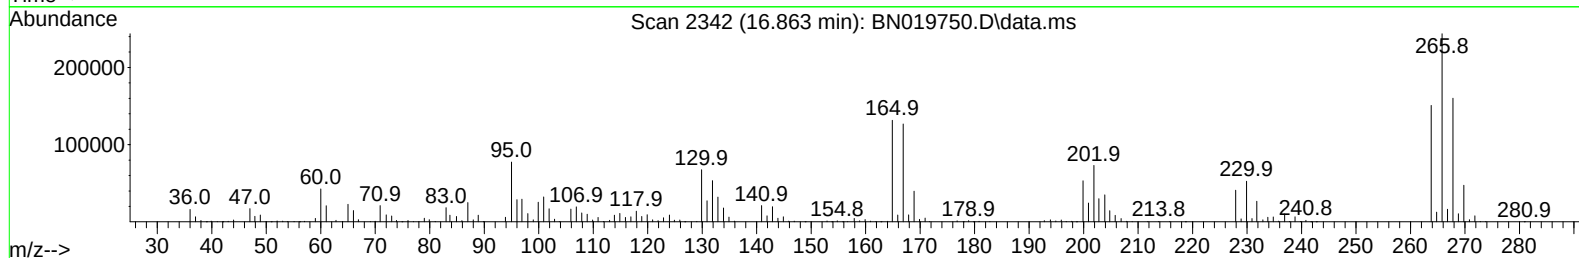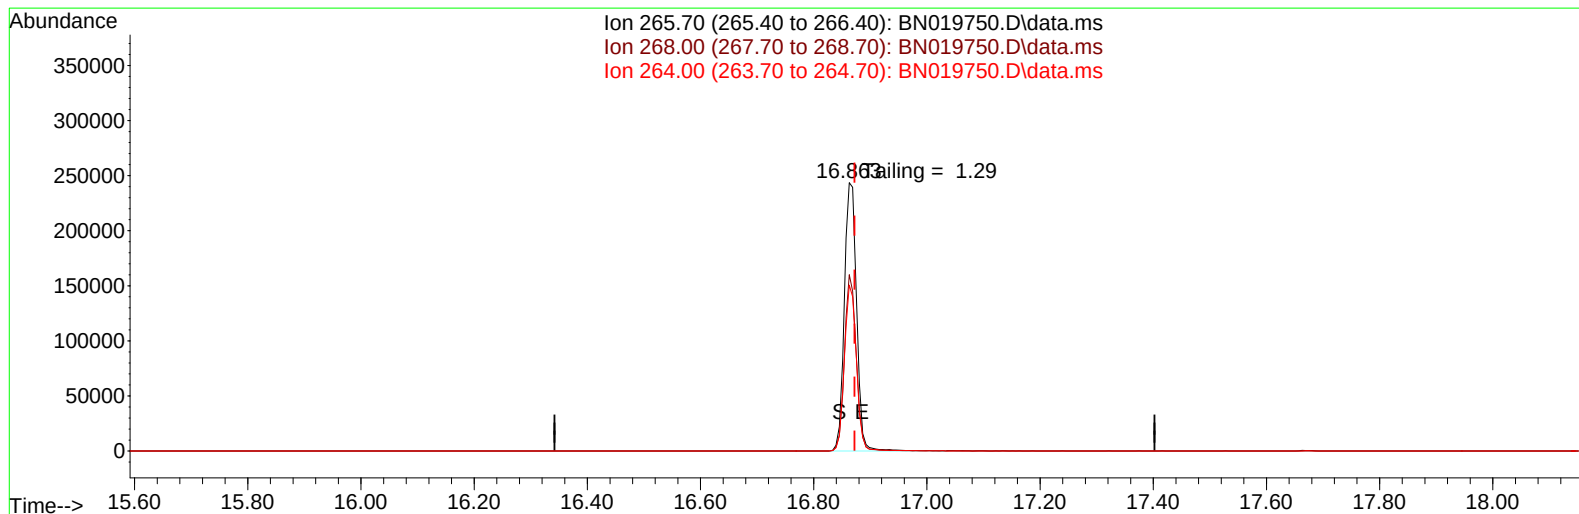

TIC: BN019750.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 21328.48 ng




response 367735

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.69
264.00	61.60	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
Data File : BN019750.D
Acq On : 12 May 2022 15:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 02:49:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

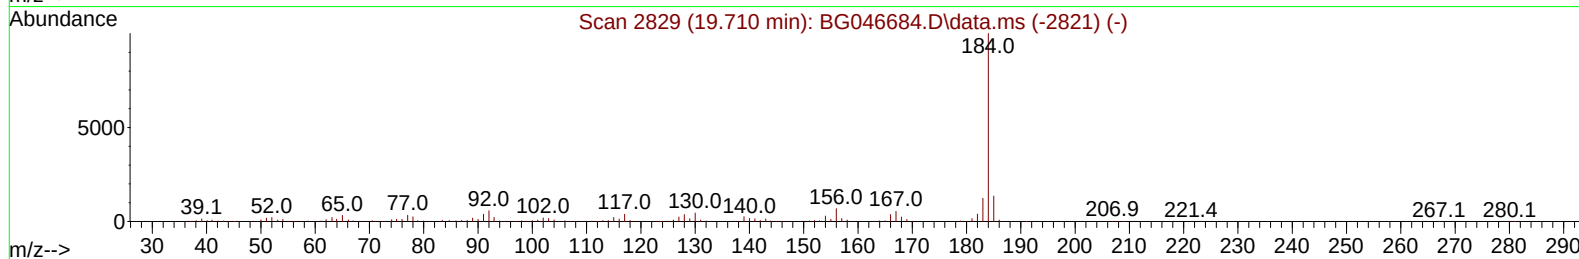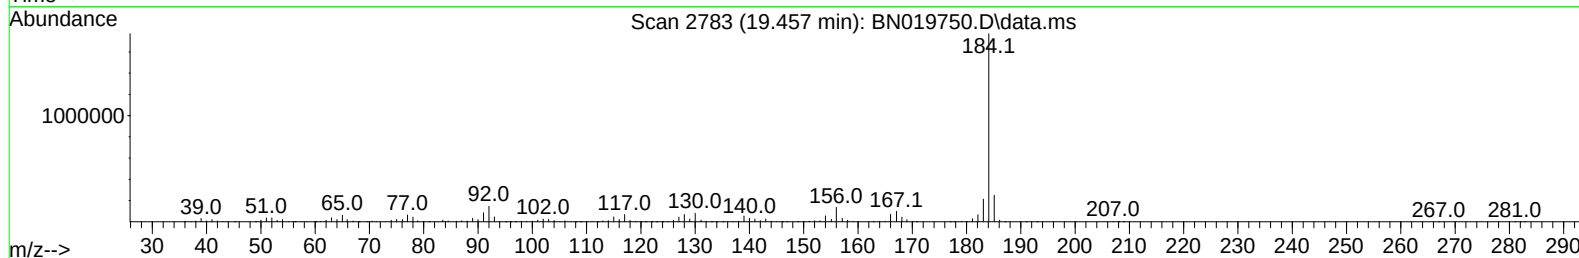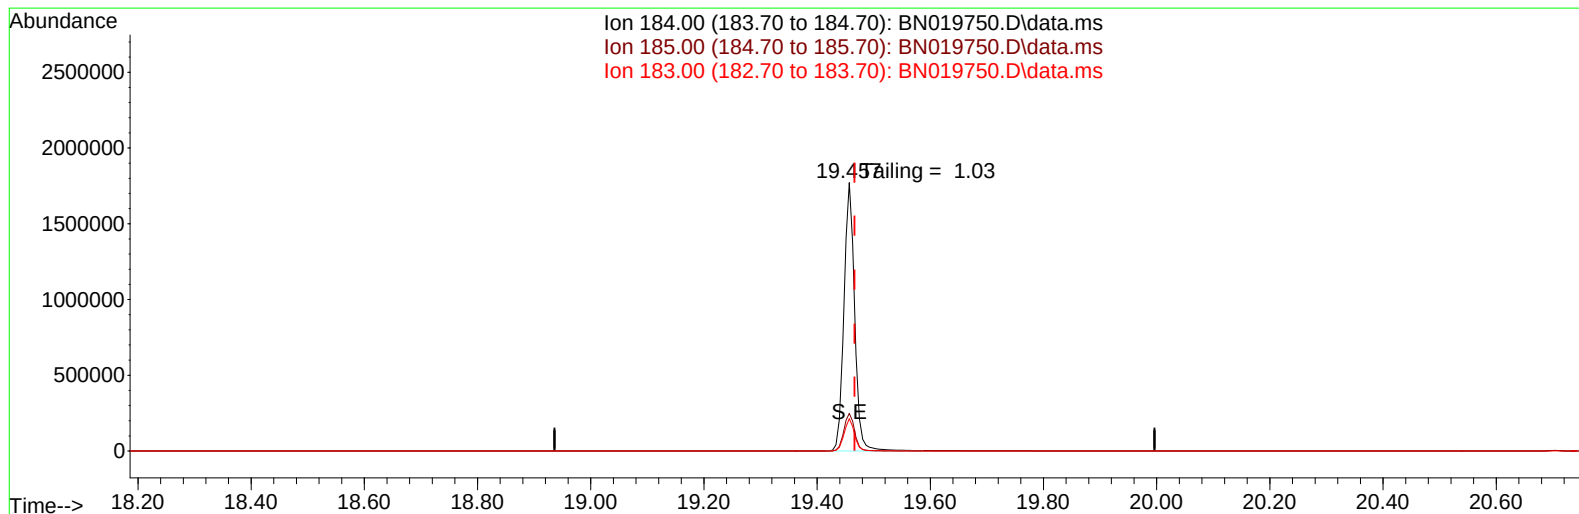

TIC: BN019750.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 2337810

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	12.03
0.00	0.00	0.00