


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
 Data File : BN019763.D
 Acq On : 13 May 2022 08:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 18 07:42:52 2022

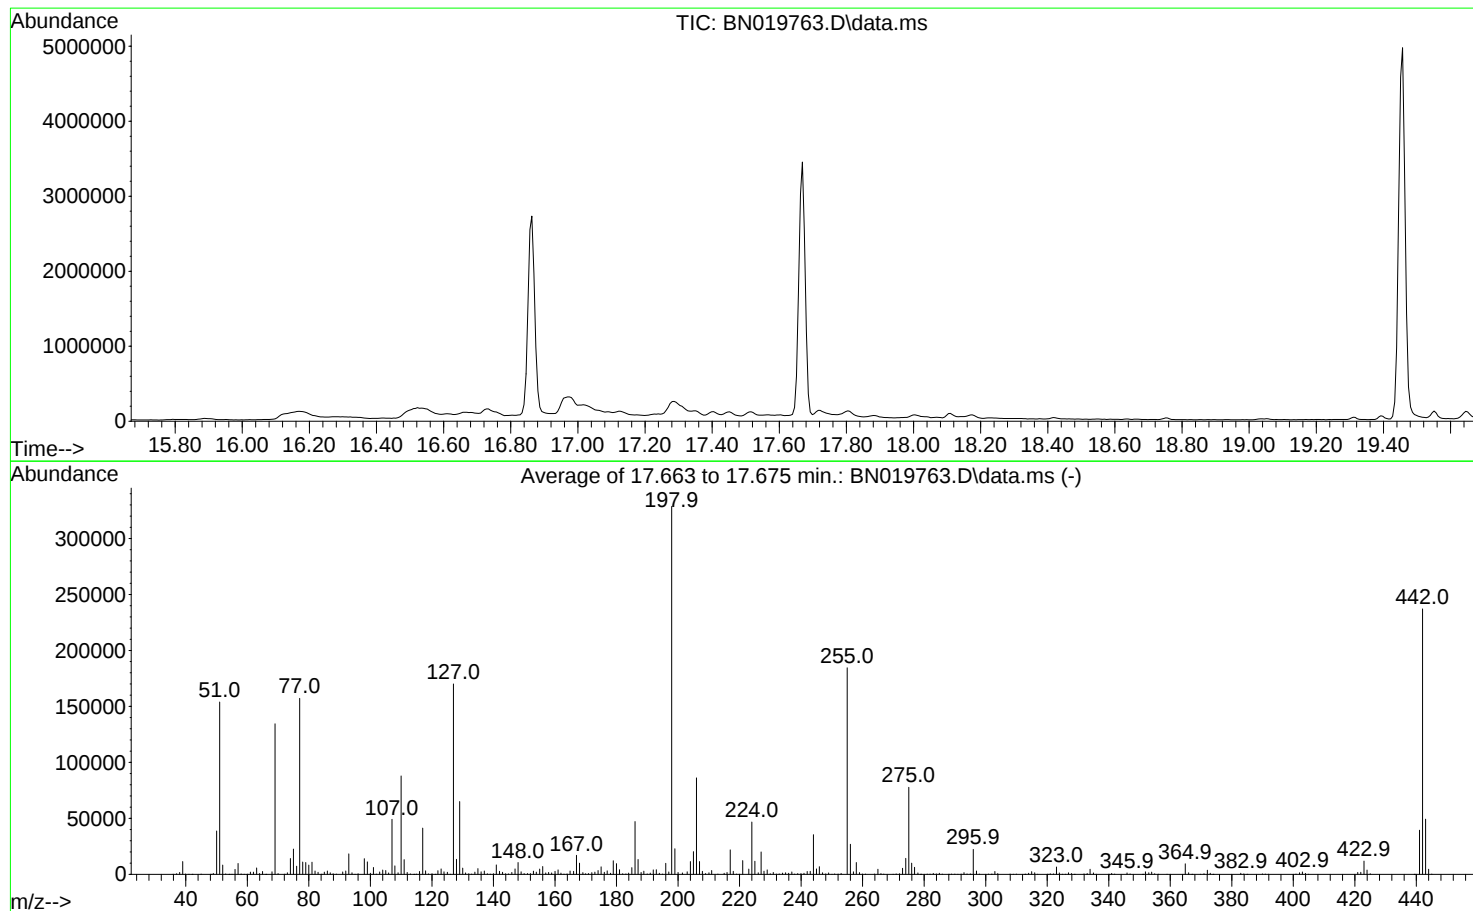

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	153971	PASS
68	69	0.00	2	1.7	2264	PASS
69	198	0.00	100	40.9	134531	PASS
70	69	0.00	2	0.5	704	PASS
127	198	10	80	51.8	170134	PASS
197	198	0.00	2	0.7	2136	PASS
198	198	100	100	100.0	328555	PASS
199	198	5	9	7.0	22891	PASS
275	198	10	60	23.7	77805	PASS
365	198	1	100	2.9	9433	PASS
441	198	0.01	100	12.0	39507	PASS
442	442	50	100	100.0	237141	PASS
443	442	15	24	20.8	49275	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2022	BNA_N	<u>BN019763.D</u>
Compound Name	Response	Retention Time
DDT	1130227	20.698
DDD	15257	20.257
DDE	377	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15634	1145861	1.36

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
Data File : BN019763.D
Acq On : 13 May 2022 08:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 06:10:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

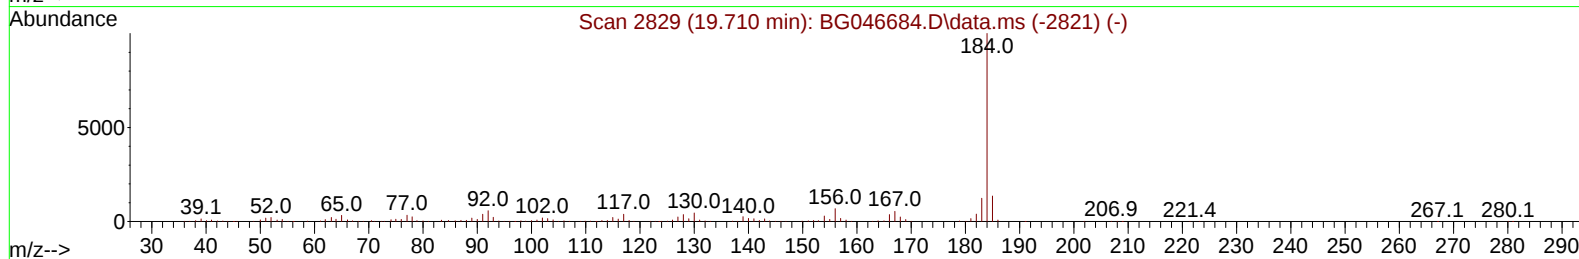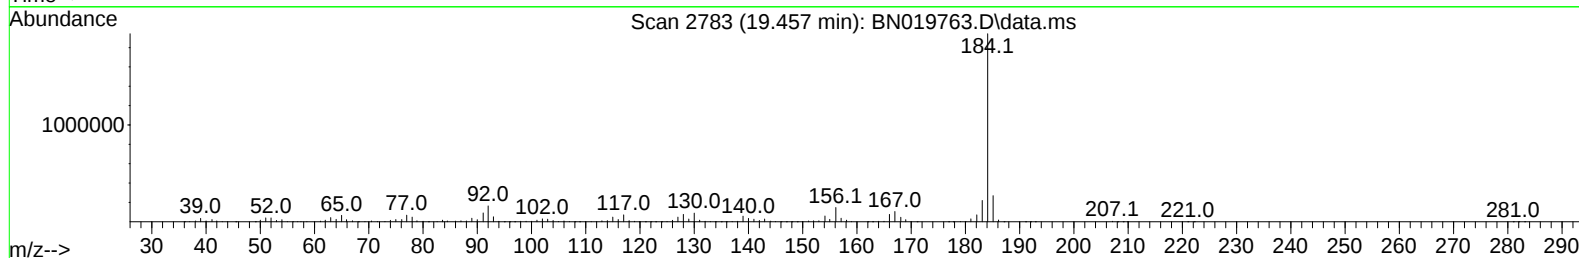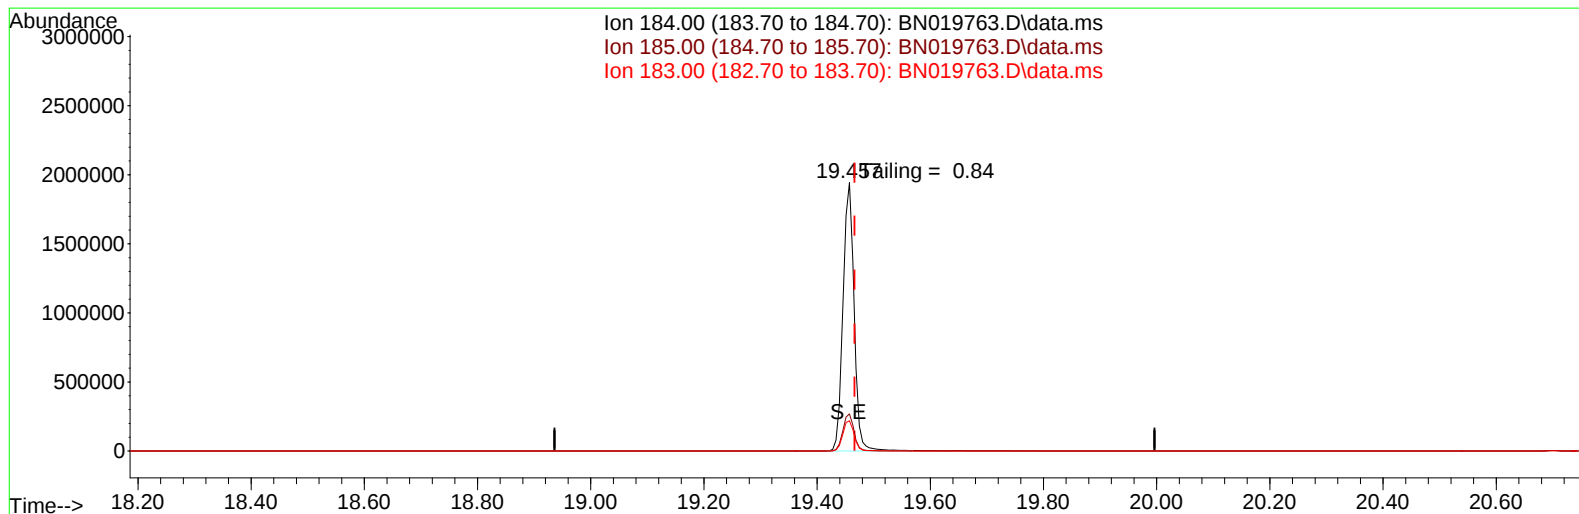

TIC: BN019763.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng




response 2653746

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	11.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
 Data File : BN019763.D
 Acq On : 13 May 2022 08:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 14 06:10:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

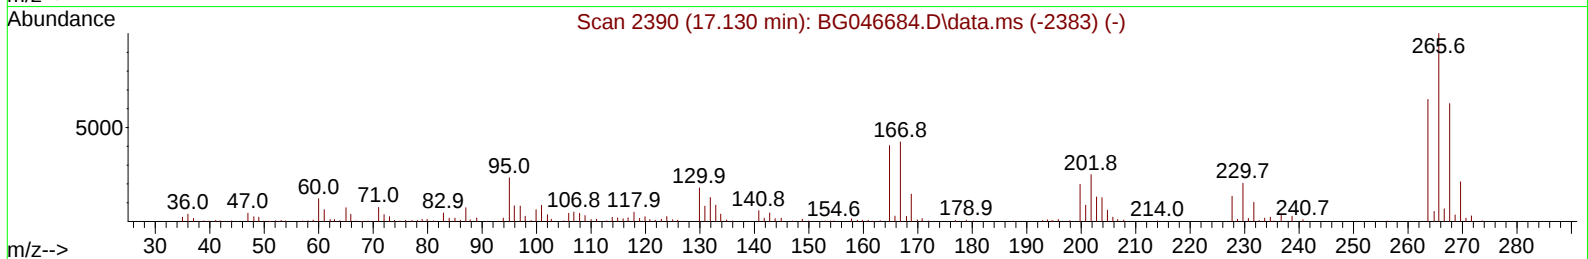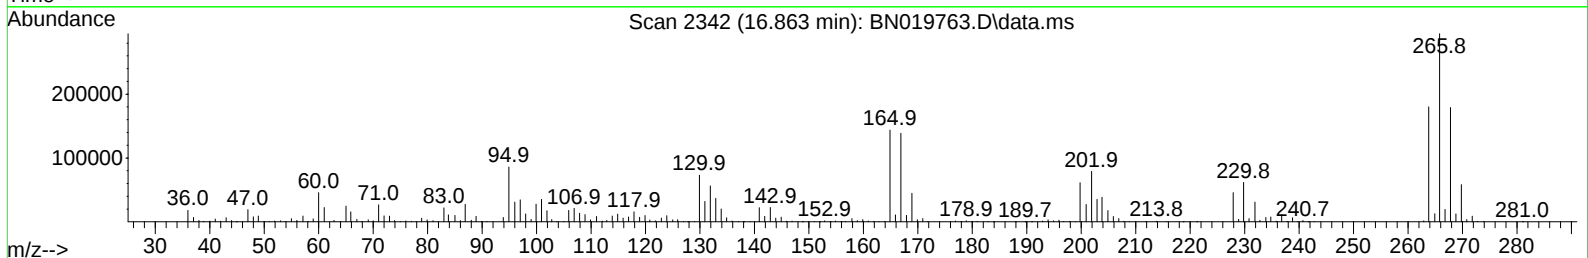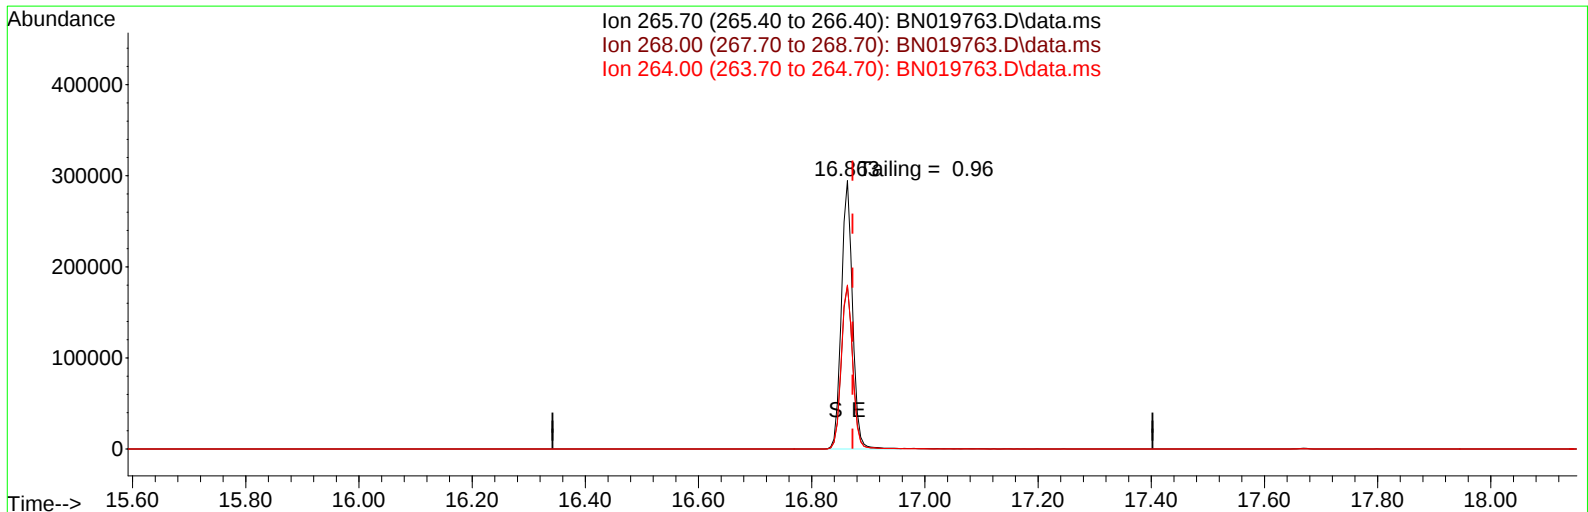

TIC: BN019763.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 20811.33 ng

response 402589

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.82
264.00	61.60	61.12
0.00	0.00	0.00