


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
 Data File : BN019771.D
 Acq On : 13 May 2022 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 18 07:42:52 2022

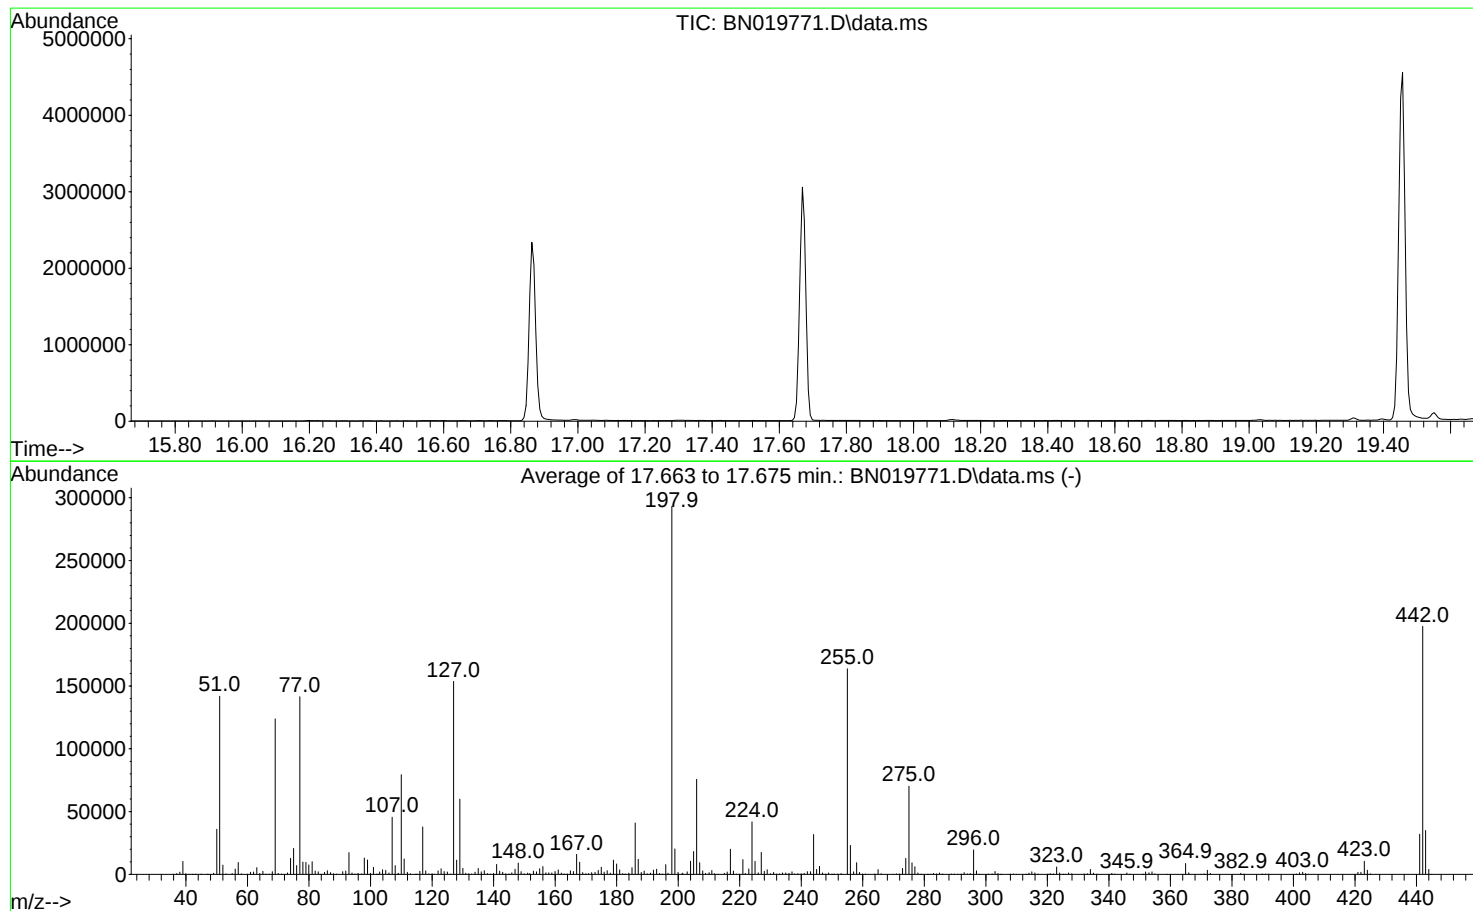

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	141885	PASS
68	69	0.00	2	1.8	2179	PASS
69	198	0.00	100	42.3	123948	PASS
70	69	0.00	2	0.6	730	PASS
127	198	10	80	52.5	153707	PASS
197	198	0.00	2	0.3	937	PASS
198	198	100	100	100.0	293035	PASS
199	198	5	9	6.9	20323	PASS
275	198	10	60	24.0	70208	PASS
365	198	1	100	3.0	8674	PASS
441	198	0.01	100	10.9	32029	PASS
442	442	50	100	100.0	197536	PASS
443	442	15	24	17.7	34957	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/13/2022	BNA_N	<u>BN019771.D</u>
Compound Name	Response	Retention Time
DDT	1070471	20.698
DDD	10263	20.257
DDE	129	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10392	1080863	0.96

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
 Data File : BN019771.D
 Acq On : 13 May 2022 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 14 06:17:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

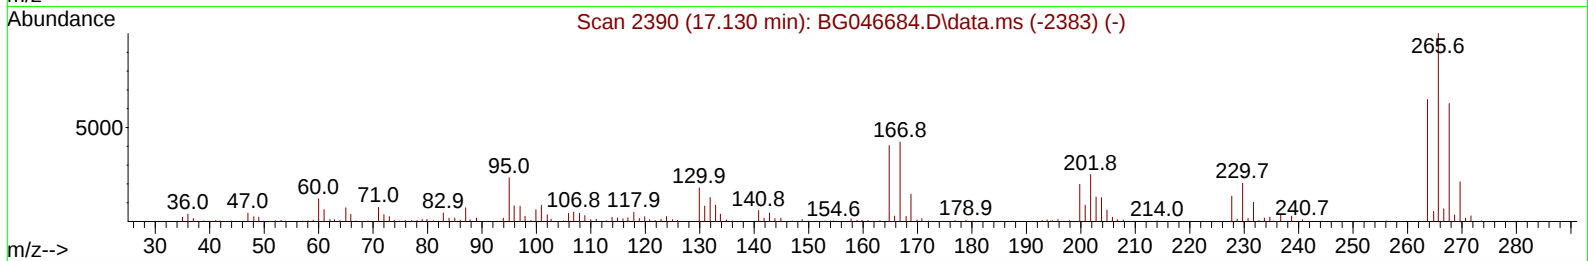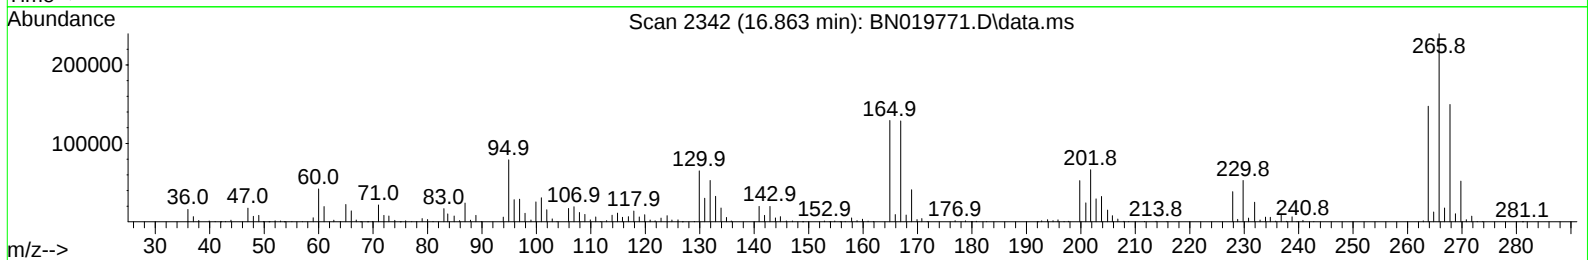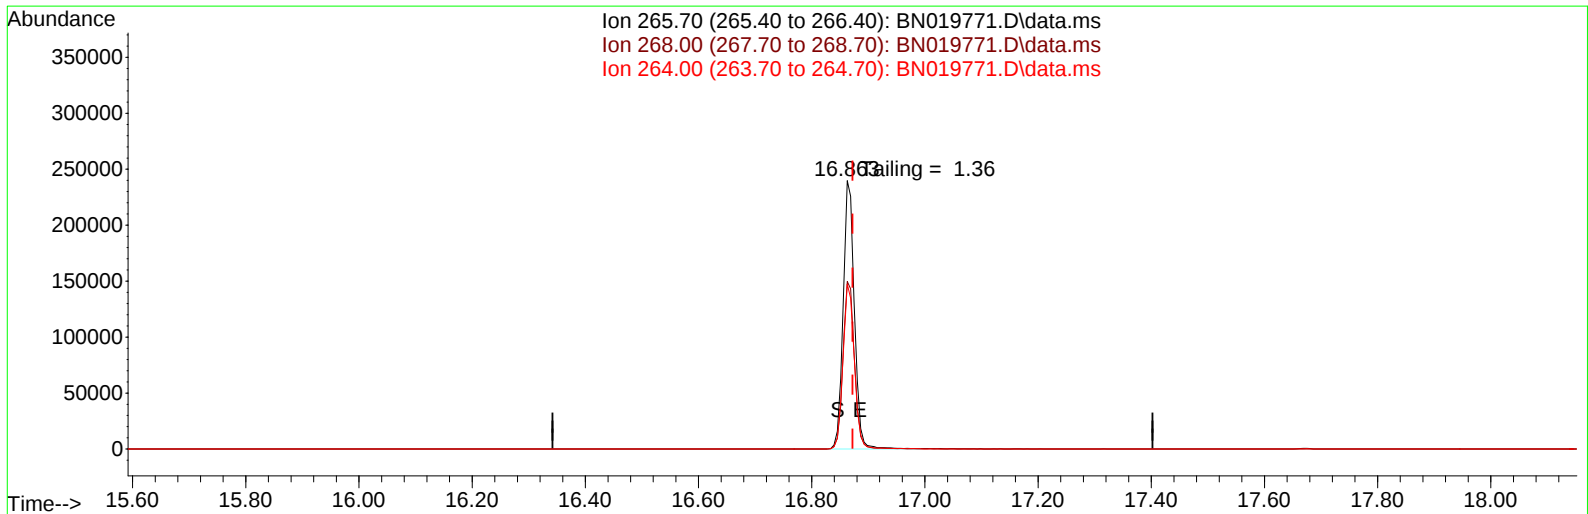

TIC: BN019771.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 18702.05 ng




response 330964

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.45
264.00	61.60	61.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051322\
Data File : BN019771.D
Acq On : 13 May 2022 16:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 06:17:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

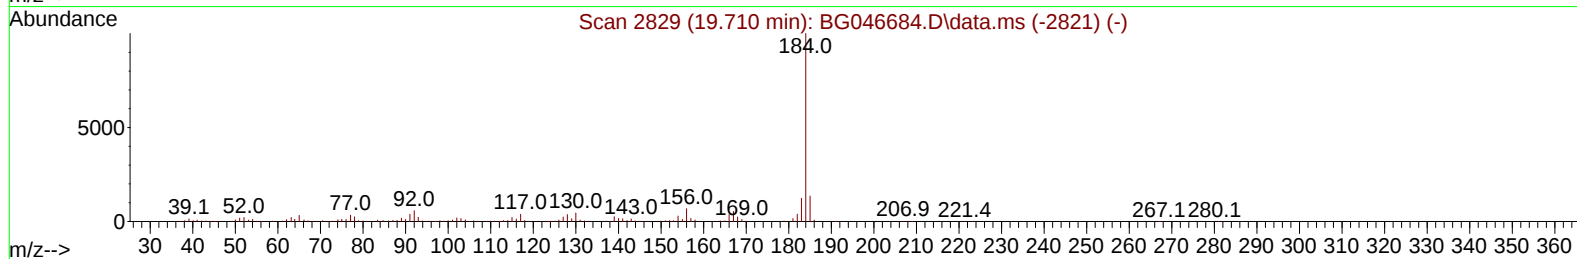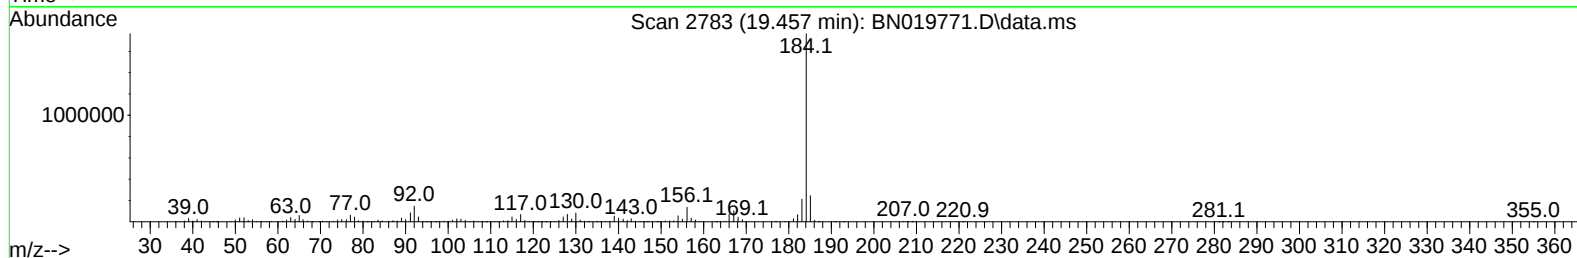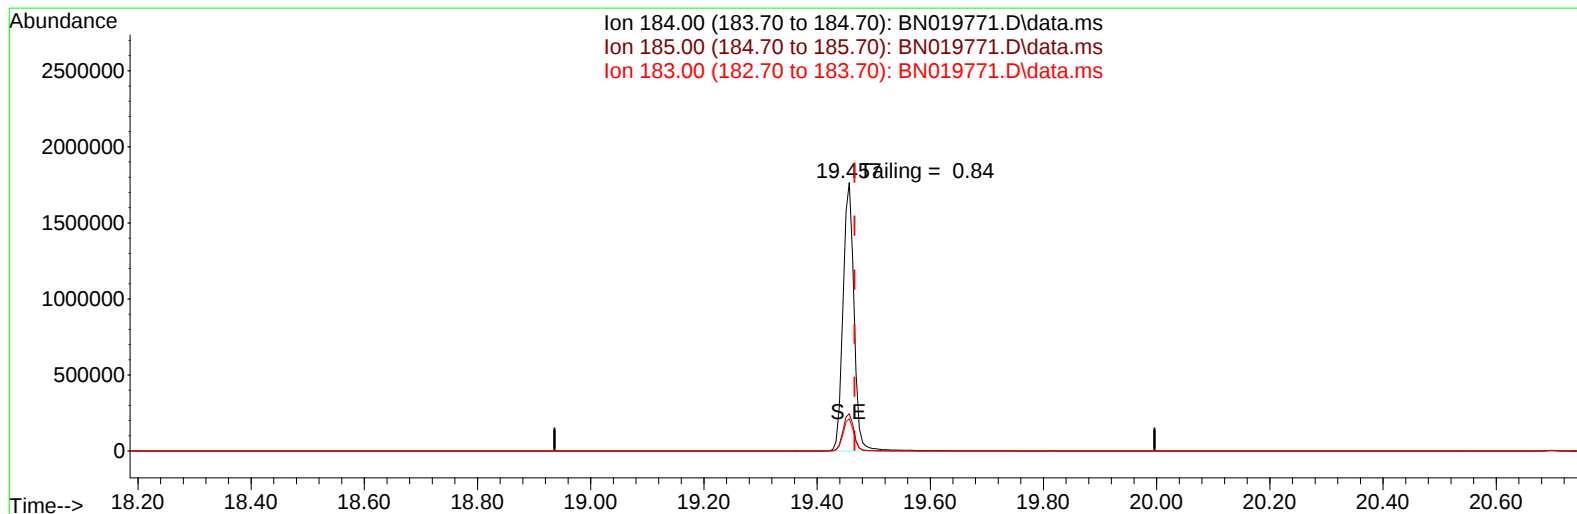

TIC: BN019771.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 2394067

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	12.04
0.00	0.00	0.00