

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051819\
 Data File : BN005754.D
 Acq On : 18 May 2019 15:52
 Operator : JU/SJ
 Sample : PB119473BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK73

Quant Time: May 20 04:03:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 20 03:44:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	100205	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	450678	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	321323	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	792505	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	860518	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	964068	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	13125	7.33	ng/uL	0.00
5) Phenol-d5	6.76	99	247408	31.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	141310	34.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	210922	33.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	216758	32.73	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	114476	34.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	138381	36.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	207444	28.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	334100	41.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	952198	38.51	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	1116087	37.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	114430	32.85	ng/ul	0.00
57) Fluorene-d10	15.22	176	800974	37.72	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	142544	29.92	ng/ul	0.00
70) Anthracene-d10	17.07	188	1316639	38.46	ng/ul	0.00
78) Pyrene-d10	19.39	212	1559798	36.79	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	1634245	37.79	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.28	70	5469	1.068	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051819\
Data File : BN005754.D
Acq On : 18 May 2019 15:52
Operator : JU/SJ
Sample : PB119473BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK73

Quant Time: May 20 04:03:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 20 03:44:27 2019
Response via : Initial Calibration

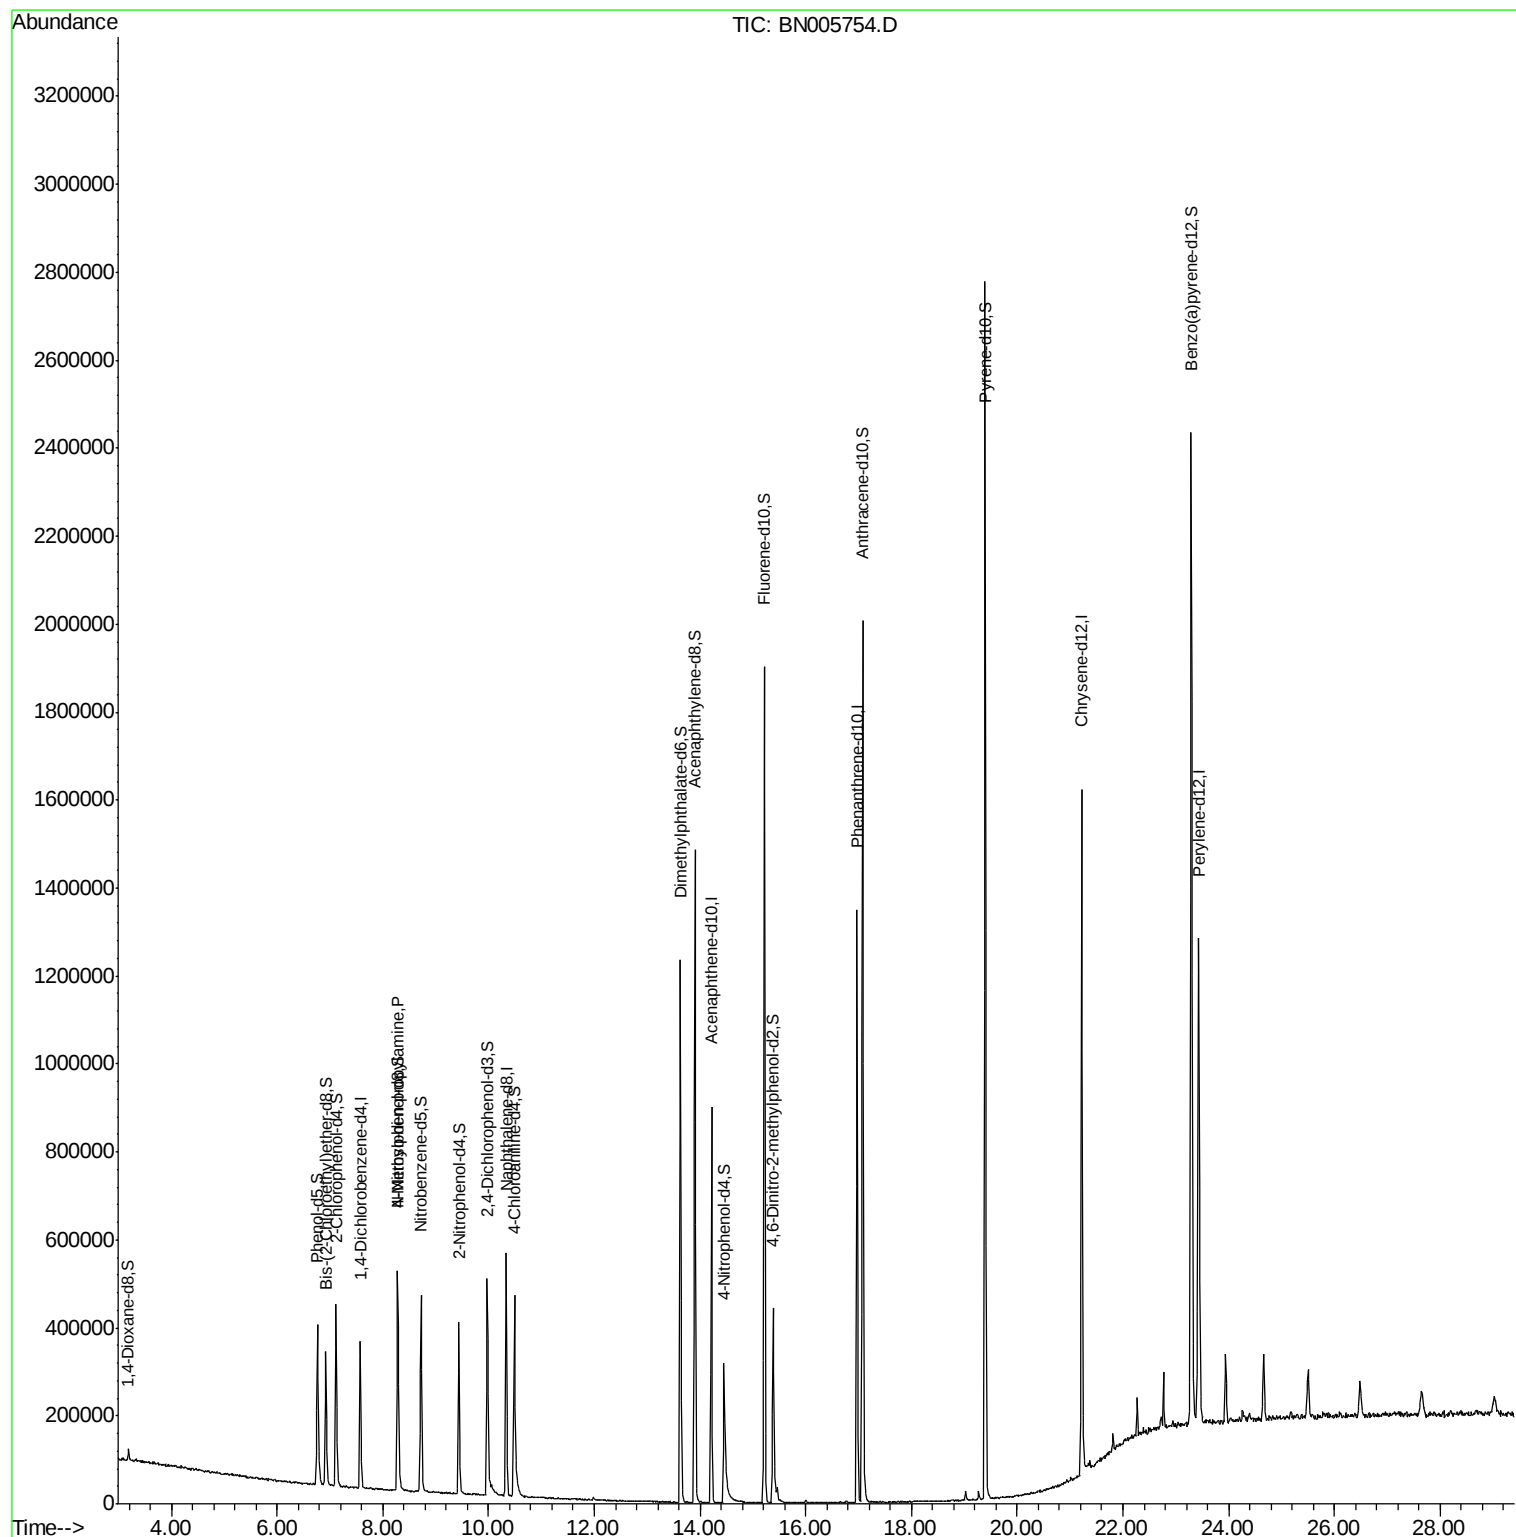

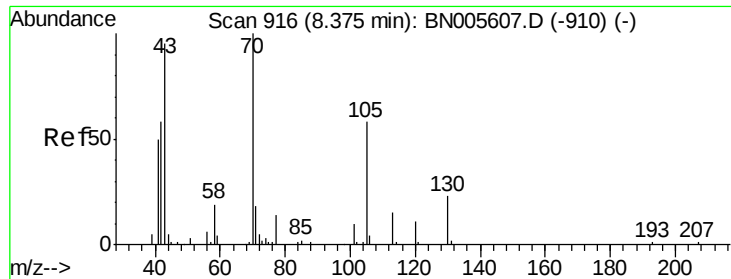

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.068 ng/ul
 RT: 8.28 min Scan# 900
 Delta R.T. -0.09 min
 Lab File: BN005754.D
 Acq: 18 May 2019 15:52

Instrument :
 BNA_N
 ClientSampleId :
 SBLK73

Tgt Ion:	70	Resp:	5469
Ion	Ratio	Lower	Upper
70	100		
42	344.9	53.8	80.8#
101	0.0	7.7	11.5#
130	0.0	15.0	22.4#

