


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051819\
Data File : BN005744.D
Acq On : 18 May 2019 09:20
Operator : JU/SJ
Sample : SSTD00573
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 20 03:39:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 18 11:54:52 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SSTD00573

Manual Integrations APPROVED

Sohil
5/21/2019 7:09:38 PM

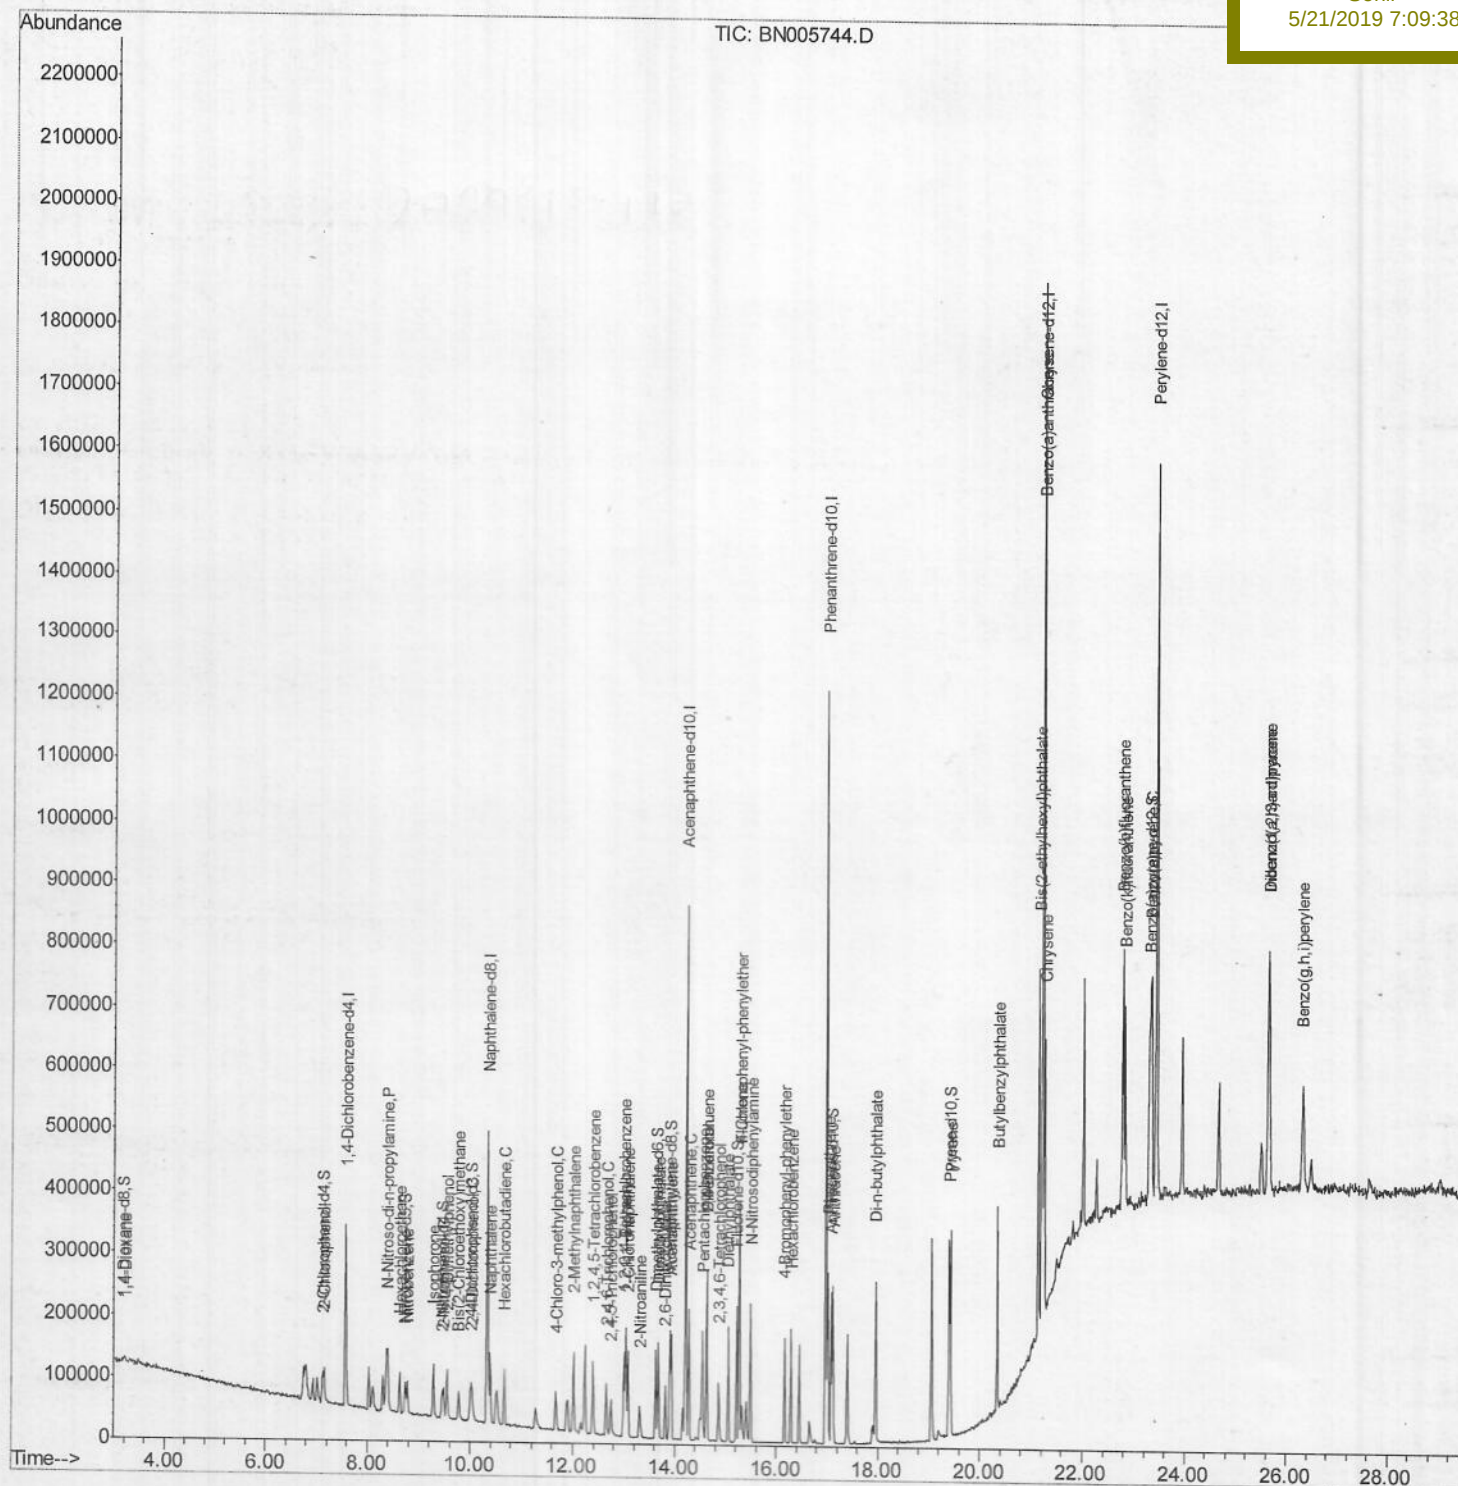

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051819\

Data File : BN005744.D

Acq On : 18 May 2019 09:20

Operator : JU/SJ

Sample : SST000573

Misc :

ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 18 12:04:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat May 18 11:54:52 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

SSTD000573

Manual Integrations
APPROVED

Sohil

5/21/2019 7:09:38 PM

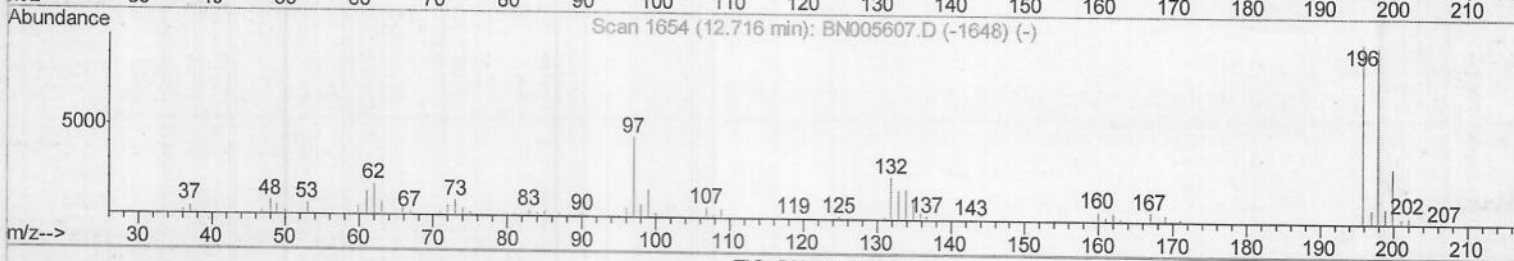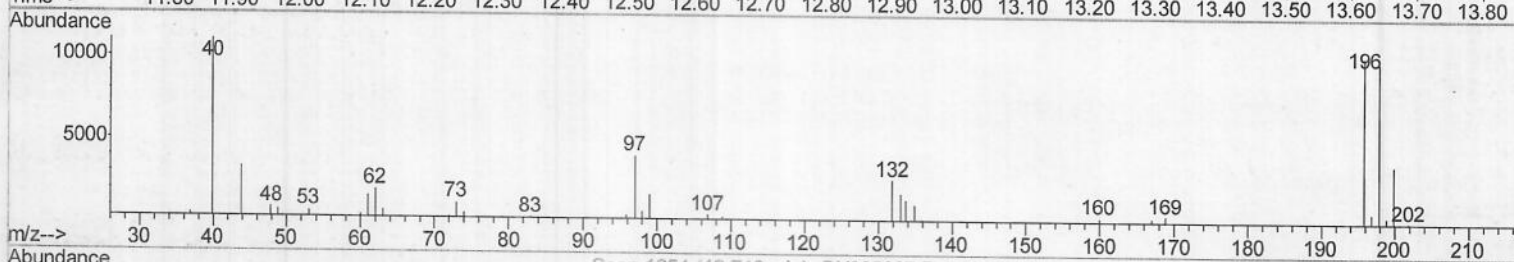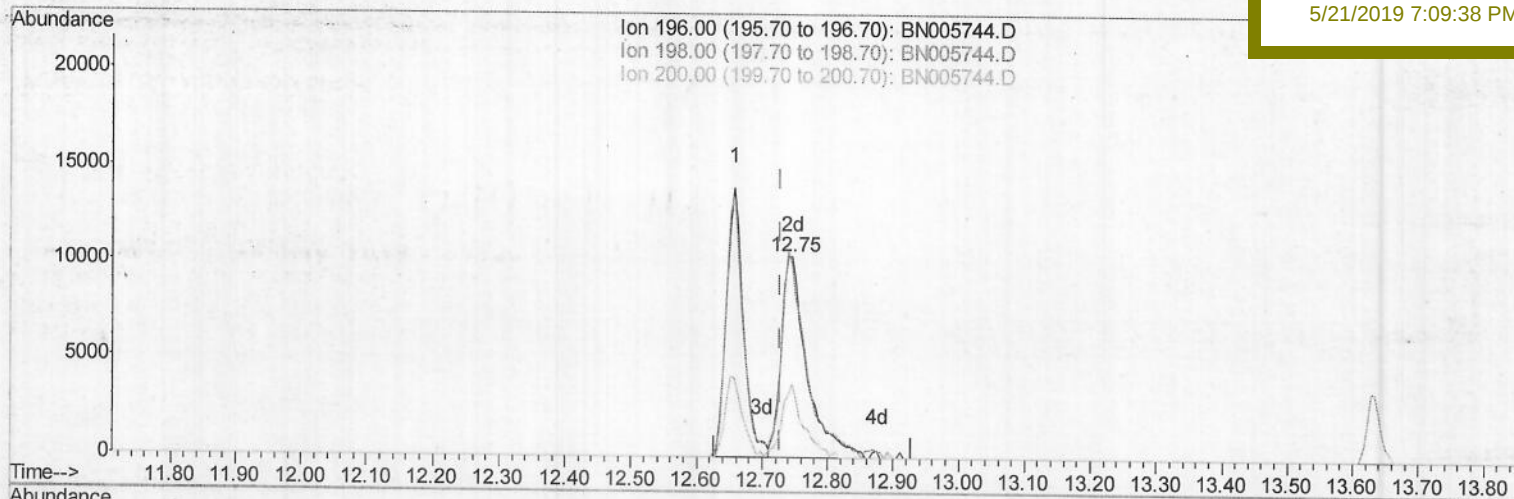

TIC: BN005744.D

(39) 2,4,5-Trichlorophenol

12.746min (+0.018) 5.01ng/ul m

> JU/05/22/19

response 28341

Ion	Exp%	Act%
196.00	100	100
198.00	93.70	96.35
200.00	30.30	36.47#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051819\

Data File : BN005744.D

Acq On : 18 May 2019 09:20

Operator : JU/SJ

Sample : SSTD00573

Misc :

ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 18 12:04:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat May 18 11:54:52 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




SSTD00573

Manual Integrations

APPROVED

Sohil

5/21/2019 7:09:38 PM

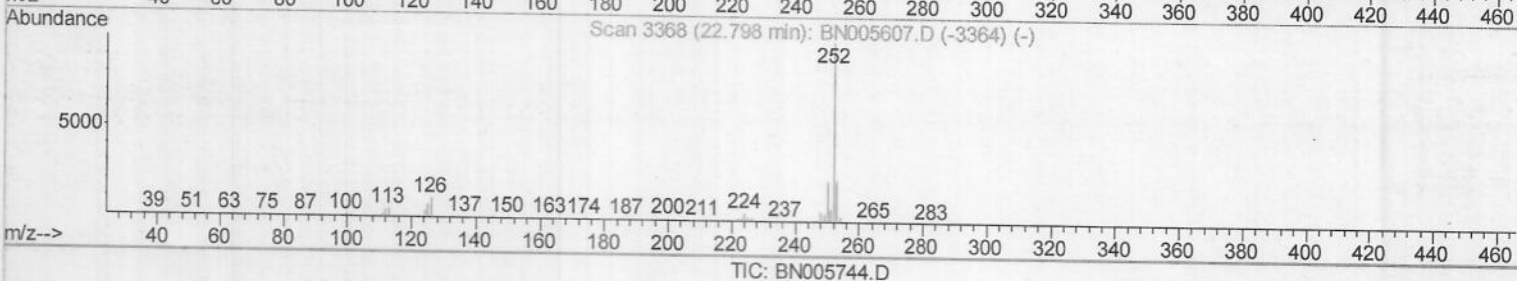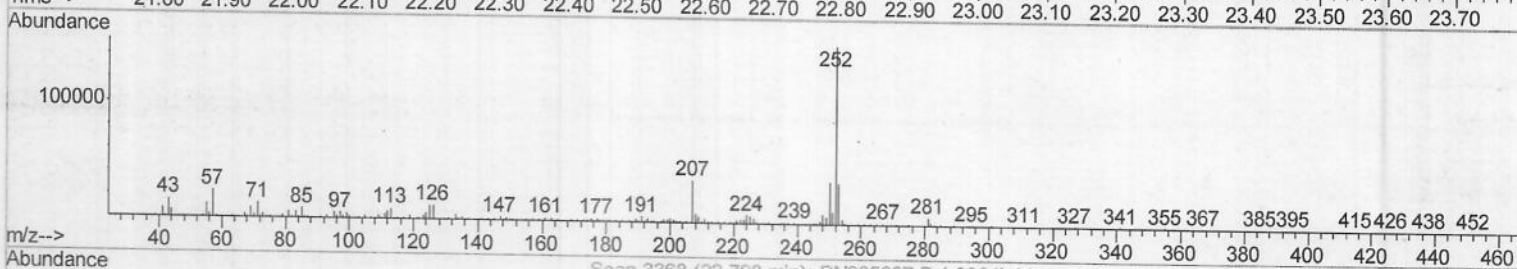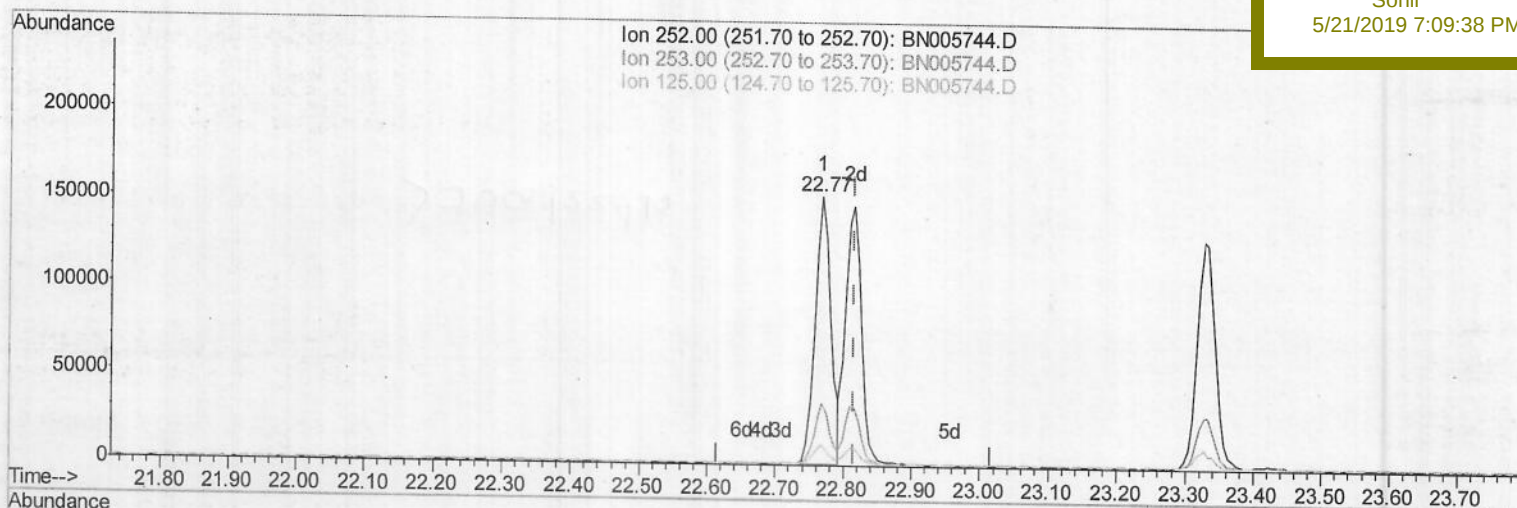

(88) Benzo(k)fluoranthene

22.769min (-0.047) 4.87ng/ul

response 243944

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.66
125.00	9.40	7.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051819\

Data File : BN005744.D

Acq On : 18 May 2019 09:20

Operator : JU/SJ

Sample : SST00573

Misc :

ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 18 12:04:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat May 18 11:54:52 2019

Response via : Initial Calibration

Instrument :

BNA_N




Client Sample Id :

SSTD00573

Manual Integrations
APPROVED

Sohil

5/21/2019 7:09:38 PM

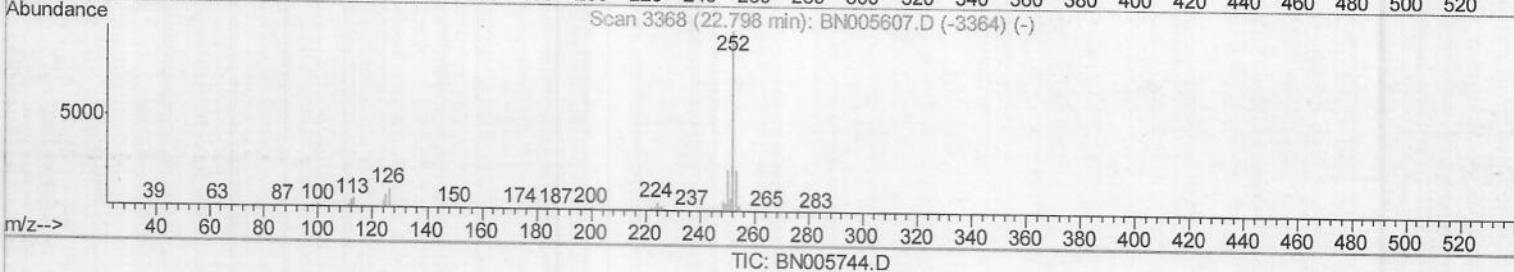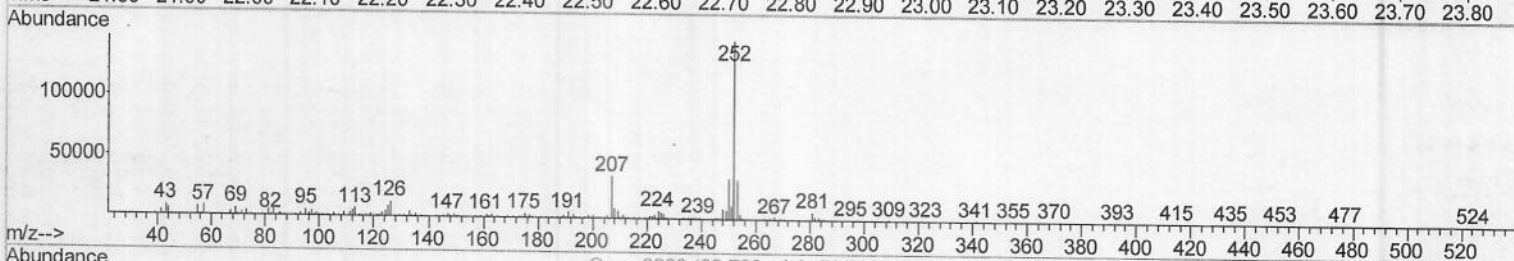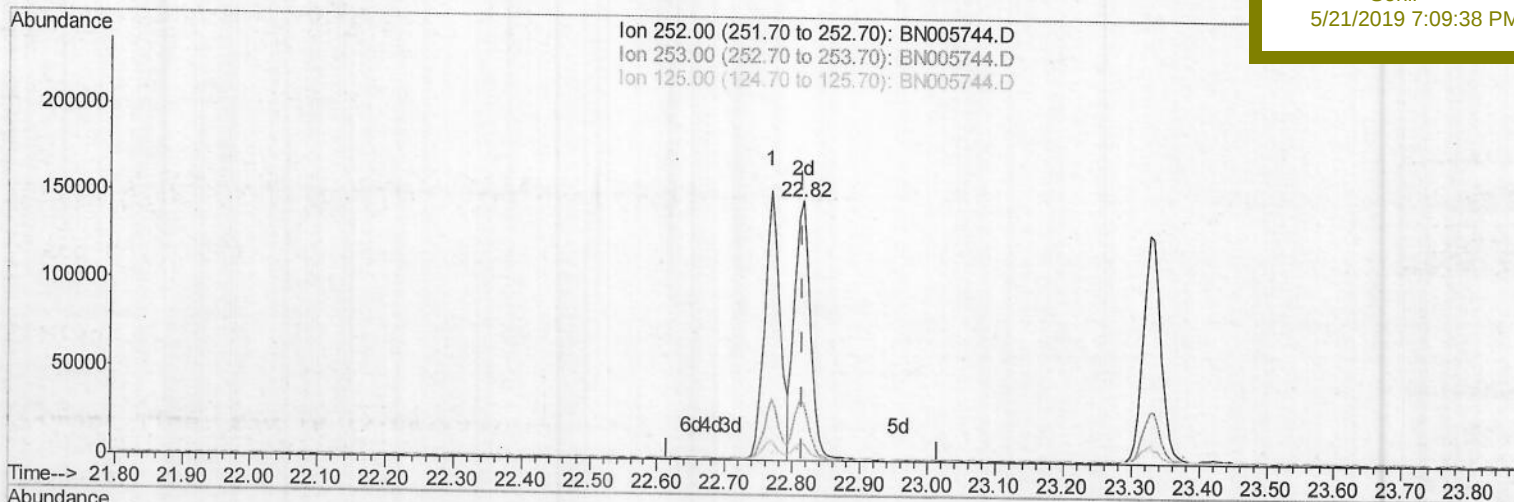

(88) Benzo(k)fluoranthene

22.816min (+0.000) 4.82ng/ul m

response 241310

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.19
125.00	9.40	6.54#
0.00	0.00	0.00

> JU/05/22/19

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051819\
 Data File : BN005744.D
 Acq On : 18 May 2019 09:20
 Operator : JU/SJ
 Sample : SST00573
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 SST00573

Quant Time: May 20 03:39:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 18 11:54:52 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 5/21/2019 7:09:38 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	87166	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	398112	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	282274	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	729205	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	782316	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	932719	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	3237	1.79	ng/uL	0.00
5) Phenol-d5	0.00	99	0d	0.00	ng/ul	
7) Bis-(2-Chloroethyl) ether-d	0.00	67	0d	0.00	ng/ul	
9) 2-Chlorophenol-d4	7.12	132	24694	4.71	ng/ul	0.00
13) 4-Methylphenol-d8	0.00	113	0d	0.00	ng/ul	
19) Nitrobenzene-d5	8.73	128	13347	5.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	14249	5.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	28502	5.01	ng/ul	0.02
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.63	166	104674	5.11	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	125328	4.98	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
57) Fluorene-d10	15.22	176	90132	5.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
70) Anthracene-d10	17.08	188	148570	4.86	ng/ul	0.00
78) Pyrene-d10	19.39	212	177808	4.44	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	199589	4.90	ng/ul	0.00

Target Compounds

					Qvalue	
2) 1,4-Dioxane	3.22	88	3416	1.759	ng/uL#	90
10) 2-Chlorophenol	7.15	128	25313	4.673	ng/ul	92
15) N-Nitroso-di-n-propylamine	8.38	70	21178	4.623	ng/ul#	89
17) Hexachloroethane	8.63	117	11845	5.036	ng/ul	89
20) Nitrobenzene	8.78	77	31378	4.653	ng/ul	93
21) Isophorone	9.28	82	62769	4.701	ng/ul	95
23) 2-Nitrophenol	9.48	139	15266	5.423	ng/ul	95
24) 2,4-Dimethylphenol	9.55	107	33320	4.727	ng/ul	98
25) Bis(2-Chloroethoxy)methane	9.78	93	35680	4.252	ng/ul	97
27) 2,4-Dichlorophenol	10.02	162	26824	4.773	ng/ul	95
28) Naphthalene	10.39	128	91419	4.940	ng/ul	96
31) Hexachlorobutadiene	10.66	225	21451	5.405	ng/ul	94
33) 4-Chloro-3-methylphenol	11.66	107	32195	5.088	ng/ul	93
34) 2-Methylnaphthalene	12.02	142	69887	5.157	ng/ul	97
36) 1,2,4,5-Tetrachlorobenzene	12.40	216	41959	4.803	ng/ul	97
38) 2,4,6-Trichlorophenol	12.66	196	24591	4.668	ng/ul	97
39) 2,4,5-Trichlorophenol	12.75	196	28341m	5.007	ng/ul	97
40) 1,1'-Biphenyl	13.04	154	97740	4.647	ng/ul#	97
41) 2-Chloronaphthalene	13.09	162	76007	4.699	ng/ul	99
42) 2-Nitroaniline	13.31	65	19777	4.610	ng/ul	96
44) Dimethylphthalate	13.68	163	103943	5.091	ng/ul#	99
45) 2,6-Dinitrotoluene	13.82	165	19704	5.589	ng/ul	93
47) Acenaphthylene	13.93	152	121106	4.897	ng/ul	100

5/21/2019 7:09:38 PM

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051819\
 Data File : BN005744.D
 Acq On : 18 May 2019 09:20
 Operator : JU/SJ
 Sample : SSTD00573
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 20 03:39:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 18 11:54:52 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 Client Sampled :
 SSTD00573

Manual Integrations
 APPROVED

Sohil
 5/21/2019 7:09:38 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Acenaphthene	14.28	153	82947	4.913	ng/ul	96
53) Dibenzofuran	14.63	168	123291	5.072	ng/ul	97
54) 2,4-Dinitrotoluene	14.63	165	29889	5.881	ng/ul#	74
55) 2,3,4,6-Tetrachlorophenol	14.87	232	24448	5.192	ng/ul#	91
56) Diethylphthalate	15.05	149	104989	5.128	ng/ul	98
58) Fluorene	15.27	166	100881	5.318	ng/ul	98
59) 4-Chlorophenyl-phenylether	15.27	204	55112	5.477	ng/ul	96
64) N-Nitrosodiphenylamine	15.49	169	87668	4.393	ng/ul	96
65) 4-Bromophenyl-phenylether	16.17	248	35593	4.845	ng/ul	91
66) Hexachlorobenzene	16.29	284	40881	5.226	ng/ul	94
69) Phenanthrene	17.02	178	176311	4.965	ng/ul	98
71) Anthracene	17.12	178	172187	4.760	ng/ul	100
72) 1,2,3,4-Tetrachlorobenzene	13.01	216	44266	4.156	ng/uL	98
73) Pentachlorobenzene	14.55	250	45419	4.738	ng/uL	95
75) Di-n-butylphthalate	17.96	149	186068	4.772	ng/ul	98
79) Pyrene	19.42	202	226740	4.501	ng/ul#	90
80) Butylbenzylphthalate	20.34	149	91145	4.570	ng/ul	95
82) Benzo(a)anthracene	21.20	228	237873	4.888	ng/ul	98
83) Bis(2-ethylhexyl)phthalate	21.13	149	140822	4.586	ng/ul#	97
84) Chrysene	21.25	228	226784	5.021	ng/ul	98
87) Benzo(b)fluoranthene	22.77	252	243944	4.653	ng/ul#	97
88) Benzo(k)fluoranthene	22.82	252	241310m	4.819	ng/ul	97
90) Benzo(a)pyrene	23.33	252	236413	4.797	ng/ul#	97
91) Indeno(1,2,3-cd)pyrene	25.63	276	299121	5.490	ng/ul#	92
92) Dibenzo(a,h)anthracene	25.63	278	252918	5.470	ng/ul#	94
93) Benzo(g,h,i)perylene	26.31	276	248138	5.508	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed