


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN051819\
Data File : BN005743.D
Acq On : 18 May 2019 08:45
Operator : JU/SJ
Sample : DFTPP72
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP72

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Title : SVOA CALIBRATION
Last Update : Mon May 20 03:44:27 2019

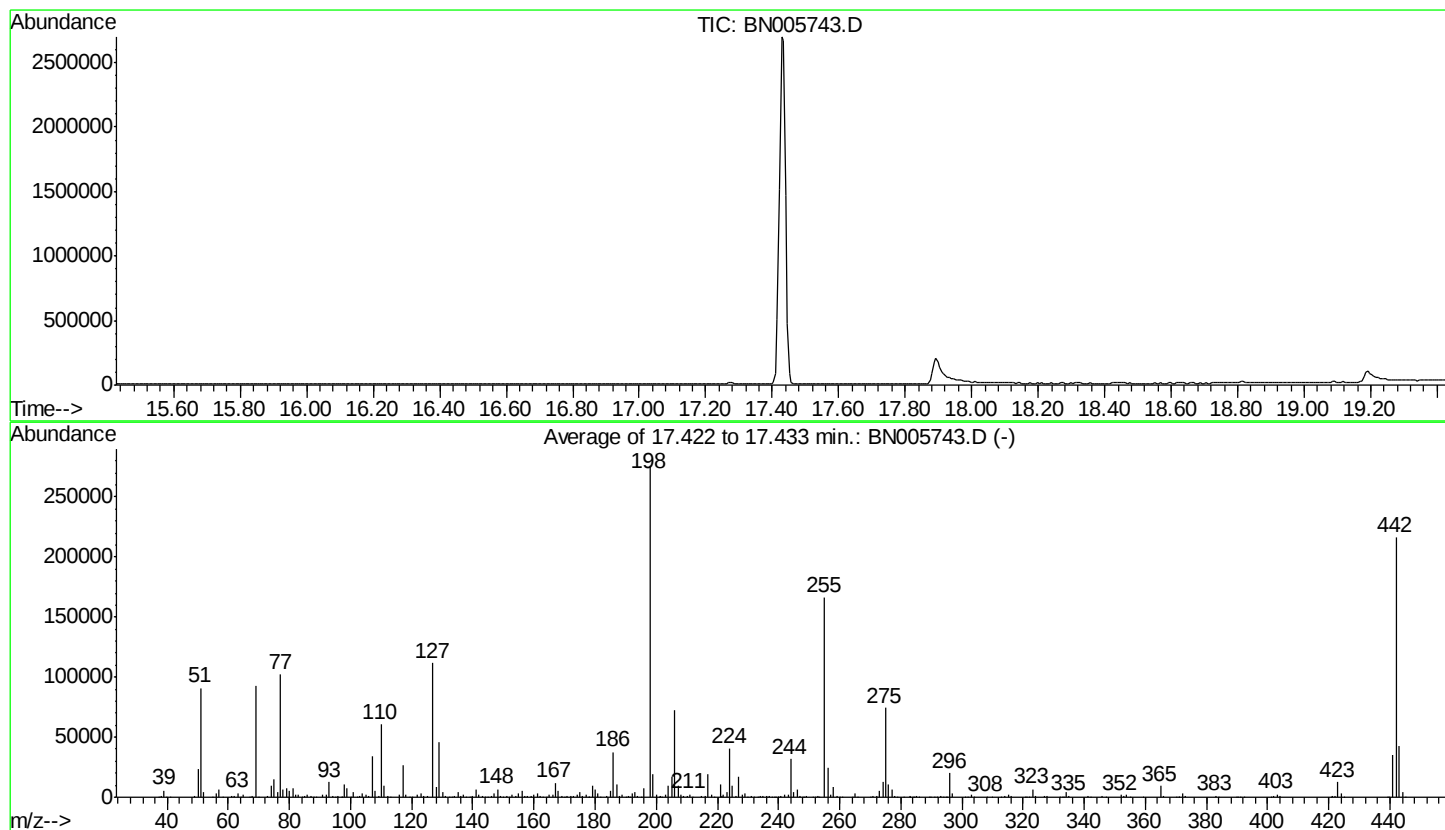

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	91114	PASS
68	69	0.00	2	1.6	1457	PASS
69	198	0.00	100	33.5	92397	PASS
70	69	0.00	2	0.6	539	PASS
127	198	10	80	40.5	111816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	276096	PASS
199	198	5	9	6.8	18783	PASS
275	198	10	60	27.0	74410	PASS
365	198	1	100	3.4	9461	PASS
441	198	0.01	100	12.8	35376	PASS
442	198	50	100	78.4	216338	PASS
443	442	15	24	19.8	42765	PASS

m/z	Abundance
40.00	1111.0
41.10	813.0
43.00	1216.0
44.00	5225.0
55.10	1221.0
55.90	343.0
57.10	1126.0
59.90	328.0
67.00	431.0
69.00	837.0
71.10	823.0
73.10	921.0
80.90	791.0
83.10	489.0
85.00	614.0
94.90	552.0
95.90	412.0
97.00	551.0
109.10	380.0
121.00	309.0
132.90	481.0
163.00	331.0
190.90	524.0
193.00	359.0
207.00	3386.0
208.00	669.0
208.90	385.0
281.10	506.0

Instrument :
BNA_N
ClientSampleId :
DFTPP72

m/z	Abundance
39.00	831.0
40.00	980.0
41.00	5472.0
42.10	1273.0
43.00	7169.0
44.00	5670.0
45.00	626.0
53.00	431.0
54.00	567.0
55.00	6021.0
56.10	1441.0
57.10	6431.0
58.00	442.0
59.00	372.0
60.00	4213.0
60.90	1271.0
67.10	1064.0
68.10	705.0
69.00	3594.0
70.10	961.0
71.10	3057.0
73.00	6422.0
73.90	540.0
78.90	326.0
81.00	1033.0
82.00	779.0
83.10	2579.0
84.00	1157.0
85.10	1963.0
86.00	431.0
87.00	1240.0
93.00	405.0
95.10	800.0
96.00	741.0
97.00	2055.0
98.00	1411.0
99.10	819.0
101.00	457.0
109.00	536.0
109.90	359.0
111.10	927.0
112.00	372.0
113.00	472.0
114.90	988.0
116.10	566.0
118.90	365.0
121.10	333.0
125.10	439.0
129.10	3068.0
130.10	386.0
133.00	551.0
135.00	323.0
137.00	320.0
143.10	582.0
157.10	443.0
171.20	610.0
185.10	1900.0
186.10	334.0
191.00	693.0
193.00	407.0
199.10	697.0
207.10	3071.0
208.00	938.0
209.00	546.0
227.10	615.0
241.20	1527.0
280.90	455.0
284.20	853.0

Instrument :
BNA_N
ClientSampleId :
DFTPP72

m/z	Abundance
39.00	1109.0
39.90	961.0
41.10	5692.0
42.00	1433.0
43.10	7692.0
44.00	5235.0
44.90	958.0
53.00	485.0
54.00	532.0
55.00	6204.0
56.00	1530.0
57.00	5892.0
58.00	489.0
59.00	421.0
60.00	5209.0
61.00	1646.0
67.00	1199.0
68.00	700.0
69.10	3634.0
70.00	846.0
71.00	3221.0
71.90	344.0
73.00	7125.0
74.00	666.0
79.00	467.0
81.00	1343.0
82.00	716.0
83.10	2440.0
84.00	1165.0
85.10	2282.0
86.90	1301.0
91.00	326.0
93.20	333.0
95.00	1054.0
96.10	652.0
97.00	2062.0
98.00	1310.0
99.10	737.0
100.90	551.0
109.00	465.0
110.00	509.0
111.00	1079.0
112.00	451.0
113.00	412.0
115.10	1179.0
116.00	412.0
125.00	427.0
127.00	382.0
129.00	3194.0
130.00	323.0
133.00	540.0
135.10	354.0
143.00	768.0
146.90	424.0
149.00	312.0
157.10	571.0
171.00	977.0
185.10	1638.0
191.10	361.0
193.00	433.0
199.10	779.0
207.00	3044.0
207.90	872.0
208.90	575.0
213.20	397.0
227.10	669.0
241.10	1588.0
242.20	431.0
255.10	361.0
281.00	530.0
284.10	1281.0
285.30	371.0

Instrument :
BNA_N
ClientSampleId :
DFTPP72

m/z	Abundance
39.00	922.0
40.00	1028.0
41.00	4311.0
42.00	1009.0
43.10	6371.0
44.00	5042.0
45.00	596.0
53.10	528.0
54.00	425.0
55.00	5399.0
56.00	1307.0
57.10	6107.0
58.00	337.0
58.90	393.0
60.00	4952.0
61.00	1609.0
66.90	858.0
67.90	592.0
69.00	2870.0
70.10	916.0
71.10	2857.0
73.00	5732.0
74.00	689.0
78.90	498.0
81.00	818.0
82.00	811.0
83.00	2164.0
84.10	970.0
85.10	2112.0
86.90	1521.0
95.00	749.0
95.90	518.0
97.00	2097.0
98.10	1300.0
99.10	651.0
101.10	485.0
109.00	507.0
110.10	311.0
111.00	662.0
112.00	518.0
115.10	840.0
116.00	388.0
121.10	329.0
125.00	437.0
129.10	2297.0
133.00	304.0
134.90	347.0
143.10	453.0
149.00	347.0
157.00	508.0
162.90	319.0
171.00	821.0
177.10	386.0
185.10	1305.0
191.10	453.0
193.00	372.0
199.00	625.0
207.00	3782.0
208.00	916.0
209.00	470.0
213.10	367.0
227.20	686.0
241.30	1693.0
242.10	355.0
255.10	394.0
280.80	722.0
284.30	1103.0
285.00	341.0

Instrument :
BNA_N
ClientSampleId :
DFTPP72