

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052019\
 Data File : BN005796.D
 Acq On : 20 May 2019 13:21
 Operator : JU/SJ
 Sample : K2693-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFHE1

Quant Time: May 21 03:33:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 03:29:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	99511	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	425418	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	294325	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	743957	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	837764	20.00	ng/ul	0.02
85) Perylene-d12	23.49	264	928063	20.00	ng/ul	0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	5475	3.08	ng/uL	0.00
5) Phenol-d5	6.76	99	98121	12.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	57889	14.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	86082	13.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	79051	12.02	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	44742	14.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	46965	13.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	86291	12.68	ng/ul	0.01
29) 4-Chloroaniline-d4	10.49	131	101955	13.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	366720	16.19	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	424651	15.43	ng/ul	0.00
51) 4-Nitrophenol-d4	14.60	143	921	0.29	ng/ul	0.14
57) Fluorene-d10	15.22	176	322107	16.56	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	26486	5.92	ng/ul	0.00
70) Anthracene-d10	17.07	188	535561	16.66	ng/ul	0.00
78) Pyrene-d10	19.39	212	674654	16.34	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	692395	16.63	ng/ul	0.04


Target Compounds					Ovalue	
44) Dimethylphthalate	13.68	163	87801	3.932	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052019\
Data File : BN005796.D
Acq On : 20 May 2019 13:21
Operator : JU/SJ
Sample : K2693-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFHE1

Quant Time: May 21 03:33:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 03:29:48 2019
Response via : Initial Calibration

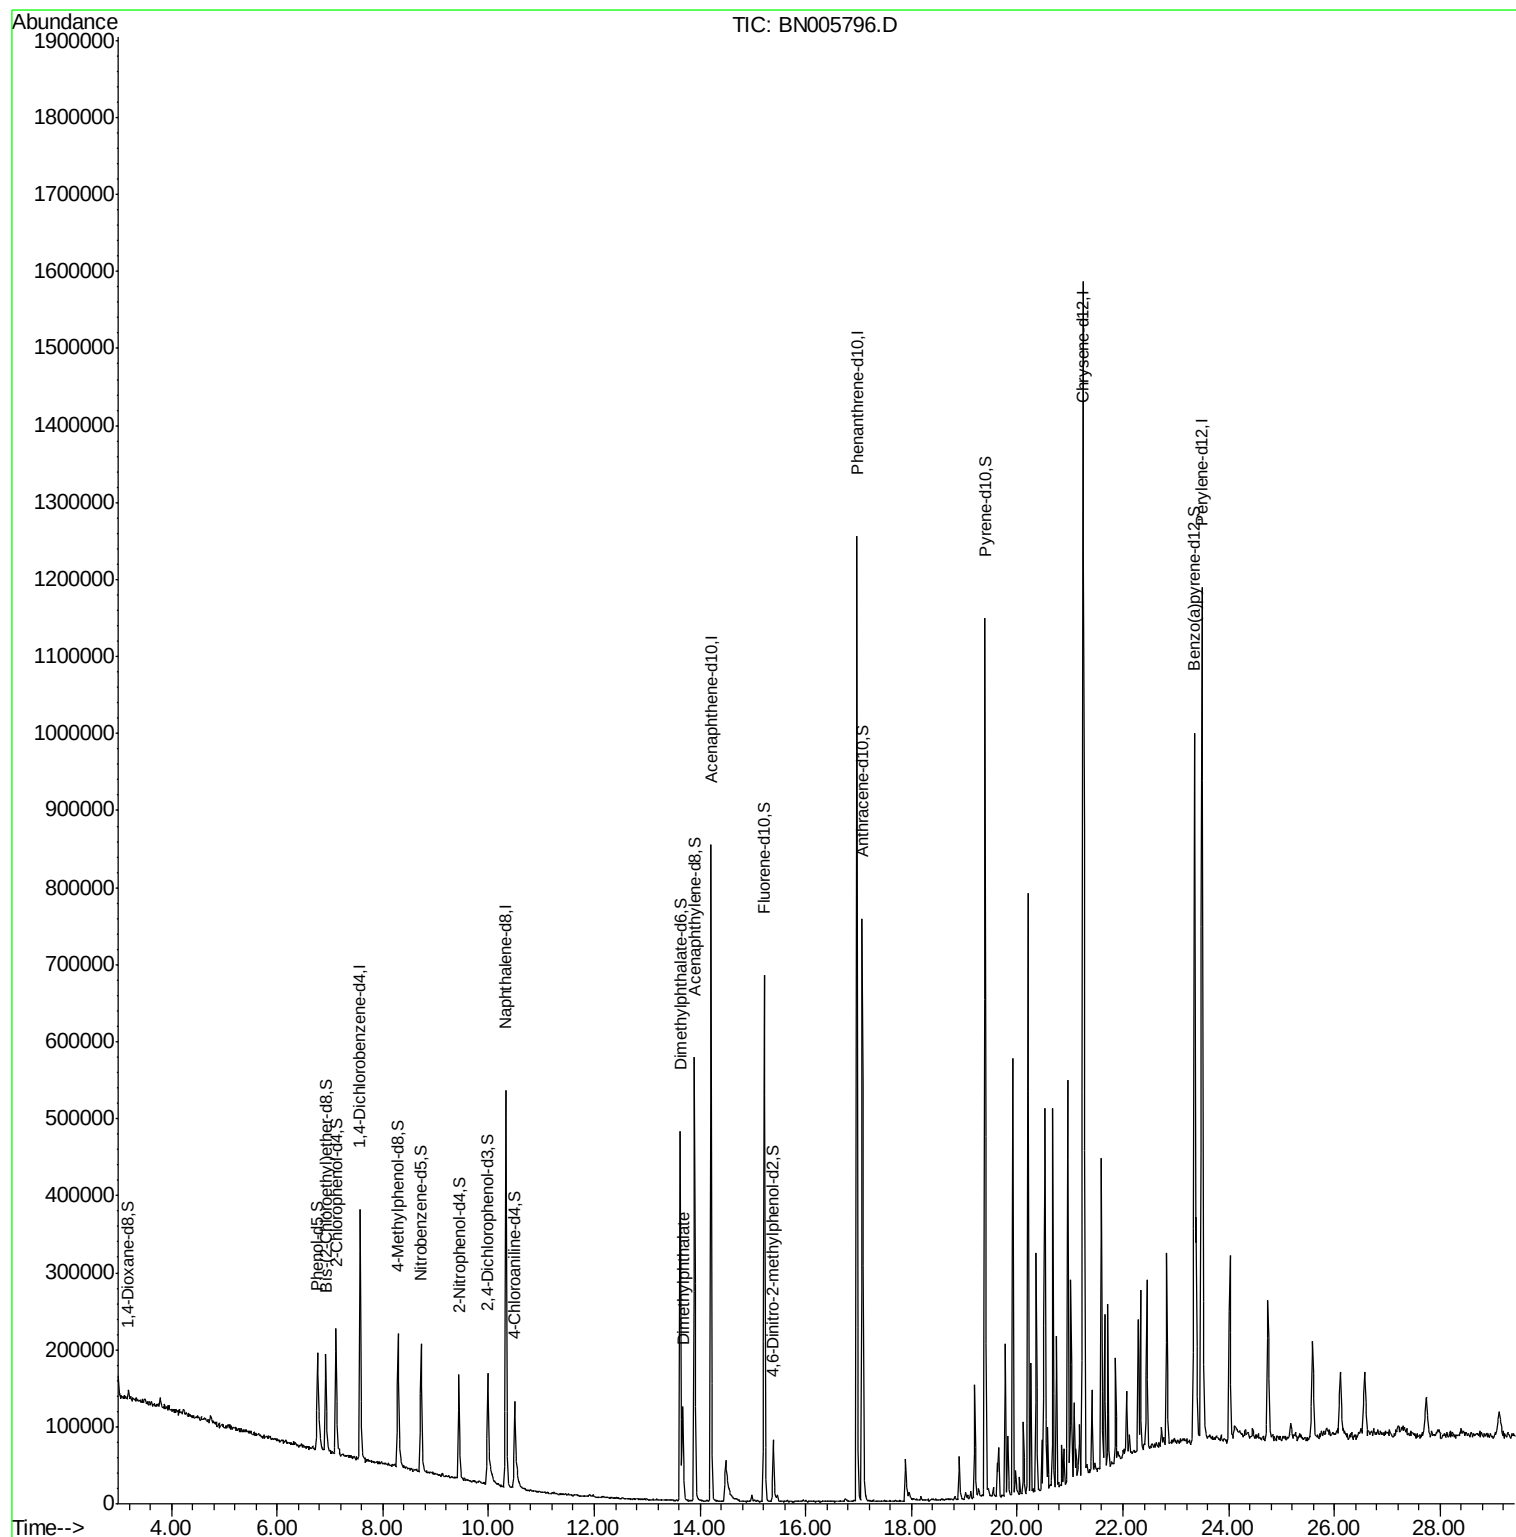

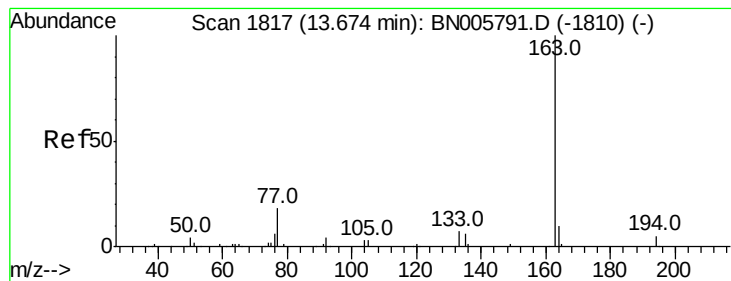

#44

Dimethylphthalate

Concen: 3.932 ng/ul

RT: 13.68 min Scan# 1817

Delta R.T. 0.00 min

Lab File: BN005796.D

Acq: 20 May 2019 13:21

Instrument :

BNA_N

ClientSampleId :

BFHE1


Tot Ion:163 Resp: 87801

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.7 8.1 12.1

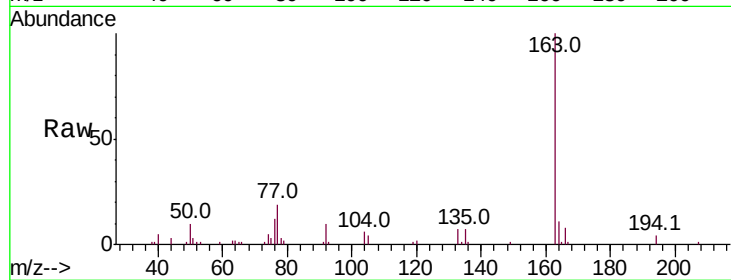

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

