

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052019\
 Data File : BN005807.D
 Acq On : 20 May 2019 19:44
 Operator : JU/SJ
 Sample : K2693-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFH63

Quant Time: May 21 04:09:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 04:05:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	91566	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	389088	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	267061	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	677519	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	583875	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	590063	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	5370	3.28	ng/uL	0.00
5) Phenol-d5	6.77	99	115223	16.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	62561	16.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	98632	17.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	84426	13.95	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	49039	17.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	52428	16.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	107016	17.19	ng/ul	0.02
29) 4-Chloroaniline-d4	10.53	131	17905	2.59	ng/ul	0.05
43) Dimethylphthalate-d6	13.62	166	363887	17.71	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	462909	18.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	31866	11.01	ng/ul	0.03
57) Fluorene-d10	15.21	176	347504	19.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	21318	5.23	ng/ul	0.01
70) Anthracene-d10	17.07	188	565507	19.32	ng/ul	0.00
78) Pyrene-d10	19.38	212	647823	22.52	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	497785	18.81	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.67	163	88470	4.367	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052019\
Data File : BN005807.D
Acq On : 20 May 2019 19:44
Operator : JU/SJ
Sample : K2693-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFH63

Quant Time: May 21 04:09:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 04:05:47 2019
Response via : Initial Calibration

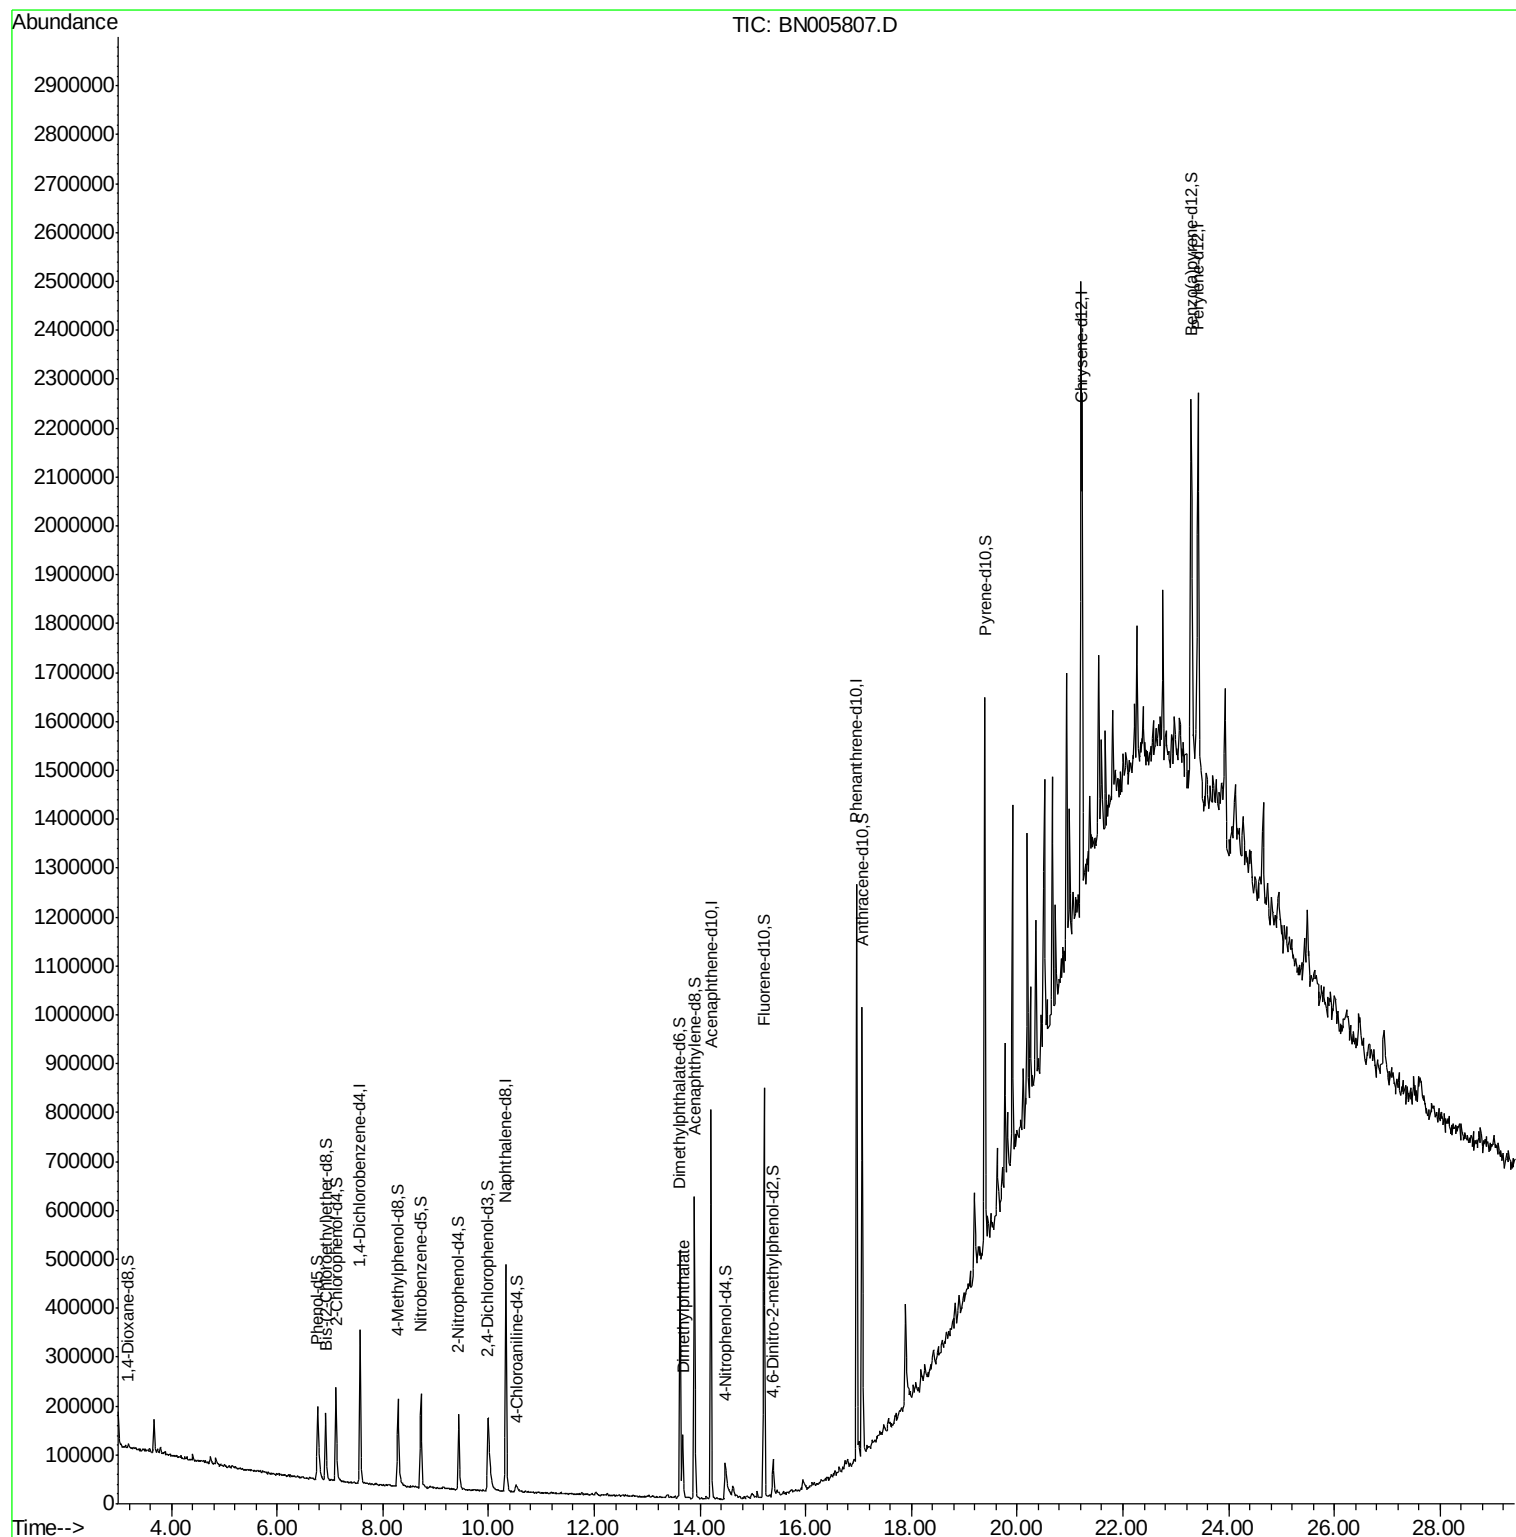

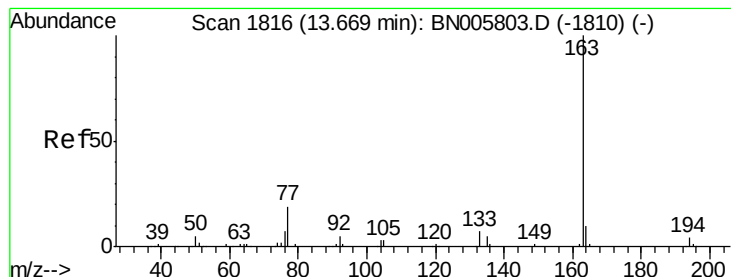

#44

Dimethylphthalate

Concen: 4.367 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. 0.01 min

Lab File: BN005807.D


Acq: 20 May 2019 19:44

Instrument :

BNA_N

ClientSampleId :

BFH63

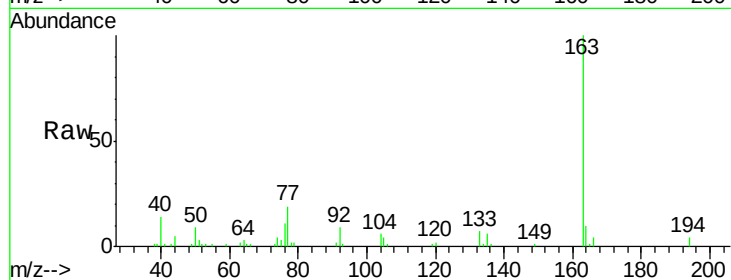


Tgt Ion:163 Resp: 88470

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.5 8.1 12.1

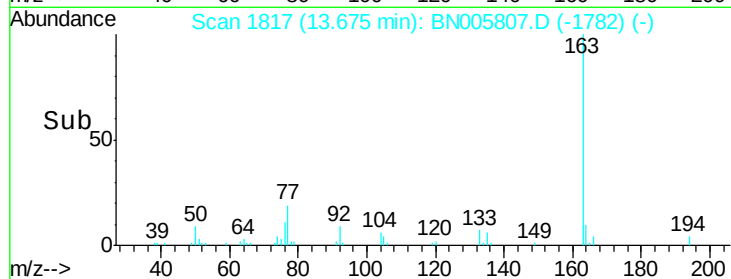

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

