

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
 Data File : BN037068.D
 Acq On : 20 May 2025 10:57
 Operator : RC/JU
 Sample : PB166510BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.023	22	23	26	rBV3	2028	1981	0.10%	0.008%
2	3.093	32	35	46	rVB	26843	39362	1.99%	0.166%
3	3.340	73	77	78	rBV4	3044	2769	0.14%	0.012%
4	3.505	101	105	122	rBV	350459	608340	30.75%	2.572%
5	3.823	155	159	164	rBV	6920	9501	0.48%	0.040%
6	3.952	178	181	186	rVB6	1405	2038	0.10%	0.009%
7	6.781	656	662	670	rBV	514422	787524	39.80%	3.329%
8	6.946	684	690	700	rVB	334809	508149	25.68%	2.148%
9	7.140	717	723	732	rBV	480172	727981	36.79%	3.077%
10	7.605	796	802	810	rBV	371067	566561	28.64%	2.395%
11	8.316	916	923	933	rBV	594835	889659	44.97%	3.761%
12	8.758	991	998	1008	rBV	463120	728703	36.83%	3.081%
13	8.887	1016	1020	1025	rBV3	5360	7841	0.40%	0.033%
14	9.481	1114	1121	1130	rBV	395858	616760	31.17%	2.607%
15	10.016	1205	1212	1224	rBV	557140	886542	44.81%	3.748%
16	10.387	1268	1275	1284	rVB	486060	785498	39.70%	3.321%
17	10.528	1293	1299	1313	rVV	531090	883256	44.64%	3.734%
18	11.599	1475	1481	1485	rVB4	1049	2086	0.11%	0.009%
19	11.993	1544	1548	1555	rVB6	5807	9034	0.46%	0.038%
20	13.675	1828	1834	1842	rBV	952967	1238838	62.62%	5.237%
21	13.951	1874	1881	1890	rBV	1006280	1380371	69.77%	5.835%
22	14.263	1927	1934	1940	rBV	730800	1057676	53.46%	4.471%
23	14.463	1962	1968	1985	rBV	522205	730120	36.90%	3.086%
24	15.257	2097	2103	2115	rVB	1214954	1656086	83.70%	7.001%
25	15.381	2118	2124	2133	rVV	499253	624164	31.55%	2.639%
26	15.493	2140	2143	2148	rVB5	4186	5623	0.28%	0.024%
27	16.793	2362	2364	2368	rVB2	2700	3724	0.19%	0.016%
28	17.010	2394	2401	2408	rBV2	909981	1208455	61.08%	5.109%
29	17.110	2411	2418	2429	rVB	1322242	1828415	92.42%	7.729%
30	17.651	2506	2510	2513	rBV4	1354	2805	0.14%	0.012%
31	17.687	2513	2516	2519	rVB2	2514	3090	0.16%	0.013%
32	17.916	2550	2555	2560	rBV5	5859	8158	0.41%	0.034%
33	18.969	2730	2734	2740	rVB3	12893	16338	0.83%	0.069%
34	19.045	2742	2747	2753	rVB2	10601	15086	0.76%	0.064%
35	19.204	2771	2774	2777	rBV4	4588	5557	0.28%	0.023%
36	19.269	2781	2785	2789	rBV	9121	12006	0.61%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037068.D
Acq On : 20 May 2025 10:57
Operator : RC/JU
Sample : PB166510BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK510

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Title : SVOA CALIBRATION

37	19.404	2803	2808	2815	rVV	1511598	1978481	100.00%	8.364%
38	21.239	3114	3120	3126	rBV	867930	1180175	59.65%	4.989%
39	23.922	3567	3576	3587	rBV	664746	1542954	77.99%	6.523%
40	24.116	3601	3609	3623	rVB2	451564	1093606	55.28%	4.623%




Sum of corrected areas: 23655313

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037068.D
Acq On : 20 May 2025 10:57
Operator : RC/JU
Sample : PB166510BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

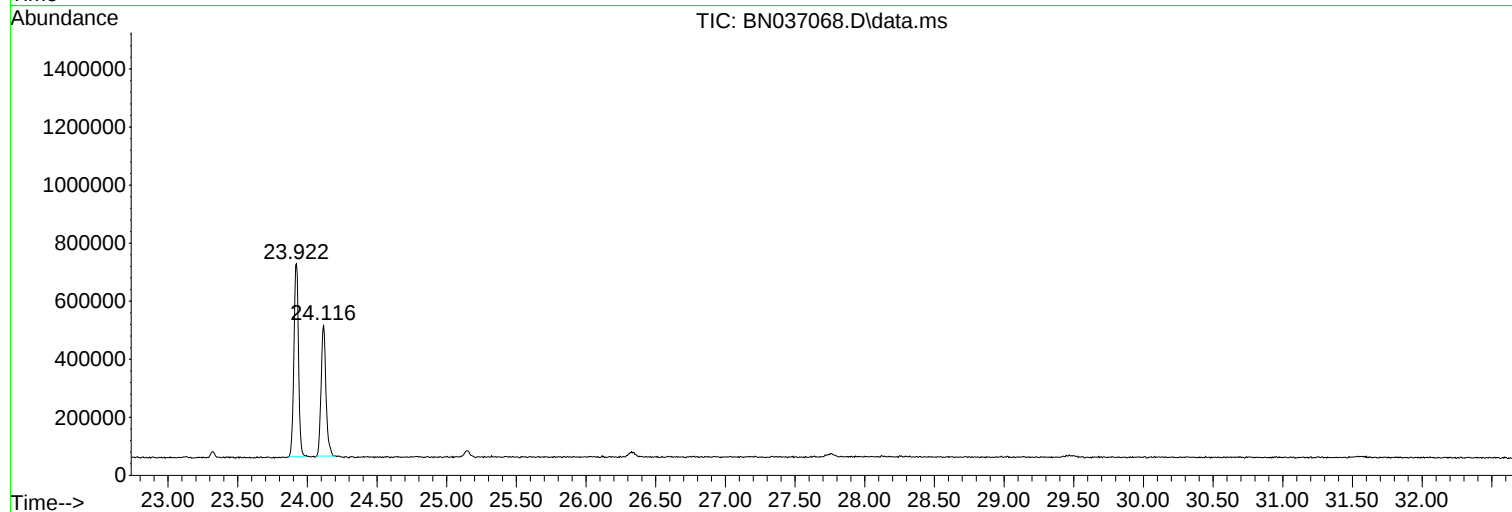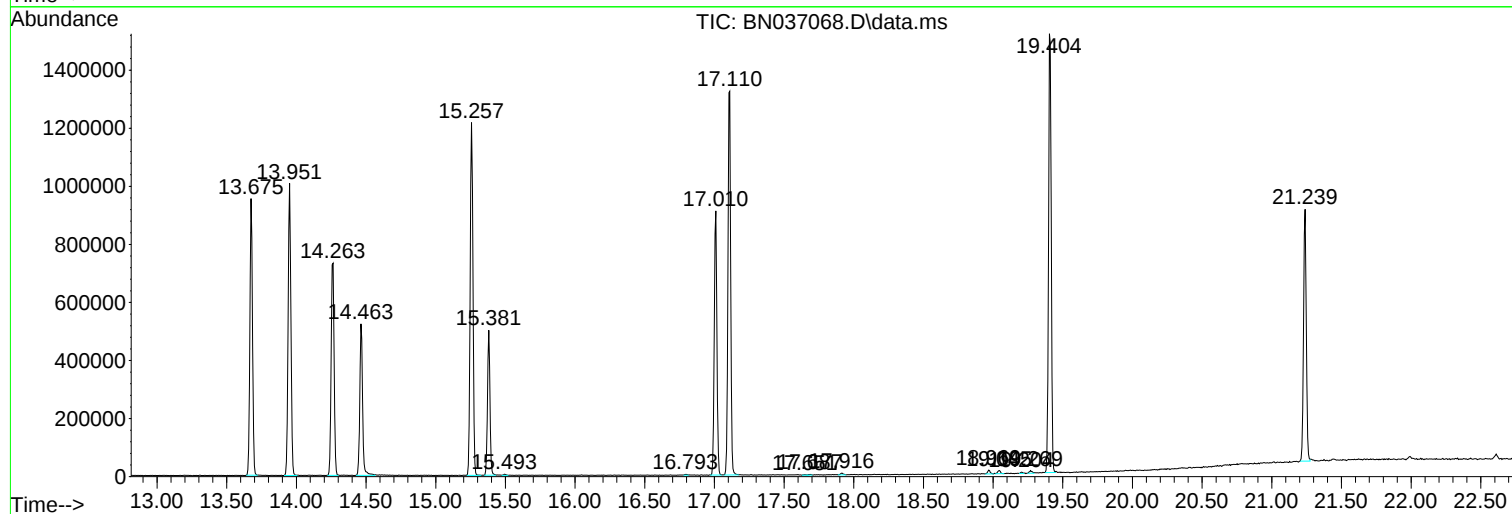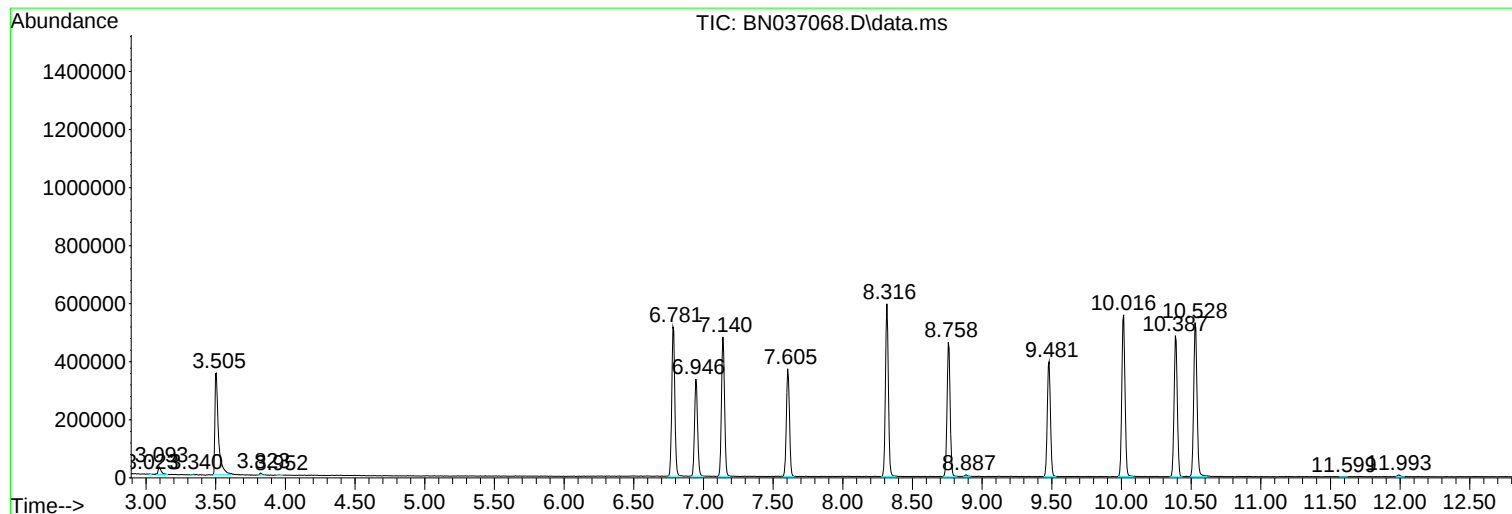

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037068.D
Acq On : 20 May 2025 10:57
Operator : RC/JU
Sample : PB166510BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037068.D
Acq On : 20 May 2025 10:57
Operator : RC/JU
Sample : PB166510BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc