

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
 Data File : BN037070.D
 Acq On : 20 May 2025 12:16
 Operator : RC/JU
 Sample : Q1994-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	42	44	47	rBV4	1366	1588	0.15%	0.030%
2	3.258	61	63	66	rVB4	1688	1965	0.18%	0.037%
3	3.334	75	76	78	rBV2	1529	1127	0.11%	0.021%
4	3.446	93	95	98	rVB3	2107	1334	0.12%	0.025%
5	3.828	156	160	164	rBV4	5047	5654	0.53%	0.107%
6	4.334	244	246	250	rBV5	1033	1702	0.16%	0.032%
7	5.575	455	457	460	rVB3	1110	1073	0.10%	0.020%
8	5.705	476	479	481	rBV4	952	1415	0.13%	0.027%
9	5.975	523	525	528	rVV4	1234	1342	0.13%	0.025%
10	6.028	532	534	538	rVV3	886	1150	0.11%	0.022%
11	6.105	544	547	550	rVB3	1267	1787	0.17%	0.034%
12	6.134	550	552	556	rBV4	1361	1823	0.17%	0.034%
13	6.175	556	559	561	rVV4	1266	1779	0.17%	0.034%
14	6.234	565	569	572	rBV4	1121	1380	0.13%	0.026%
15	6.522	614	618	619	rBV3	1159	1272	0.12%	0.024%
16	6.552	621	623	624	rBV2	1547	1281	0.12%	0.024%
17	7.011	696	701	702	rVB5	970	1340	0.12%	0.025%
18	7.169	724	728	729	rBV2	960	1207	0.11%	0.023%
19	7.275	744	746	749	rVB4	1318	1332	0.12%	0.025%
20	7.310	749	752	755	rVB4	1529	1933	0.18%	0.036%
21	7.334	755	756	760	rBV4	1263	1543	0.14%	0.029%
22	7.516	786	787	790	rVB3	1336	1215	0.11%	0.023%
23	7.605	796	802	810	rBV	323296	515656	48.06%	9.721%
24	7.793	831	834	839	rBV4	941	1139	0.11%	0.021%
25	8.205	902	904	909	rBV3	637	1212	0.11%	0.023%
26	8.381	929	934	936	rVB4	911	1162	0.11%	0.022%
27	8.481	948	951	953	rBV5	1091	1306	0.12%	0.025%
28	8.663	980	982	985	rBV3	1482	1106	0.10%	0.021%
29	8.852	1012	1014	1016	rVB2	1616	1083	0.10%	0.020%
30	8.940	1027	1029	1034	rBV4	858	1417	0.13%	0.027%
31	9.034	1042	1045	1047	rVB4	1103	1255	0.12%	0.024%
32	9.134	1059	1062	1065	rBV3	1102	1530	0.14%	0.029%
33	9.469	1116	1119	1122	rVB2	1212	1216	0.11%	0.023%
34	9.687	1153	1156	1158	rVB2	1458	1325	0.12%	0.025%
35	10.152	1234	1235	1240	rBV2	1043	1402	0.13%	0.026%
36	10.393	1268	1276	1286	rBV	427423	695843	64.86%	13.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
 Data File : BN037070.D
 Acq On : 20 May 2025 12:16
 Operator : RC/JU
 Sample : Q1994-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
 Title : SVOA CALIBRATION

37	10.557	1302	1304	1308	rVV2	797	1253	0.12%	0.024%
38	10.857	1354	1355	1358	rBV2	1227	1121	0.10%	0.021%
39	11.140	1401	1403	1406	rBV3	810	1099	0.10%	0.021%
40	11.175	1406	1409	1412	rVB4	906	1086	0.10%	0.020%
41	11.222	1414	1417	1420	rVV3	940	1164	0.11%	0.022%
42	11.263	1420	1424	1428	rVB4	766	1360	0.13%	0.026%
43	12.410	1616	1619	1620	rVB2	1346	1163	0.11%	0.022%
44	12.828	1689	1690	1695	rVB4	944	1205	0.11%	0.023%
45	13.116	1737	1739	1742	rVB2	1096	1229	0.11%	0.023%
46	13.175	1747	1749	1754	rVB2	1641	1973	0.18%	0.037%
47	13.704	1837	1839	1844	rVB2	948	1373	0.13%	0.026%
48	13.787	1850	1853	1854	rVB2	1495	1478	0.14%	0.028%
49	13.816	1854	1858	1862	rBV4	1055	2260	0.21%	0.043%
50	13.857	1862	1865	1868	rVV3	1136	1111	0.10%	0.021%
51	14.040	1893	1896	1898	rBV3	920	1112	0.10%	0.021%
52	14.128	1909	1911	1914	rVB2	1177	1185	0.11%	0.022%
53	14.257	1927	1933	1944	rVB	648296	932041	86.87%	17.570%
54	14.675	2001	2004	2008	rBV4	1070	1444	0.13%	0.027%
55	15.022	2060	2063	2066	rVB4	1123	1555	0.14%	0.029%
56	15.445	2134	2135	2138	rBV3	1334	1073	0.10%	0.020%
57	15.969	2221	2224	2227	rVB4	1202	1683	0.16%	0.032%
58	16.010	2227	2231	2235	rBV4	1314	2634	0.25%	0.050%
59	16.286	2275	2278	2279	rBV2	1026	1324	0.12%	0.025%
60	16.392	2292	2296	2298	rBV3	1230	1481	0.14%	0.028%
61	16.804	2359	2366	2370	rBV5	2065	4081	0.38%	0.077%
62	17.010	2393	2401	2414	rBV	780286	1072869	100.00%	20.225%
63	17.110	2414	2418	2422	rBV5	2000	3719	0.35%	0.070%
64	17.486	2478	2482	2484	rBV4	1333	1492	0.14%	0.028%
65	17.522	2486	2488	2492	rVB5	909	1102	0.10%	0.021%
66	17.598	2499	2501	2502	rBV2	1141	1084	0.10%	0.020%
67	17.663	2510	2512	2514	rVV2	1119	1354	0.13%	0.026%
68	17.710	2516	2520	2521	rVV4	1502	1568	0.15%	0.030%
69	17.798	2531	2535	2537	rBV4	1339	1335	0.12%	0.025%
70	17.986	2566	2567	2570	rBV3	1578	1448	0.13%	0.027%
71	18.116	2585	2589	2590	rBV3	1697	1788	0.17%	0.034%
72	18.398	2634	2637	2639	rBV3	1438	1286	0.12%	0.024%
73	18.451	2642	2646	2649	rVB4	911	1388	0.13%	0.026%
74	18.622	2673	2675	2678	rVB4	1426	1643	0.15%	0.031%
75	18.651	2678	2680	2681	rBV2	2235	1639	0.15%	0.031%
76	18.733	2692	2694	2697	rVB3	1359	1124	0.10%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037070.D
Acq On : 20 May 2025 12:16
Operator : RC/JU
Sample : Q1994-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Title : SVOA CALIBRATION

77	19.251	2778	2782	2785	rBV6	1793	2143	0.20%	0.040%
78	19.363	2797	2801	2802	rBV2	1681	1409	0.13%	0.027%
79	19.410	2807	2809	2811	rVB3	1799	1138	0.11%	0.021%
80	19.627	2842	2846	2847	rBV4	2144	2792	0.26%	0.053%
81	19.704	2857	2859	2860	rBV2	1816	1627	0.15%	0.031%
82	21.239	3114	3120	3132	rBV	720490	1032500	96.24%	19.464%
83	24.115	3600	3609	3621	rBV2	375658	936773	87.31%	17.660%




Sum of corrected areas: 5304603

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037070.D
Acq On : 20 May 2025 12:16
Operator : RC/JU
Sample : Q1994-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

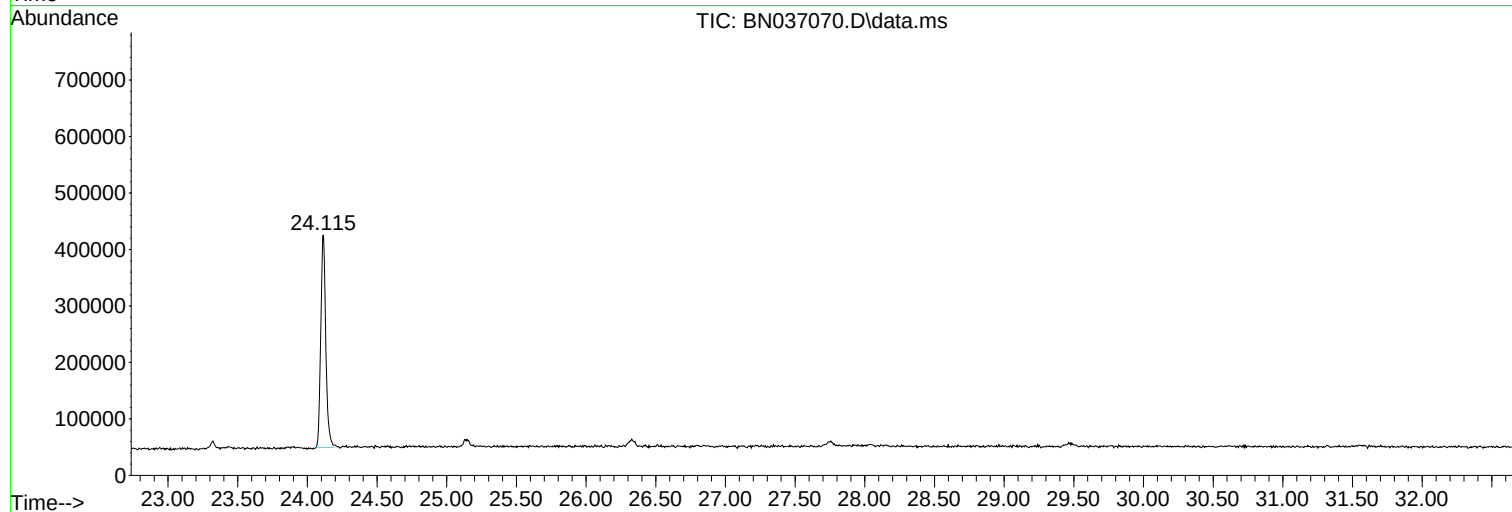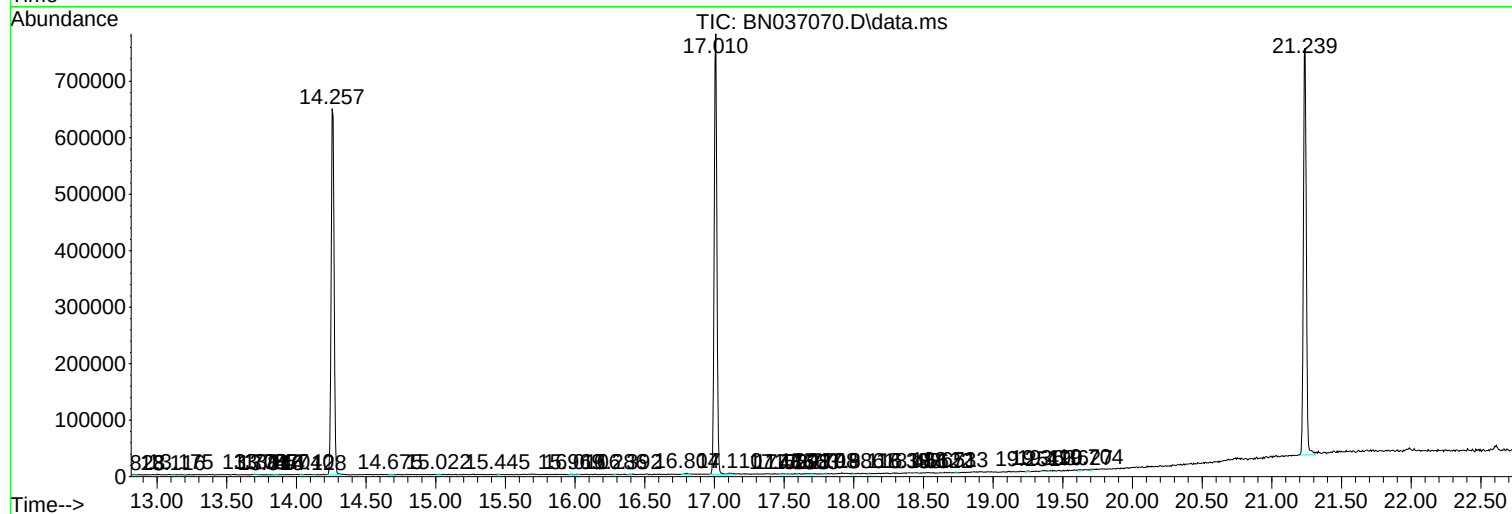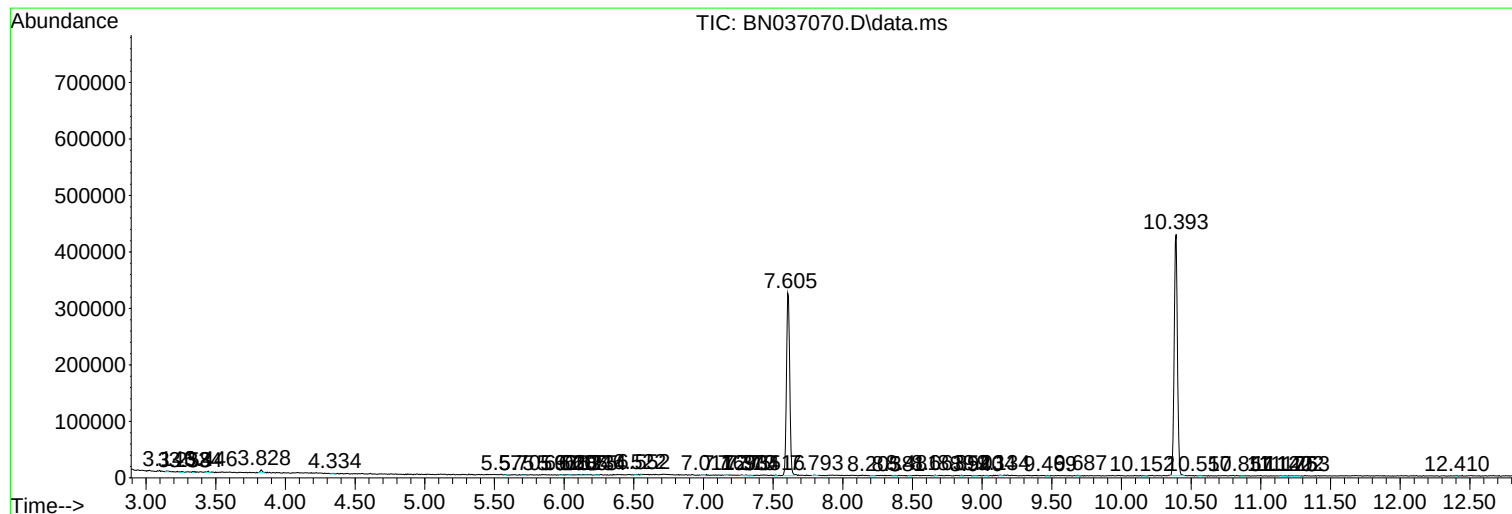

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037070.D
Acq On : 20 May 2025 12:16
Operator : RC/JU
Sample : Q1994-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052025\
Data File : BN037070.D
Acq On : 20 May 2025 12:16
Operator : RC/JU
Sample : Q1994-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051625.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------