


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052119\
Data File : BN005842.D
Acq On : 22 May 2019 02:31
Operator : JU/SJ
Sample : K2862-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: May 22 04:26:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 22 04:04:33 2019
Response via : Initial Calibration

Instrument :
BNA_N
Client Sample ID :
BFHJ9

Manual Integrations
APPROVED

mohammad
5/23/2019 4:02:54 AM

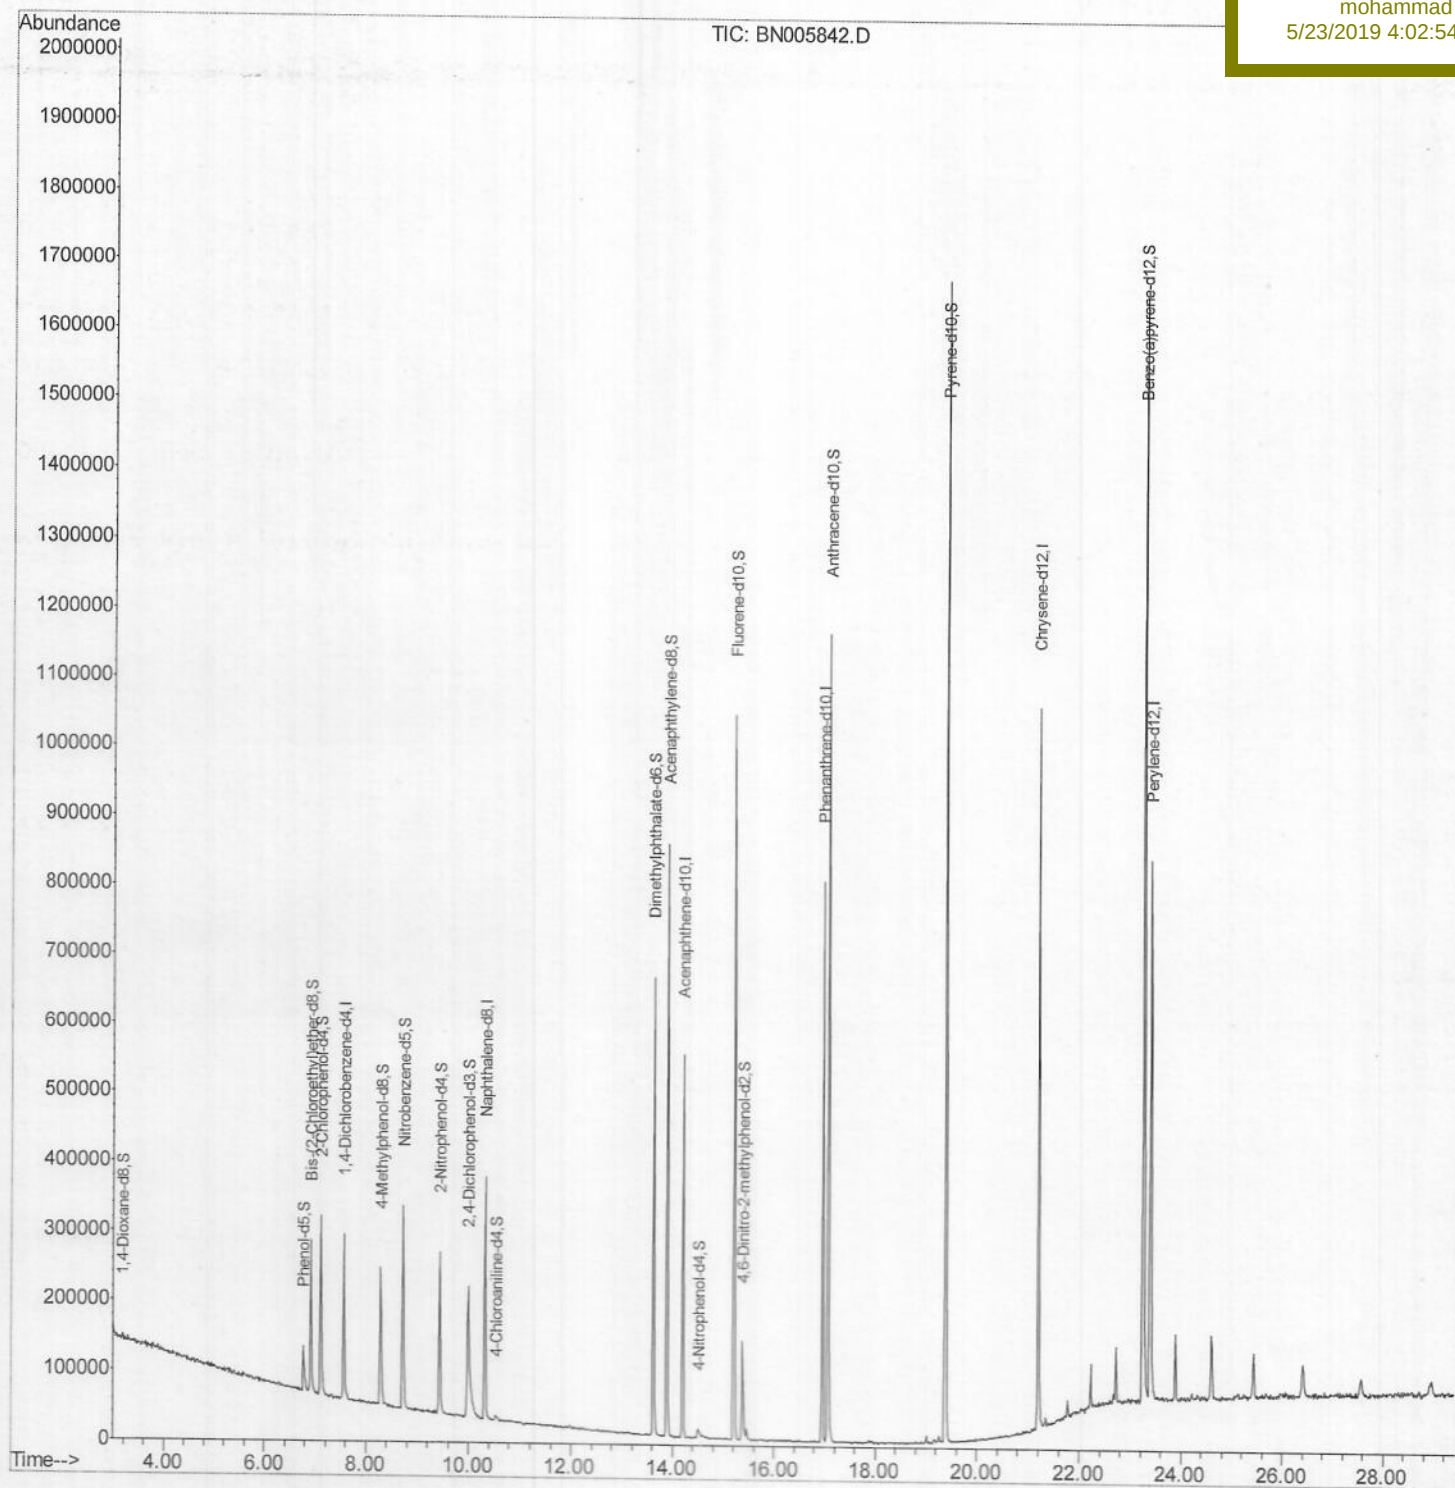

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052119\

Data File : BN005842.D

Acq On : 22 May 2019 02:31

Operator : JU/SJ

Sample : K2862-01

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: May 22 04:09:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed May 22 04:04:33 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

BFHJ9

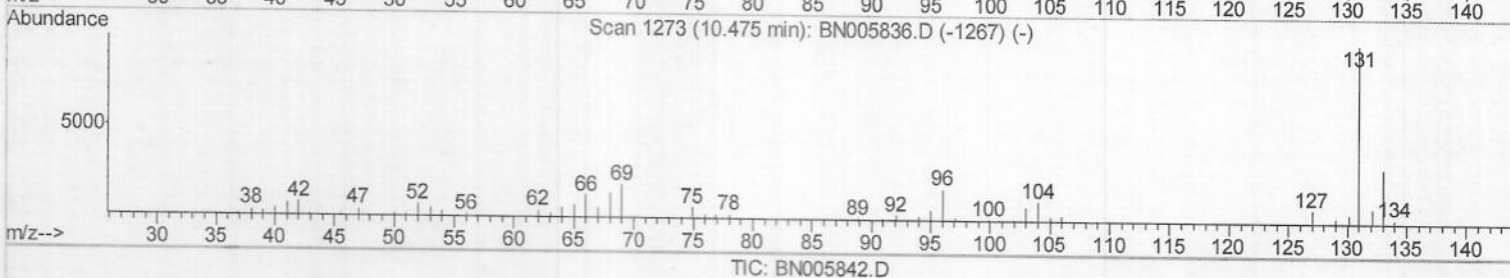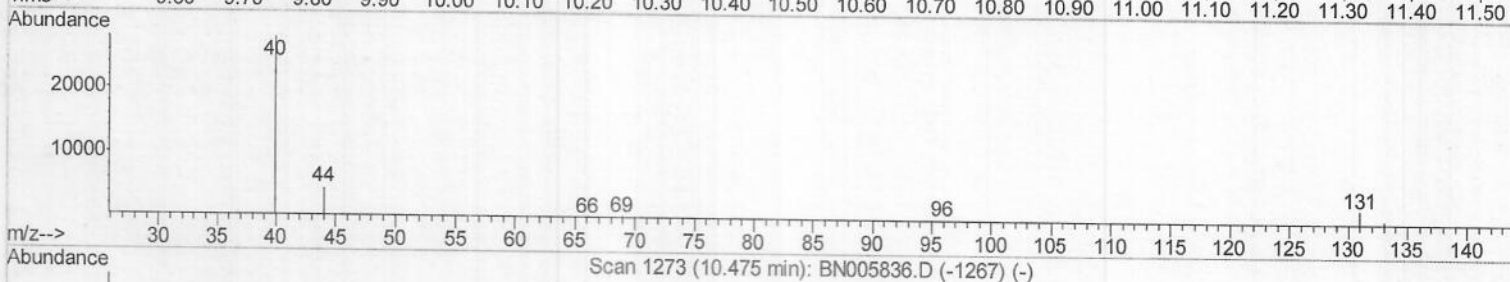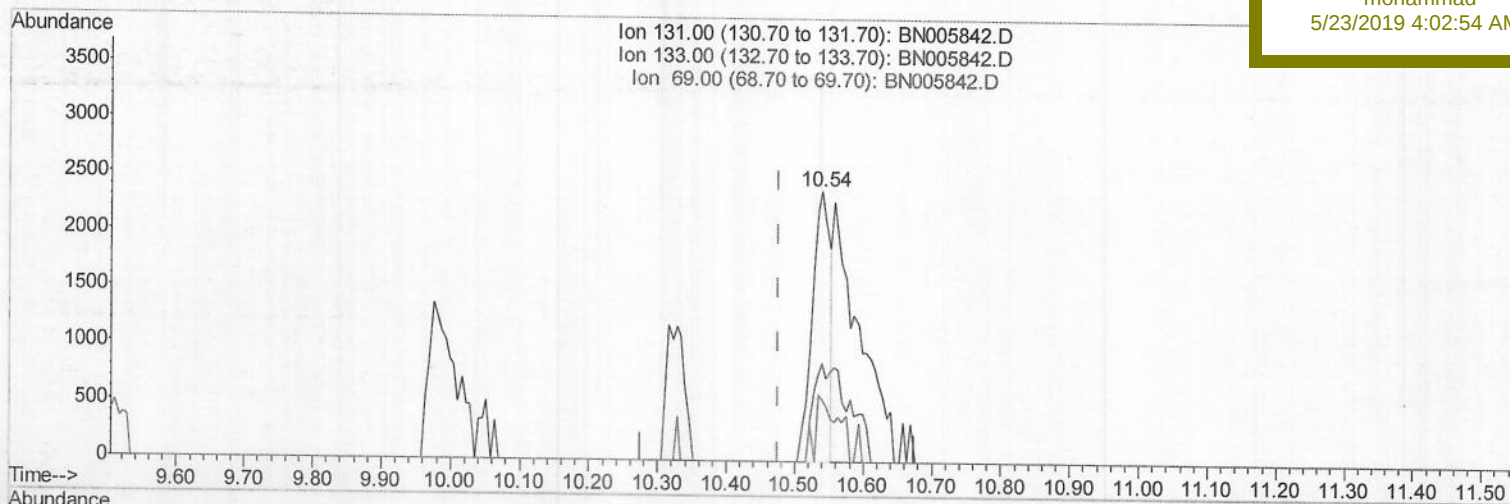Manual Integrations
APPROVEDmohammad
5/23/2019 4:02:54 AM

(29) 4-Chloroaniline-d4 (S)

10.540min (+0.065) 0.83ng/ul

response 4264

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	35.87
69.00	18.90	22.53
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052119\

Data File : BN005842.D

Acq On : 22 May 2019 02:31

Operator : JU/SJ

Sample : K2862-01

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: May 22 04:09:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed May 22 04:04:33 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




BFHJ9

Manual Integrations

APPROVED

mohammad

5/23/2019 4:02:54 AM

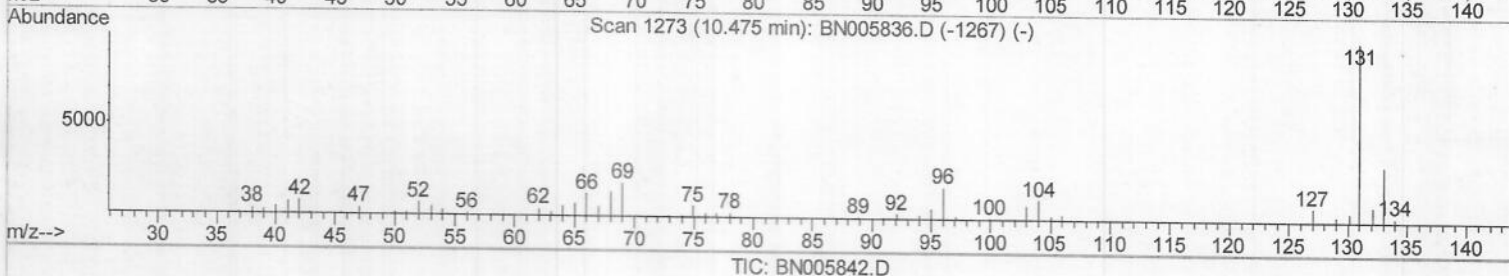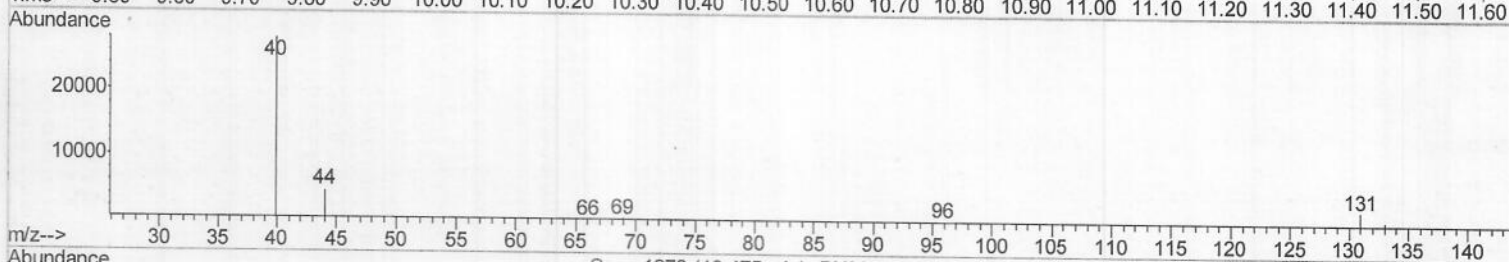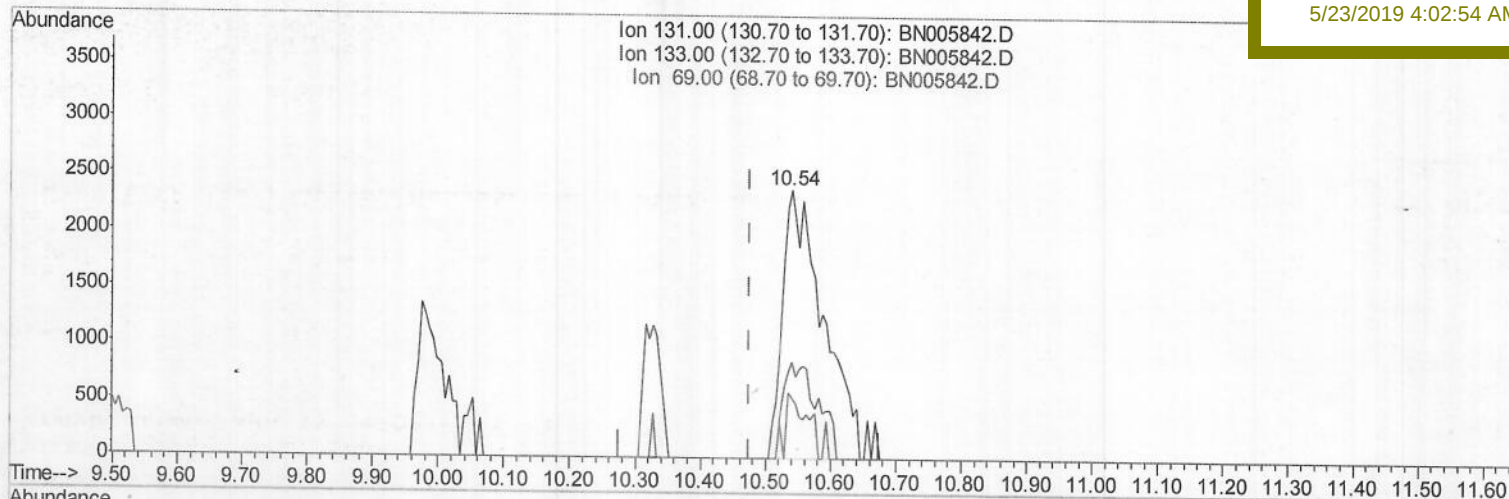

(29) 4-Chloroaniline-d4 (S)

10.540min (+0.065) 1.98ng/ul m

response 10242

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	35.87
69.00	18.90	22.53
0.00	0.00	0.00

JU
05/28/19

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052119\
Data File : BN005842.D
Acq On : 22 May 2019 02:31
Operator : JU/SJ
Sample : K2862-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: May 22 04:09:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 22 04:04:33 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
BFHJ9

Manual Integrations
APPROVED

mohammad
5/23/2019 4:02:54 AM

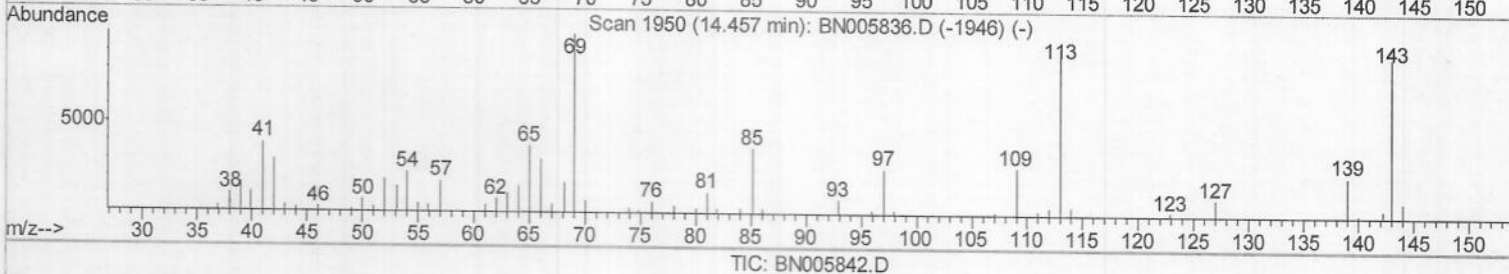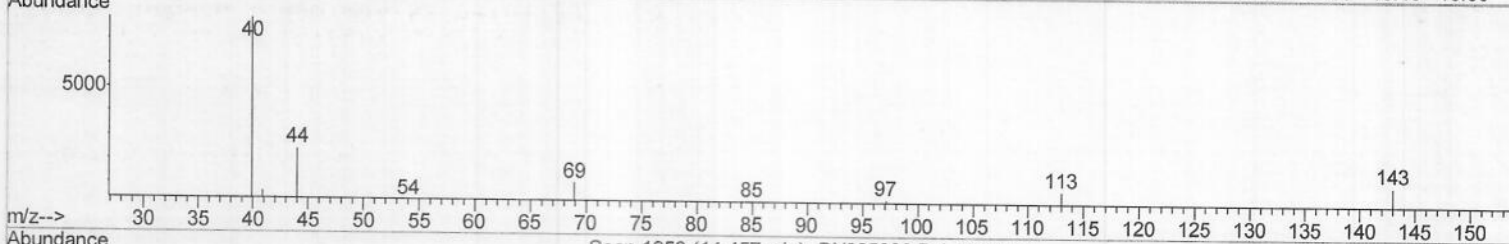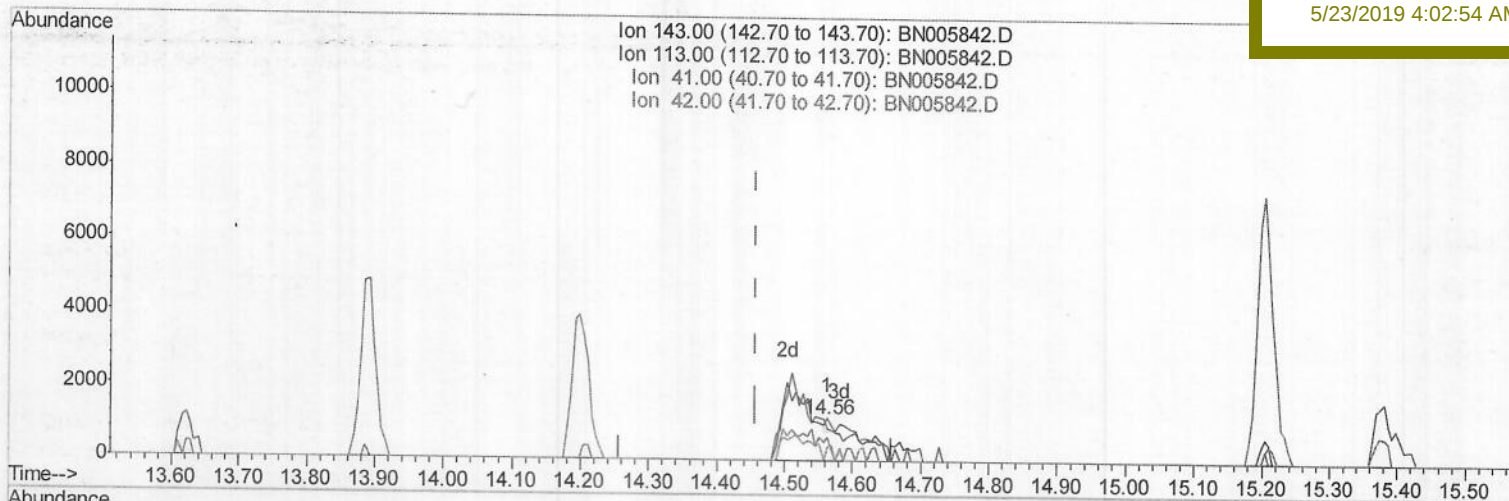

TIC: BN005842.D

(51) 4-Nitrophenol-d4 (S)

14.563min (+0.106) 0.09ng/ul

response 186

Ion	Exp%	Act%
143.00	100	100
113.00	82.50	73.91
41.00	47.90	53.22
42.00	31.70	30.82

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052119\

Data File : BN005842.D

Acq On : 22 May 2019 02:31

Operator : JU/SJ

Sample : K2862-01

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: May 22 04:09:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed May 22 04:04:33 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

BFHJ9

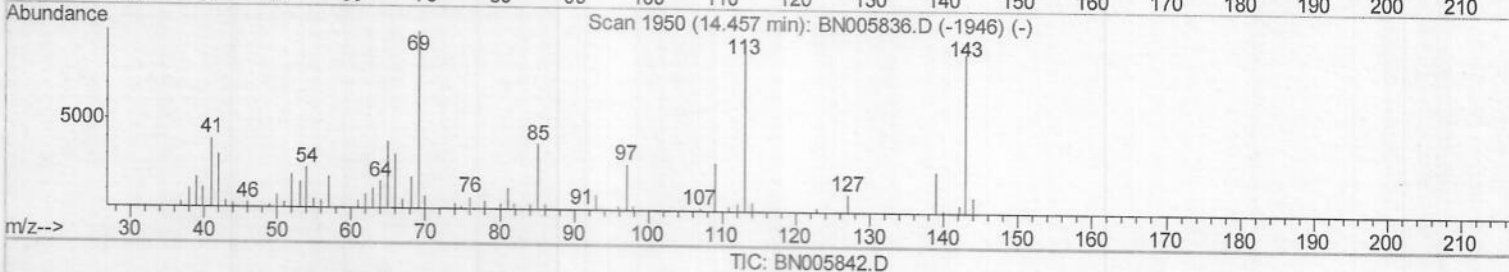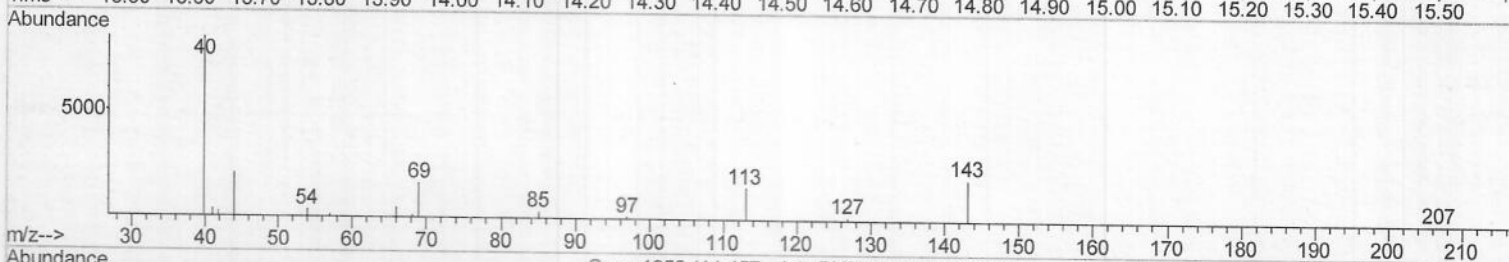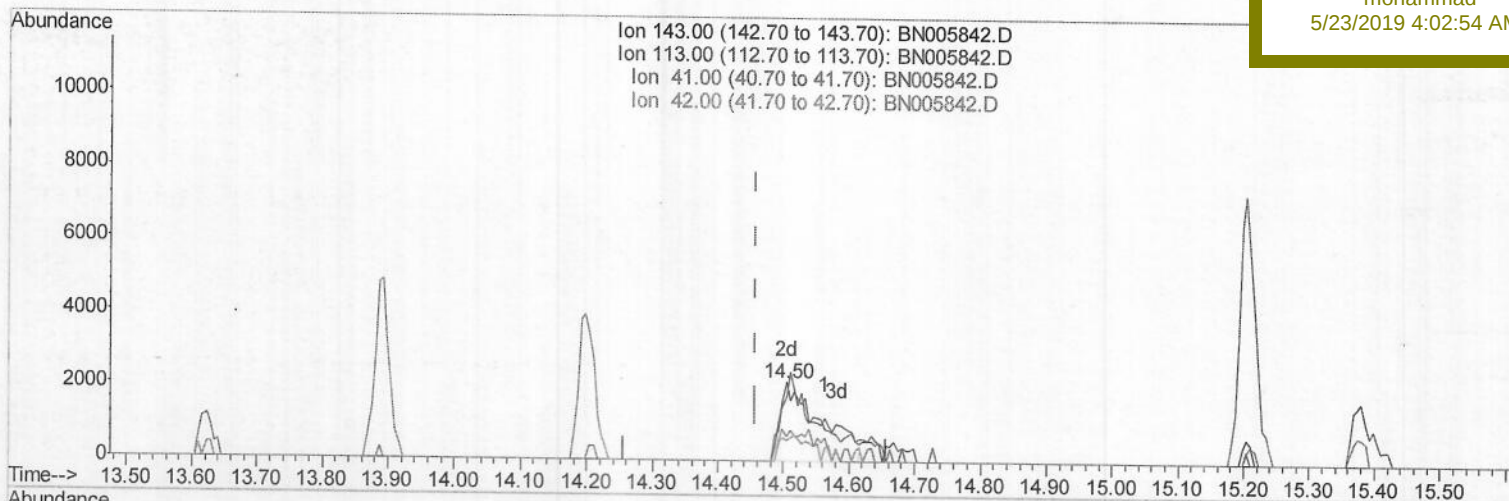Manual Integrations
APPROVEDmohammad
5/23/2019 4:02:54 AM

(51) 4-Nitrophenol-d4 (S)

14.504min (+0.047) 4.53ng/ul m

response 9222

Ion	Exp%	Act%
143.00	100	100
113.00	82.50	81.42
41.00	47.90	30.93#
42.00	31.70	25.88

JU
05/28/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052119\
 Data File : BN005842.D
 Acq On : 22 May 2019 02:31
 Operator : JU/SJ
 Sample : K2862-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 BFHJ9

Quant Time: May 22 04:26:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 22 04:04:33 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 5/23/2019 4:02:54 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	73302	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	290518	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	187820	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	487289	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	582921	20.00	ng/ul	0.00
85) Perylene-d12	23.39	264	684764	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	3431	2.62	ng/uL	0.00
5) Phenol-d5	6.77	99	52049	9.19	ng/ul	0.01
7) Bis-(2-Chloroethyl) ether-d	6.91	67	98870	33.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	132651	29.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	88795	18.33	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	72815	34.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	76019	31.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	145212	31.24	ng/ul	0.01
29) 4-Chloroaniline-d4	10.54	131	10242m	1.98	ng/ul	0.06
43) Dimethylphthalate-d6	13.62	166	523330	36.21	ng/ul	0.00
46) Acenaphthylene-d8	13.89	160	641643	36.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	9222m	4.53	ng/ul	0.05
57) Fluorene-d10	15.20	176	471178	37.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	43571	14.88	ng/ul	0.00
70) Anthracene-d10	17.06	188	773971	36.77	ng/ul	0.00
78) Pyrene-d10	19.37	212	991129	34.51	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.25	264	1163564	37.88	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} JU
 05/28/19