

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052119\
 Data File : BN005832.D
 Acq On : 21 May 2019 19:34
 Operator : JU/SJ
 Sample : K2693-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFHF0

Quant Time: May 22 03:46:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 04:05:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	59423	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	240909	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	156647	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	389629	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	442109	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	535441	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	8388	7.90	ng/uL	-0.01
5) Phenol-d5	6.76	99	156012	33.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	87921	36.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	137808	37.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	131450	33.47	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	67703	38.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	76371	37.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	137331	35.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	166787	38.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.62	166	489814	40.64	ng/ul	0.00
46) Acenaphthylene-d8	13.89	160	603837	41.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	48639	28.65	ng/ul	0.02
57) Fluorene-d10	15.20	176	433815	41.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	49312	21.06	ng/ul	0.00
70) Anthracene-d10	17.06	188	698248	41.48	ng/ul	0.00
78) Pyrene-d10	19.38	212	850120	39.02	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	1015615	42.28	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.79	94	9355	1.998	ng/ul# 76
44) Dimethylphthalate	13.67	163	99367	8.362	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN052119\
 Data File : BN005832.D
 Acq On : 21 May 2019 19:34
 Operator : JU/SJ
 Sample : K2693-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFHF0

Quant Time: May 22 03:46:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 04:05:47 2019
 Response via : Initial Calibration




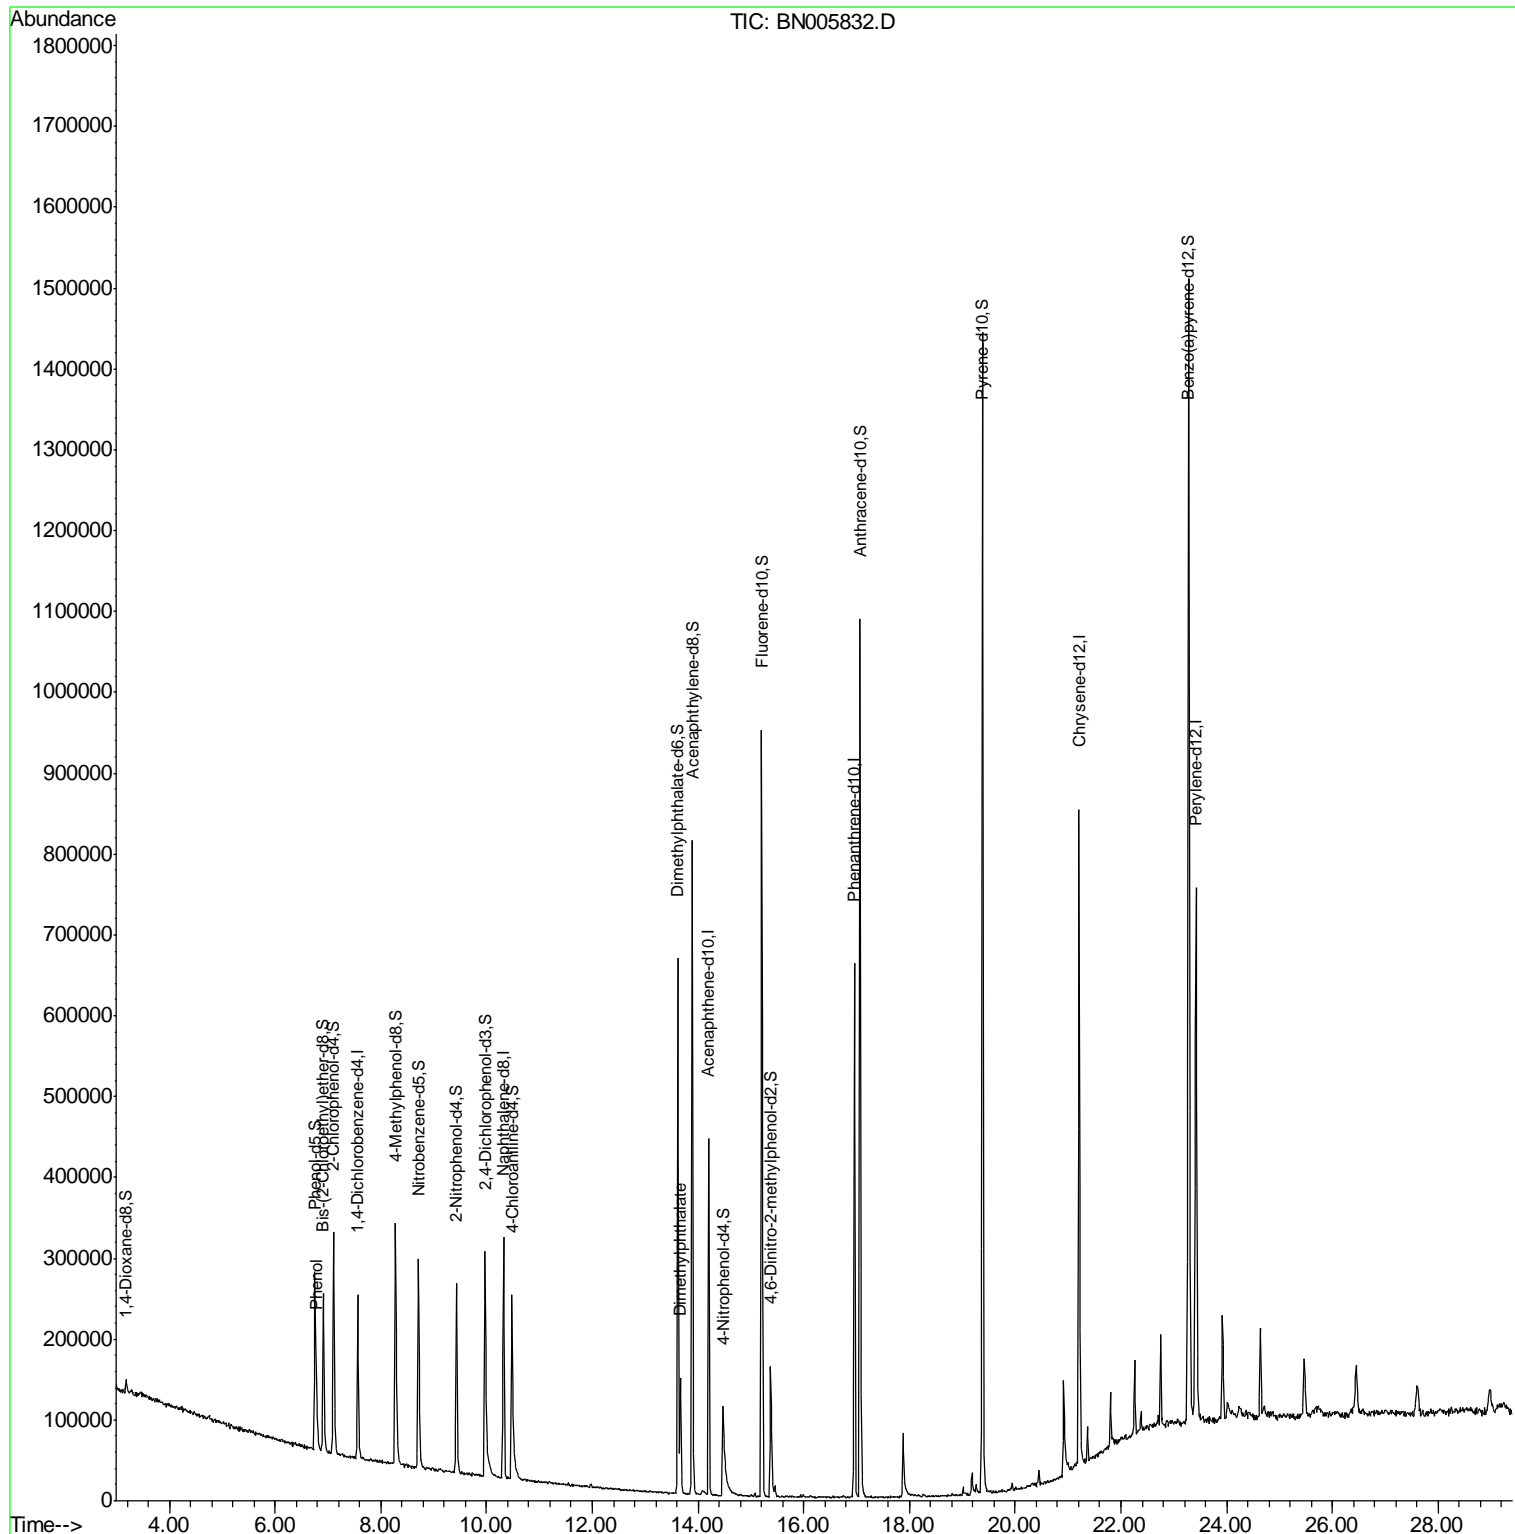


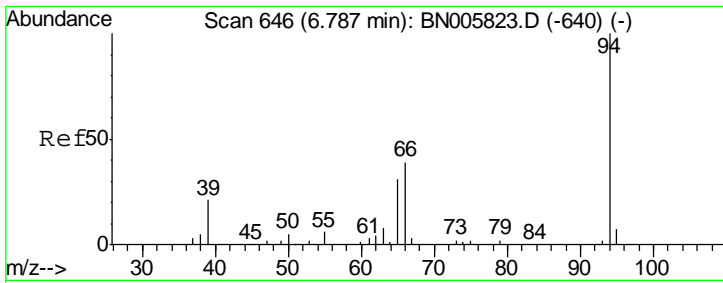

#6
 Phenol
 Concen: 1.998 ng/ul
 RT: 6.79 min Scan# 646
 Delta R.T. 0.00 min
 Lab File: BN005832.D
 Acq: 21 May 2019 19:34

Instrument :
 BNA_N
ClientSampled :
 BFHF0

Tgt Ion	Resp	Lower	Upper
94	100		
65	32.4	24.2	36.4
66	66.9	33.8	50.6

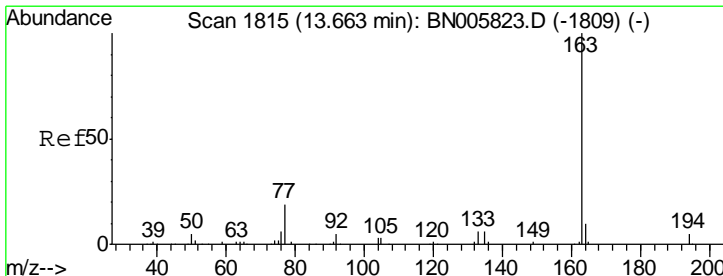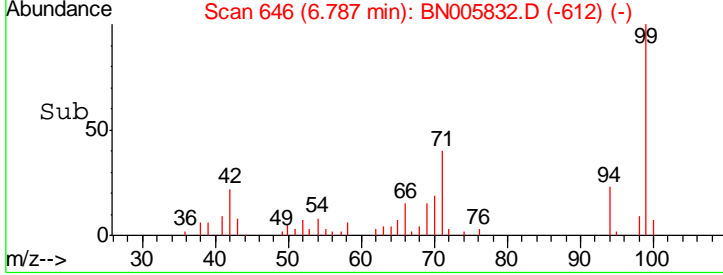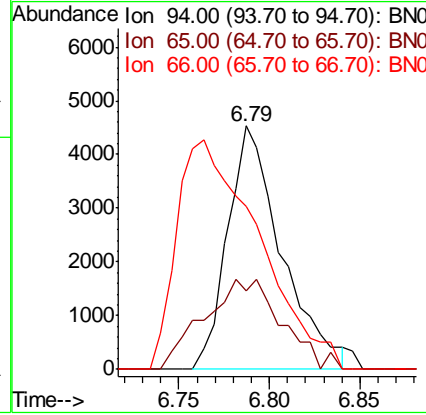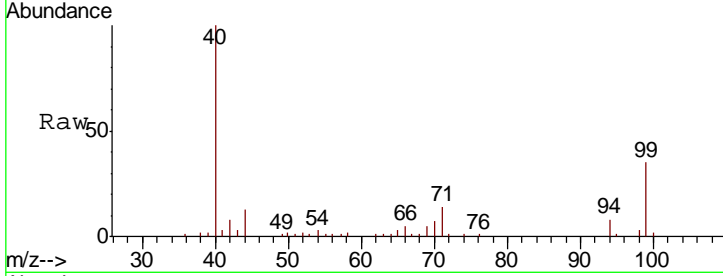

#44
 Dimethylphthalate
 Concen: 8.362 ng/ul
 RT: 13.67 min Scan# 1816
 Delta R.T. 0.00 min
 Lab File: BN005832.D
 Acq: 21 May 2019 19:34

Tgt Ion	Resp	Lower	Upper
163	100		
194	4.6	3.4	5.0
164	9.8	8.1	12.1

