


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052120\
 Data File : BN010730.D
 Acq On : 21 May 2020 15:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 21 16:54:53 2020

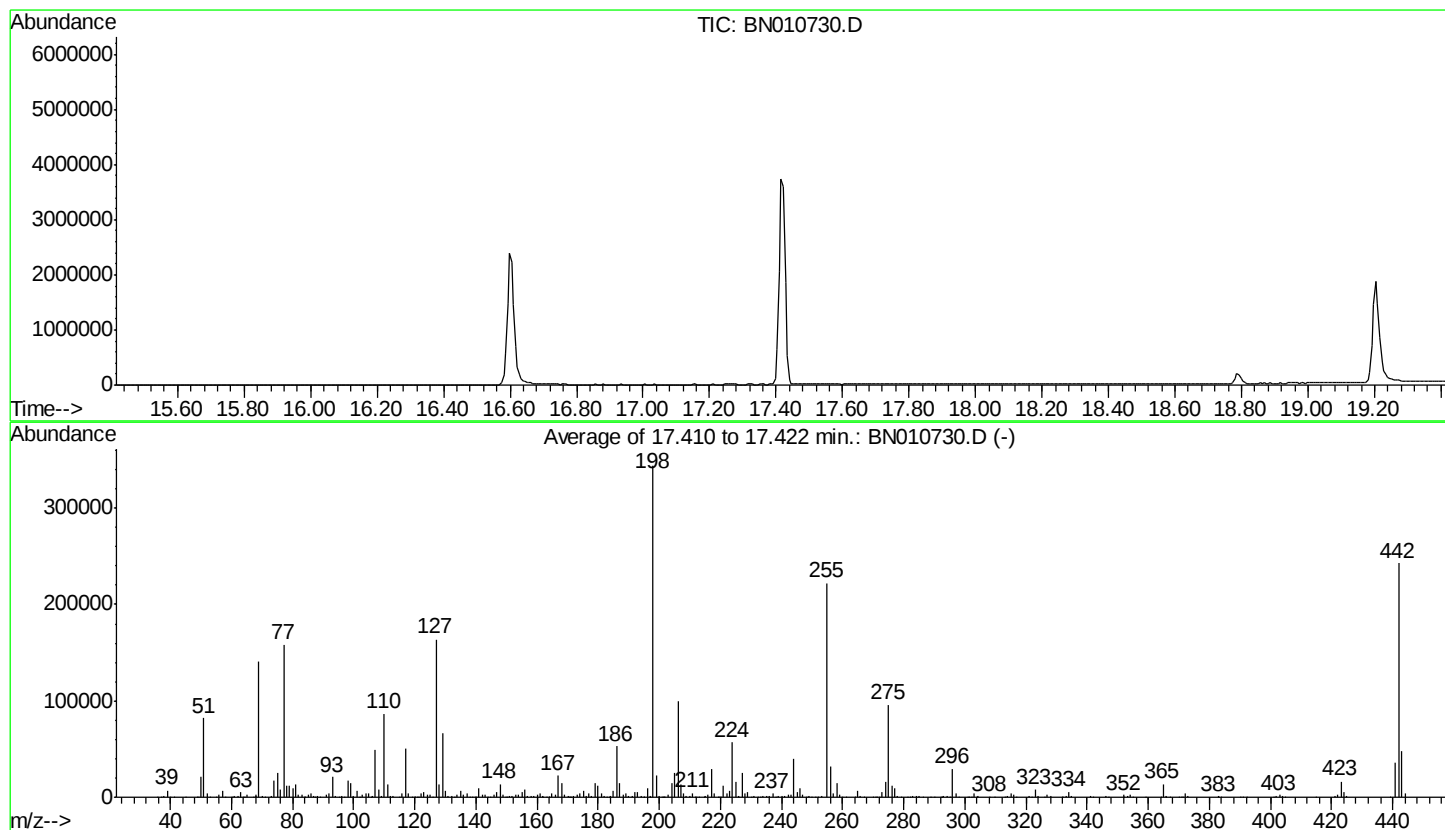

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	82266	PASS
68	69	0.00	2	1.5	2174	PASS
69	198	0.00	100	40.9	140917	PASS
70	69	0.00	2	0.6	911	PASS
127	198	10	80	47.6	163648	PASS
197	198	0.00	2	0.4	1247	PASS
198	198	100	100	100.0	344149	PASS
199	198	5	9	6.6	22742	PASS
275	198	10	60	27.9	96080	PASS
365	198	1	100	4.0	13894	PASS
441	198	0.01	100	10.3	35328	PASS
442	198	50	100	70.6	242912	PASS
443	442	15	24	19.5	47394	PASS