

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN052219\
 Data File : BN005860.D
 Acq On : 22 May 2019 20:35
 Operator : JU/SJ
 Sample : K2925-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4298

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.769	639	643	657	rVB2	52662	140131	6.33%	0.826%
2	6.911	663	667	681	rVB	70492	136841	6.19%	0.807%
3	7.111	696	701	713	rVB2	78614	166723	7.54%	0.983%
4	7.564	772	778	791	rVB	188874	381706	17.25%	2.250%
5	8.293	897	902	916	rBV2	71859	164954	7.46%	0.972%
6	8.722	970	975	986	rVB	96385	185033	8.36%	1.091%
7	9.434	1091	1096	1107	rBV	68274	147508	6.67%	0.869%
8	9.999	1186	1192	1203	rBV2	55520	164123	7.42%	0.967%
9	10.322	1241	1247	1259	rVB	340398	608593	27.51%	3.587%
10	10.499	1272	1277	1294	rBV3	46223	140959	6.37%	0.831%
11	13.622	1801	1808	1813	rBV	311481	492314	22.25%	2.902%
12	13.669	1813	1816	1827	rVB	65274	121319	5.48%	0.715%
13	13.893	1848	1854	1864	rBV	329857	524626	23.72%	3.092%
14	14.087	1885	1887	1891	rBV2	1725	2319	0.10%	0.014%
15	14.199	1900	1906	1924	rVB2	602137	974388	44.05%	5.743%
16	14.522	1957	1961	1967	rBV6	13649	36848	1.67%	0.217%
17	14.687	1985	1989	1992	rBV4	3134	4189	0.19%	0.025%
18	15.022	2042	2046	2049	rBV3	2058	3059	0.14%	0.018%
19	15.204	2071	2077	2090	rBV	422364	729446	32.97%	4.300%
20	15.387	2103	2108	2118	rBV	43225	82037	3.71%	0.484%
21	15.457	2118	2120	2125	rVB3	4547	6188	0.28%	0.036%
22	16.745	2335	2339	2343	rVB3	2090	3603	0.16%	0.021%
23	16.957	2369	2375	2381	rVV2	966561	1371197	61.98%	8.082%
24	17.004	2381	2383	2387	rVV	25378	30100	1.36%	0.177%
25	17.063	2387	2393	2406	rVB	525202	858405	38.80%	5.060%
26	17.369	2443	2445	2448	rBV2	1949	2752	0.12%	0.016%
27	17.416	2451	2453	2458	rVB5	2665	3914	0.18%	0.023%
28	17.875	2523	2531	2535	rBV3	27488	48598	2.20%	0.286%
29	17.939	2541	2542	2546	rVB3	4504	4148	0.19%	0.024%
30	17.992	2546	2551	2555	rVB3	6209	9524	0.43%	0.056%
31	18.045	2555	2560	2565	rBV4	13072	24903	1.13%	0.147%
32	18.081	2565	2566	2571	rVV5	5212	6887	0.31%	0.041%
33	18.163	2576	2580	2583	rBV3	2589	3868	0.17%	0.023%
34	18.263	2592	2597	2600	rVB3	2719	3031	0.14%	0.018%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN052219\
 Data File : BN005860.D
 Acq On : 22 May 2019 20:35
 Operator : JU/SJ
 Sample : K2925-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4298

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Title : SVOA CALIBRATION

35	18.298	2600	2603	2607	rBV3	4487	5188	0.23%	0.031%
36	18.363	2610	2614	2617	rBV3	5871	7692	0.35%	0.045%
37	18.434	2620	2626	2631	rBV5	4454	7819	0.35%	0.046%
38	18.657	2660	2664	2668	rBV2	3489	4846	0.22%	0.029%
39	18.698	2668	2671	2674	rVB2	2851	3000	0.14%	0.018%
40	18.781	2681	2685	2688	rBV2	7711	9993	0.45%	0.059%
41	18.845	2693	2696	2699	rVV4	3961	5616	0.25%	0.033%
42	18.934	2705	2711	2718	rVB7	7060	14765	0.67%	0.087%
43	19.010	2718	2724	2725	rBV2	7028	7304	0.33%	0.043%
44	19.039	2725	2729	2736	rVB	137108	192892	8.72%	1.137%
45	19.175	2748	2752	2753	rBV3	8692	9829	0.44%	0.058%
46	19.286	2762	2771	2775	rBV5	5980	15398	0.70%	0.091%
47	19.375	2781	2786	2800	rVB3	760846	1339892	60.57%	7.898%
48	19.498	2803	2807	2810	rBV3	9607	12117	0.55%	0.071%
49	19.604	2818	2825	2830	rBV3	9679	17493	0.79%	0.103%
50	19.686	2837	2839	2844	rVB4	2093	2518	0.11%	0.015%
51	19.757	2844	2851	2859	rBV5	12487	30174	1.36%	0.178%
52	19.828	2861	2863	2869	rBV6	1754	2468	0.11%	0.015%
53	19.892	2869	2874	2875	rBV3	8827	16084	0.73%	0.095%
54	19.922	2875	2879	2887	rVB6	19848	41479	1.88%	0.244%
55	20.022	2891	2896	2900	rBV3	9994	14105	0.64%	0.083%
56	20.081	2902	2906	2911	rVB3	19486	28206	1.28%	0.166%
57	20.122	2911	2913	2917	rVB4	4266	4582	0.21%	0.027%
58	20.163	2917	2920	2923	rBV4	5422	7485	0.34%	0.044%
59	20.222	2926	2930	2934	rBV5	9873	13890	0.63%	0.082%
60	20.269	2934	2938	2942	rBV4	11844	19083	0.86%	0.112%
61	20.304	2942	2944	2946	rBV3	3191	2799	0.13%	0.016%
62	20.381	2954	2957	2958	rBV2	3089	3073	0.14%	0.018%
63	20.422	2961	2964	2966	rVV2	12127	14588	0.66%	0.086%
64	20.445	2966	2968	2971	rVV3	12864	11929	0.54%	0.070%
65	20.481	2971	2974	2977	rVV5	4684	4746	0.21%	0.028%
66	20.545	2982	2985	2990	rVB4	15597	21060	0.95%	0.124%
67	20.598	2990	2994	2998	rBV4	5556	7529	0.34%	0.044%
68	20.692	3006	3010	3012	rVB3	17921	21491	0.97%	0.127%
69	20.845	3034	3036	3038	rVB2	14595	11411	0.52%	0.067%
70	20.875	3038	3041	3044	rBV3	15943	18573	0.84%	0.109%
71	20.916	3044	3048	3058	rVB7	40808	80227	3.63%	0.473%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052219\
Data File : BN005860.D
Acq On : 22 May 2019 20:35
Operator : JU/SJ
Sample : K2925-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4298

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Title : SVOA CALIBRATION

72	20.998	3058	3062	3069	rVB2	20711	39049	1.77%	0.230%
73	21.081	3071	3076	3077	rBV5	8352	11267	0.51%	0.066%
74	21.198	3088	3096	3101	rBV	1466045	2212173	100.00%	13.039%
75	21.357	3119	3123	3128	rBV	41354	46609	2.11%	0.275%
76	21.433	3134	3136	3138	rBV3	10601	7789	0.35%	0.046%
77	21.757	3188	3191	3193	rBV	22322	24858	1.12%	0.147%
78	21.780	3193	3195	3198	rVV	38231	40986	1.85%	0.242%
79	22.239	3269	3273	3277	rBV	87728	110403	4.99%	0.651%
80	22.357	3290	3293	3297	rVB3	24655	29483	1.33%	0.174%
81	22.727	3352	3356	3365	rBV3	114345	325237	14.70%	1.917%
82	23.210	3434	3438	3440	rBV2	35780	55084	2.49%	0.325%
83	23.257	3440	3446	3462	rVB2	779144	1708557	77.23%	10.071%
84	23.398	3463	3470	3482	rVV	1145857	2181643	98.62%	12.859%
85	23.892	3549	3554	3562	rVB2	119540	210045	9.49%	1.238%
86	24.610	3670	3676	3685	rBV3	96514	202896	9.17%	1.196%
87	25.439	3812	3817	3825	rVB3	66932	144008	6.51%	0.849%


Sum of corrected areas: 16965665

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN052219\
Data File : BN005860.D
Acq On : 22 May 2019 20:35
Operator : JU/SJ
Sample : K2925-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4298

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

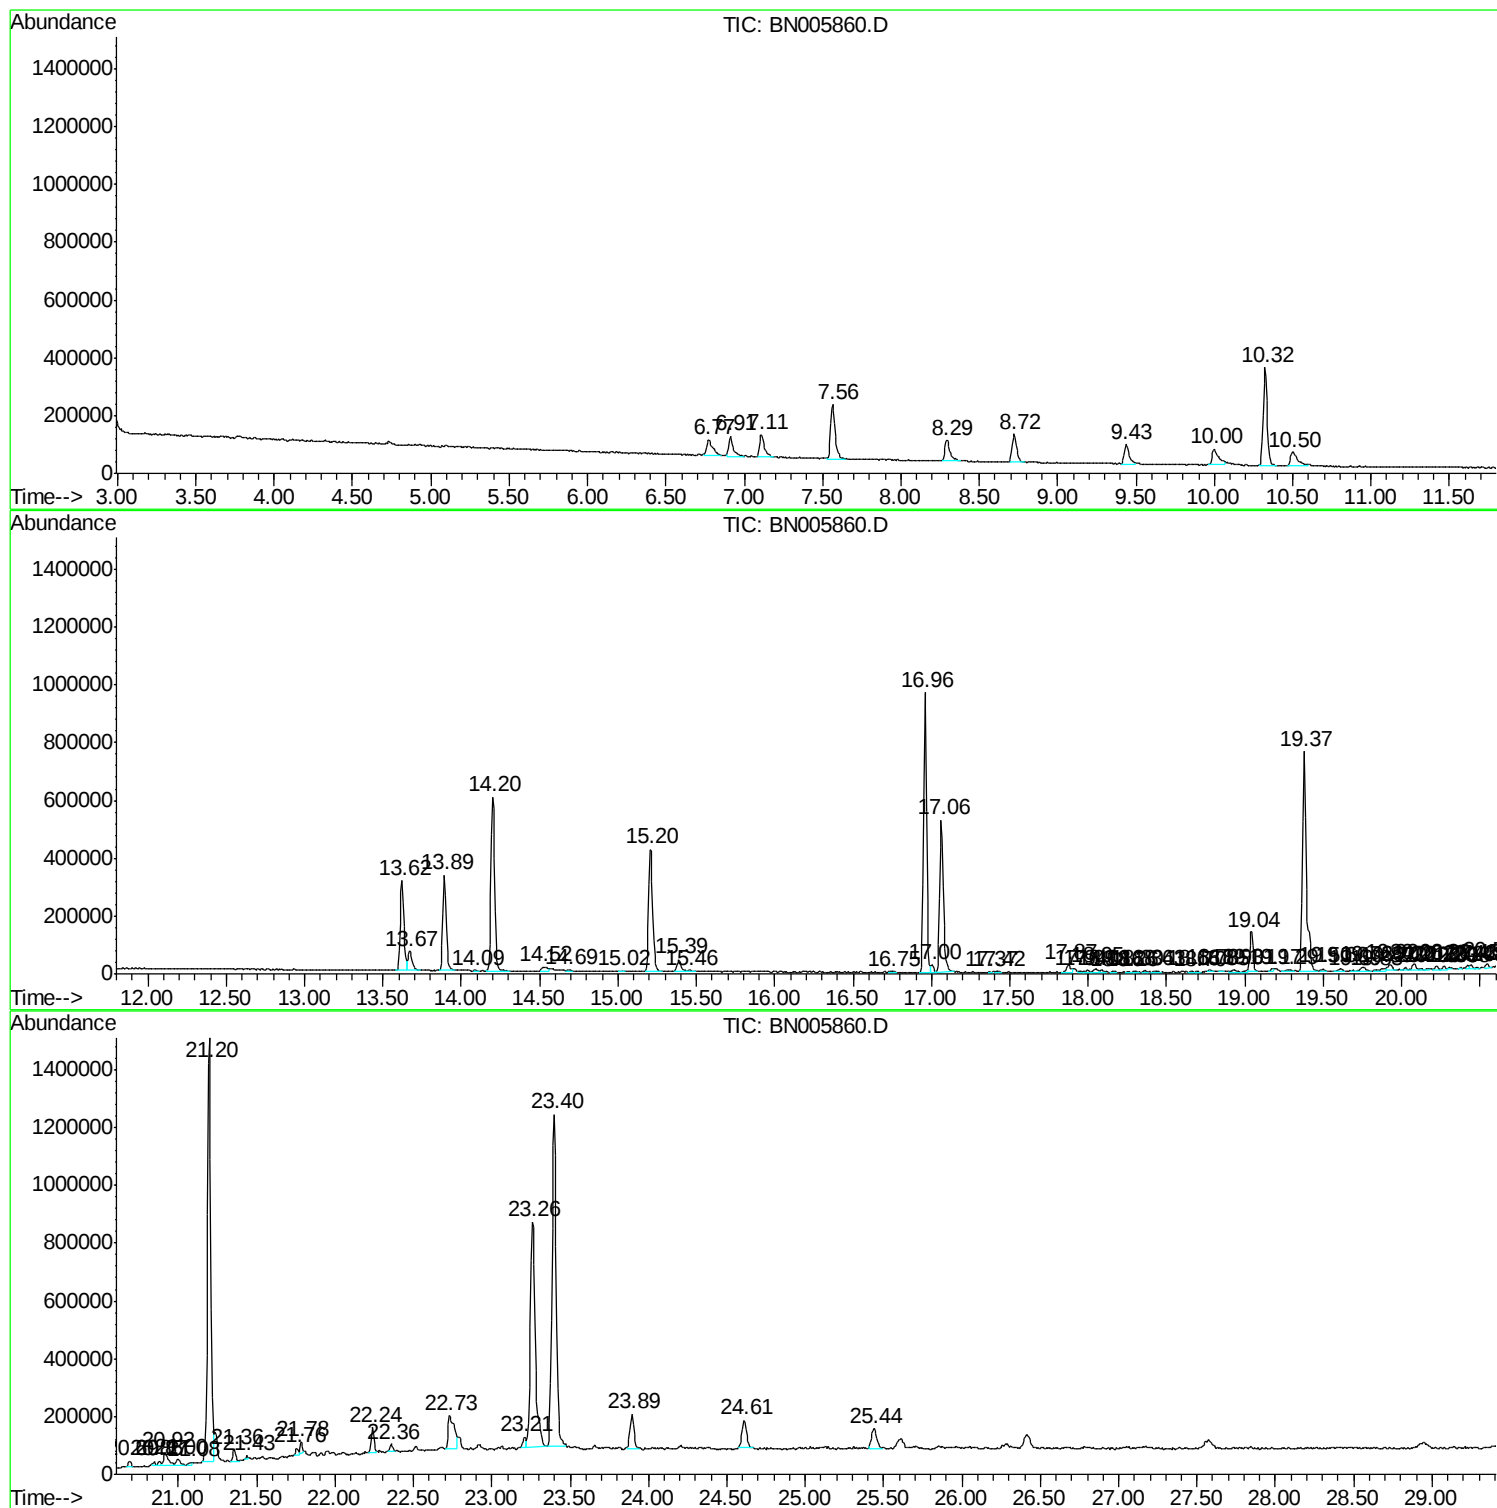

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052219\
Data File : BN005860.D
Acq On : 22 May 2019 20:35
Operator : JU/SJ
Sample : K2925-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4298

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052219\
Data File : BN005860.D
Acq On : 22 May 2019 20:35
Operator : JU/SJ
Sample : K2925-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4298

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
