

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052419\
 Data File : BN005903.D
 Acq On : 24 May 2019 22:54
 Operator : JU/SJ
 Sample : K2924-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4267

Manual Integrations
 APPROVED

mohammad
 5/27/2019 3:55:02 AM

Quant Time: May 25 00:15:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 22 04:04:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	77398	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	323023	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	225784	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	600452	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	683523	20.00	ng/ul	0.00
85) Perylene-d12	23.40	264	746420	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	8125	5.88	ng/uL	-0.01
5) Phenol-d5	6.76	99	148981	24.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	84849	27.19	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	126183	26.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	130997	25.61	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	64953	27.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	67663	24.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	141402m	27.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	150356	26.20	ng/ul	0.00
43) Dimethylphthalate-d6	13.62	166	559621	32.21	ng/ul	0.00
46) Acenaphthylene-d8	13.89	160	651545	30.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	46021m	18.80	ng/ul	0.05
57) Fluorene-d10	15.20	176	499141	33.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	35836	9.93	ng/ul	0.01
70) Anthracene-d10	17.06	188	853556	32.91	ng/ul	0.00
78) Pyrene-d10	19.37	212	1109398	32.94	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.26	264	1136719	33.95	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.66	163	175723	10.259	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052419\
Data File : BN005903.D
Acq On : 24 May 2019 22:54
Operator : JU/SJ
Sample : K2924-06
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4267

Manual Integrations
APPROVED

mohammad
5/27/2019 3:55:02 AM

Quant Time: May 25 00:15:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN051819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 22 04:04:33 2019
Response via : Initial Calibration

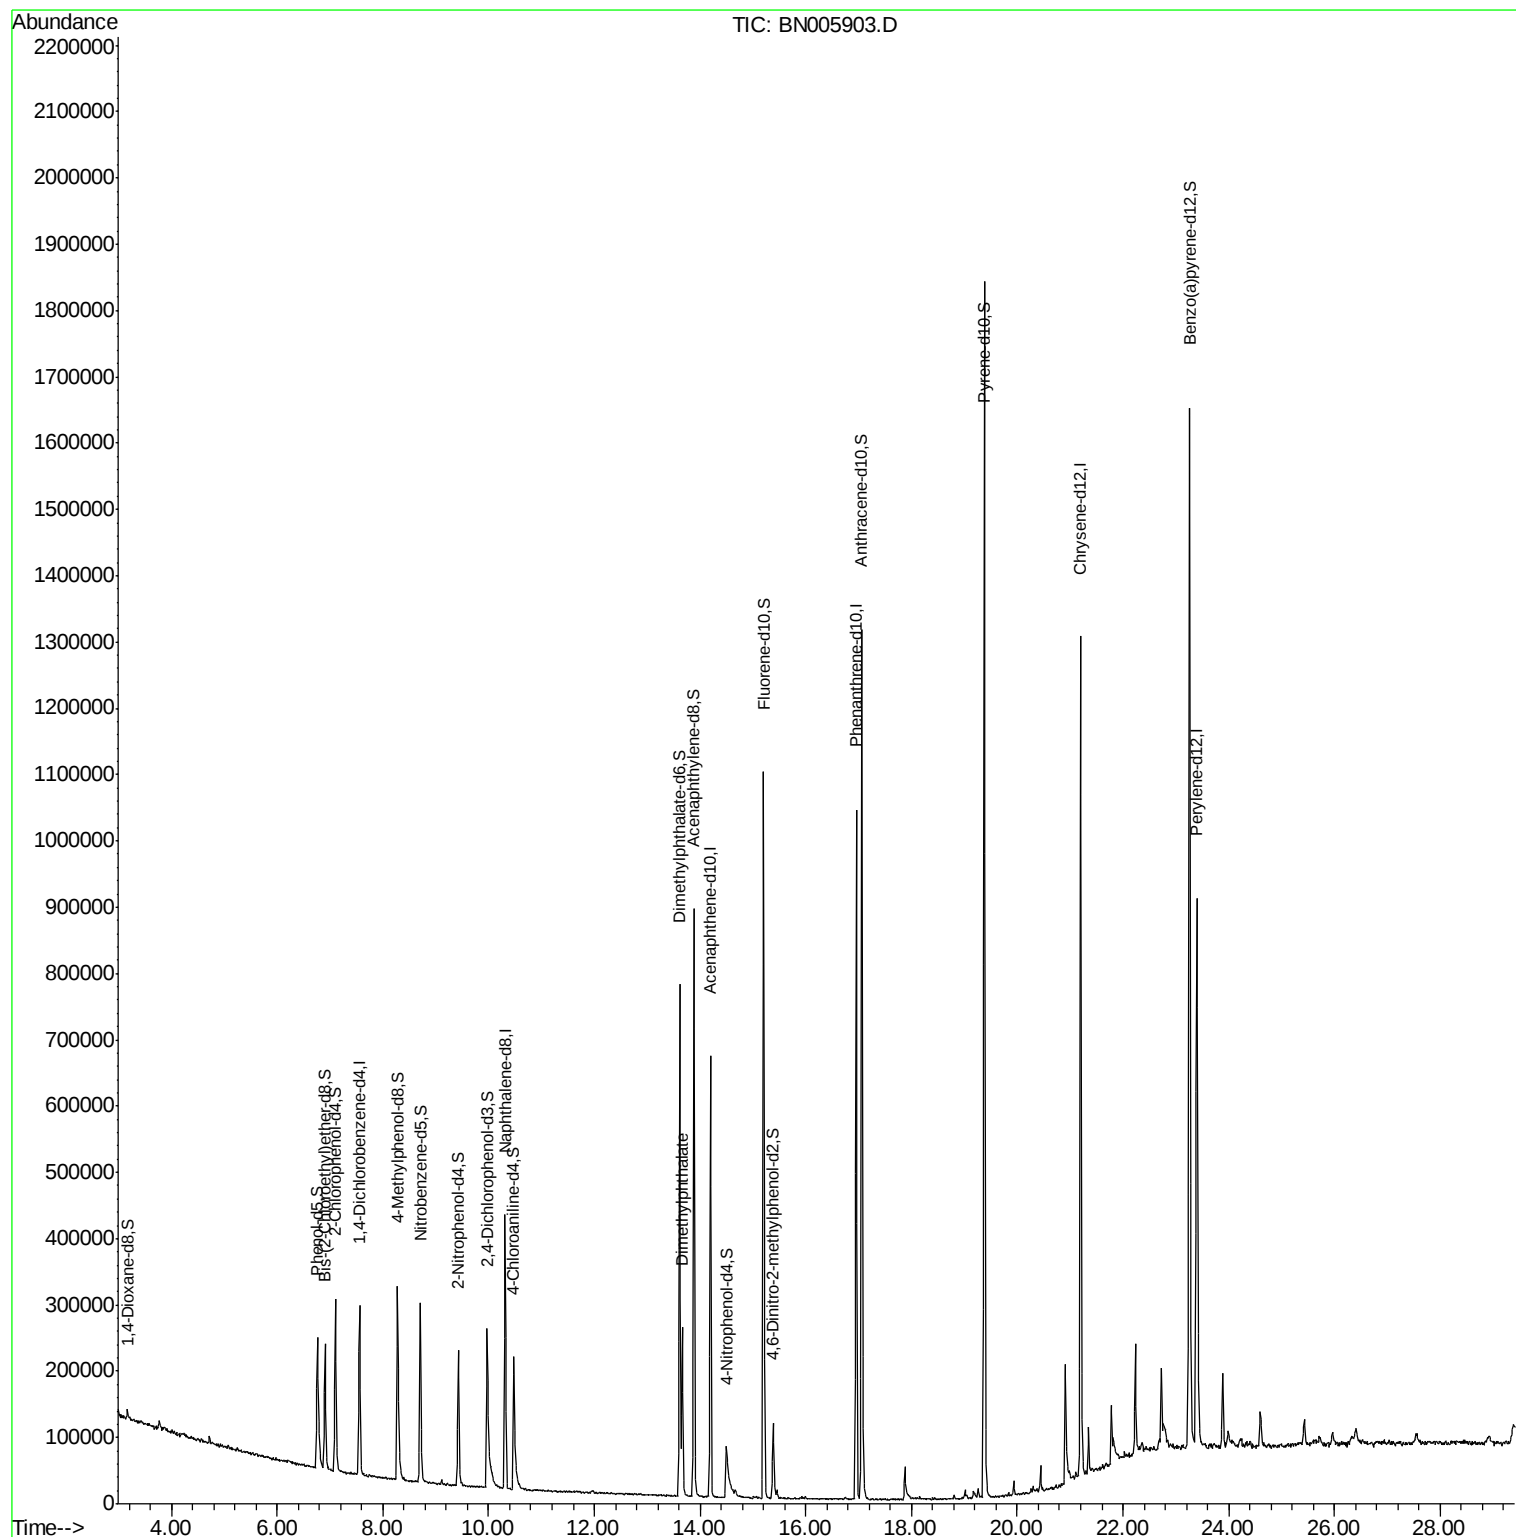

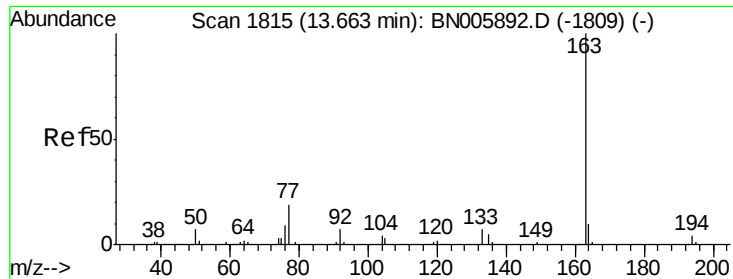

#44

Dimethylphthalate

Concen: 10.259 ng/ul

RT: 13.66 min Scan# 1815

Delta R.T. -0.00 min

Lab File: BN005903.D

Acq: 24 May 2019 22:54

Instrument :

BNA_N

ClientSampleId :

A4267

Tot Ion:	163	Resp:	175723
Ion Ratio	Lower	Upper	
163	100		
194	4.6	3.4	5.0
164	9.8	8.1	12.1

Manual Integrations
APPROVED

mohammad
5/27/2019 3:55:02 AM

