
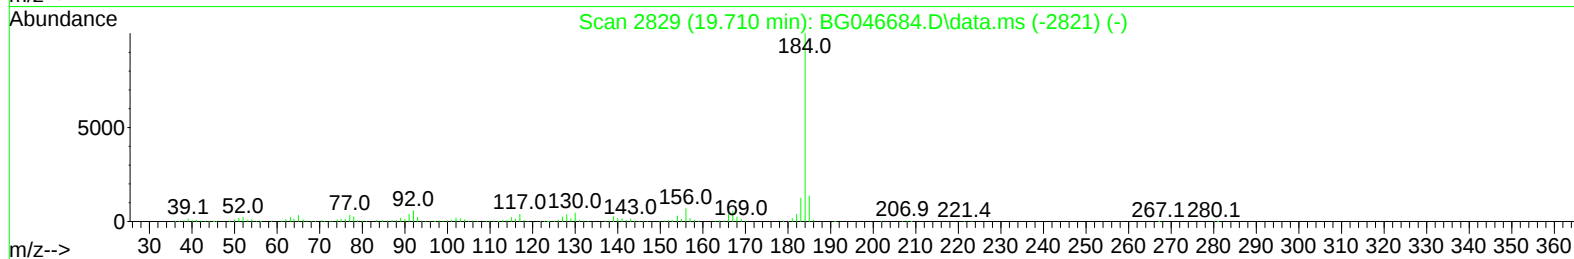
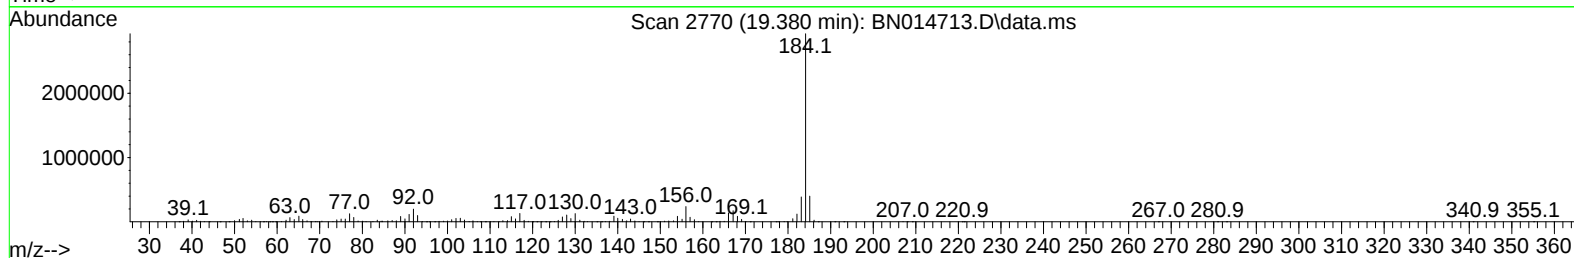


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052421\
Data File : BN014713.D
Acq On : 24 May 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 11:42:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

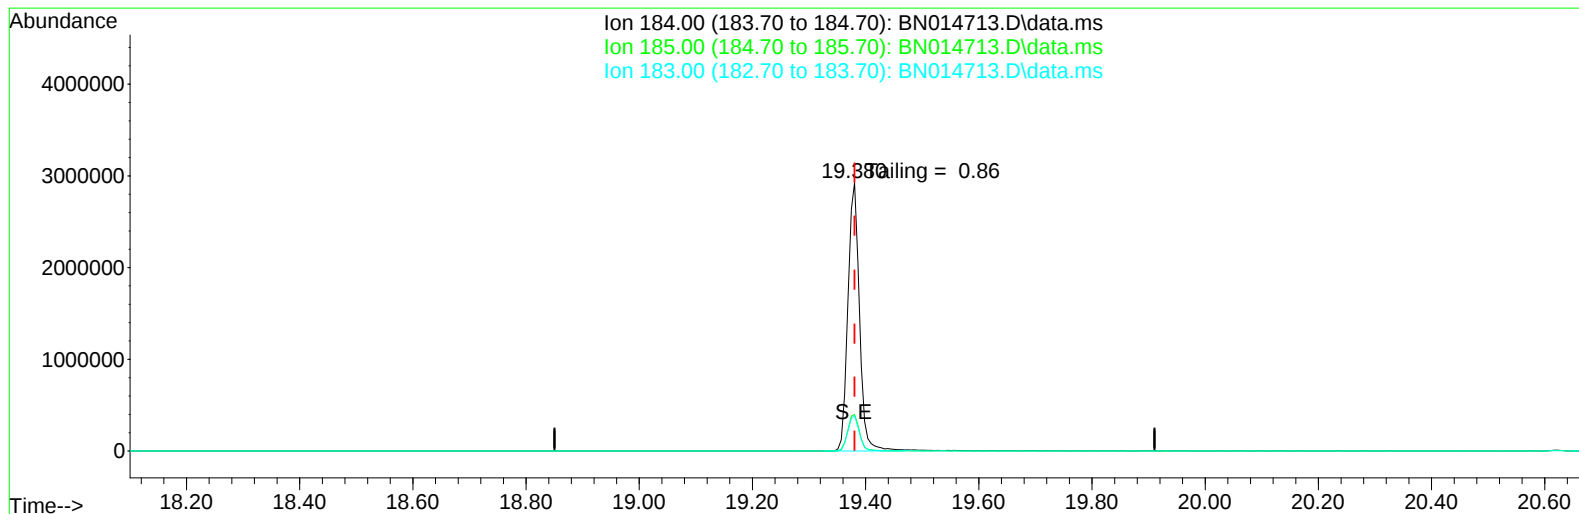




TIC: BN014713.D\data.ms

(77) Benzidine**19.380min (+ 0.000) 1202890.85 ng****response 4189990**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.64
183.00	13.20	13.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052421\
Data File : BN014713.D
Acq On : 24 May 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 11:42:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

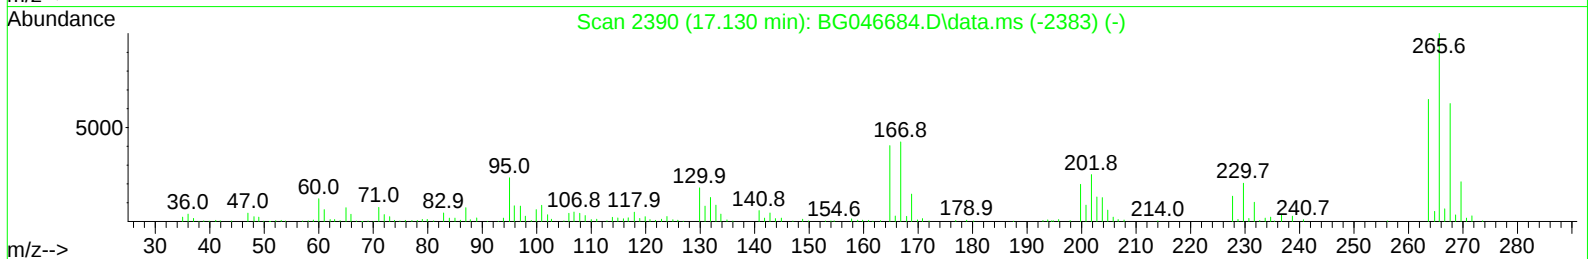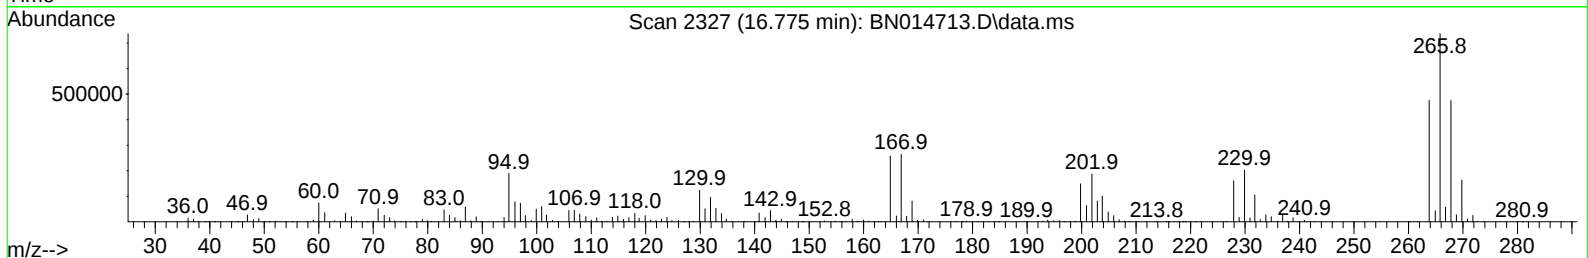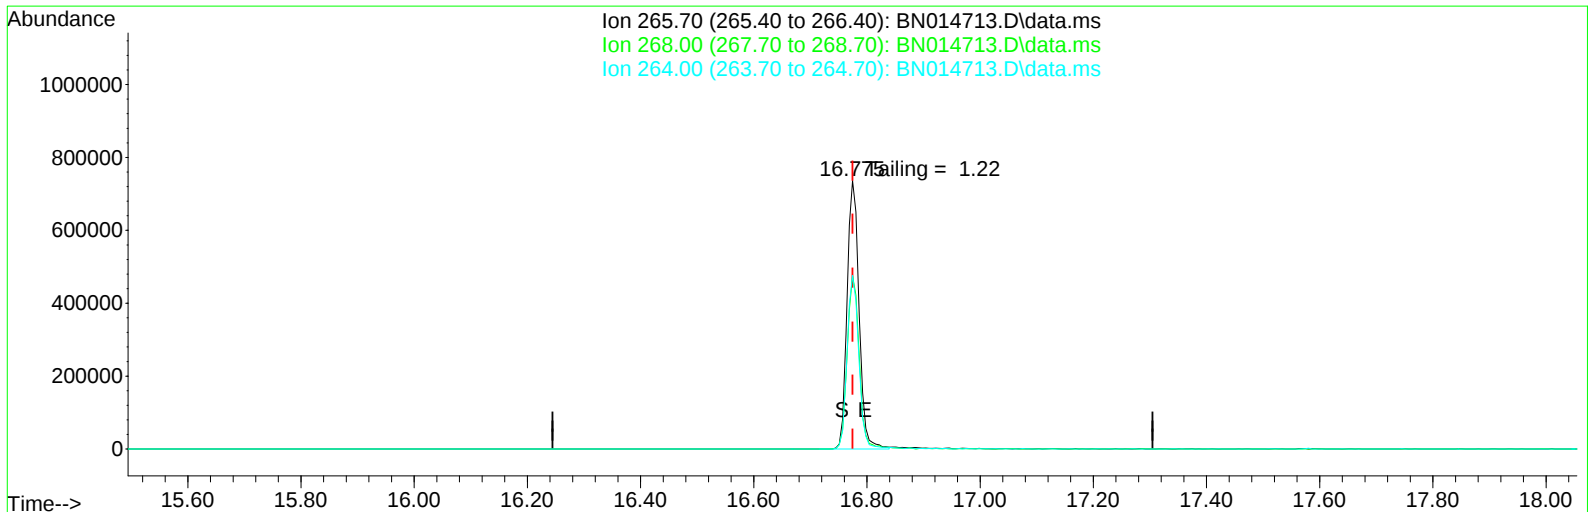

TIC: BN014713.D\data.ms

(70) Pentachlorophenol (C)

16.775min (+ 0.000) 206303.86 ng

response 1092839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.57
264.00	61.60	64.62
0.00	0.00	0.00