


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052421\
 Data File : BN014713.D
 Acq On : 24 May 2021 09:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 21 11:30:28 2021

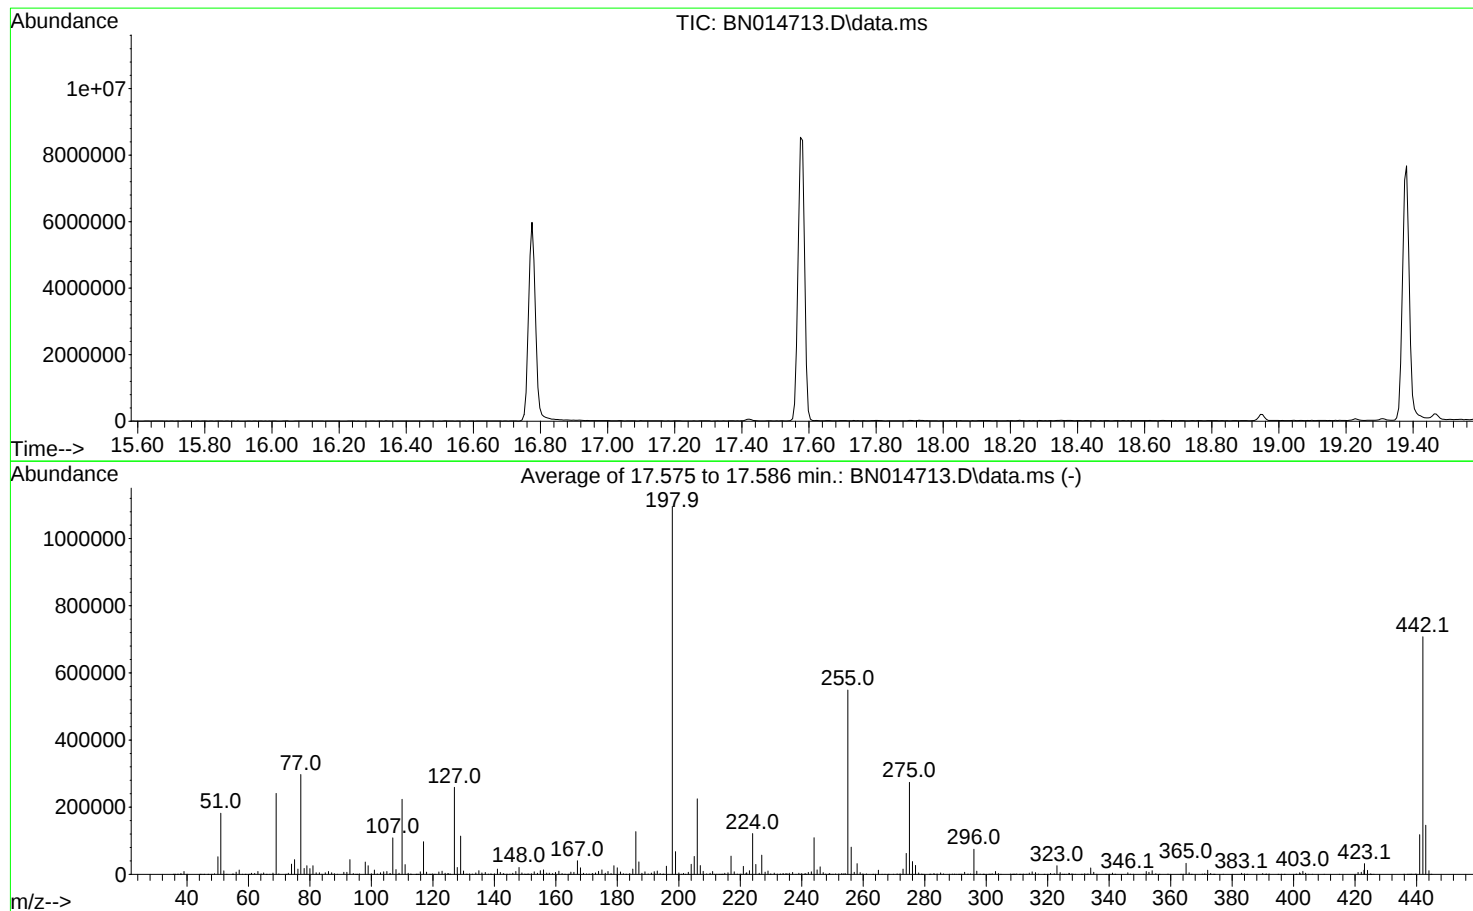

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	16.6	182131	PASS
68	69	0.00	2	1.5	3695	PASS
69	198	0.00	100	22.0	240981	PASS
70	69	0.00	2	0.6	1543	PASS
127	198	10	80	23.6	259093	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1095552	PASS
199	198	5	9	6.2	67555	PASS
275	198	10	60	25.0	274240	PASS
365	198	1	100	3.0	32872	PASS
441	198	0.01	100	10.8	118163	PASS
442	442	50	100	100.0	707520	PASS
443	442	15	24	20.7	146357	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/24/2021	BNA_N	<u>BN014713.D</u>
Compound Name	Response	Retention Time
DDT	2753714	20.62
DDD	40240	20.17
DDE	10026	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
50266	2803980	1.79

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052421\
Data File : BN014713.D
Acq On : 24 May 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 24 11:42:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

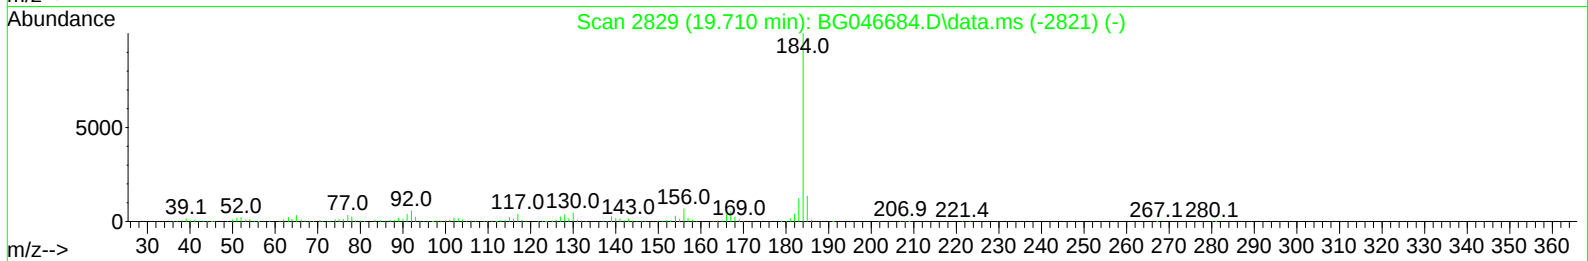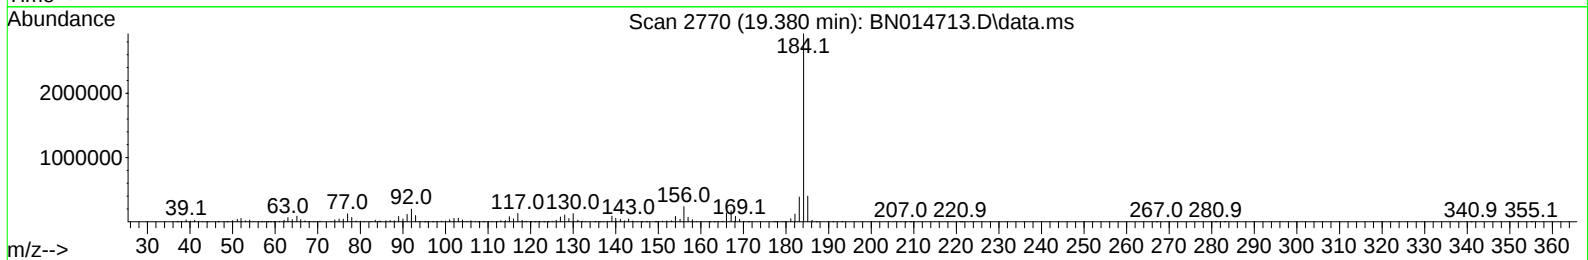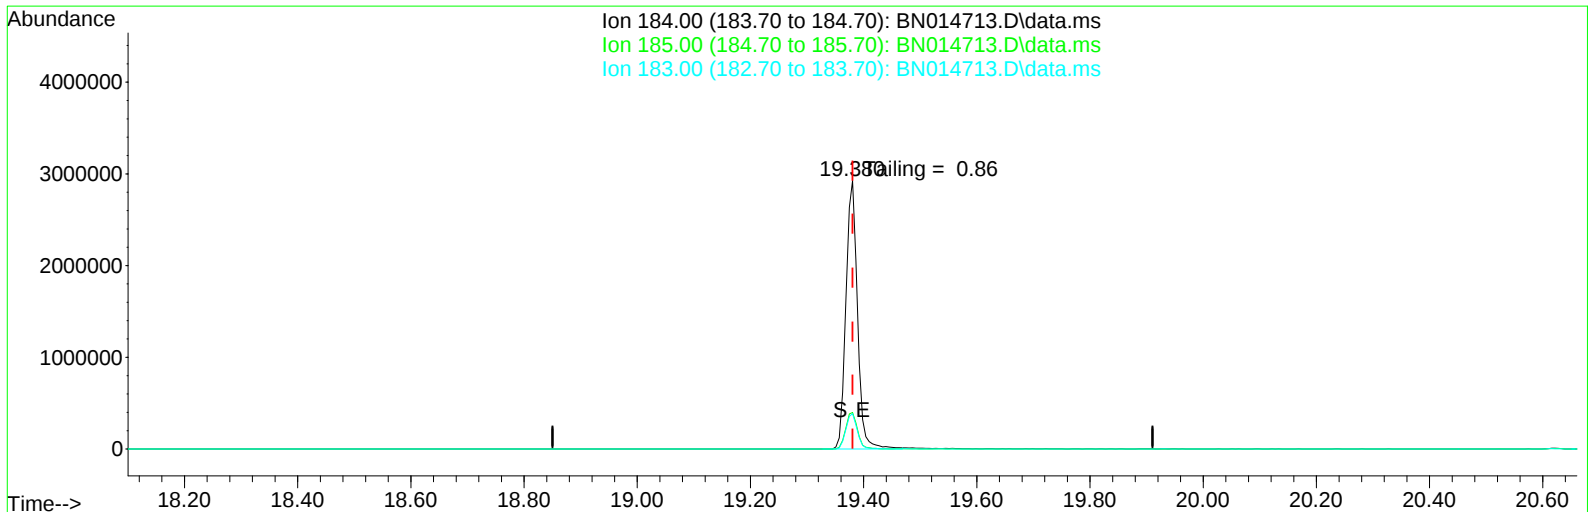

TIC: BN014713.D\data.ms

(77) Benzidine

19.380min (+ 0.000) 1202890.85 ng




response 4189990

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.64
183.00	13.20	13.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052421\
Data File : BN014713.D
Acq On : 24 May 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 24 11:42:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

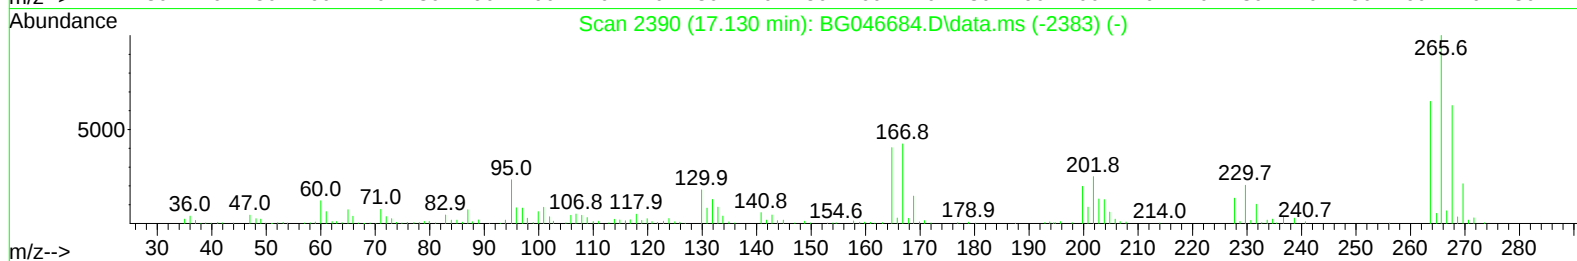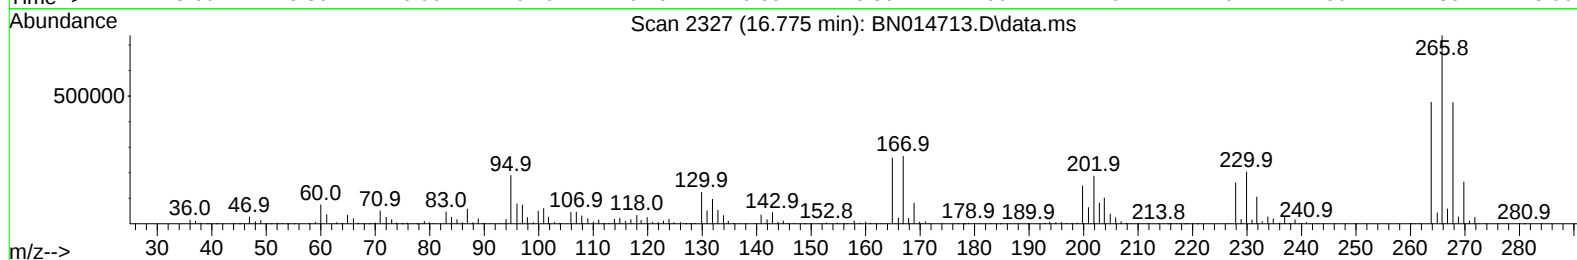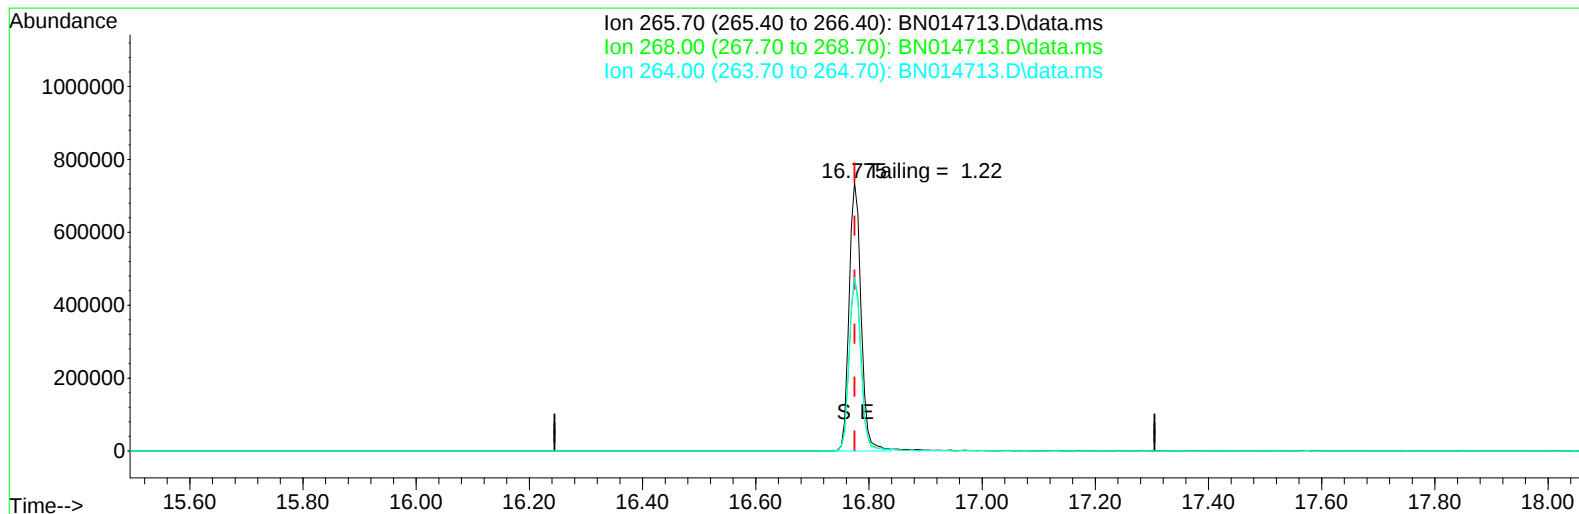

TIC: BN014713.D\data.ms

(70) Pentachlorophenol (C)

16.775min (+ 0.000) 206303.86 ng

response 1092839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.57
264.00	61.60	64.62
0.00	0.00	0.00