

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052424\
 Data File : BN031667.D
 Acq On : 24 May 2024 18:58
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020262

Quant Time: May 24 22:44:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 23:42:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	504928	20.000	ng/u1	0.00
20) Naphthalene-d8	10.469	136	1957960	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.328	164	951345	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.069	188	1589712	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1431211	20.000	ng/u1	0.00
88) Perylene-d12	24.233	264	1757235	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	101836	7.994	ng/uL	0.00
4) Pyridine-d5	3.599	84	712537	20.043	ng/u1	0.00
7) Phenol-d5	6.858	99	849260	20.432	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	496012	19.897	ng/u1	0.00
11) 2-Chlorophenol-d4	7.222	132	658775	20.569	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	623971	19.392	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	301099	20.319	ng/u1	0.00
24) 2-Nitrophenol-d4	9.558	143	291010	20.566	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	548968	19.842	ng/u1	0.00
31) 4-Chloroaniline-d4	10.610	131	752296	18.863	ng/u1	0.00
46) Dimethylphthalate-d6	13.746	166	1221001	20.366	ng/u1	0.00
49) Acenaphthylene-d8	14.022	160	1549517	20.621	ng/u1	0.00
54) 4-Nitrophenol-d4	14.522	143	206260	18.183	ng/u1	0.00
60) Fluorene-d10	15.322	176	995973	19.169	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.440	200	107470	15.637	ng/u1	0.00
73) Anthracene-d10	17.169	188	1344149	19.974	ng/u1	0.00
81) Pyrene-d10	19.463	212	1497720	16.683	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.033	264	1629177	19.696	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.234	88	110563	8.236	ng/uL	97
5) Pyridine	3.623	79	708235	20.242	ng/u1	98
6) Benzaldehyde	6.840	77	471921	22.166	ng/u1	99
8) Phenol	6.881	94	855209	20.020	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.122	93	716668	20.217	ng/u1	97
12) 2-Chlorophenol	7.252	128	681110	20.278	ng/u1	99
13) 2-Methylphenol	8.128	108	627812	19.619	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.211	45	790605	19.307	ng/u1	99
16) Acetophenone	8.511	105	980246	19.531	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.493	70	470007	18.228	ng/u1	100
18) 4-Methylphenol	8.452	108	653961	19.229	ng/u1	97
19) Hexachloroethane	8.758	117	284947	19.855	ng/u1	96
22) Nitrobenzene	8.887	77	739761	20.379	ng/u1	97
23) Isophorone	9.410	82	1293725	18.736	ng/u1	98
25) 2-Nitrophenol	9.593	139	318064	20.167	ng/u1	98
26) 2,4-Dimethylphenol	9.652	107	633069	19.650	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.893	93	844703	19.190	ng/u1	99
29) 2,4-Dichlorophenol	10.116	162	534141	19.474	ng/u1	98
30) Naphthalene	10.522	128	1999237	19.841	ng/u1	99
32) 4-Chloroaniline	10.634	127	737627	18.955	ng/u1	99
33) Hexachlorobutadiene	10.805	225	357365	21.291	ng/u1	97
34) Caprolactam	11.393	113	150556	16.948	ng/u1	98
35) 4-Chloro-3-methylphenol	11.757	107	526998	17.692	ng/u1	100
36) 2-Methylnaphthalene	12.134	142	1219531	18.494	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052424\
 Data File : BN031667.D
 Acq On : 24 May 2024 18:58
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 SSTD020262


Quant Time: May 24 22:44:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 23:42:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.357	142	1220374	18.696	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.504	216	587625	21.825	ng/ul	96
40) Hexachlorocyclopentadiene	12.487	237	249777	15.476	ng/ul	98
41) 2,4,6-Trichlorophenol	12.751	196	351267	21.113	ng/ul	94
42) 2,4,5-Trichlorophenol	12.816	196	370480	20.570	ng/ul	97
43) 1,1'-Biphenyl	13.157	154	1451879	21.169	ng/ul	98
44) 2-Chloronaphthalene	13.198	162	1147635	21.132	ng/ul	98
45) 2-Nitroaniline	13.404	65	281395	19.793	ng/ul	99
47) Dimethylphthalate	13.787	163	1245293	20.355	ng/ul	99
48) 2,6-Dinitrotoluene	13.910	165	231704	19.873	ng/ul	96
50) Acenaphthylene	14.046	152	1785526	20.584	ng/ul	100
51) 3-Nitroaniline	14.234	138	268853	20.315	ng/ul	97
52) Acenaphthene	14.393	153	1148288	20.431	ng/ul	94
53) 2,4-Dinitrophenol	14.440	184	72646	13.568	ng/ul	98
55) 4-Nitrophenol	14.540	109	159200	18.626	ng/ul	98
56) Dibenzofuran	14.728	168	1487949	19.832	ng/ul	98
57) 2,4-Dinitrotoluene	14.693	165	304541	19.497	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	14.951	232	259950	19.869	ng/ul	96
59) Diethylphthalate	15.157	149	1148556	19.924	ng/ul	97
61) Fluorene	15.375	166	1163945	19.804	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.375	204	561971	19.862	ng/ul	99
63) 4-Nitroaniline	15.398	138	262779	22.140	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.451	198	119579	15.865	ng/ul	95
67) N-Nitrosodiphenylamine	15.587	169	946712	20.230	ng/ul	98
68) 4-Bromophenyl-phenylether	16.269	248	310147	19.377	ng/ul	98
69) Hexachlorobenzene	16.375	284	337891	19.560	ng/ul	89
70) Atrazine	16.540	200	253237	20.107	ng/ul	95
71) Pentachlorophenol	16.716	266	195085	19.799	ng/ul	97
72) Phenanthrene	17.116	178	1635021	20.266	ng/ul	97
74) Anthracene	17.204	178	1627653	20.108	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.116	216	550287	21.775	ng/ul	98
76) Pentachlorobenzene	14.640	250	459832	20.094	ng/ul	90
77) Carbazole	17.475	167	1488830	21.554	ng/ul	99
78) Di-n-butylphthalate	18.045	149	1665094	20.994	ng/ul	99
80) Fluoranthene	19.133	202	1804694	16.264	ng/ul	99
82) Pyrene	19.498	202	1867590	16.411	ng/ul	99
83) Butylbenzylphthalate	20.410	149	718361	18.600	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.216	252	557140	20.245	ng/ul	99
85) Benzo(a)anthracene	21.286	228	1903662	19.780	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.222	149	1009090	19.082	ng/ul	98
87) Chrysene	21.345	228	1806356	20.319	ng/ul	99
89) Di-n-octyl phthalate	22.339	149	1761899	17.543	ng/ul	100
90) Benzo(b)fluoranthene	23.310	252	1974958	19.259	ng/ul	98
91) Benzo(k)fluoranthene	23.374	252	2043843	19.553	ng/ul	98
93) Benzo(a)pyrene	24.098	252	1945293	19.749	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	27.533	276	1199562	10.147	ng/ul	98
95) Dibenzo(a,h)anthracene	27.598	278	1972894	20.265	ng/ul	99
96) Benzo(g,h,i)perylene	28.562	276	1932722	19.787	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 24 22:44:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 23:42:49 2024
Response via : Initial Calibration




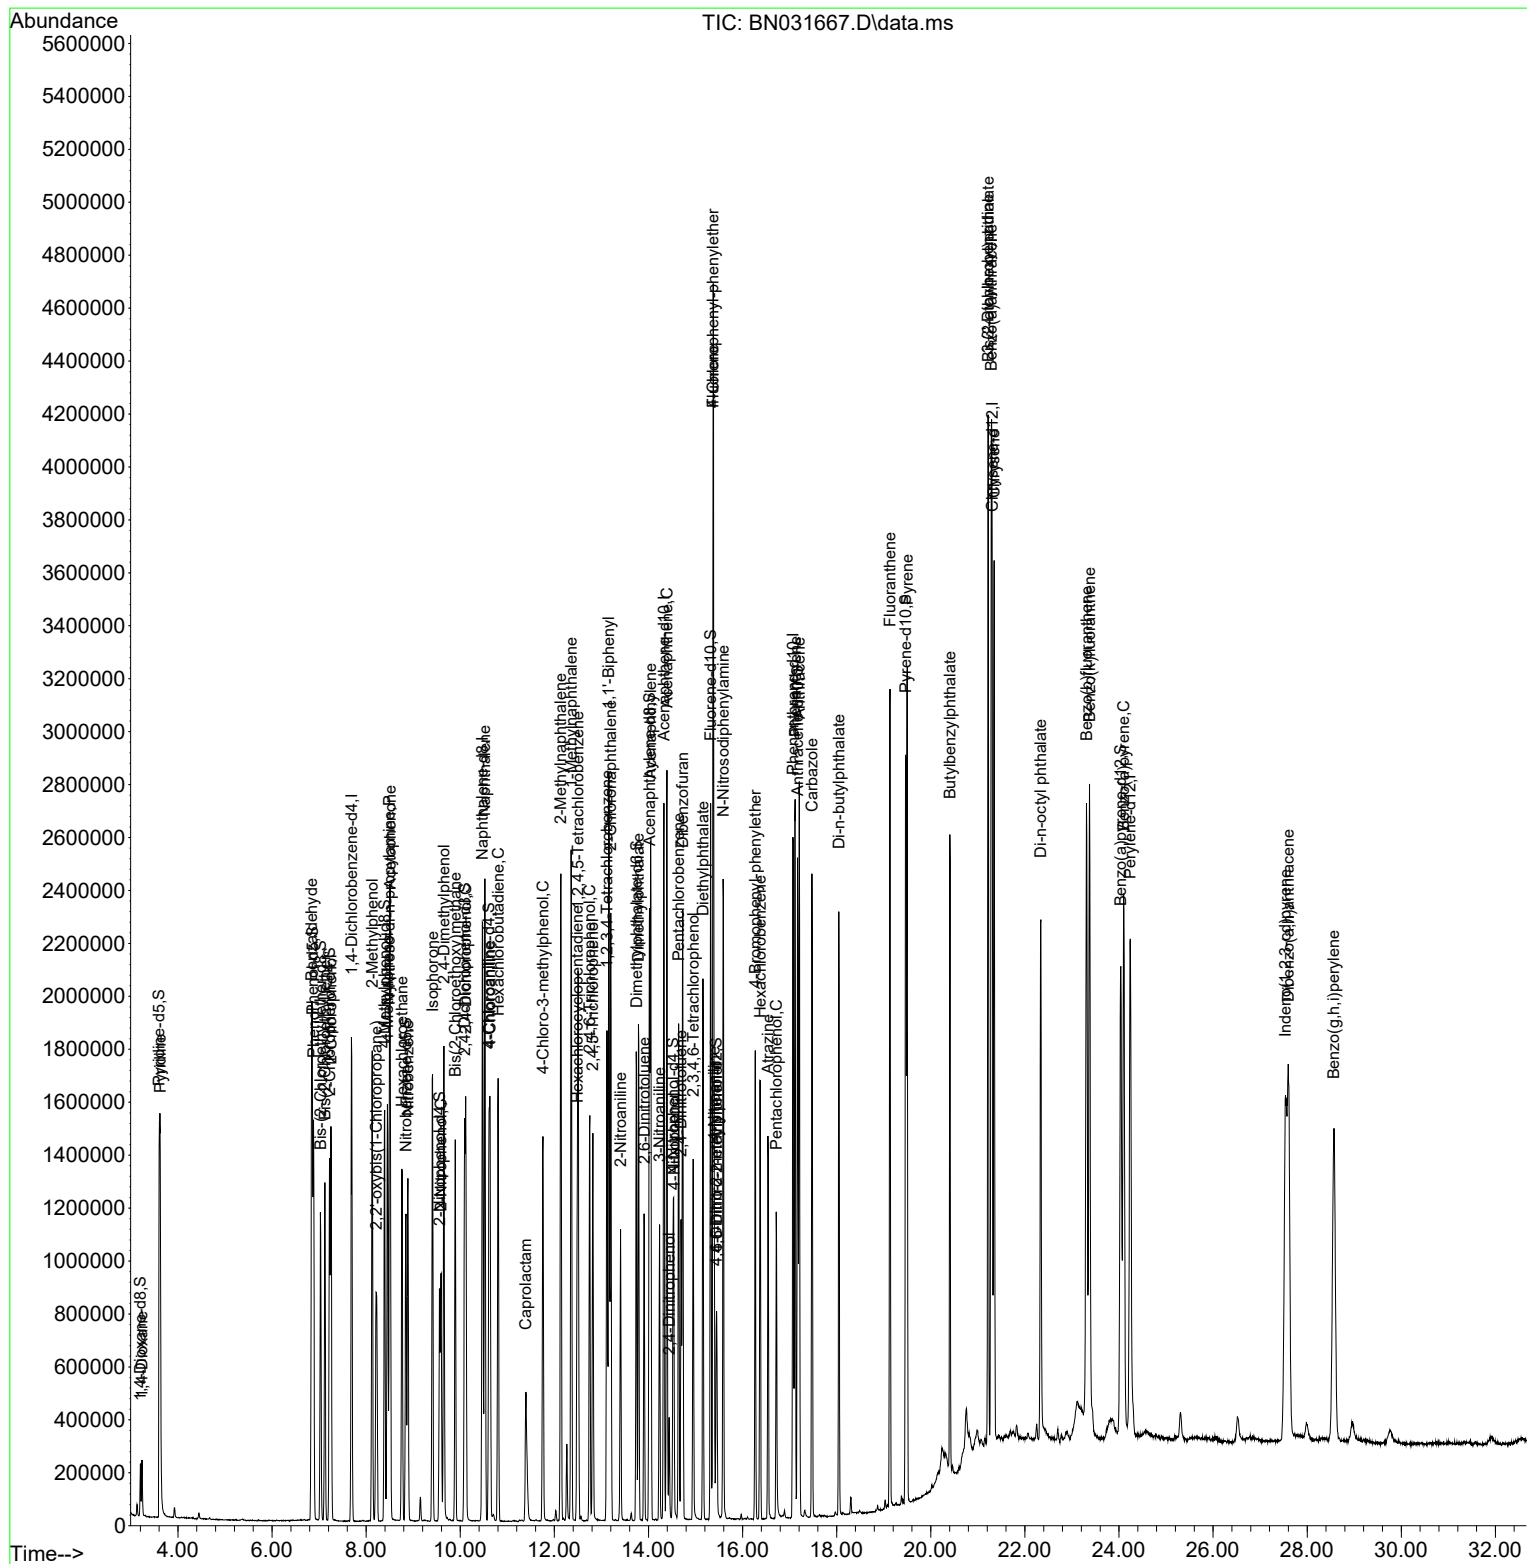




#2
1,4-Dioxane
Concen: 8.236 ng/uL
RT: 3.234 min Scan# 41
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion: 88 Resp: 110563
Ion Ratio Lower Upper
88 100
43 24.8 18.3 27.5
58 67.3 55.5 83.3

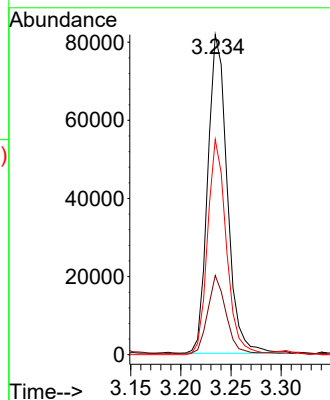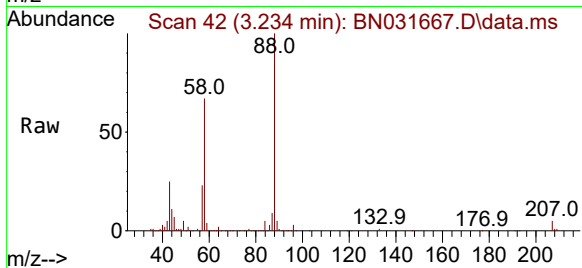

#5
Pyridine
Concen: 20.242 ng/uL
RT: 3.623 min Scan# 108
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion: 79 Resp: 708235
Ion Ratio Lower Upper
79 100
52 63.8 52.3 78.5
51 29.7 24.4 36.6



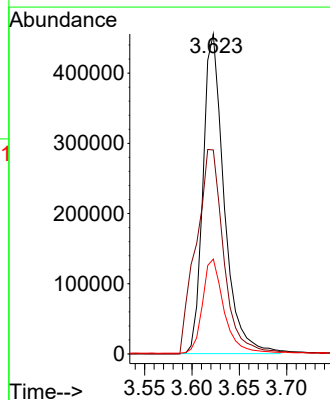
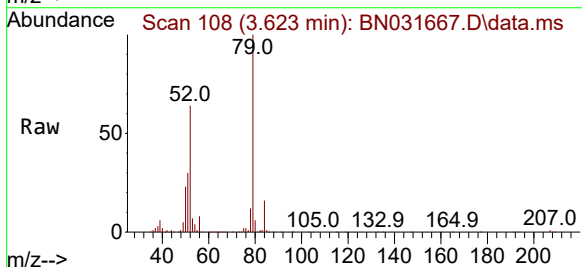




#6
Benzaldehyde
Concen: 22.166 ng/ul
RT: 6.840 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion: 77 Resp: 471921
Ion Ratio Lower Upper
77 100
105 100.7 82.1 123.1
106 94.7 75.5 113.3

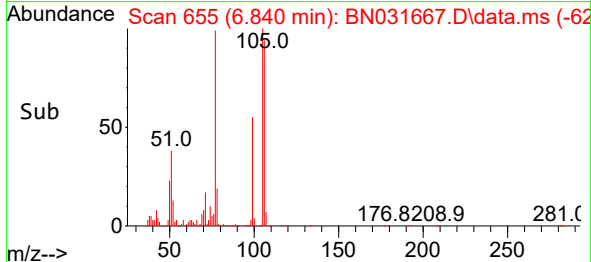

#8
Phenol
Concen: 20.020 ng/ul
RT: 6.881 min Scan# 662
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion: 94 Resp: 855209
Ion Ratio Lower Upper
94 100
65 25.4 20.8 31.2
66 33.4 26.7 40.1









#10
Bis(2-Chloroethyl)ether
Concen: 20.217 ng/ul
RT: 7.122 min Scan# 703
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion: 93 Resp: 716668
Ion Ratio Lower Upper
93 100
63 67.2 56.3 84.5
95 32.5 25.2 37.8

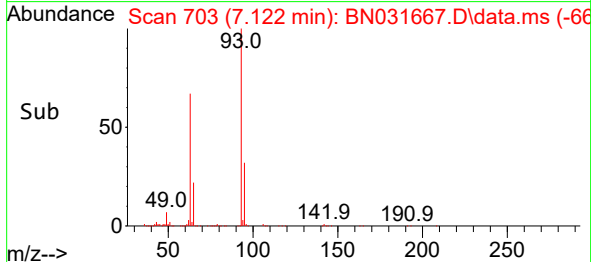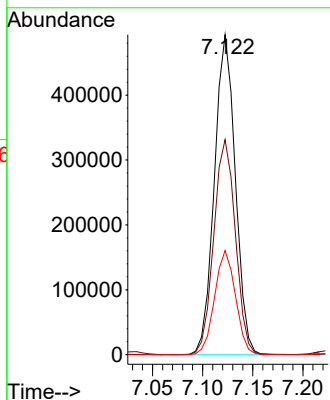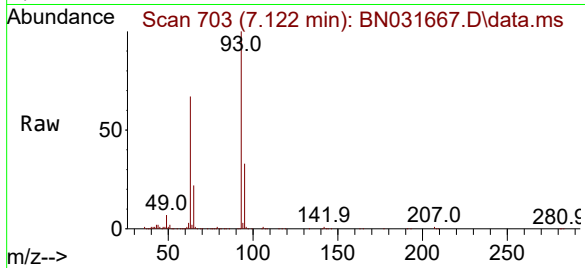

#12
2-Chlorophenol
Concen: 20.278 ng/ul
RT: 7.252 min Scan# 725
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:128 Resp: 681110
Ion Ratio Lower Upper
128 100
64 44.0 36.1 54.1
130 31.9 26.0 39.0



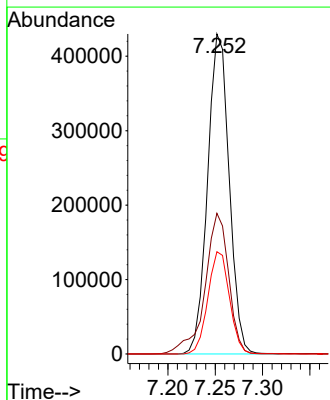
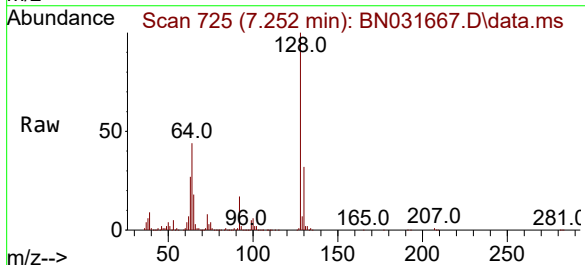




#13
2-Methylphenol
Concen: 19.619 ng/ul
RT: 8.128 min Scan# 873
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:108 Resp: 627812
Ion Ratio Lower Upper
108 100
107 90.0 71.0 106.6

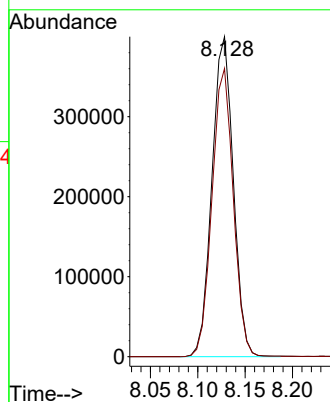

#14
2,2'-oxybis(1-Chloropropane)
Concen: 19.307 ng/ul
RT: 8.211 min Scan# 888
Delta R.T. -0.012 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion: 45 Resp: 790605
Ion Ratio Lower Upper
45 100
77 16.9 13.2 19.8
79 12.7 10.6 16.0



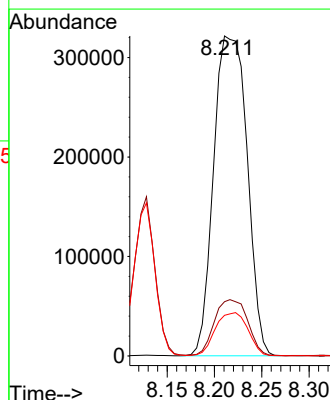





#16
Acetophenone
Concen: 19.531 ng/ul
RT: 8.511 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:105 Resp: 980246
Ion Ratio Lower Upper
105 100
77 72.9 60.7 91.1
51 21.6 18.6 28.0

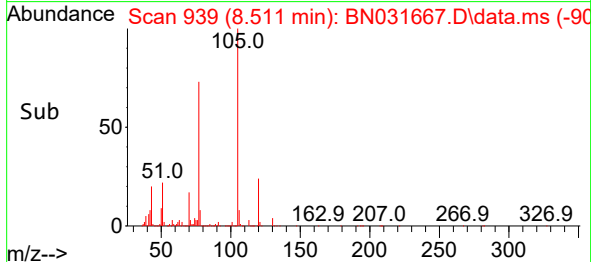

#17
N-Nitroso-di-n-propylamine
Concen: 18.228 ng/ul
RT: 8.493 min Scan# 936
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion: 70 Resp: 470007
Ion Ratio Lower Upper
70 100
42 48.0 38.2 57.4
101 10.1 8.1 12.1
130 21.7 17.7 26.5









#18
4-Methylphenol
Concen: 19.229 ng/ul
RT: 8.452 min Scan# 911
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:108 Resp: 653961
Ion Ratio Lower Upper
108 100
107 113.0 87.6 131.4

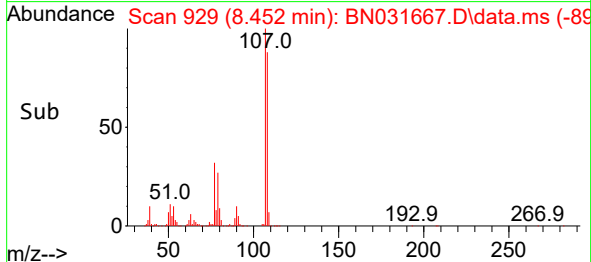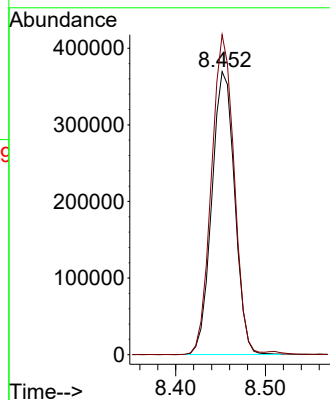

#19
Hexachloroethane
Concen: 19.855 ng/ul
RT: 8.758 min Scan# 981
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:117 Resp: 284947
Ion Ratio Lower Upper
117 100
201 93.8 72.6 109.0
199 60.2 45.6 68.4



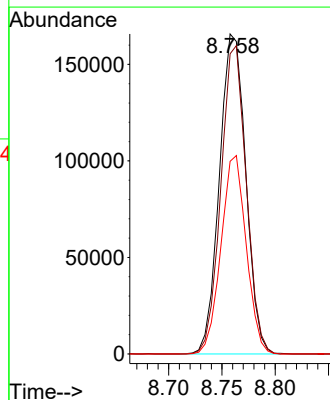
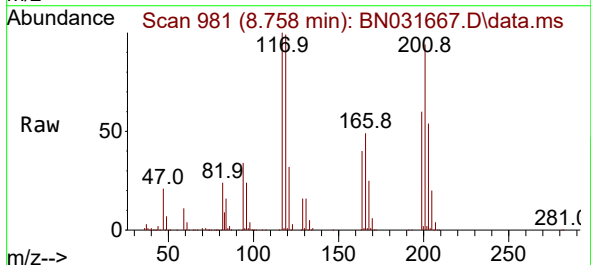




#22
Nitrobenzene
Concen: 20.379 ng/ul
RT: 8.887 min Scan# 1003
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion: 77 Resp: 739761
Ion Ratio Lower Upper
77 100
123 45.7 34.7 52.1
65 12.4 10.1 15.1



#23
Isophorone
Concen: 18.736 ng/ul
RT: 9.410 min Scan# 1092
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion: 82 Resp: 1293725
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.2
138 17.9 13.4 20.2









#25
2-Nitrophenol
Concen: 20.167 ng/ul
RT: 9.593 min Scan# 1123
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:139 Resp: 318064
Ion Ratio Lower Upper
139 100
65 48.6 38.6 58.0
109 30.7 23.2 34.8

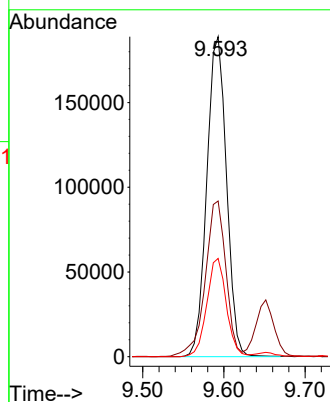

#26
2,4-Dimethylphenol
Concen: 19.650 ng/ul
RT: 9.652 min Scan# 1133
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:107 Resp: 633069
Ion Ratio Lower Upper
107 100
121 49.9 40.9 61.3
122 87.5 69.5 104.3

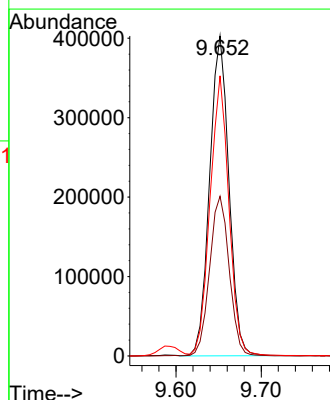



#27

Bis(2-Chloroethoxy)methane

Concen: 19.190 ng/ul

RT: 9.893 min Scan# 1174

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion: 93 Resp: 844703

Ion Ratio Lower Upper

93 100

95 32.3 26.2 39.2

123 11.3 9.1 13.7

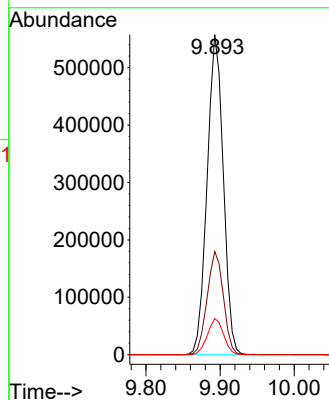

#29

2,4-Dichlorophenol

Concen: 19.474 ng/ul

RT: 10.116 min Scan# 1212

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion: 162 Resp: 534141


Ion Ratio Lower Upper

162 100

164 65.4 51.2 76.8

98 38.3 29.0 43.4



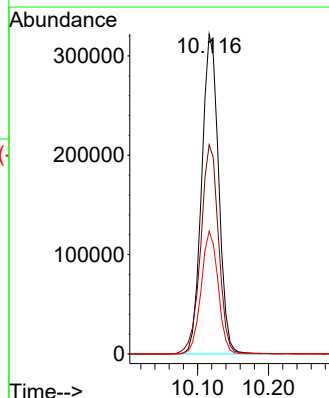



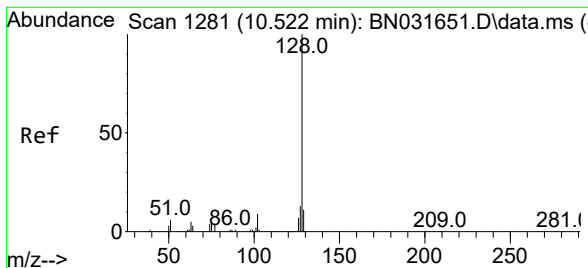

#30
Naphthalene
Concen: 19.841 ng/ul
RT: 10.522 min Scan# 1281
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:128 Resp: 1999237
Ion Ratio Lower Upper
128 100
129 10.6 8.8 13.2
127 13.0 10.2 15.2

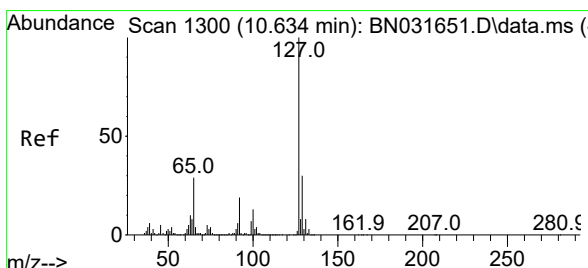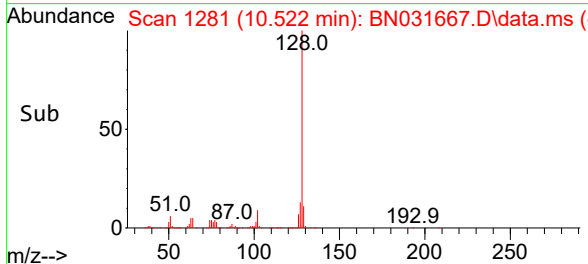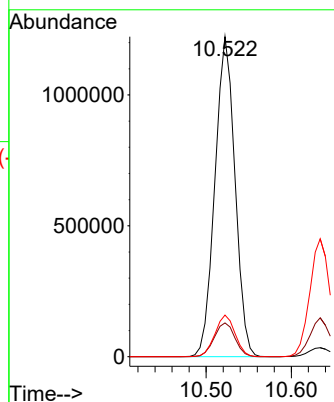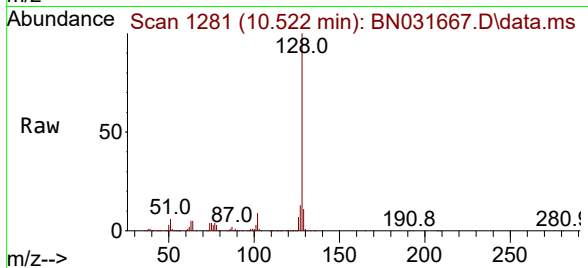

#32
4-Chloroaniline
Concen: 18.955 ng/ul
RT: 10.634 min Scan# 1300
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:127 Resp: 737627
Ion Ratio Lower Upper
127 100
129 33.0 25.8 38.6


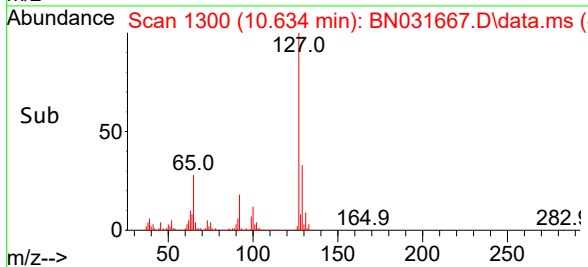
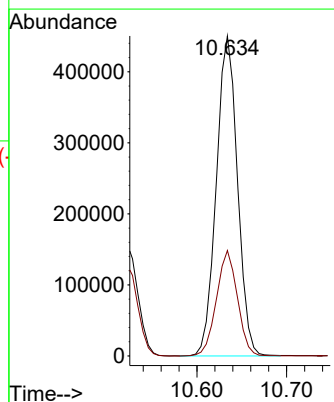
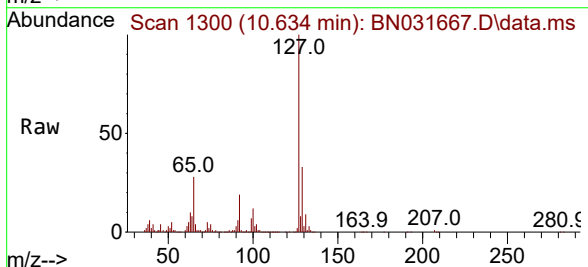




#33
Hexachlorobutadiene
Concen: 21.291 ng/ul
RT: 10.805 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:225 Resp: 357365
Ion Ratio Lower Upper
225 100
223 60.6 49.5 74.3
227 59.4 50.2 75.2

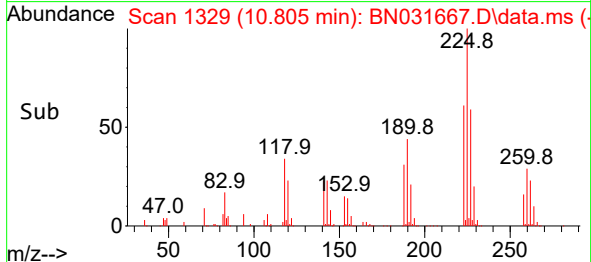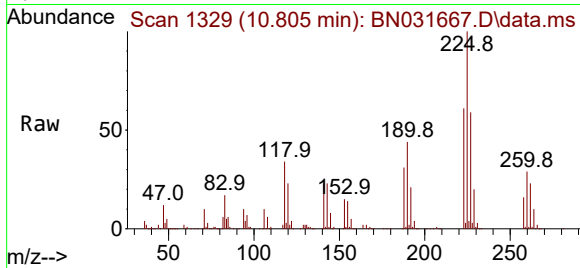

#34
Caprolactam
Concen: 16.948 ng/ul
RT: 11.393 min Scan# 1429
Delta R.T. -0.012 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:113 Resp: 150556
Ion Ratio Lower Upper
113 100
55 146.2 114.6 172.0
56 108.1 84.3 126.5




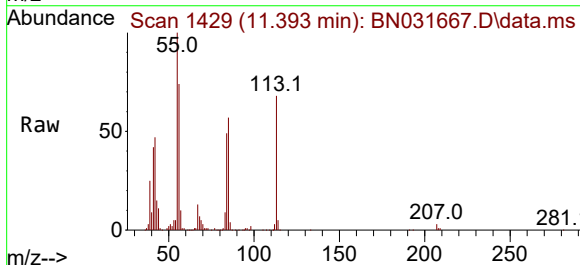




#35
4-Chloro-3-methylphenol
Concen: 17.692 ng/ul
RT: 11.757 min Scan# 1491
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:107 Resp: 526998
Ion Ratio Lower Upper
107 100
144 26.8 21.4 32.0
142 81.8 65.0 97.6

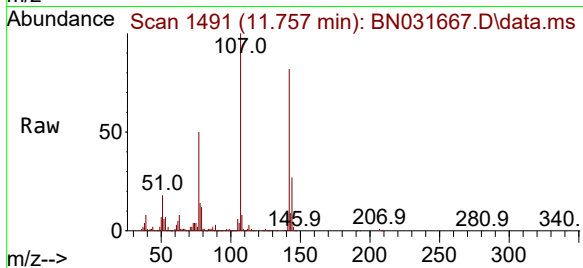

#36
2-Methylnaphthalene
Concen: 18.494 ng/ul
RT: 12.134 min Scan# 1555
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:142 Resp: 1219531
Ion Ratio Lower Upper
142 100
141 84.0 70.5 105.7


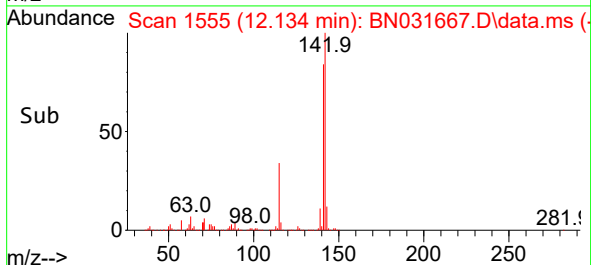

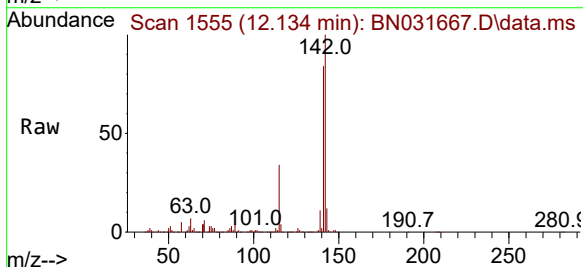


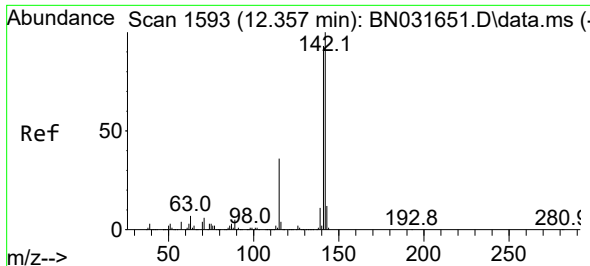

#37
1-Methylnaphthalene
Concen: 18.696 ng/ul
RT: 12.357 min Scan# 1593
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:142 Resp: 1220374
Ion Ratio Lower Upper
142 100
141 93.9 77.0 115.6
116 3.7 3.0 4.6

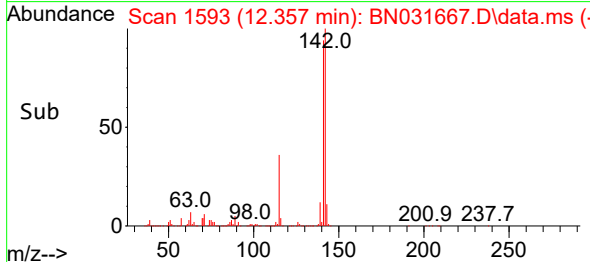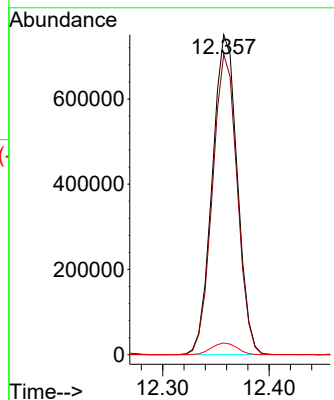

#39
1,2,4,5-Tetrachlorobenzene
Concen: 21.825 ng/ul
RT: 12.504 min Scan# 1618
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:216 Resp: 587625
Ion Ratio Lower Upper
216 100
214 74.8 64.0 96.0
179 20.5 16.8 25.2
108 18.8 15.5 23.3

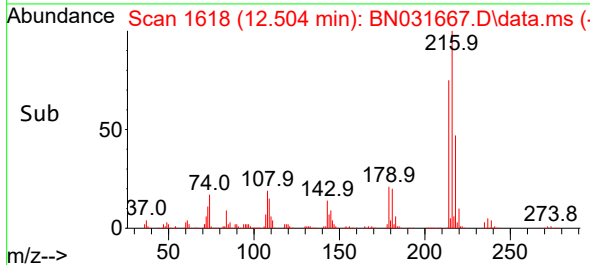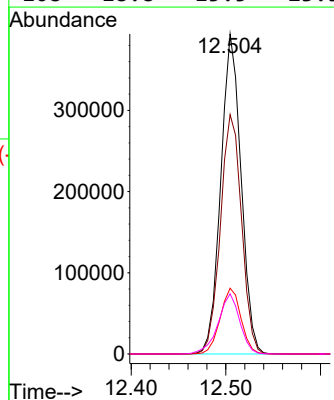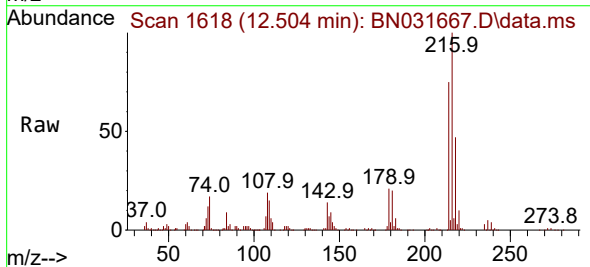



#40

Hexachlorocyclopentadiene

Concen: 15.476 ng/ul

RT: 12.487 min Scan# 1615

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:237 Resp: 249777

Ion Ratio Lower Upper

237 100

235 62.5 51.3 76.9

272 13.8 10.1 15.1

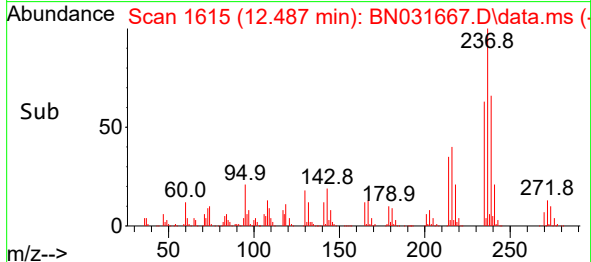

#41

2,4,6-Trichlorophenol

Concen: 21.113 ng/ul

RT: 12.751 min Scan# 1660

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:196 Resp: 351267


Ion Ratio Lower Upper

196 100

198 91.1 79.4 119.2


200 29.9 24.0 36.0

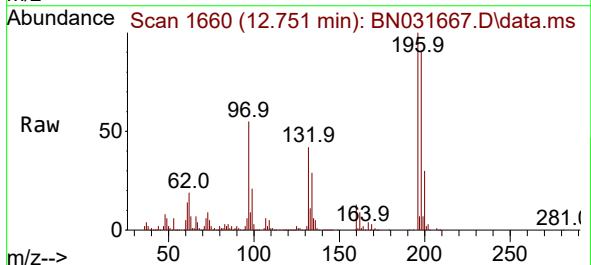






#42
2,4,5-Trichlorophenol
Concen: 20.570 ng/ul
RT: 12.816 min Scan# 1671
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Instrument :
BNA_N
ClientSampleId :
SSTD020262







Tgt Ion:196 Resp: 370480
Ion Ratio Lower Upper
196 100
198 94.0 71.9 107.9
200 29.4 23.2 34.8

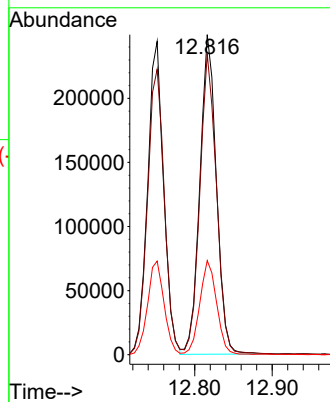

#43
1,1'-Biphenyl
Concen: 21.169 ng/ul
RT: 13.157 min Scan# 1729
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:154 Resp: 1451879
Ion Ratio Lower Upper
154 100
153 39.6 32.6 48.8
76 13.4 11.3 16.9

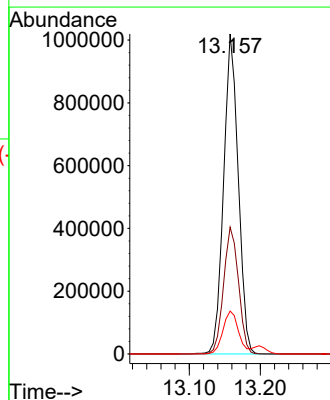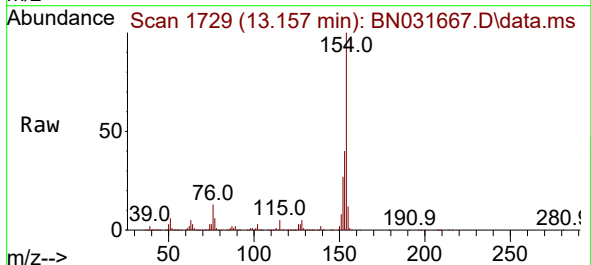



#44

2-Chloronaphthalene

Concen: 21.132 ng/ul

RT: 13.198 min Scan# 1736

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:162 Resp: 1147635

Ion Ratio Lower Upper

162 100

164 34.0 26.6 39.8

127 40.5 30.8 46.2



#45

2-Nitroaniline

Concen: 19.793 ng/ul

RT: 13.404 min Scan# 1771

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion: 65 Resp: 281395


Ion Ratio Lower Upper

65 100

92 76.3 60.2 90.4

138 110.0 88.6 132.8







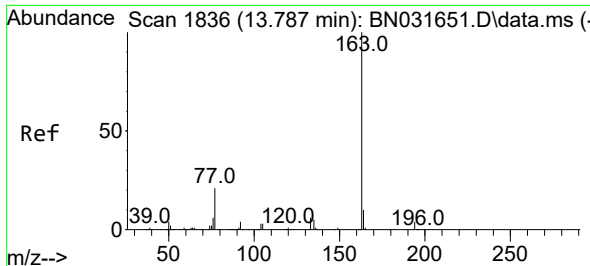

#47
Dimethylphthalate
Concen: 20.355 ng/ul
RT: 13.787 min Scan# 1836
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:163 Resp: 1245293
Ion Ratio Lower Upper
163 100
194 3.8 3.2 4.8
164 10.2 7.8 11.6

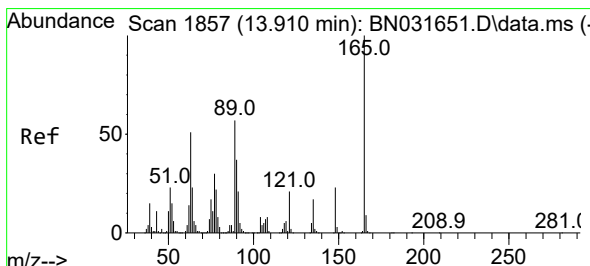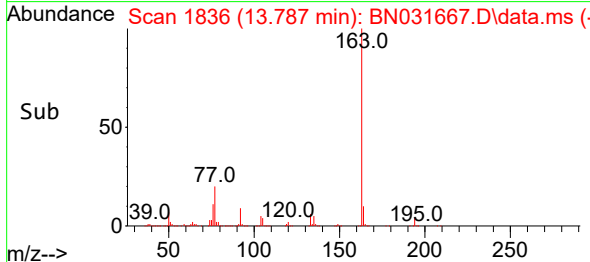

#48
2,6-Dinitrotoluene
Concen: 19.873 ng/ul
RT: 13.910 min Scan# 1857
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:165 Resp: 231704
Ion Ratio Lower Upper
165 100
89 55.3 47.0 70.6
121 21.9 18.7 28.1


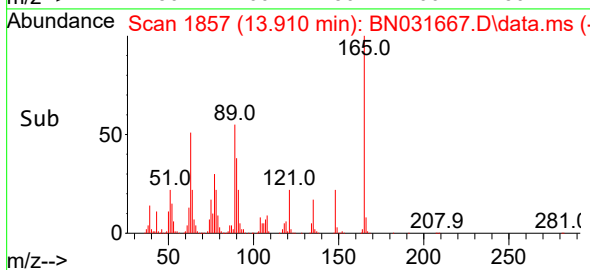

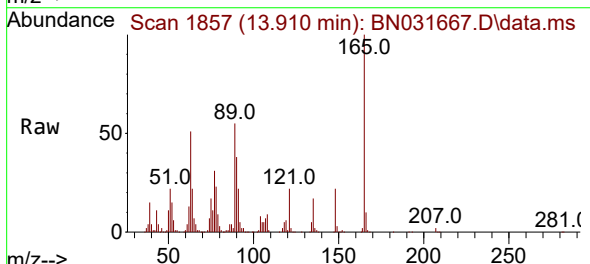


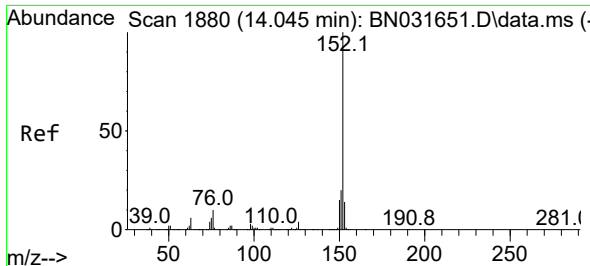

#50
Acenaphthylene
Concen: 20.584 ng/ul
RT: 14.046 min Scan# 1880
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:152 Resp: 1785526
Ion Ratio Lower Upper
152 100
151 19.5 15.6 23.4
153 13.2 10.8 16.2

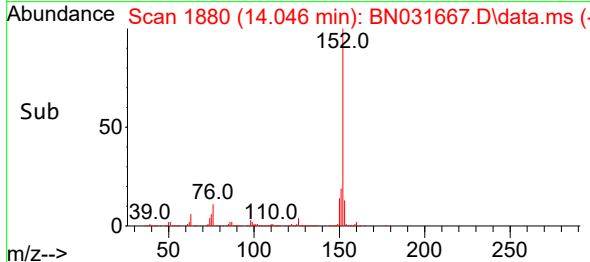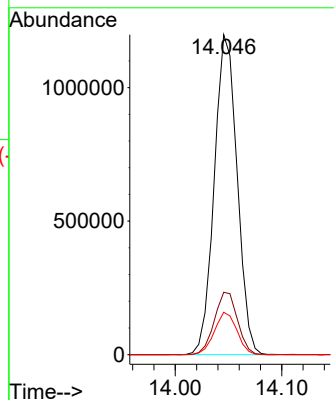

#51
3-Nitroaniline
Concen: 20.315 ng/ul
RT: 14.234 min Scan# 1912
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:138 Resp: 268853
Ion Ratio Lower Upper
138 100
108 12.9 10.7 16.1
92 114.7 94.6 141.8


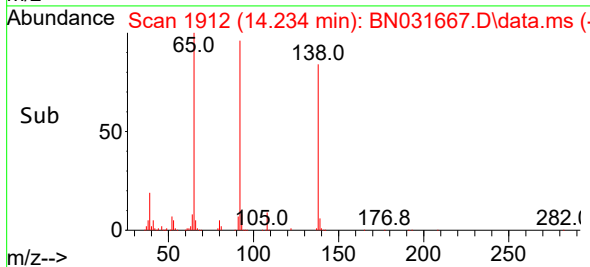
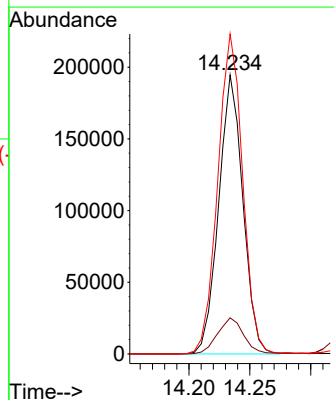
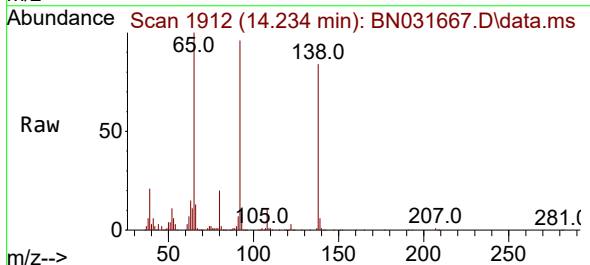




#52
Acenaphthene
Concen: 20.431 ng/ul
RT: 14.393 min Scan# 1939
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:153 Resp: 1148288
Ion Ratio Lower Upper
153 100
152 48.0 40.5 60.7
154 88.5 76.6 114.8

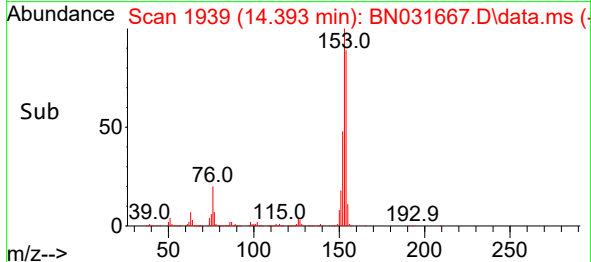

#53
2,4-Dinitrophenol
Concen: 13.568 ng/ul
RT: 14.440 min Scan# 1947
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:184 Resp: 72646
Ion Ratio Lower Upper
184 100
63 60.4 50.7 76.1
154 62.0 49.1 73.7









#55
4-Nitrophenol
Concen: 18.626 ng/ul
RT: 14.540 min Scan# 1964
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:109 Resp: 159200
Ion Ratio Lower Upper
109 100
139 147.5 113.8 170.6
65 126.0 101.1 151.7

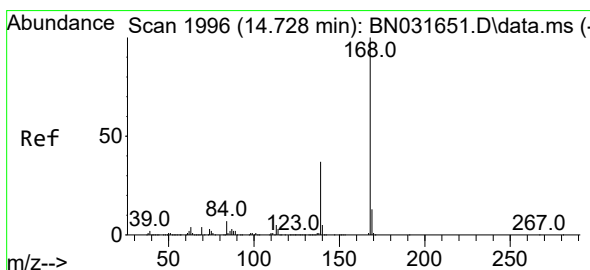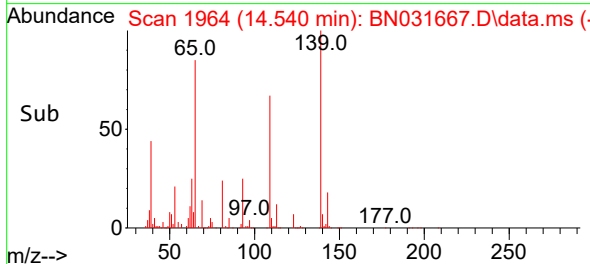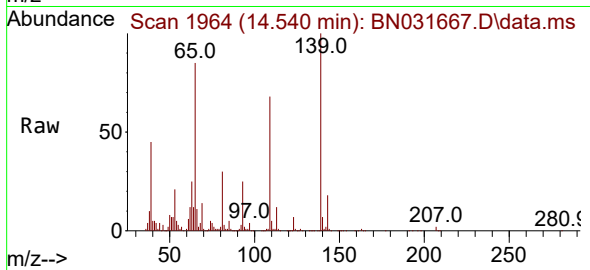

#56
Dibenzofuran
Concen: 19.832 ng/ul
RT: 14.728 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:168 Resp: 1487949
Ion Ratio Lower Upper
168 100
139 37.6 29.2 43.8




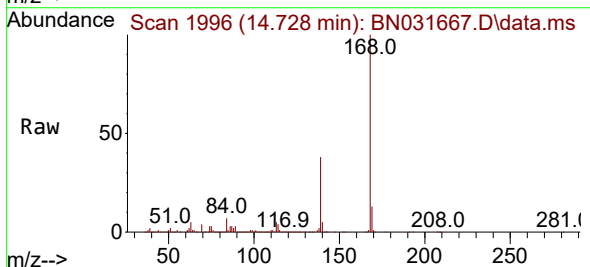


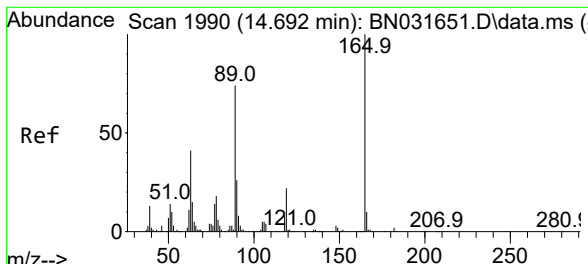

#57
 2,4-Dinitrotoluene
 Concen: 19.497 ng/ul
 RT: 14.693 min Scan# 1990
 Delta R.T. 0.000 min
 Lab File: BN031667.D
 Acq: 24 May 2024 18:58




Instrument :
 BNA_N
 ClientSampleId :
 SST020262


Tgt Ion:	165	Resp:	304541
Ion Ratio	Lower	Upper	
165	100		
63	42.2	35.1	52.7
182	3.0	2.4	3.6

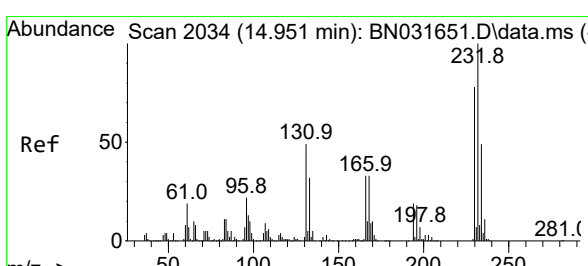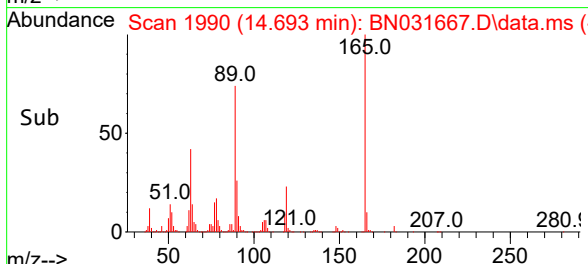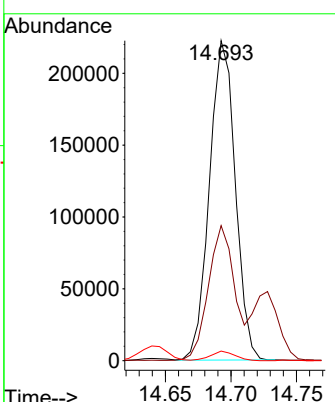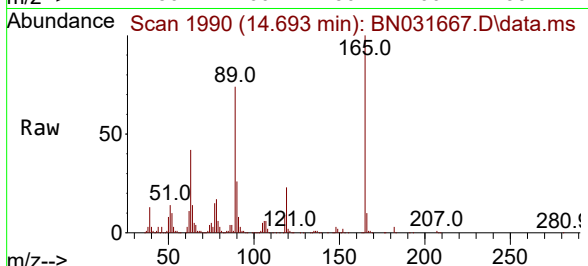

#58
 2,3,4,6-Tetrachlorophenol
 Concen: 19.869 ng/ul
 RT: 14.951 min Scan# 2034
 Delta R.T. 0.000 min
 Lab File: BN031667.D
 Acq: 24 May 2024 18:58

Tgt Ion:	232	Resp:	259950
Ion Ratio	Lower	Upper	
232	100		
131	45.8	39.2	58.8
130	2.3	2.1	3.1
166	30.8	26.3	39.5


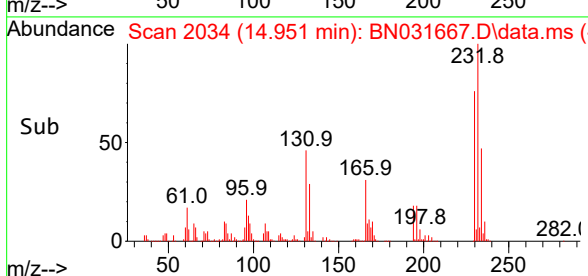
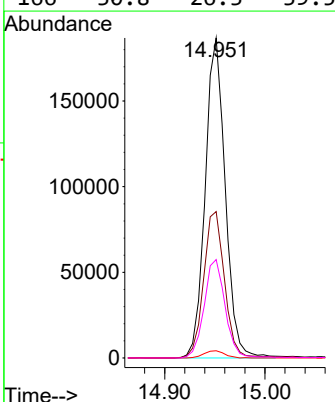
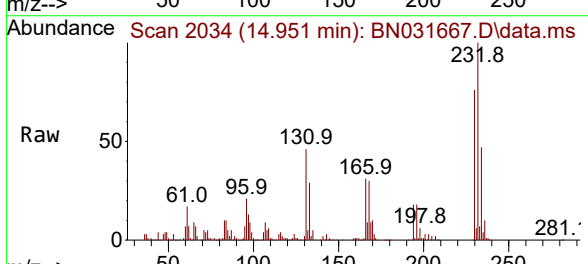


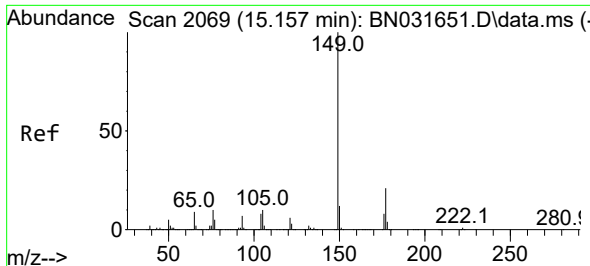

#59
Diethylphthalate
Concen: 19.924 ng/ul
RT: 15.157 min Scan# 2069
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:149 Resp: 1148556
Ion Ratio Lower Upper
149 100
177 22.4 16.3 24.5
150 12.8 10.0 15.0

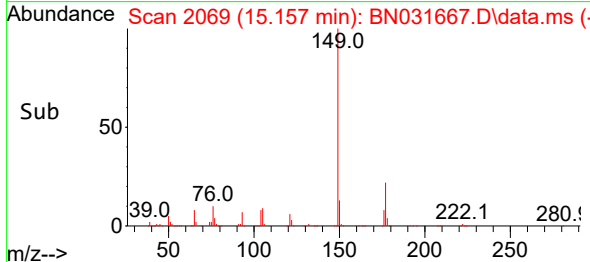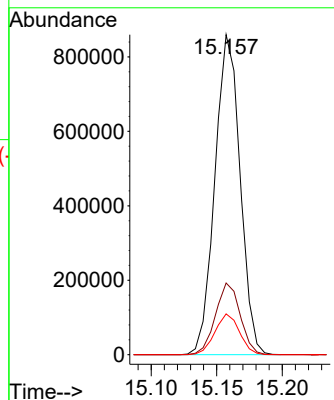

#61
Fluorene
Concen: 19.804 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:166 Resp: 1163945
Ion Ratio Lower Upper
166 100
165 95.5 77.0 115.6
167 13.5 10.9 16.3


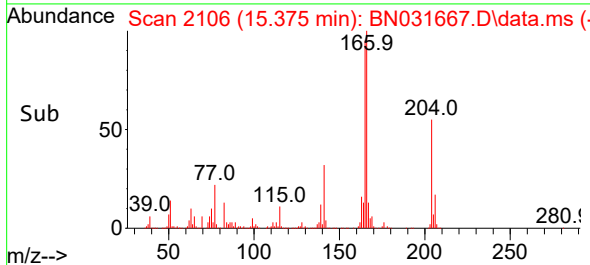
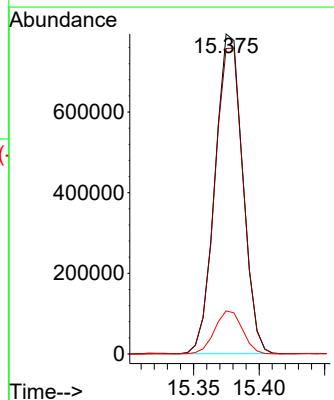
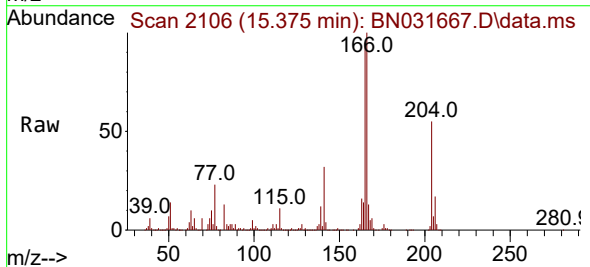


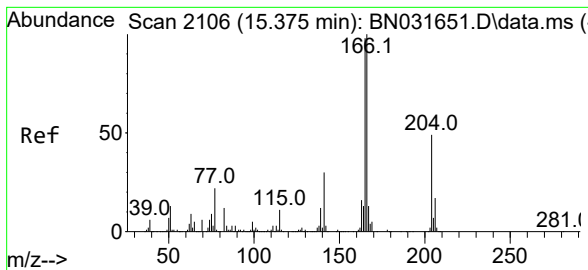

#62
4-Chlorophenyl-phenylether
Concen: 19.862 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:204 Resp: 561971
Ion Ratio Lower Upper
204 100
206 30.9 25.8 38.8
141 57.7 46.5 69.7

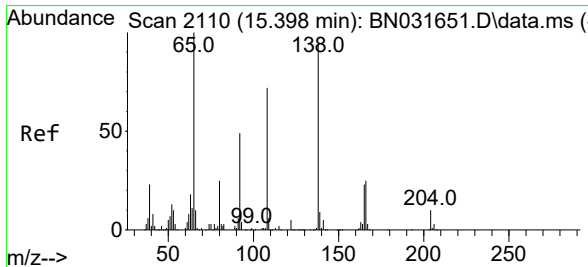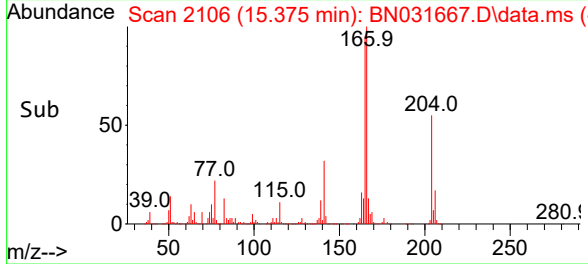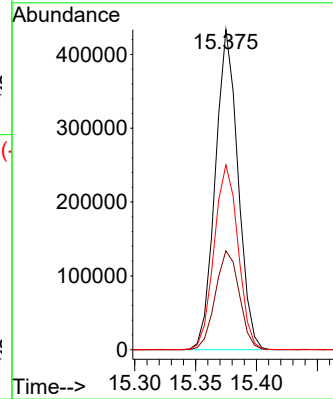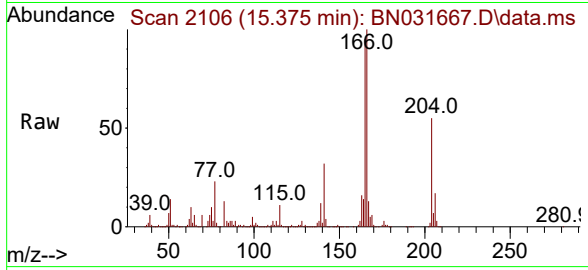

#63
4-Nitroaniline
Concen: 22.140 ng/ul
RT: 15.398 min Scan# 2110
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:138 Resp: 262779
Ion Ratio Lower Upper
138 100
92 51.8 40.7 61.1
108 74.5 57.1 85.7


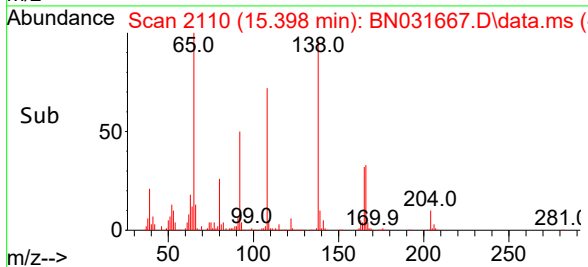
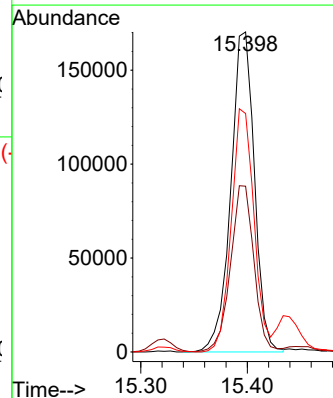
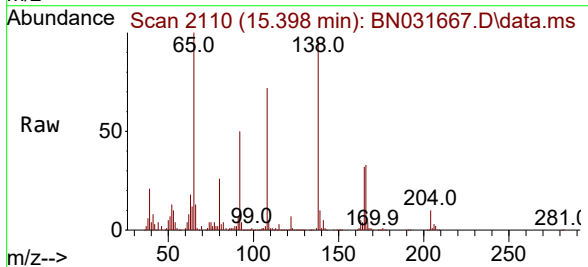


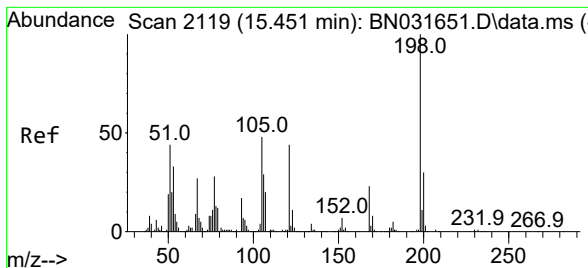

#66
4,6-Dinitro-2-methylphenol
Concen: 15.865 ng/ul
RT: 15.451 min Scan# 2119
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:198 Resp: 119579
Ion Ratio Lower Upper
198 100
182 4.3 3.9 5.9
77 27.3 24.2 36.2

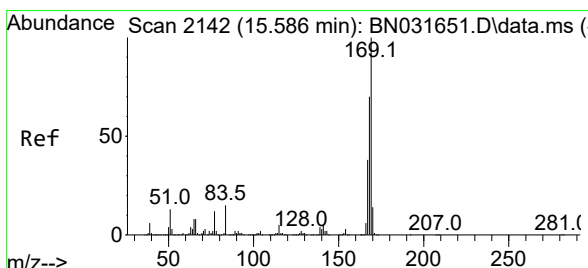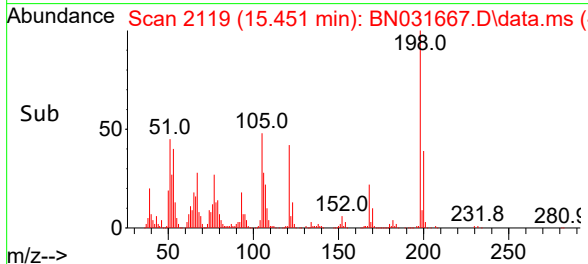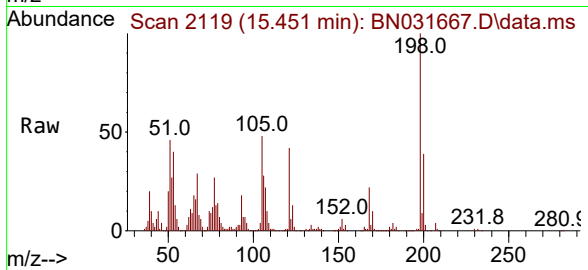

#67
N-Nitrosodiphenylamine
Concen: 20.230 ng/ul
RT: 15.587 min Scan# 2142
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:169 Resp: 946712
Ion Ratio Lower Upper
169 100
168 66.5 52.5 78.7
167 35.6 29.8 44.8


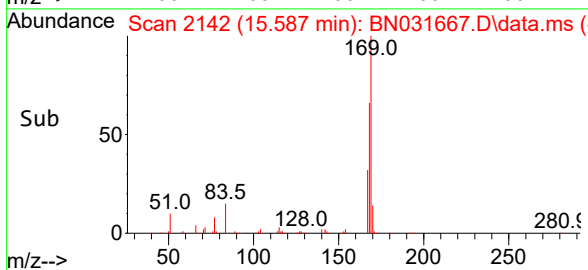

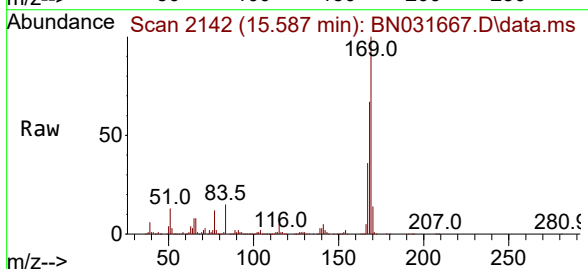




#68
4-Bromophenyl-phenylether
Concen: 19.377 ng/ul
RT: 16.269 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:248 Resp: 310147
Ion Ratio Lower Upper
248 100
250 98.9 79.6 119.4
141 79.2 61.4 92.0



#69
Hexachlorobenzene
Concen: 19.560 ng/ul
RT: 16.375 min Scan# 2276
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:284 Resp: 337891
Ion Ratio Lower Upper
284 100
142 34.2 33.0 49.4
249 26.9 26.4 39.6

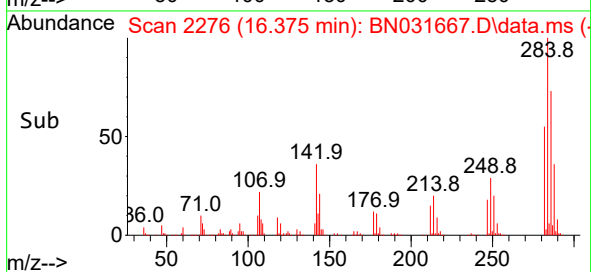



#70

Atrazine

Concen: 20.107 ng/ul

RT: 16.540 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:200 Resp: 253237

Ion Ratio Lower Upper

200 100

173 26.2 22.1 33.1

215 44.9 39.4 59.0



#71

Pentachlorophenol

Concen: 19.799 ng/ul

RT: 16.716 min Scan# 2334

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:266 Resp: 195085


Ion Ratio Lower Upper

266 100

264 58.8 45.8 68.6

268 55.9 47.4 71.0







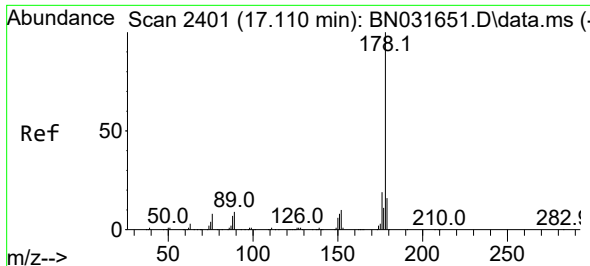

#72
Phenanthrene
Concen: 20.266 ng/ul
RT: 17.116 min Scan# 2401
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:178 Resp: 1635021
Ion Ratio Lower Upper
178 100
179 14.6 12.6 18.8
176 20.2 15.2 22.8

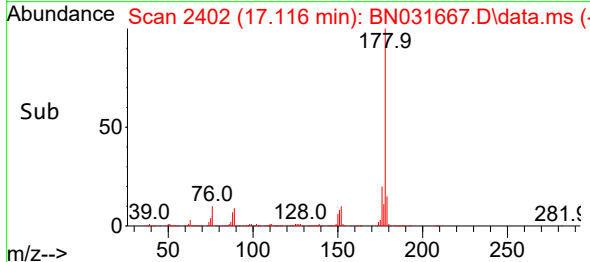

#74
Anthracene
Concen: 20.108 ng/ul
RT: 17.204 min Scan# 2417
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:178 Resp: 1627653
Ion Ratio Lower Upper
178 100
179 16.0 11.9 17.9
176 18.0 15.4 23.2

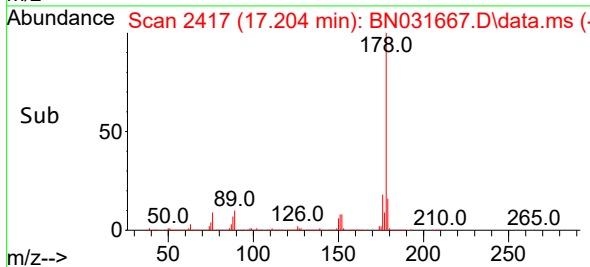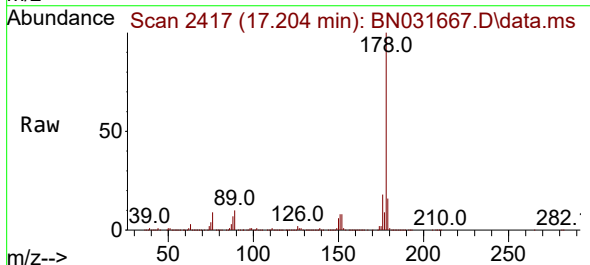



#75

1,2,3,4-Tetrachlorobenzene

Concen: 21.775 ng/uL

RT: 13.116 min Scan# 11

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:216 Resp: 550287

Ion Ratio Lower Upper

216 100

214 77.2 61.7 92.5

218 45.9 39.0 58.6



#76

Pentachlorobenzene

Concen: 20.094 ng/uL

RT: 14.640 min Scan# 1981

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:250 Resp: 459832


Ion Ratio Lower Upper

250 100

248 70.8 47.3 70.9

252 68.2 51.0 76.4









#77
 Carbazole
 Concen: 21.554 ng/ul
 RT: 17.475 min Scan# 2463
 Delta R.T. 0.000 min
 Lab File: BN031667.D
 Acq: 24 May 2024 18:58

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020262

Tgt Ion:167 Resp: 1488830




Ion	Ratio	Lower	Upper
167	100		
166	21.2	16.7	25.1
139	12.9	10.5	15.7

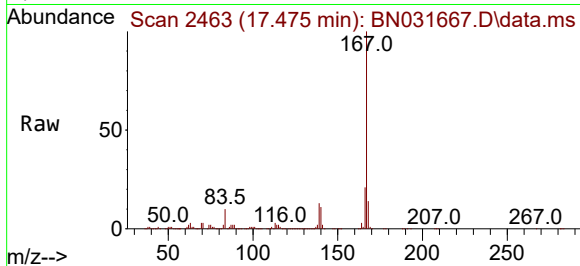


#78
 Di-n-butylphthalate
 Concen: 20.994 ng/ul
 RT: 18.045 min Scan# 2560
 Delta R.T. -0.006 min
 Lab File: BN031667.D
 Acq: 24 May 2024 18:58

Tgt Ion:149 Resp: 1665094

Ion	Ratio	Lower	Upper
149	100		
150	9.0	7.0	10.6
104	4.8	4.2	6.2

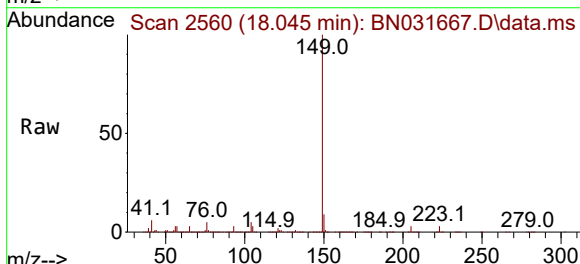



#80

Fluoranthene

Concen: 16.264 ng/ul

RT: 19.133 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:202 Resp: 1804694

Ion Ratio Lower Upper

202 100

101 12.1 10.1 15.1

100 9.4 8.0 12.0



#82

Pyrene

Concen: 16.411 ng/ul

RT: 19.498 min Scan# 2807

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:202 Resp: 1867590


Ion Ratio Lower Upper

202 100

101 14.4 11.4 17.2

100 11.9 9.3 13.9





#83

Butylbenzylphthalate

Concen: 18.600 ng/ul

RT: 20.410 min Scan# 2961

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:149 Resp: 718361

Ion Ratio Lower Upper

149 100

91 69.3 60.8 91.2

206 20.4 15.8 23.8

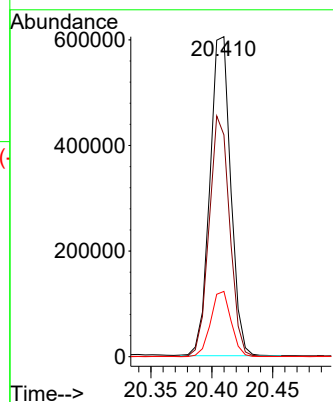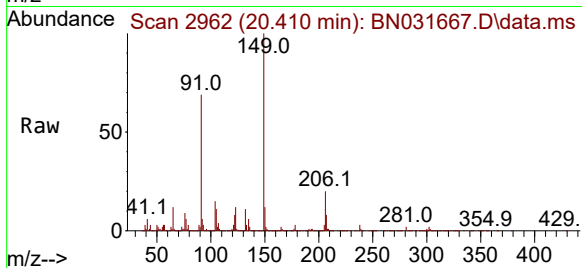

#84

3,3'-Dichlorobenzidine

Concen: 20.245 ng/ul

RT: 21.216 min Scan# 3099

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:252 Resp: 557140


Ion Ratio Lower Upper

252 100

254 63.0 51.4 77.0

126 13.2 10.6 15.8

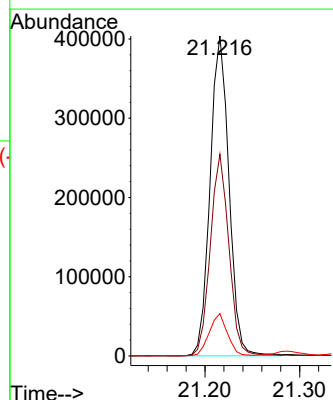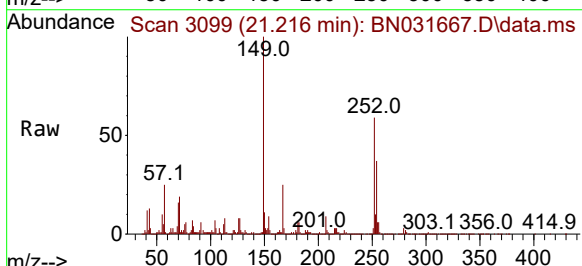



#85

Benzo(a)anthracene

Concen: 19.780 ng/ul

RT: 21.286 min Scan# 3111

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:228 Resp: 1903662

Ion Ratio Lower Upper

228 100

229 20.6 15.7 23.5

226 28.0 21.9 32.9

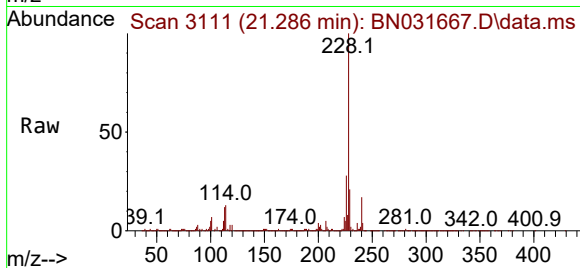

#86

Bis(2-ethylhexyl)phthalate

Concen: 19.082 ng/ul

RT: 21.222 min Scan# 3100

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:149 Resp: 1009090


Ion Ratio Lower Upper

149 100

167 28.3 21.6 32.4

279 3.7 2.8 4.2




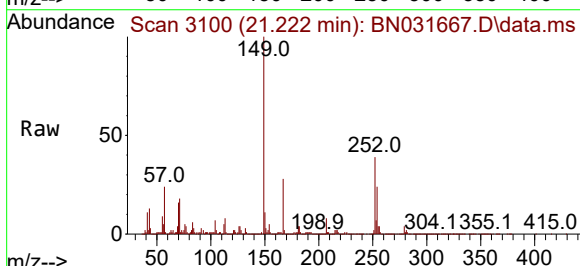




#87
Chrysene
Concen: 20.319 ng/ul
RT: 21.345 min Scan# 3121
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58




Instrument :
BNA_N
ClientSampleId :
SSTD020262


Tgt Ion:228 Resp: 1806356
Ion Ratio Lower Upper
228 100
226 27.9 22.9 34.3
229 18.4 15.2 22.8

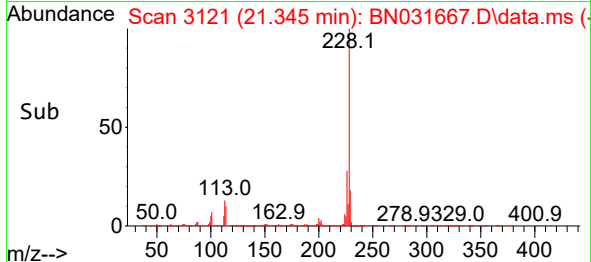

#89
Di-n-octyl phthalate
Concen: 17.543 ng/ul
RT: 22.339 min Scan# 3290
Delta R.T. 0.000 min
Lab File: BN031667.D
Acq: 24 May 2024 18:58

Tgt Ion:149 Resp: 1761899

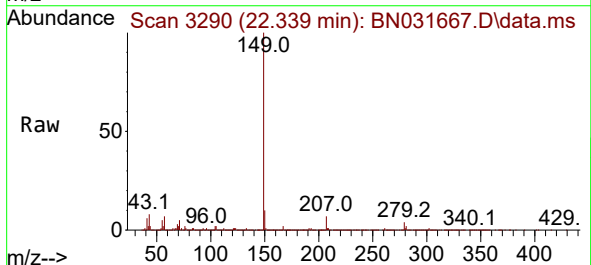



#90

Benzo(b)fluoranthene

Concen: 19.259 ng/ul

RT: 23.310 min Scan# 3455

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:252 Resp: 1974958

Ion Ratio Lower Upper

252 100

253 22.0 16.8 25.2

125 12.2 9.3 13.9



#91

Benzo(k)fluoranthene

Concen: 19.553 ng/ul

RT: 23.374 min Scan# 3466

Delta R.T. 0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:252 Resp: 2043843


Ion Ratio Lower Upper

252 100

253 22.6 17.4 26.0

125 12.0 9.3 13.9





#93

Benzo(a)pyrene

Concen: 19.749 ng/ul

RT: 24.098 min Scan# 3589

Delta R.T. -0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:252 Resp: 1945293

Ion Ratio Lower Upper

252 100

253 22.1 16.6 24.8

125 13.9 9.8 14.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 10.147 ng/ul

RT: 27.533 min Scan# 4173

Delta R.T. 0.000 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58




Tgt Ion:276 Resp: 1199562


Ion Ratio Lower Upper

276 100

138 22.6 19.8 29.6

277 22.8 18.2 27.4





#95

Dibenzo(a,h)anthracene

Concen: 20.265 ng/ul

RT: 27.598 min Scan# 4184

Delta R.T. 0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Instrument :

BNA_N

ClientSampleId :

SSTD020262





Tgt Ion:278 Resp: 1972894

Ion Ratio Lower Upper

278 100

139 19.2 15.2 22.8

279 22.2 18.4 27.6

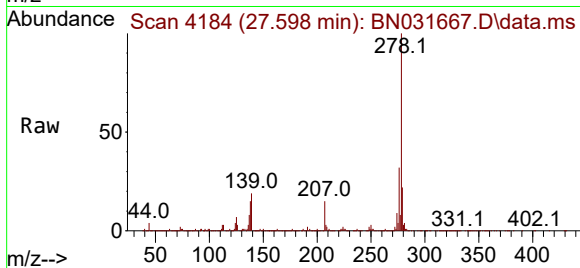

#96

Benzo(g,h,i)perylene

Concen: 19.787 ng/ul

RT: 28.562 min Scan# 4348

Delta R.T. 0.006 min

Lab File: BN031667.D

Acq: 24 May 2024 18:58

Tgt Ion:276 Resp: 1932722

Ion Ratio Lower Upper

276 100

138 26.5 19.5 29.3

277 22.0 17.6 26.4

