

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052424\
 Data File : BN031652.D
 Acq On : 24 May 2024 09:04
 Operator : MA/JU
 Sample : PB161058BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	33	37	50	rVB	184144	268729	2.10%	0.167%
2	3.605	102	105	124	rBV	2402699	3735085	29.18%	2.320%
3	3.928	155	160	167	rVB	42429	66142	0.52%	0.041%
4	6.852	650	657	674	rVV	2894183	4679594	36.55%	2.907%
5	7.028	678	687	700	rVB	2441691	3898625	30.45%	2.422%
6	7.222	712	720	734	rBV	2877020	4686790	36.61%	2.912%
7	7.687	791	799	809	rBV	2427164	3963700	30.96%	2.462%
8	8.387	907	918	932	rBV	3734865	5998573	46.86%	3.726%
9	8.846	987	996	1007	rBV	2822938	4641504	36.26%	2.883%
10	9.558	1108	1117	1132	rBV	2172240	3578045	27.95%	2.223%
11	10.087	1198	1207	1222	rBV	3458769	5890264	46.01%	3.659%
12	10.469	1264	1272	1283	rVB	3654430	6147224	48.02%	3.819%
13	10.610	1287	1296	1312	rBV	3747538	6373823	49.79%	3.960%
14	12.063	1536	1543	1550	rVB	68458	115158	0.90%	0.072%
15	13.228	1734	1741	1747	rBV	33699	55958	0.44%	0.035%
16	13.293	1747	1752	1758	rVB3	9839	16109	0.13%	0.010%
17	13.740	1820	1828	1839	rBV	5767436	8520877	66.56%	5.293%
18	14.016	1867	1875	1887	rBV	6834523	10751742	83.98%	6.679%
19	14.328	1920	1928	1935	rBV	5458383	8154121	63.69%	5.065%
20	14.410	1938	1942	1946	rVB6	9802	13801	0.11%	0.009%
21	14.522	1953	1961	1977	rBV	2921222	4168455	32.56%	2.590%
22	14.746	1995	1999	2003	rVB4	10581	16358	0.13%	0.010%
23	15.322	2090	2097	2110	rBV	8799662	12621186	98.59%	7.841%
24	15.434	2110	2116	2130	rVV	1919183	2724117	21.28%	1.692%
25	15.557	2132	2137	2144	rVB	42027	70410	0.55%	0.044%
26	16.098	2226	2229	2237	rVB4	9711	16503	0.13%	0.010%
27	16.751	2336	2340	2343	rBV3	12419	13334	0.10%	0.008%
28	16.857	2354	2358	2362	rVB2	12763	18920	0.15%	0.012%
29	17.069	2387	2394	2404	rBV	6124642	8836342	69.02%	5.489%
30	17.169	2404	2411	2425	rVB2	8756900	12802255	100.00%	7.953%
31	17.310	2431	2435	2443	rBV7	13561	26245	0.21%	0.016%
32	17.445	2453	2458	2462	rBV4	12293	19922	0.16%	0.012%
33	18.298	2599	2603	2607	rBV6	7914	12955	0.10%	0.008%
34	19.028	2722	2727	2734	rBV2	105232	146823	1.15%	0.091%
35	19.098	2734	2739	2744	rBV	101311	139665	1.09%	0.087%
36	19.169	2749	2751	2755	rVB4	12055	12997	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052424\
Data File : BN031652.D
Acq On : 24 May 2024 09:04
Operator : MA/JU
Sample : PB161058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION

37	19.410	2789	2792	2795	rBV3	30208	34455	0.27%	0.021%
38	19.469	2795	2802	2813	rVV	8644793	12528363	97.86%	7.783%
39	20.457	2968	2970	2976	rVB5	27449	30436	0.24%	0.019%
40	21.298	3107	3113	3126	rBV2	4493438	6809668	53.19%	4.230%
41	24.033	3569	3578	3596	rVB2	4553509	11030903	86.16%	6.853%
42	24.233	3603	3612	3630	rBV	2942265	7337758	57.32%	4.558%




Sum of corrected areas: 160973934

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052424\
Data File : BN031652.D
Acq On : 24 May 2024 09:04
Operator : MA/JU
Sample : PB161058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

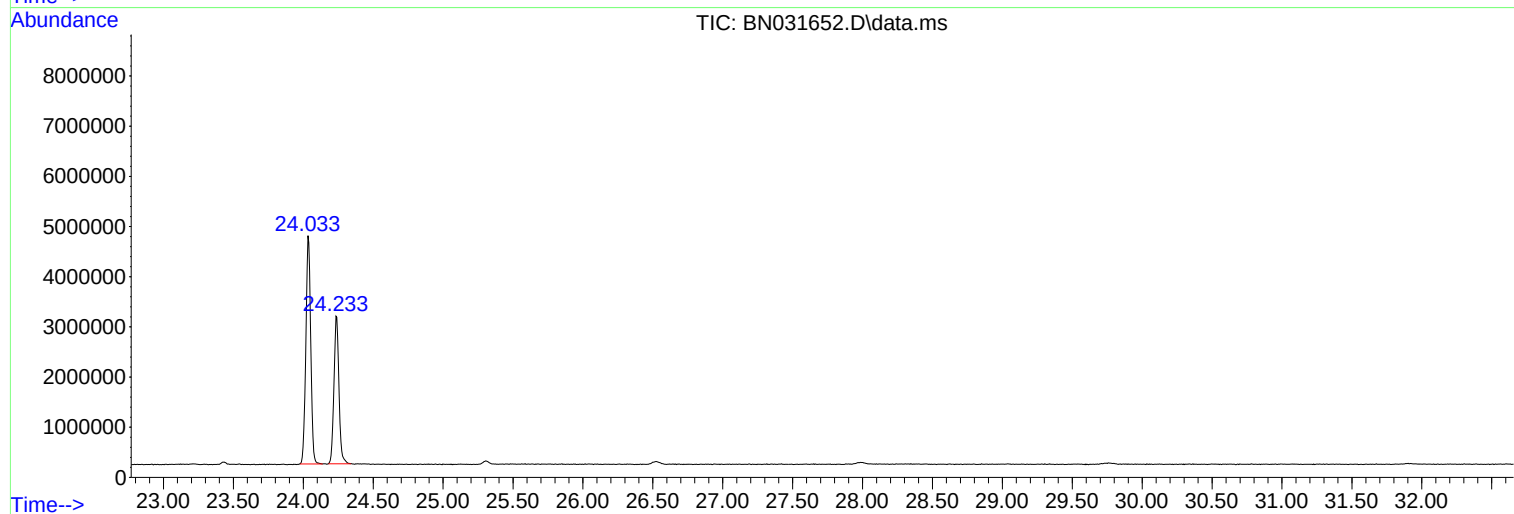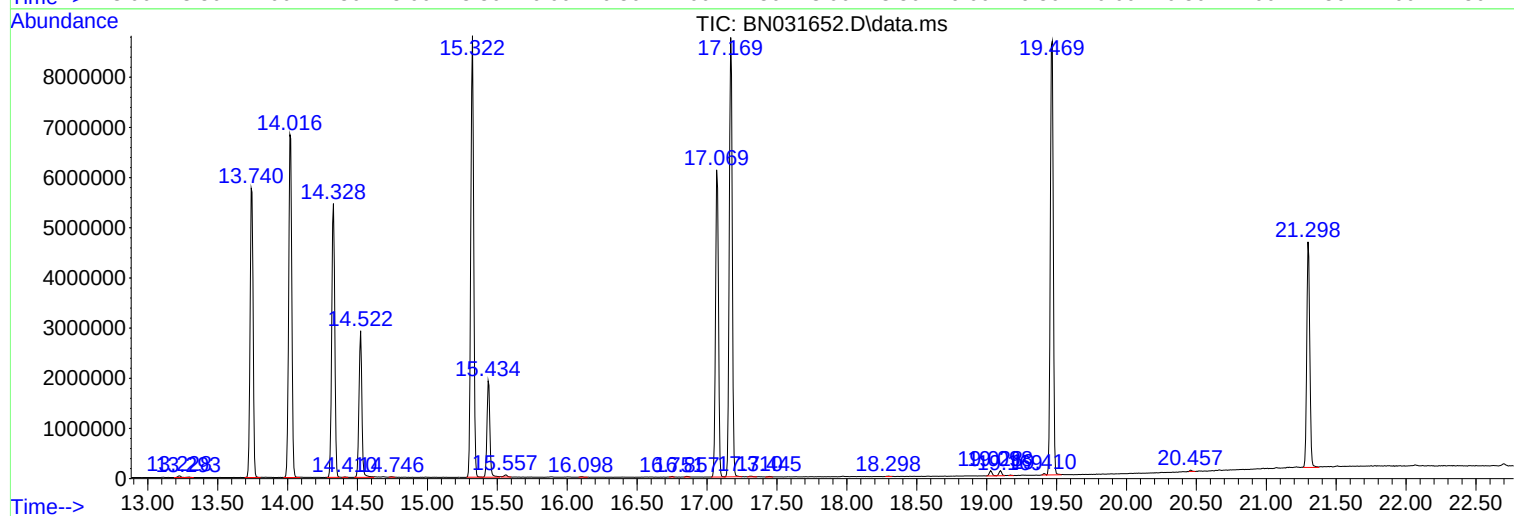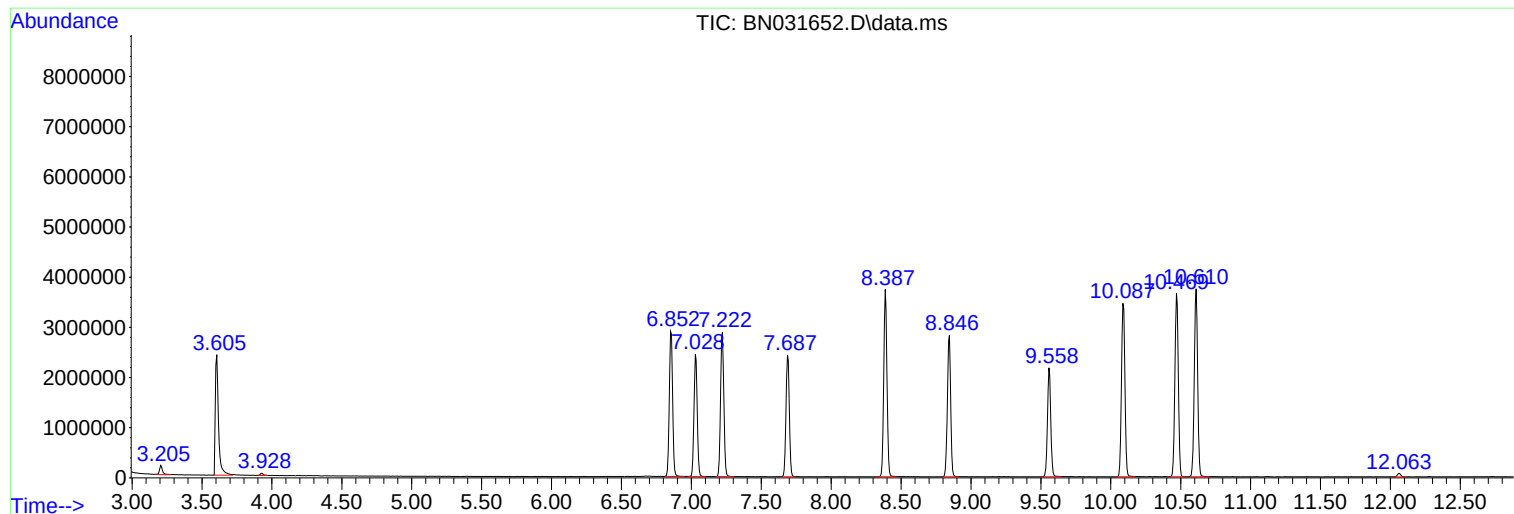

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052424\
Data File : BN031652.D
Acq On : 24 May 2024 09:04
Operator : MA/JU
Sample : PB161058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052424\
Data File : BN031652.D
Acq On : 24 May 2024 09:04
Operator : MA/JU
Sample : PB161058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------