


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052521\
Data File : BN014758.D
Acq On : 26 May 2021 05:31
Operator : CG/JU
Sample : M2493-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
GB431

Quant Time: May 26 06:15:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
5/26/2021 4:28:13 PM

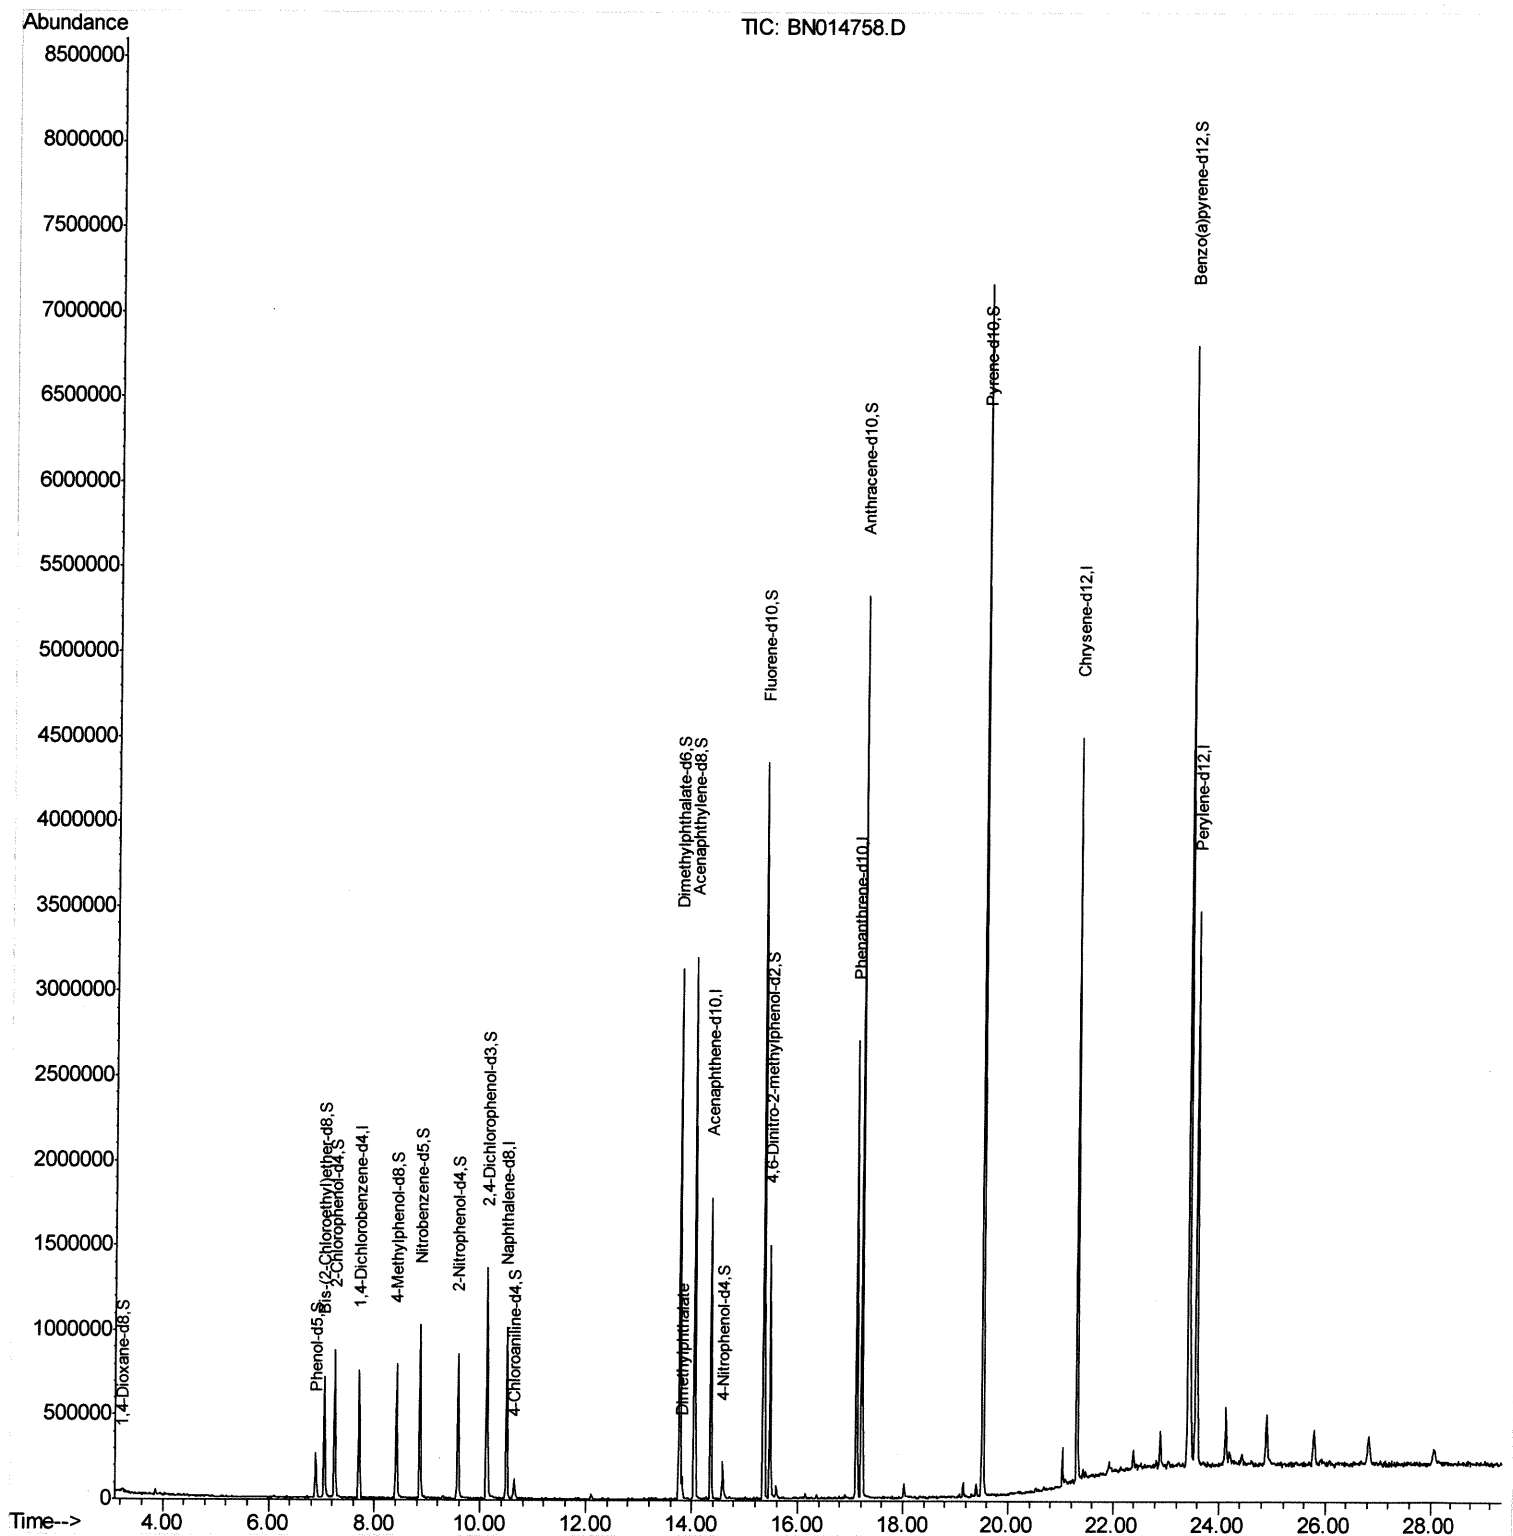


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052521\
 Data File : BN014758.D
 Acq On : 26 May 2021 05:31
 Operator : CG/JU
 Sample : M2493-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB431

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:13 PM

Quant Time: May 26 06:13:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

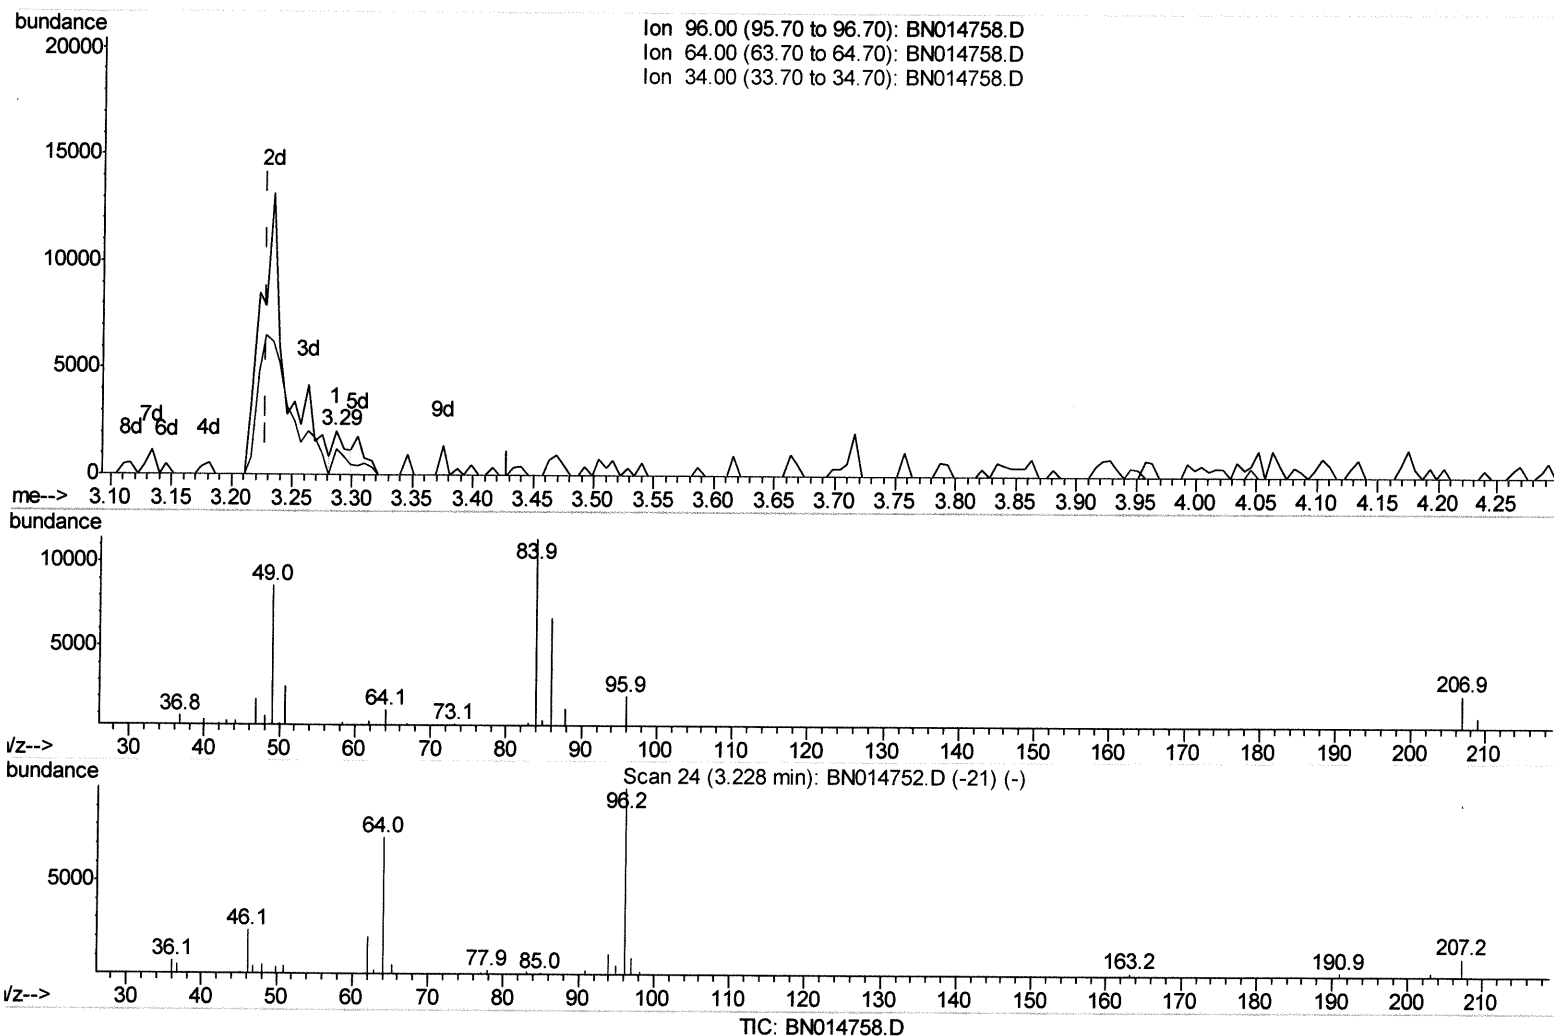

(3) 1,4-Dioxane-d8 (S)

3.287min (+0.058) 0.35ng/uL

response 1542

Ion	Exp%	Act%
96.00	100	100
64.00	64.30	58.85
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052521\
Data File : BN014758.D
Acq On : 26 May 2021 05:31
Operator : CG/JU
Sample : M2493-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB431

Manual Integrations
APPROVED

mohammad
5/26/2021 4:28:13 PM

Quant Time: May 26 06:13:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration

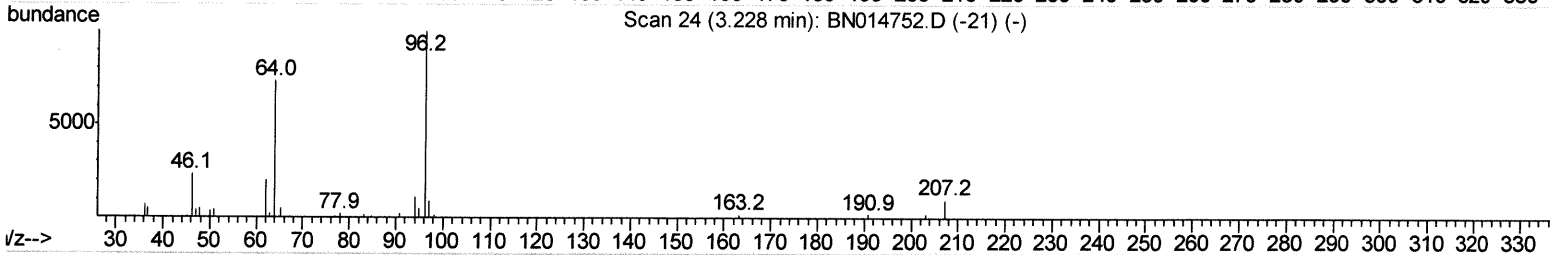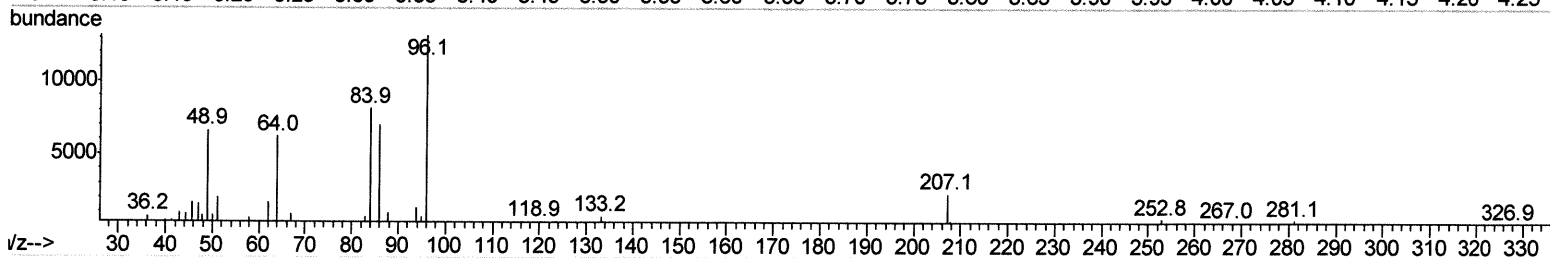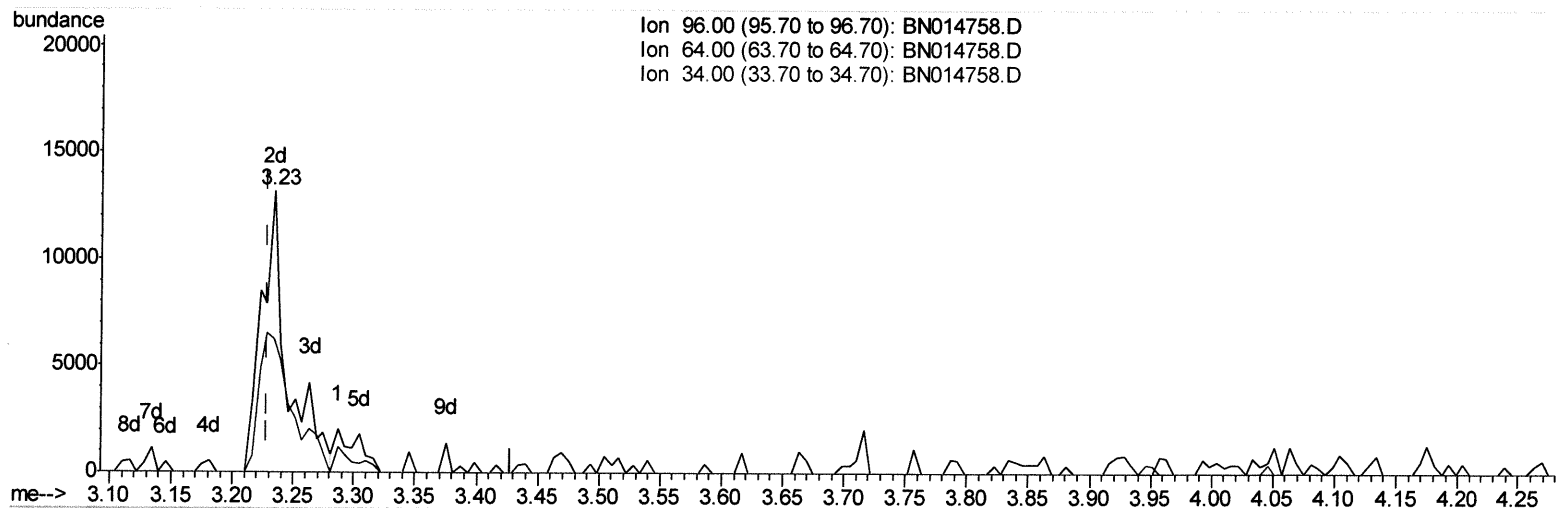

TIC: BN014758.D

(3) 1,4-Dioxane-d8 (S)

3.234min (+0.006) 4.52ng/uL m

response 19761

Ion	Exp%	Act%
96.00	100	100
64.00	64.30	47.21#
34.00	0.00	0.00
0.00	0.00	0.00

JU 5/27/21

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014758.D
 Acq On : 26 May 2021 05:31
 Operator : CG/JU
 Sample : M2493-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB431

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:13 PM

Quant Time: May 26 06:15:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	177914	20.00	ng/ul	0.00
20) Naphthalene-d8	10.49	136	743437	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.36	164	596279	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.12	188	1511636	20.00	ng/ul	0.00
79) Chrysene-d12	21.31	240	2114967	20.00	ng/ul	0.00
88) Perylene-d12	23.57	264	2421965	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	19761m	4.52	ng/uL	0.00
4) Pividine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.89	99	155505	8.93	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.05	67	302379	34.91	ng/ul	0.00
11) 2-Chlorophenol-d4	7.25	132	330896	30.67	ng/ul	0.00
15) 4-Methylphenol-d8	8.42	113	274619	20.28	ng/ul	0.00
21) Nitrobenzene-d5	8.86	128	208024	37.15	ng/ul	0.00
24) 2-Nitrophenol-d4	9.58	143	231439	38.45	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.12	165	448518	32.68	ng/ul	0.00
31) 4-Chloroaniline-d4	10.64	131	48783	3.01	ng/ul	0.00
46) Dimethylphthalate-d6	13.77	166	1916523	40.46	ng/ul	0.00
49) Acenaphthylene-d8	14.05	160	2118483	38.67	ng/ul	0.00
54) 4-Nitrophenol-d4	14.58	143	45186	6.00	ng/ul	0.00
60) Fluorene-d10	15.36	176	1714488	42.00	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.47	200	294899	35.67	ng/ul	0.00
73) Anthracene-d10	17.22	188	2937627	41.60	ng/ul	0.00
81) Pyrene-d10	19.52	212	3810149	38.21	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.43	264	5241485	40.63	ng/ul	0.00

Target Compounds

					Ovalue	
47) Dimethylphthalate	13.82	163	67976	1.451	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed