

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014730.D
 Acq On : 25 May 2021 11:43
 Operator : CG/JU
 Sample : M2493-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB428

Quant Time: May 25 12:12:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	186435	20.00	ng/ul	0.00
20) Naphthalene-d8	10.498	136	721040	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	571456	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	1373822	20.00	ng/ul	0.00
79) Chrysene-d12	21.321	240	1953094	20.00	ng/ul	0.00
88) Perylene-d12	23.586	264	2232857	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	11733	2.56	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	
7) Phenol-d5	6.893	99	92037	5.04	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.052	67	243646	26.84	ng/ul	0.00
11) 2-Chlorophenol-d4	7.252	132	244093	21.59	ng/ul	0.00
15) 4-Methylphenol-d8	8.422	113	168671	11.88	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	159746	29.41	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	151948	26.03	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	327763	24.62	ng/ul	0.00
31) 4-Chloroaniline-d4	10.646	131	24853	1.58	ng/ul	0.01
46) Dimethylphthalate-d6	13.775	166	1377969	30.35	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160	1526111	29.07	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	24245	3.36	ng/ul	0.01
60) Fluorene-d10	15.363	176	1245732	31.84	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	191838	25.53	ng/ul	0.00
73) Anthracene-d10	17.216	188	2300906	35.85	ng/ul	0.00
81) Pyrene-d10	19.522	212	3009534	32.68	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.445	264	4125125	34.68	ng/ul	0.01
Target Compounds						
47) Dimethylphthalate	13.822	163	62645	1.40	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014730.D
Acq On : 25 May 2021 11:43
Operator : CG/JU
Sample : M2493-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB428

Quant Time: May 25 12:12:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration

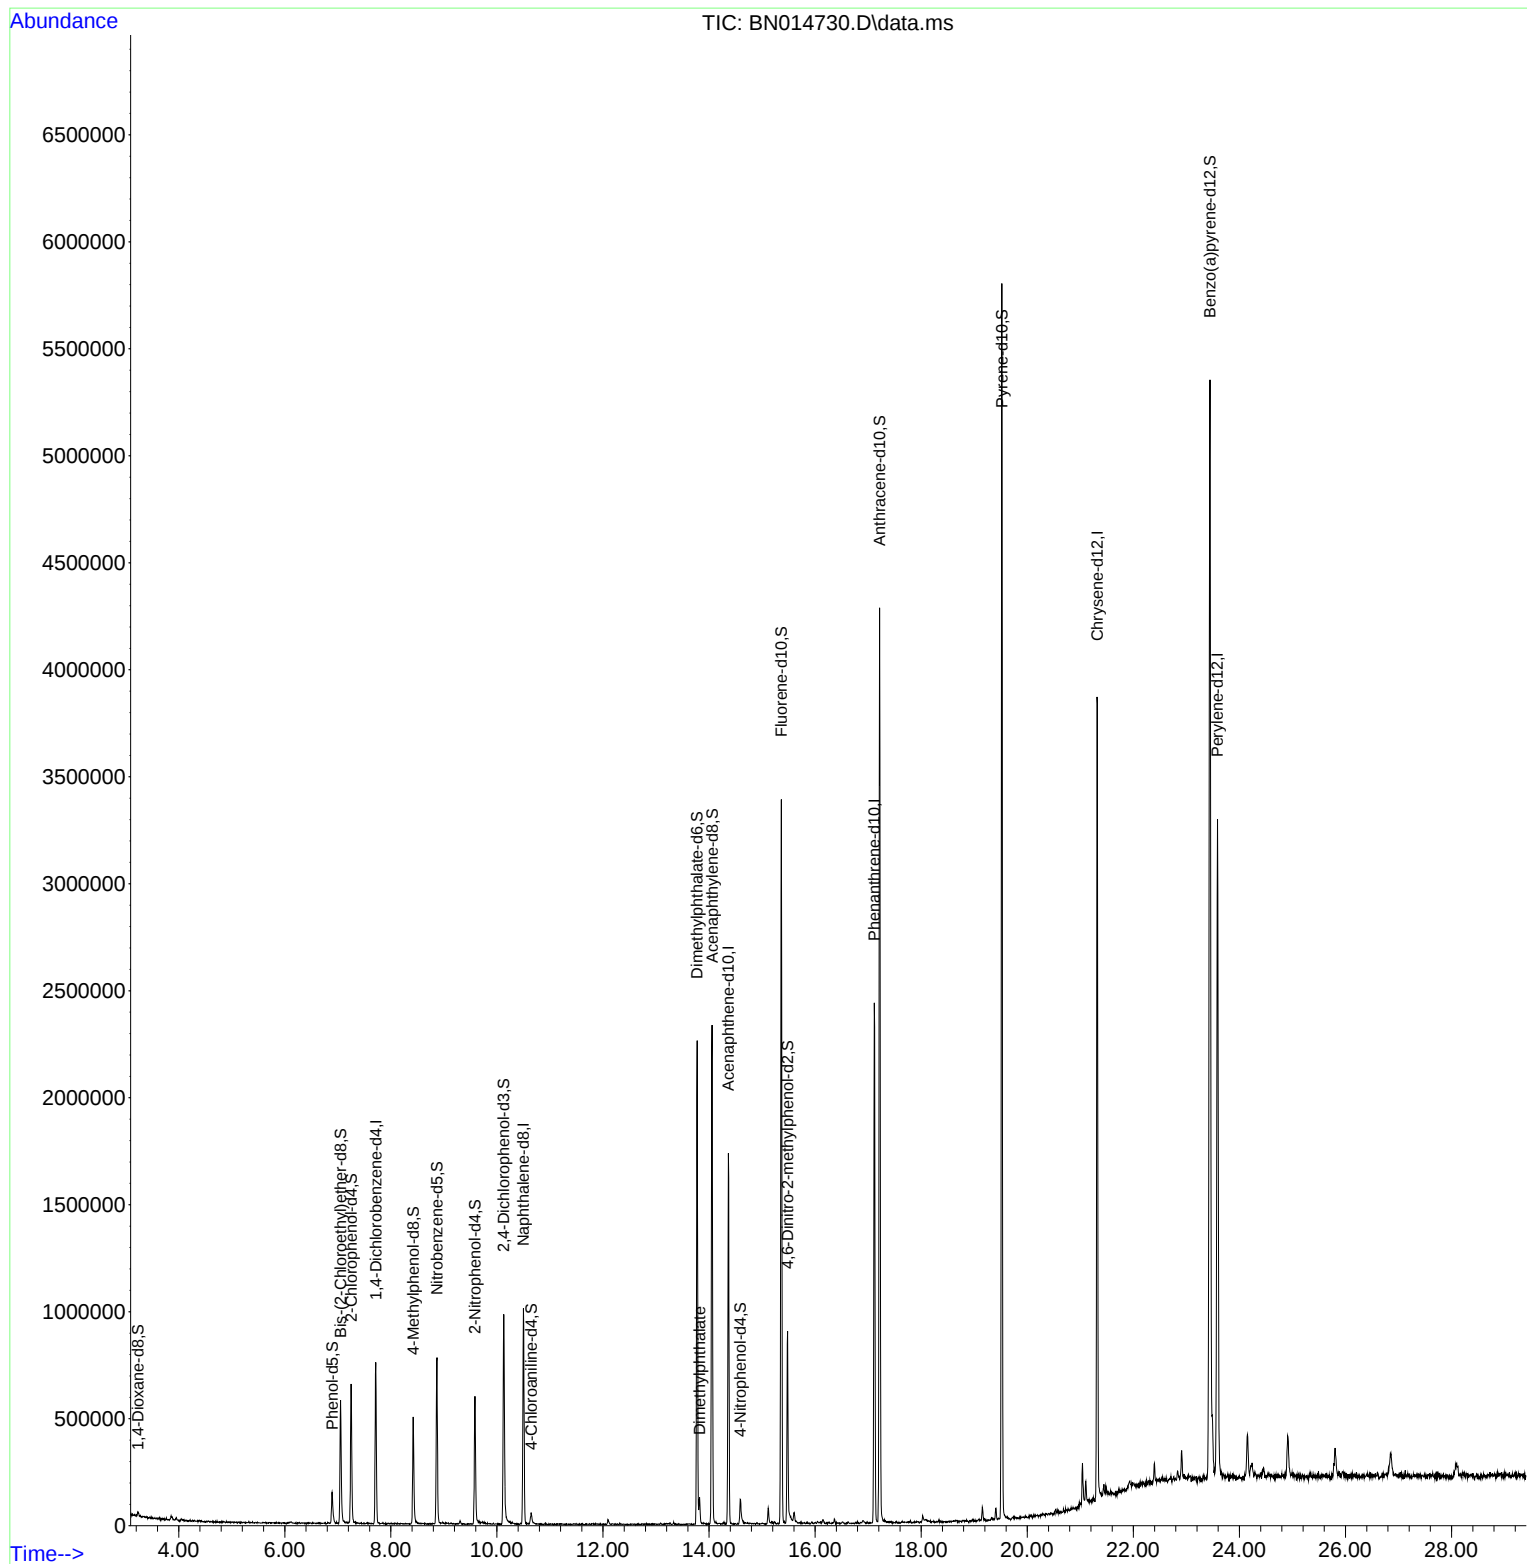

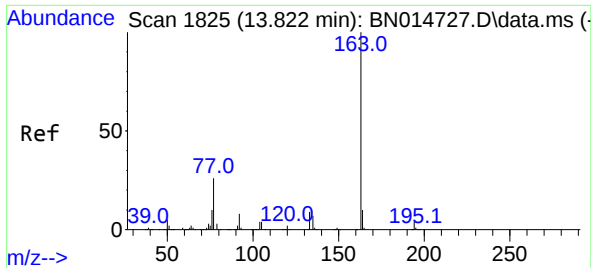

#47
 Dimethylphthalate
 Concen: 1.40 ng/ul
 RT: 13.822 min Scan# 1825
 Delta R.T. -0.000 min
 Lab File: BN014730.D
 Acq: 25 May 2021 11:43

Instrument :
 BNA_N
 ClientSampleId :
 GB428

Tgt Ion:163	Resp:	62645
Ion	Ratio	Lower Upper
163	100	
194	5.6	3.8 5.8
164	8.9	8.7 13.1

