

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014749.D
 Acq On : 25 May 2021 23:36
 Operator : CG/JU
 Sample : M2493-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB425

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:27:40 PM

Quant Time: May 26 01:06:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.711	152	209531	20.00	ng/ul	0.00
20) Naphthalene-d8	10.499	136	839498	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	675483	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	1658518	20.00	ng/ul	0.00
79) Chrysene-d12	21.310	240	2304268	20.00	ng/ul	0.00
88) Perylene-d12	23.574	264	2642164	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	22775	4.43	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.887	99	123060	6.00	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	306675	30.06	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	317458	24.98	ng/ul	0.00
15) 4-Methylphenol-d8	8.422	113	200502	12.57	ng/ul	0.00
21) Nitrobenzene-d5	8.863	128	200544	31.71	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	215680	31.73	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	422005	27.23	ng/ul	0.00
31) 4-Chloroaniline-d4	10.646	131	15614m	0.85	ng/ul	0.01
46) Dimethylphthalate-d6	13.775	166	1741870	32.46	ng/ul	0.00
49) Acenaphthylene-d8	14.051	160	1912279	30.82	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143	35449	4.16	ng/ul	0.00
60) Fluorene-d10	15.357	176	1608488	34.79	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	290515	32.03	ng/ul	0.00
73) Anthracene-d10	17.216	188	2809344	36.26	ng/ul	0.00
81) Pyrene-d10	19.516	212	3633384	33.44	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	4985268	35.42	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.816	163	94090	1.77	ng/ul#	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014749.D
Acq On : 25 May 2021 23:36
Operator : CG/JU
Sample : M2493-10
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GB425

Manual Integrations
APPROVED

mohammad
5/26/2021 4:27:40 PM


Quant Time: May 26 01:06:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration

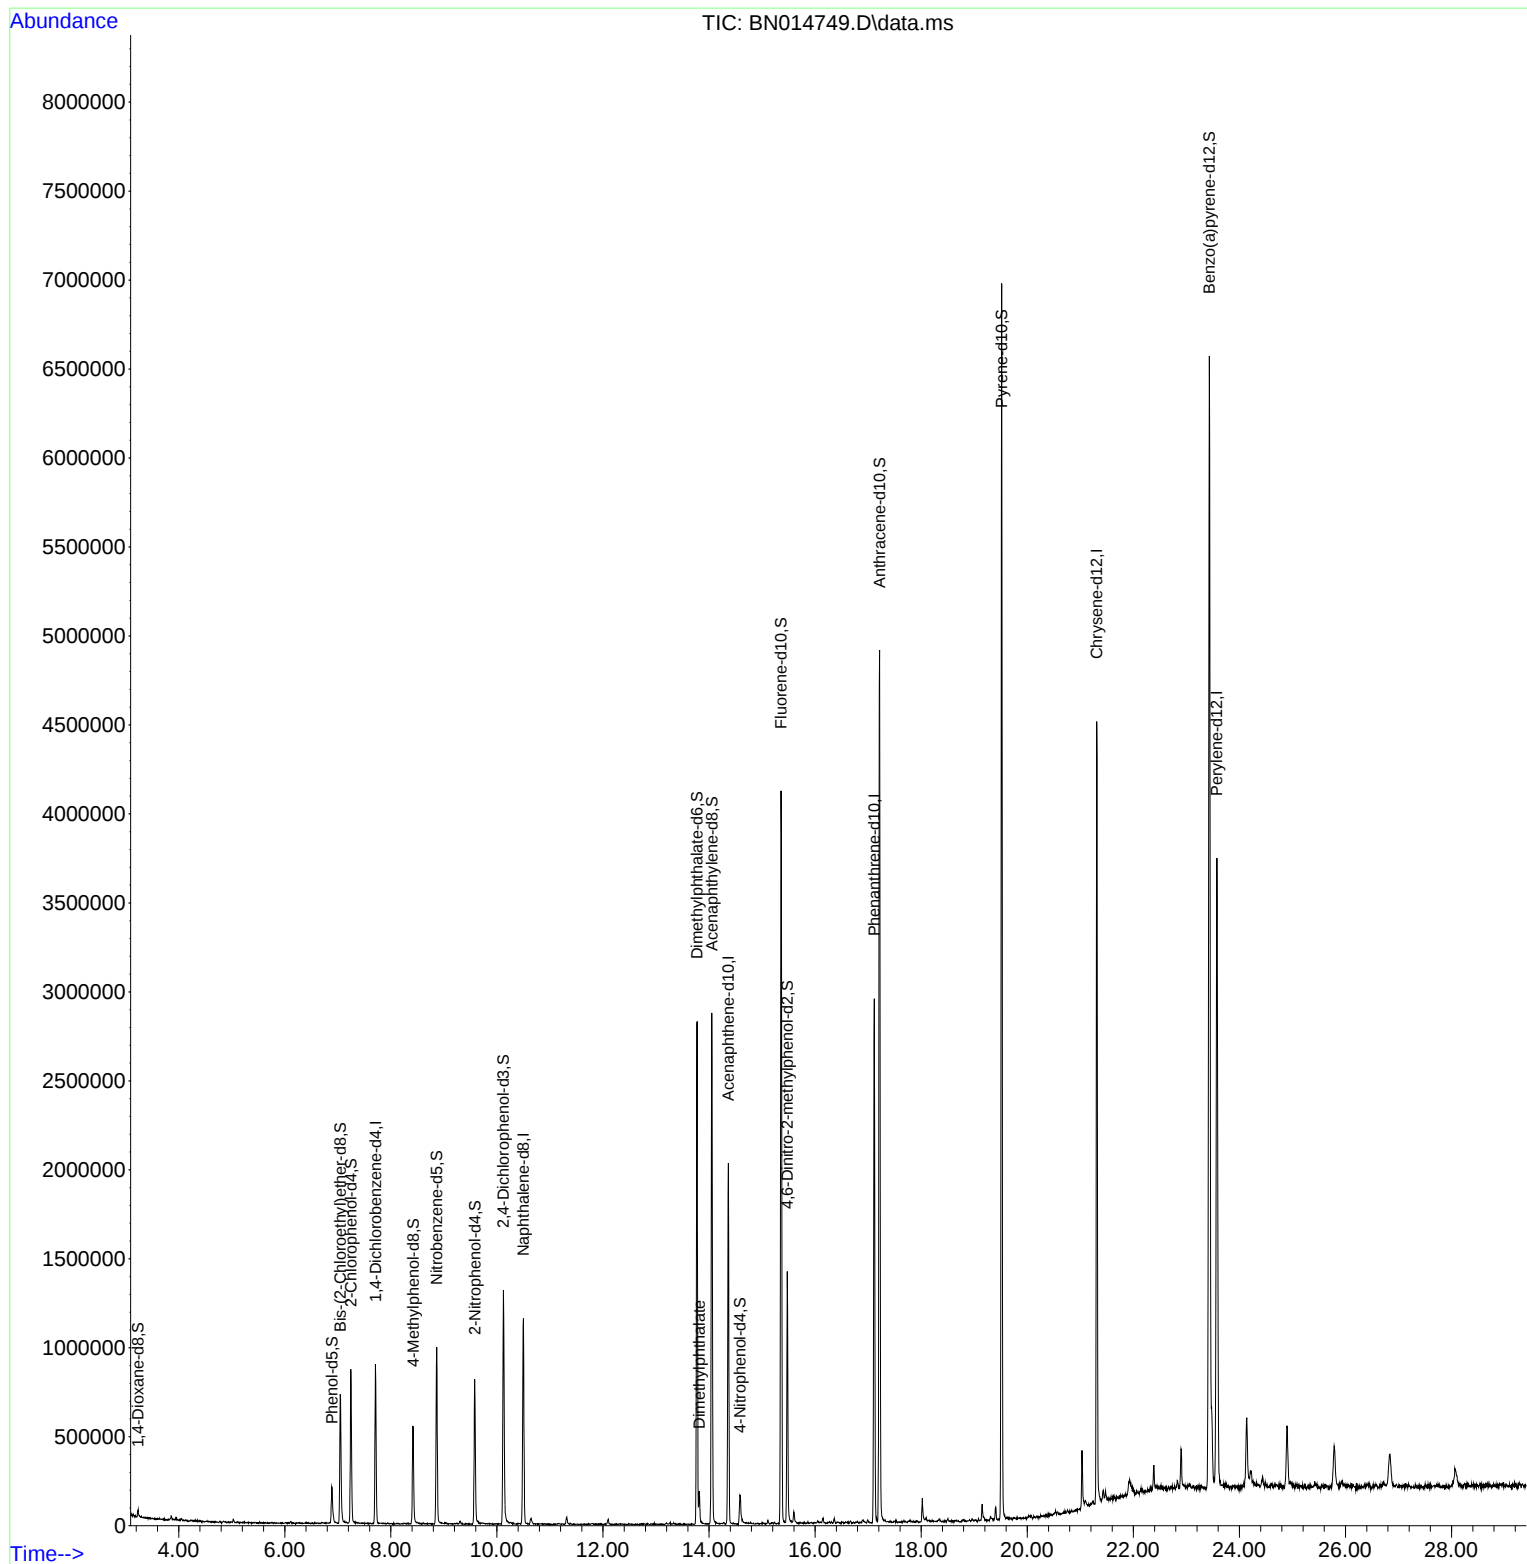

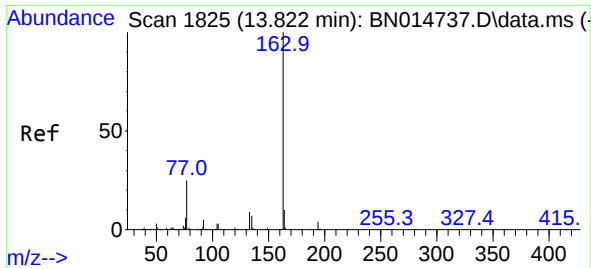

#47
 Dimethylphthalate
 Concen: 1.77 ng/ul
 RT: 13.816 min Scan# 1824
 Delta R.T. -0.006 min
 Lab File: BN014749.D
 Acq: 25 May 2021 23:36

Instrument :
 BNA_N
 ClientSampleID :
 GB425

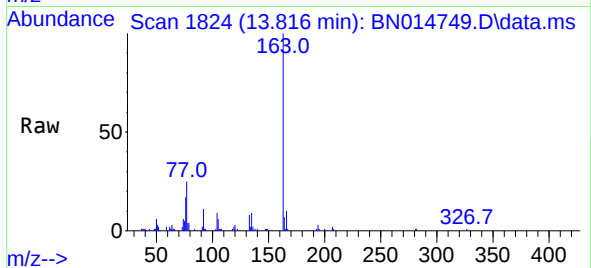

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.3	3.8	5.8#
164	6.8	8.7	13.1#

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:27:40 PM

