

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014759.D
 Acq On : 26 May 2021 06:06
 Operator : CG/JU
 Sample : M2495-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB436

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:16 PM

Quant Time: May 26 06:39:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	178143	20.00	ng/ul	0.00
20) Naphthalene-d8	10.498	136	735194	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	599779	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	1499974	20.00	ng/ul	0.00
79) Chrysene-d12	21.309	240	2027761	20.00	ng/ul	0.00
88) Perylene-d12	23.574	264	2382372	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	14866m	3.40	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.887	99	108579	6.22	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	265936	30.66	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	286095	26.48	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	206085	15.20	ng/ul	0.00
21) Nitrobenzene-d5	8.863	128	182999	33.04	ng/ul	0.00
24) 2-Nitrophenol-d4	9.581	143	201168	33.79	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	371540	27.37	ng/ul	0.00
31) 4-Chloroaniline-d4	10.639	131	17883	1.12	ng/ul	0.00
46) Dimethylphthalate-d6	13.769	166	1660705	34.85	ng/ul	0.00
49) Acenaphthylene-d8	14.051	160	1863154	33.81	ng/ul	0.00
54) 4-Nitrophenol-d4	14.580	143	33759m	4.46	ng/ul	0.00
60) Fluorene-d10	15.357	176	1492194	36.34	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	275039	33.52	ng/ul	0.00
73) Anthracene-d10	17.216	188	2809872	40.10	ng/ul	0.00
81) Pyrene-d10	19.515	212	3728309	38.99	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	5197815	40.96	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.816	163	88882	1.89	ng/ul	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014759.D
Acq On : 26 May 2021 06:06
Operator : CG/JU
Sample : M2495-04
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GB436

Manual Integrations
APPROVED

mohammad
5/26/2021 4:28:16 PM




Quant Time: May 26 06:39:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration

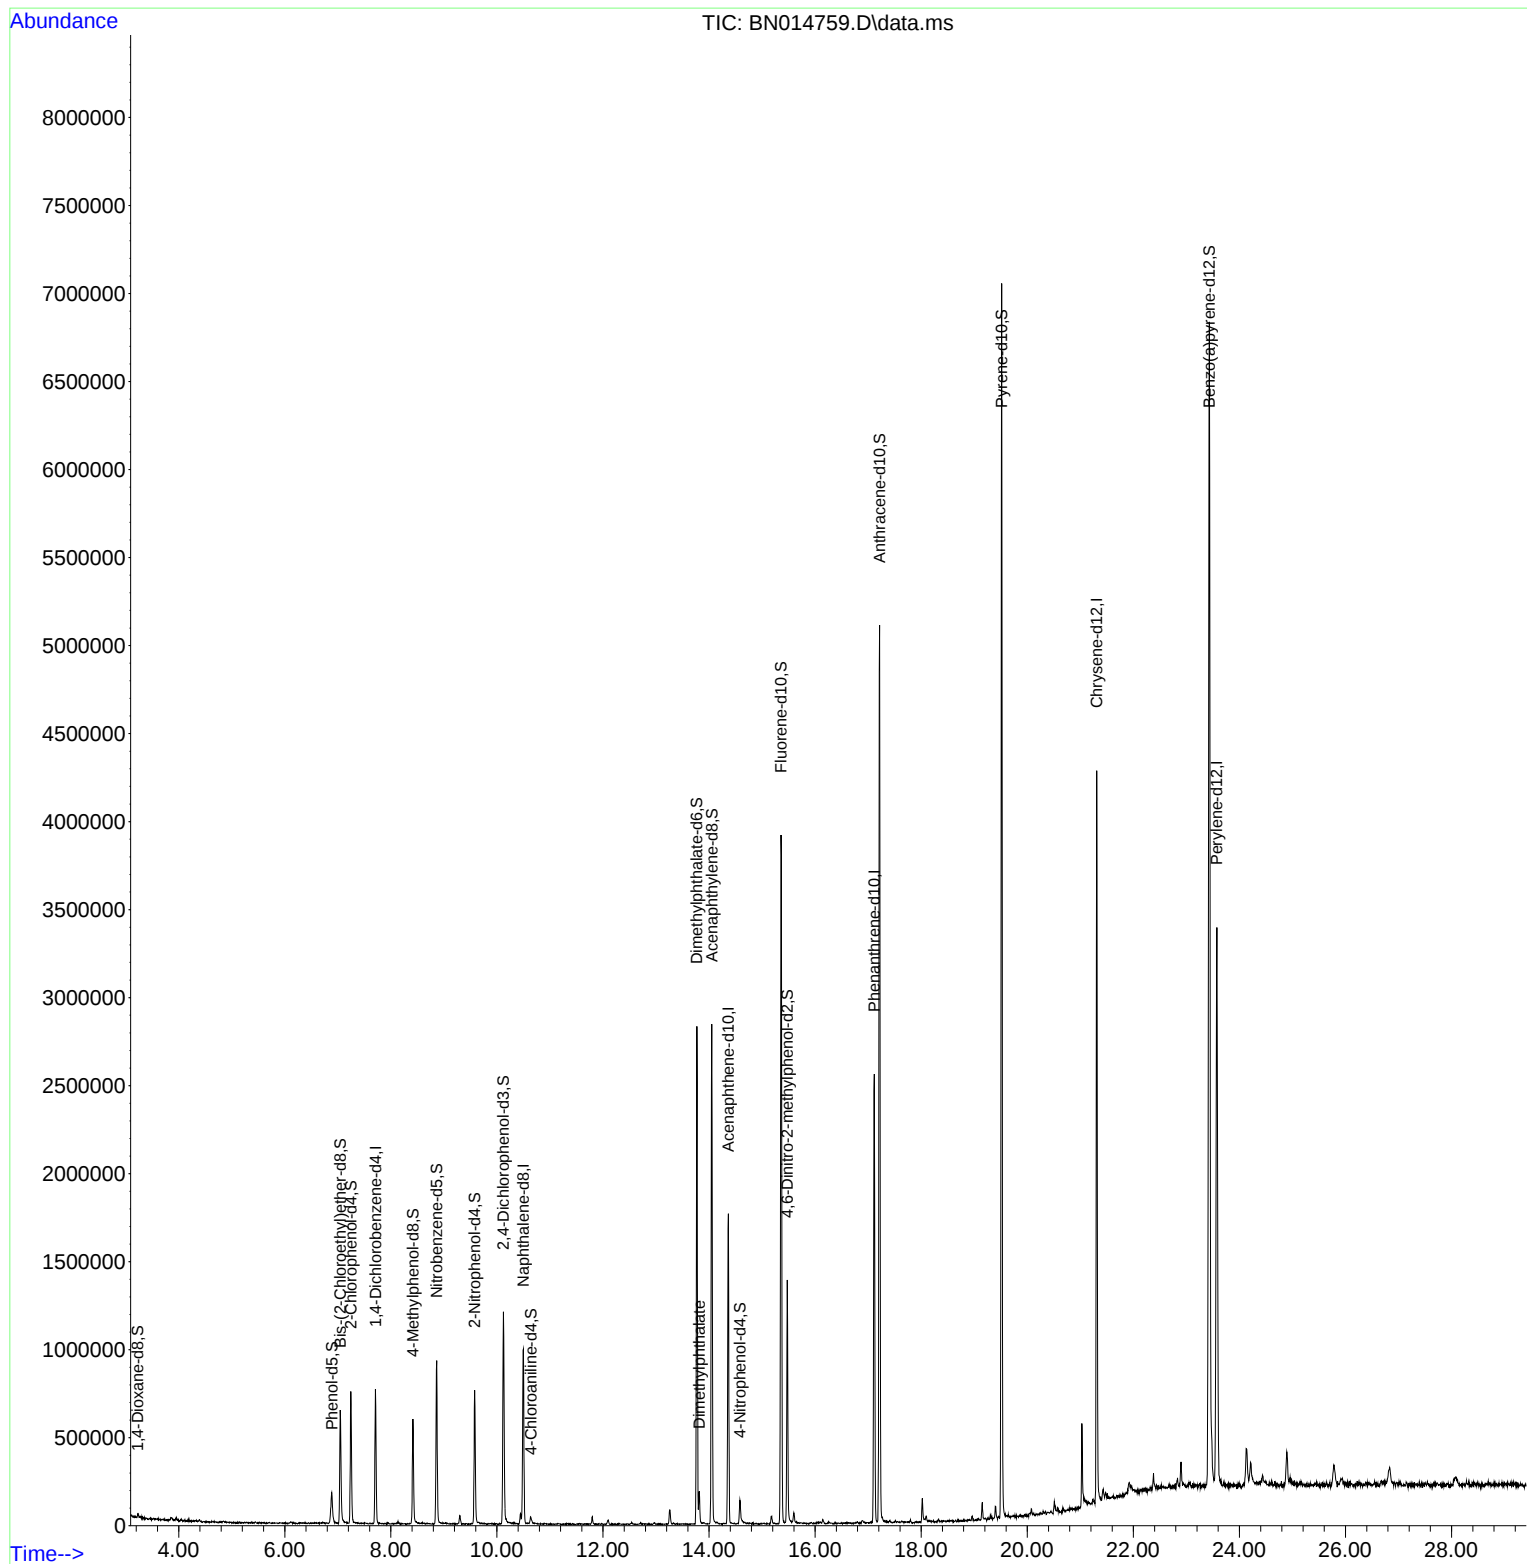

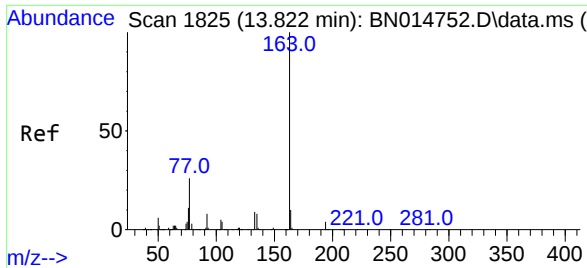

#47
Dimethylphthalate
Concen: 1.89 ng/ul
RT: 13.816 min Scan# 1824
Delta R.T. -0.006 min
Lab File: BN014759.D
Acq: 26 May 2021 06:06

Tgt Ion:163 Resp: 88882
Ion Ratio Lower Upper
163 100
194 4.5 3.8 5.8
164 12.8 8.7 13.1

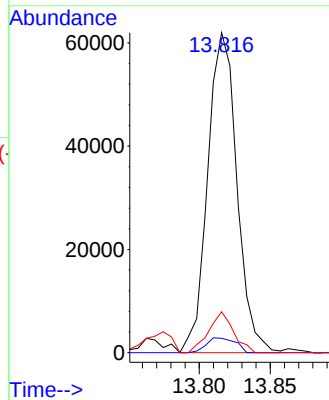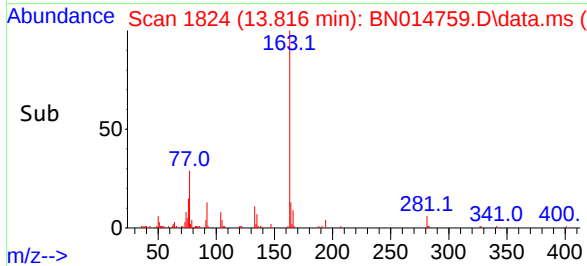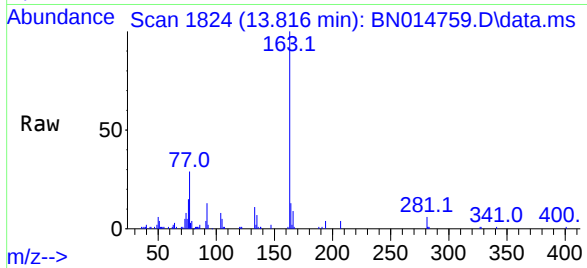

Instrument :
BNA_N
ClientSampleId :
GB436

Manual Integrations
APPROVED

mohammad
5/26/2021 4:28:16 PM