

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014760.D
 Acq On : 26 May 2021 06:41
 Operator : CG/JU
 Sample : M2495-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB430

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:19 PM

Quant Time: May 26 07:23:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	210513	20.00	ng/ul	0.00
20) Naphthalene-d8	10.499	136	825224	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	660262	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	1685315	20.00	ng/ul	0.00
79) Chrysene-d12	21.310	240	2202194	20.00	ng/ul	0.00
88) Perylene-d12	23.580	264	2528876	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	18151	3.51	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.887	99	125713	6.10	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	311466	30.39	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	334287	26.19	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	250778	15.65	ng/ul	0.00
21) Nitrobenzene-d5	8.863	128	207807	33.43	ng/ul	0.00
24) 2-Nitrophenol-d4	9.581	143	223336	33.42	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	451802	29.66	ng/ul	0.00
31) 4-Chloroaniline-d4	10.640	131	23353	1.30	ng/ul	0.00
46) Dimethylphthalate-d6	13.775	166	1900786	36.24	ng/ul	0.00
49) Acenaphthylene-d8	14.051	160	2107514	34.74	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143	41300	4.96	ng/ul	0.00
60) Fluorene-d10	15.357	176	1692931	37.46	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	315924m	34.27	ng/ul	0.00
73) Anthracene-d10	17.210	188	3087028m	39.21	ng/ul	0.00
81) Pyrene-d10	19.516	212	4044927	38.95	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	5356666	39.77	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.816	163	65774	1.27	ng/ul#	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014760.D
Acq On : 26 May 2021 06:41
Operator : CG/JU
Sample : M2495-07
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GB430

Manual Integrations
APPROVED


mohammad
5/26/2021 4:28:19 PM

Quant Time: May 26 07:23:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration


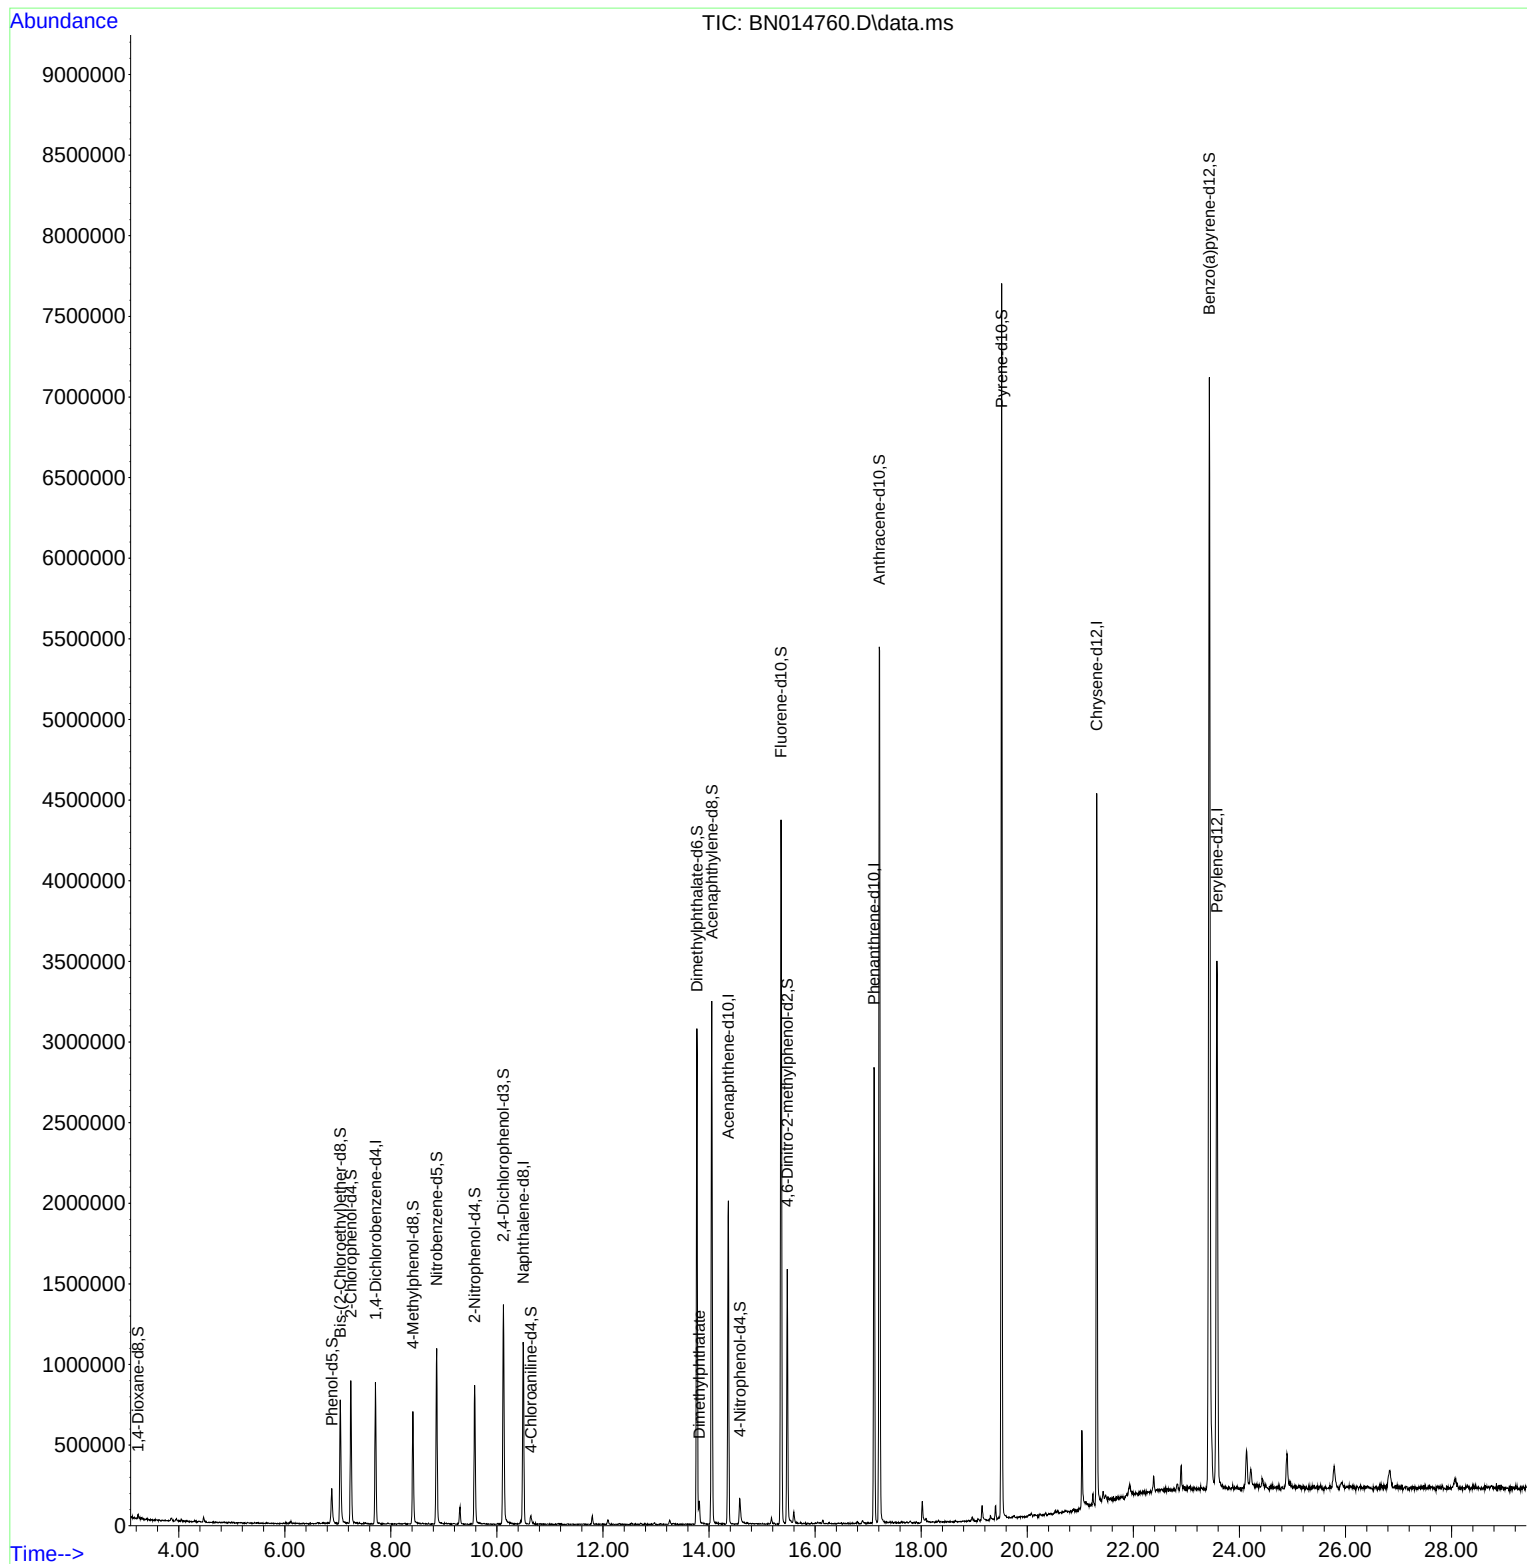


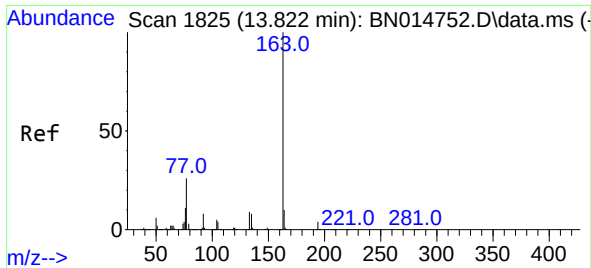

#47
 Dimethylphthalate
 Concen: 1.27 ng/ul
 RT: 13.816 min Scan# 1824
 Delta R.T. -0.006 min
 Lab File: BN014760.D
 Acq: 26 May 2021 06:41

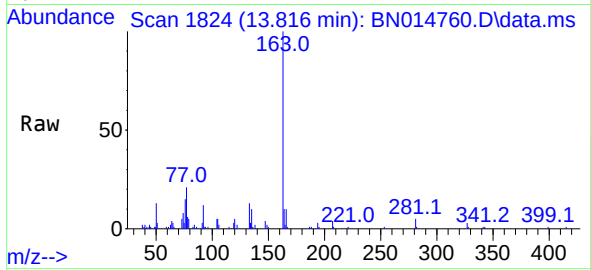

Tgt Ion:163 Resp: 65774
 Ion Ratio Lower Upper
 163 100
 194 3.4 3.8 5.8#
 164 9.8 8.7 13.1

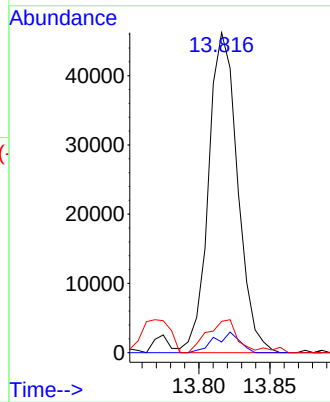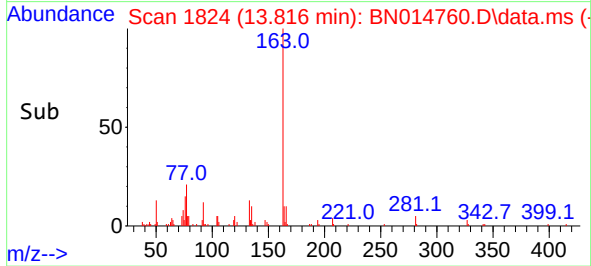

Instrument :
 BNA_N
 ClientSampleId :
 GB430

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:19 PM