

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014761.D
 Acq On : 26 May 2021 07:17
 Operator : CG/JU
 Sample : M2495-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB438

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:21 PM

Quant Time: May 26 08:02:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.711	152	206630	20.00	ng/ul	0.00
20) Naphthalene-d8	10.499	136	847558	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	665198	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	1679605	20.00	ng/ul	0.00
79) Chrysene-d12	21.310	240	2288748	20.00	ng/ul	0.00
88) Perylene-d12	23.574	264	2650467	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	19621m	3.87	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.887	99	140586	6.95	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	324900	32.29	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	336704	26.87	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	262739	16.70	ng/ul	0.00
21) Nitrobenzene-d5	8.858	128	210257	32.93	ng/ul	0.00
24) 2-Nitrophenol-d4	9.581	143	230705	33.62	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	454877	29.07	ng/ul	0.00
31) 4-Chloroaniline-d4	10.646	131	32449m	1.76	ng/ul	0.01
46) Dimethylphthalate-d6	13.769	166	1892911	35.82	ng/ul	0.00
49) Acenaphthylene-d8	14.051	160	2116689	34.64	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	46611m	5.55	ng/ul	0.00
60) Fluorene-d10	15.357	176	1700895	37.35	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	317162	34.52	ng/ul	0.00
73) Anthracene-d10	17.216	188	3148681	40.13	ng/ul	0.00
81) Pyrene-d10	19.516	212	3972336	36.81	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	5359495	37.96	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.816	163	129641	2.48	ng/ul	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014761.D
Acq On : 26 May 2021 07:17
Operator : CG/JU
Sample : M2495-06
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GB438

Manual Integrations
APPROVED

mohammad
5/26/2021 4:28:21 PM

Quant Time: May 26 08:02:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration

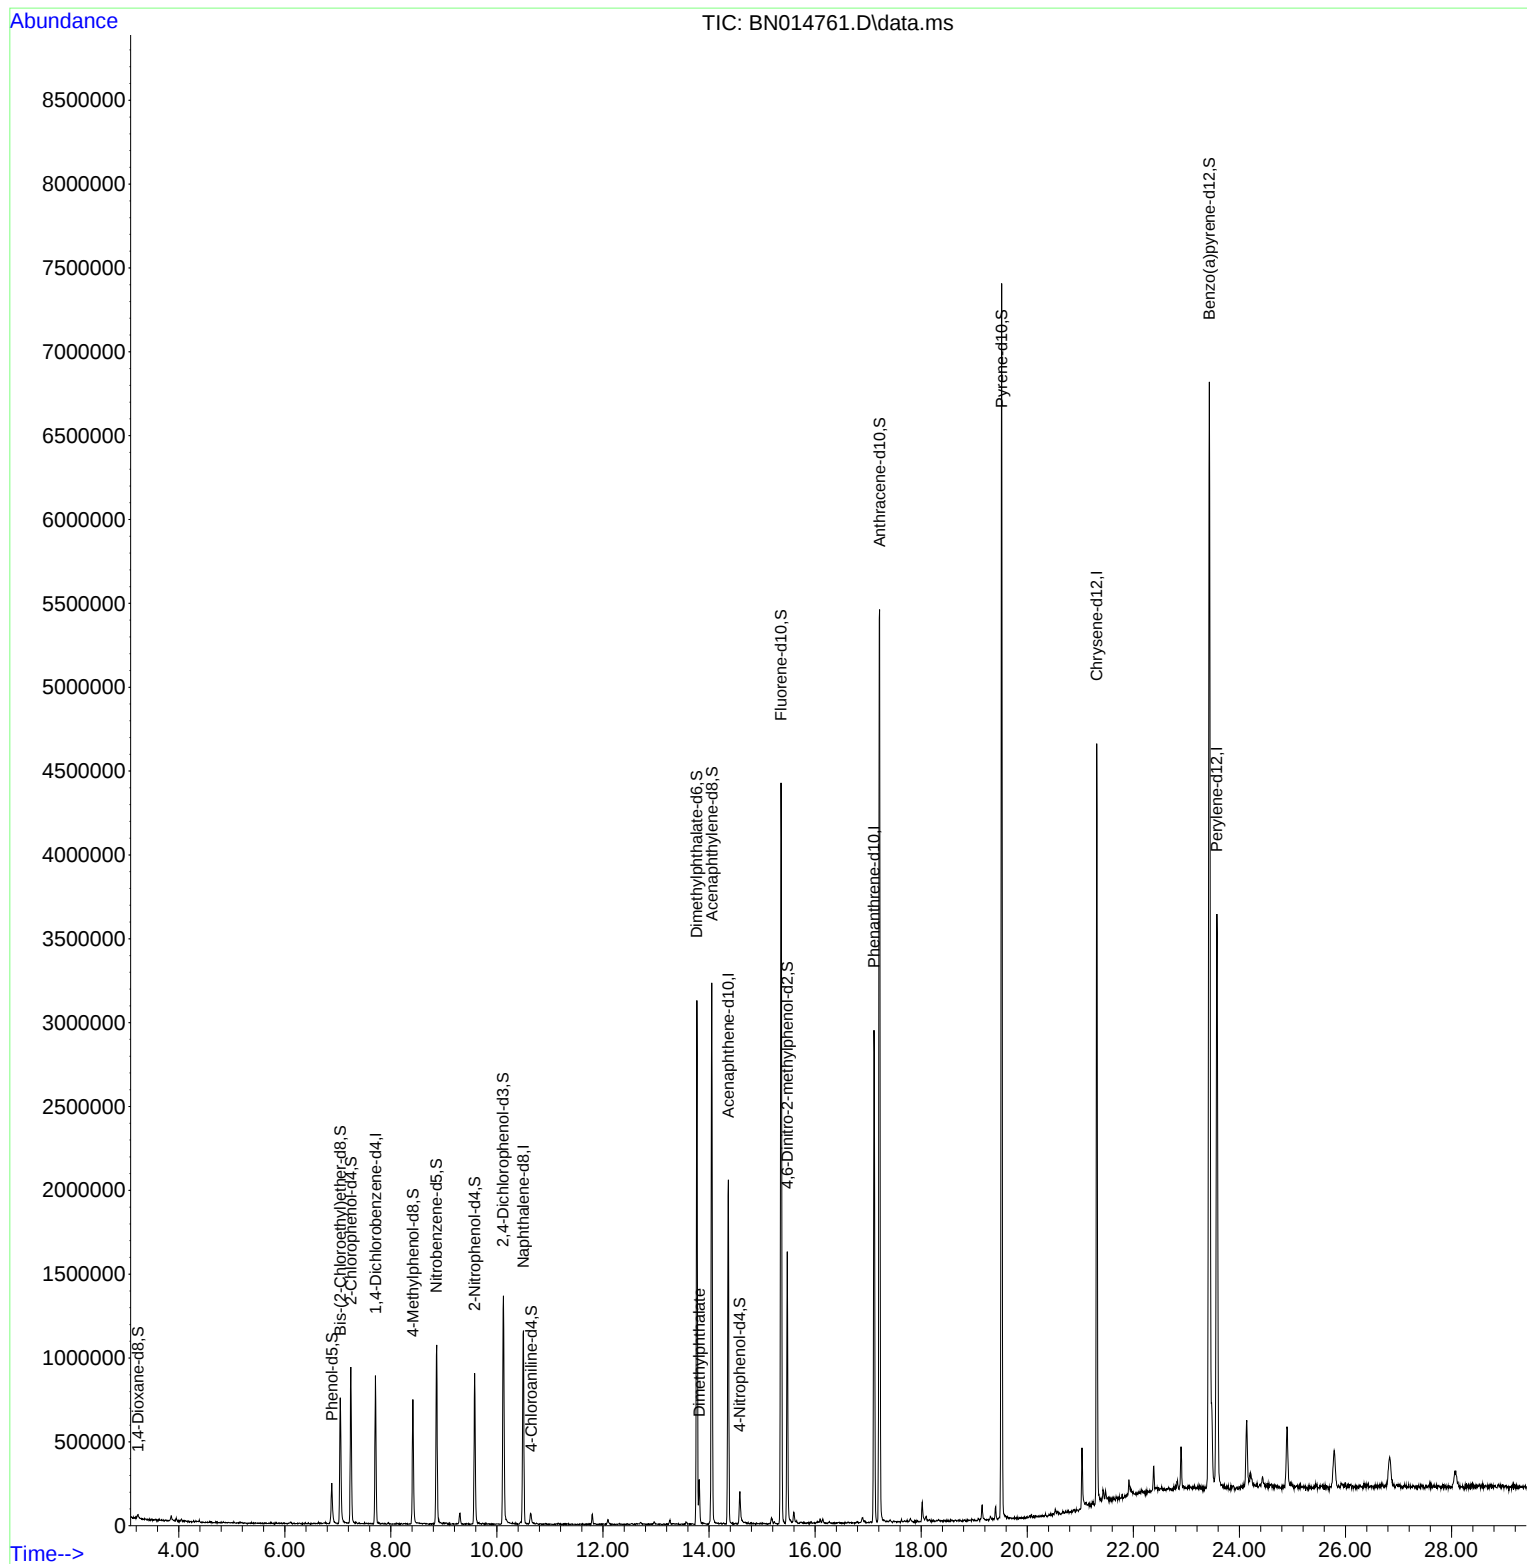

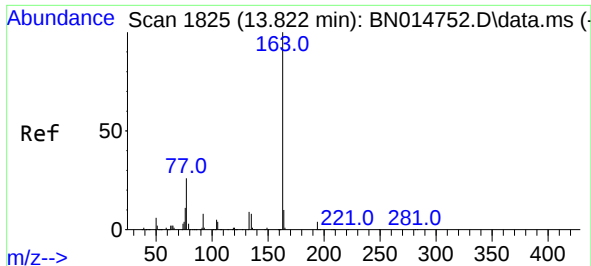

#47

Dimethylphthalate

Concen: 2.48 ng/ul

RT: 13.816 min Scan# 1824

Delta R.T. -0.006 min

Lab File: BN014761.D

Acq: 26 May 2021 07:17




Tgt Ion:163 Resp: 129641

Ion Ratio Lower Upper

163 100

194 5.0 3.8 5.8

164 9.7 8.7 13.1

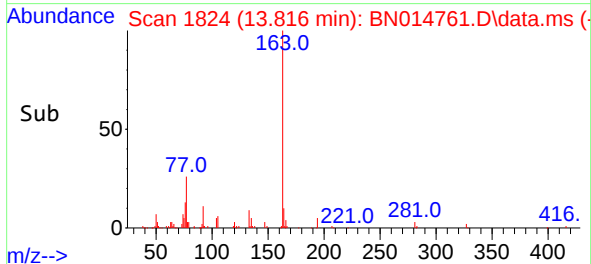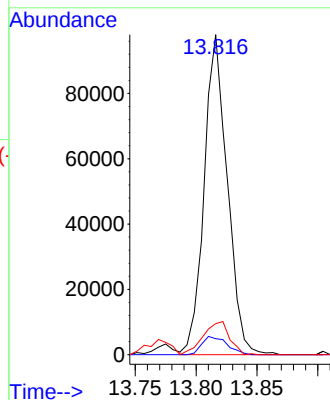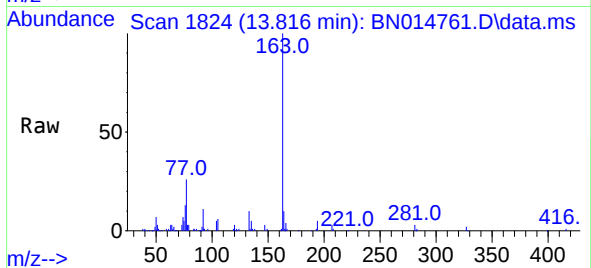

Instrument :

BNA_N

ClientSampleId :

GB438

Manual Integrations

APPROVED

mohammad
5/26/2021 4:28:21 PM