

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014762.D
 Acq On : 26 May 2021 07:52
 Operator : CG/JU
 Sample : M2495-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB437

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:24 PM

Quant Time: May 26 08:46:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 25 10:33:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.711	152	179392	20.00	ng/ul	# 0.00
20) Naphthalene-d8	10.499	136	738998	20.00	ng/ul	# 0.00
38) Acenaphthene-d10	14.357	164	602060	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	1548637	20.00	ng/ul	0.00
79) Chrysene-d12	21.310	240	2081374	20.00	ng/ul	# 0.00
88) Perylene-d12	23.580	264	2470702	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	15700m	3.56	ng/uL	0.00
4) Pyridine-d5	3.640	84	3268	0.29	ng/ul	0.00
7) Phenol-d5	6.887	99	117021	6.66	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	273129	31.27	ng/ul	0.00
11) 2-Chlorophenol-d4	7.246	132	297911	27.38	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	205836	15.07	ng/ul	0.00
21) Nitrobenzene-d5	8.863	128	192426	34.57	ng/ul	0.00
24) 2-Nitrophenol-d4	9.581	143	200445	33.50	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	382622	28.05	ng/ul	0.00
31) 4-Chloroaniline-d4	10.640	131	23947	1.49	ng/ul	0.00
46) Dimethylphthalate-d6	13.769	166	1669137	34.90	ng/ul	0.00
49) Acenaphthylene-d8	14.051	160	1908640	34.51	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	35441	4.66	ng/ul	0.01
60) Fluorene-d10	15.357	176	1546016	37.51	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	278028	32.82	ng/ul	0.00
73) Anthracene-d10	17.210	188	2802736	38.74	ng/ul	0.00
81) Pyrene-d10	19.516	212	3665855	37.35	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	5160142	39.21	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.816	163	63161	1.34	ng/ul#	Qvalue 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014762.D
Acq On : 26 May 2021 07:52
Operator : CG/JU
Sample : M2495-05
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GB437

Manual Integrations
APPROVED


mohammad
5/26/2021 4:28:24 PM

Quant Time: May 26 08:46:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 25 10:33:04 2021
Response via : Initial Calibration


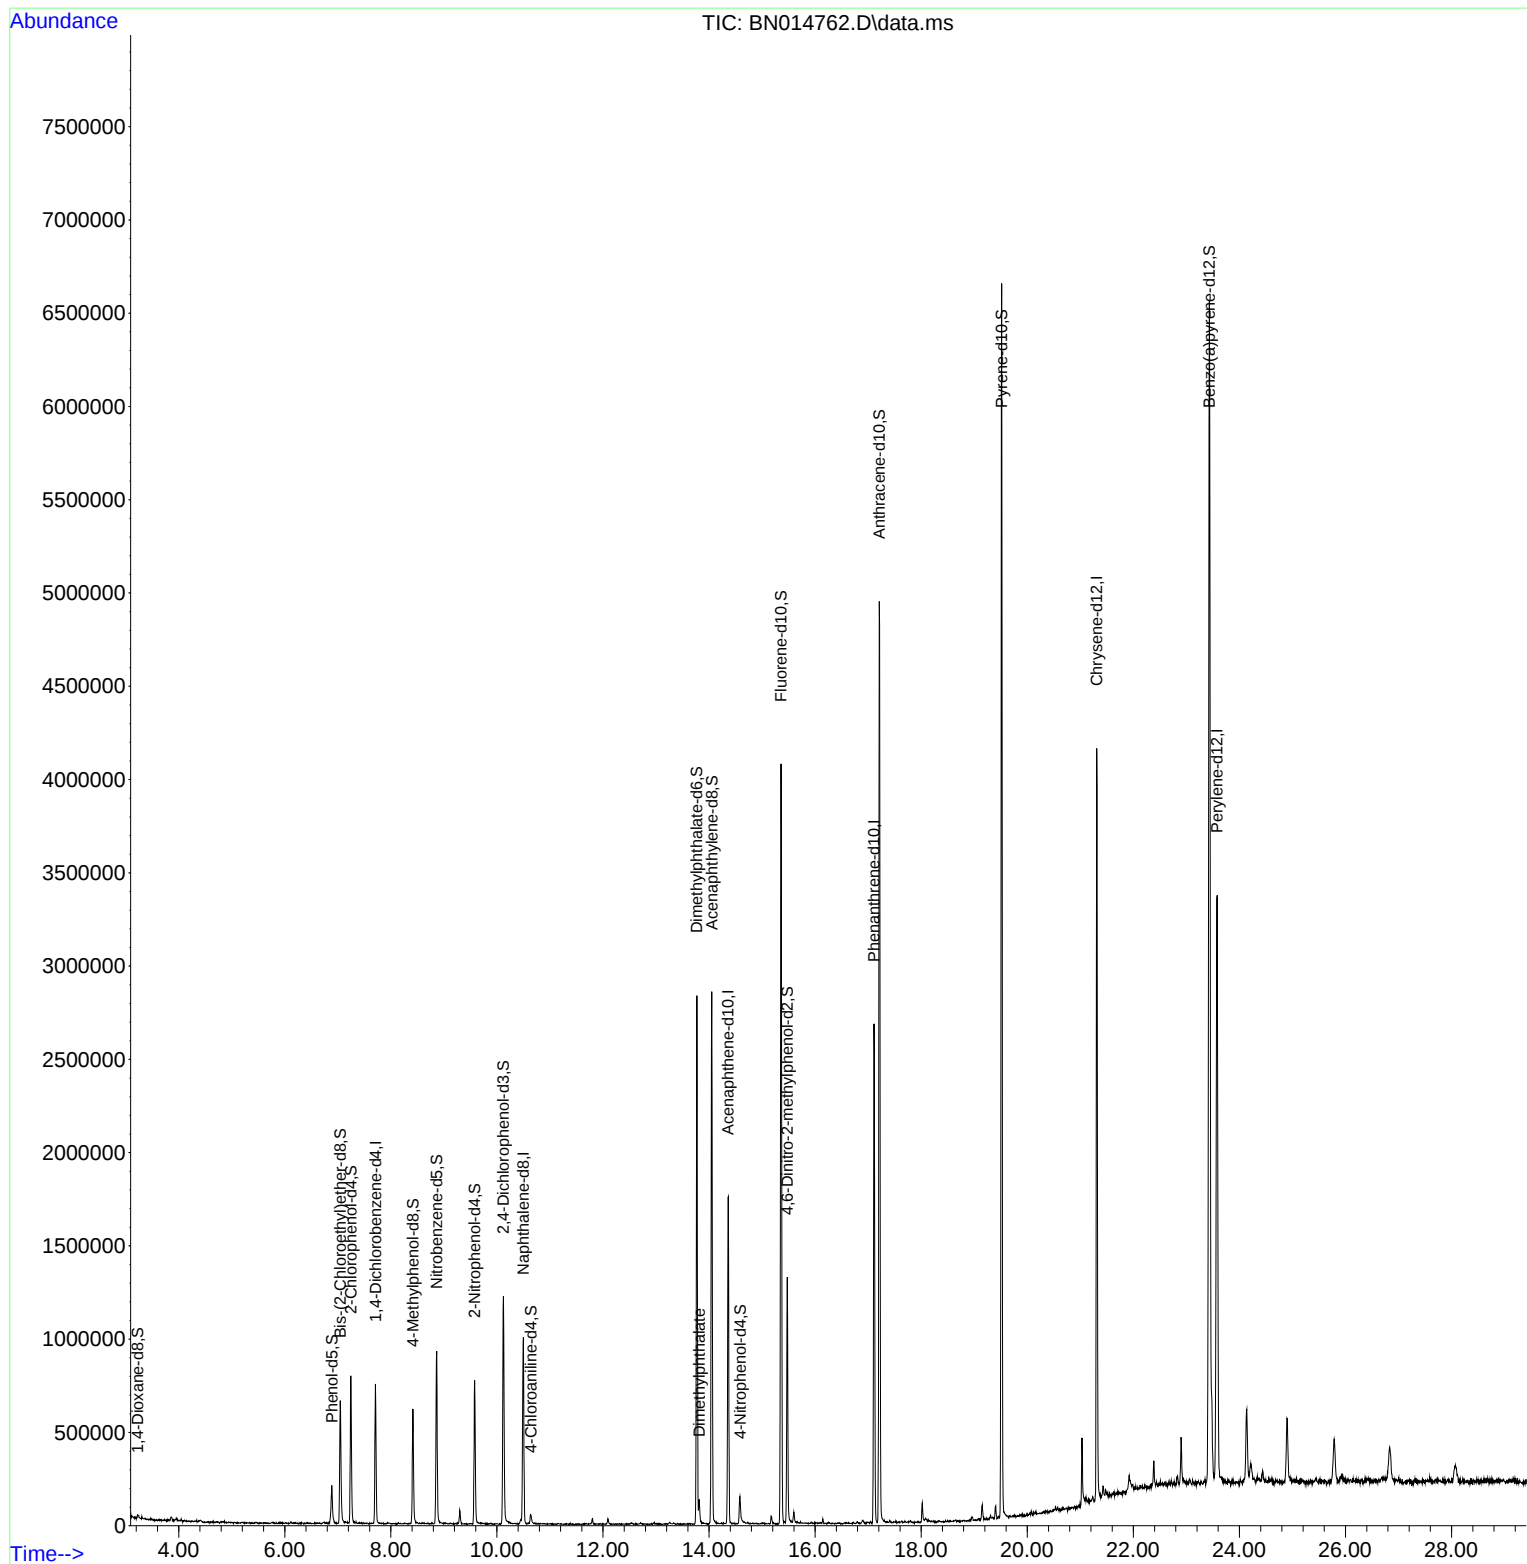


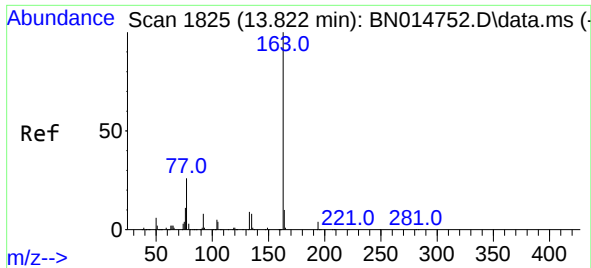

#47
 Dimethylphthalate
 Concen: 1.34 ng/ul
 RT: 13.816 min Scan# 1824
 Delta R.T. -0.006 min
 Lab File: BN014762.D
 Acq: 26 May 2021 07:52

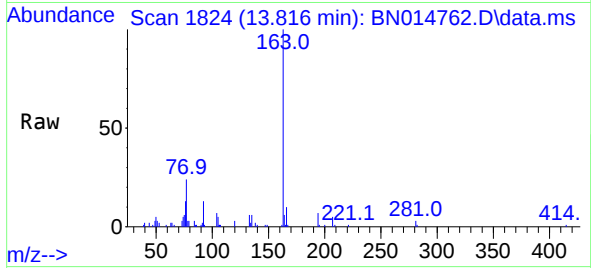

Tgt Ion:163 Resp: 63161
 Ion Ratio Lower Upper
 163 100
 194 7.1 3.8 5.8#
 164 6.5 8.7 13.1#

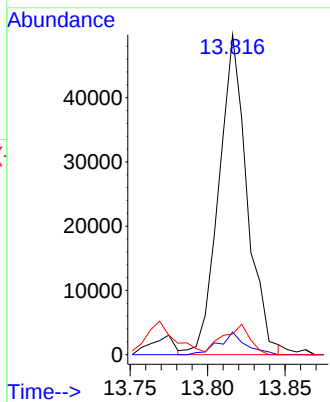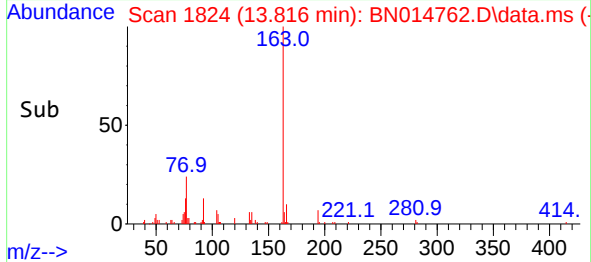

Instrument :
 BNA_N
 ClientSampleId :
 GB437

Manual Integrations
 APPROVED

mohammad
 5/26/2021 4:28:24 PM