

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014728.D
 Acq On : 25 May 2021 10:15
 Operator : CG/JU
 Sample : PB136608BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK608

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014728.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	38	rVB5	64208	133954	0.98%	0.136%
2	3.634	90	93	116	rBV	471418	1172455	8.54%	1.189%
3	3.952	143	147	150	rBV4	11397	14867	0.11%	0.015%
4	6.887	638	646	656	rBV	1192465	2079030	15.14%	2.109%
5	7.052	668	674	687	rBV	891188	1530013	11.14%	1.552%
6	7.251	699	708	722	rBV	1246684	2196774	15.99%	2.228%
7	7.710	777	786	797	rVB	859846	1439778	10.48%	1.460%
8	8.416	899	906	921	rBV2	1616800	2783928	20.27%	2.824%
9	8.863	975	982	993	rBV	1282538	2097817	15.27%	2.128%
10	9.581	1097	1104	1114	rBV	982225	1676820	12.21%	1.701%
11	10.128	1189	1197	1210	rBV	1649849	2937445	21.39%	2.980%
12	10.498	1253	1260	1269	rVB	1189370	1994847	14.52%	2.024%
13	10.634	1272	1283	1291	rBV	1630371	2785527	20.28%	2.826%
14	12.098	1527	1532	1538	rVB3	32396	55545	0.40%	0.056%
15	13.334	1738	1742	1746	rVB4	8494	15162	0.11%	0.015%
16	13.775	1809	1817	1828	rBV	3462901	4989252	36.32%	5.061%
17	14.051	1857	1864	1873	rBV	3446707	5174138	37.67%	5.249%
18	14.363	1910	1917	1924	rBV	1995709	3031801	22.07%	3.075%
19	14.575	1946	1953	1972	rBV	1369951	2302312	16.76%	2.335%
20	15.363	2080	2087	2097	rVB	4587888	6855937	49.91%	6.955%
21	15.475	2101	2106	2117	rBV	1333603	1941966	14.14%	1.970%
22	15.598	2123	2127	2135	rVB4	69312	116808	0.85%	0.118%
23	16.145	2215	2220	2226	rBV6	27717	41480	0.30%	0.042%
24	16.792	2324	2330	2331	rVV5	8751	13795	0.10%	0.014%
25	17.116	2378	2385	2393	rBV	3005152	4205961	30.62%	4.266%
26	17.216	2395	2402	2417	rVV2	5444370	8030303	58.46%	8.146%
27	18.092	2549	2551	2556	rVB6	10553	14446	0.11%	0.015%
28	19.080	2716	2719	2724	rVB7	17012	20925	0.15%	0.021%
29	19.151	2724	2731	2735	rBV	92530	124378	0.91%	0.126%
30	19.404	2770	2774	2780	rBV	88468	122795	0.89%	0.125%
31	19.516	2787	2793	2802	rBV2	6993232	10394432	75.68%	10.544%
32	20.527	2963	2965	2966	rBV2	18097	14742	0.11%	0.015%
33	20.998	3041	3045	3046	rBV3	36907	34922	0.25%	0.035%
34	21.039	3049	3052	3055	rVV4	33082	49264	0.36%	0.050%
35	21.098	3058	3062	3067	rBV	112237	165739	1.21%	0.168%
36	21.315	3093	3099	3108	rBV	4469883	6173935	44.95%	6.263%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014728.D
Acq On : 25 May 2021 10:15
Operator : CG/JU
Sample : PB136608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK608

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Title : SVOA CALIBRATION

37	22.392	3278	3282	3287	rVB8	69853	113547	0.83%	0.115%
38	22.898	3365	3368	3374	rBV8	113417	198023	1.44%	0.201%
39	23.439	3451	3460	3472	rBV2	6472770	13735482	100.00%	13.933%
40	23.580	3477	3484	3497	rVB	3729818	7079171	51.54%	7.181%
41	24.139	3574	3579	3587	rBV5	179166	435353	3.17%	0.442%
42	24.904	3705	3709	3715	rVB8	146239	286971	2.09%	0.291%


Sum of corrected areas: 98581840

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014728.D
Acq On : 25 May 2021 10:15
Operator : CG/JU
Sample : PB136608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK608

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

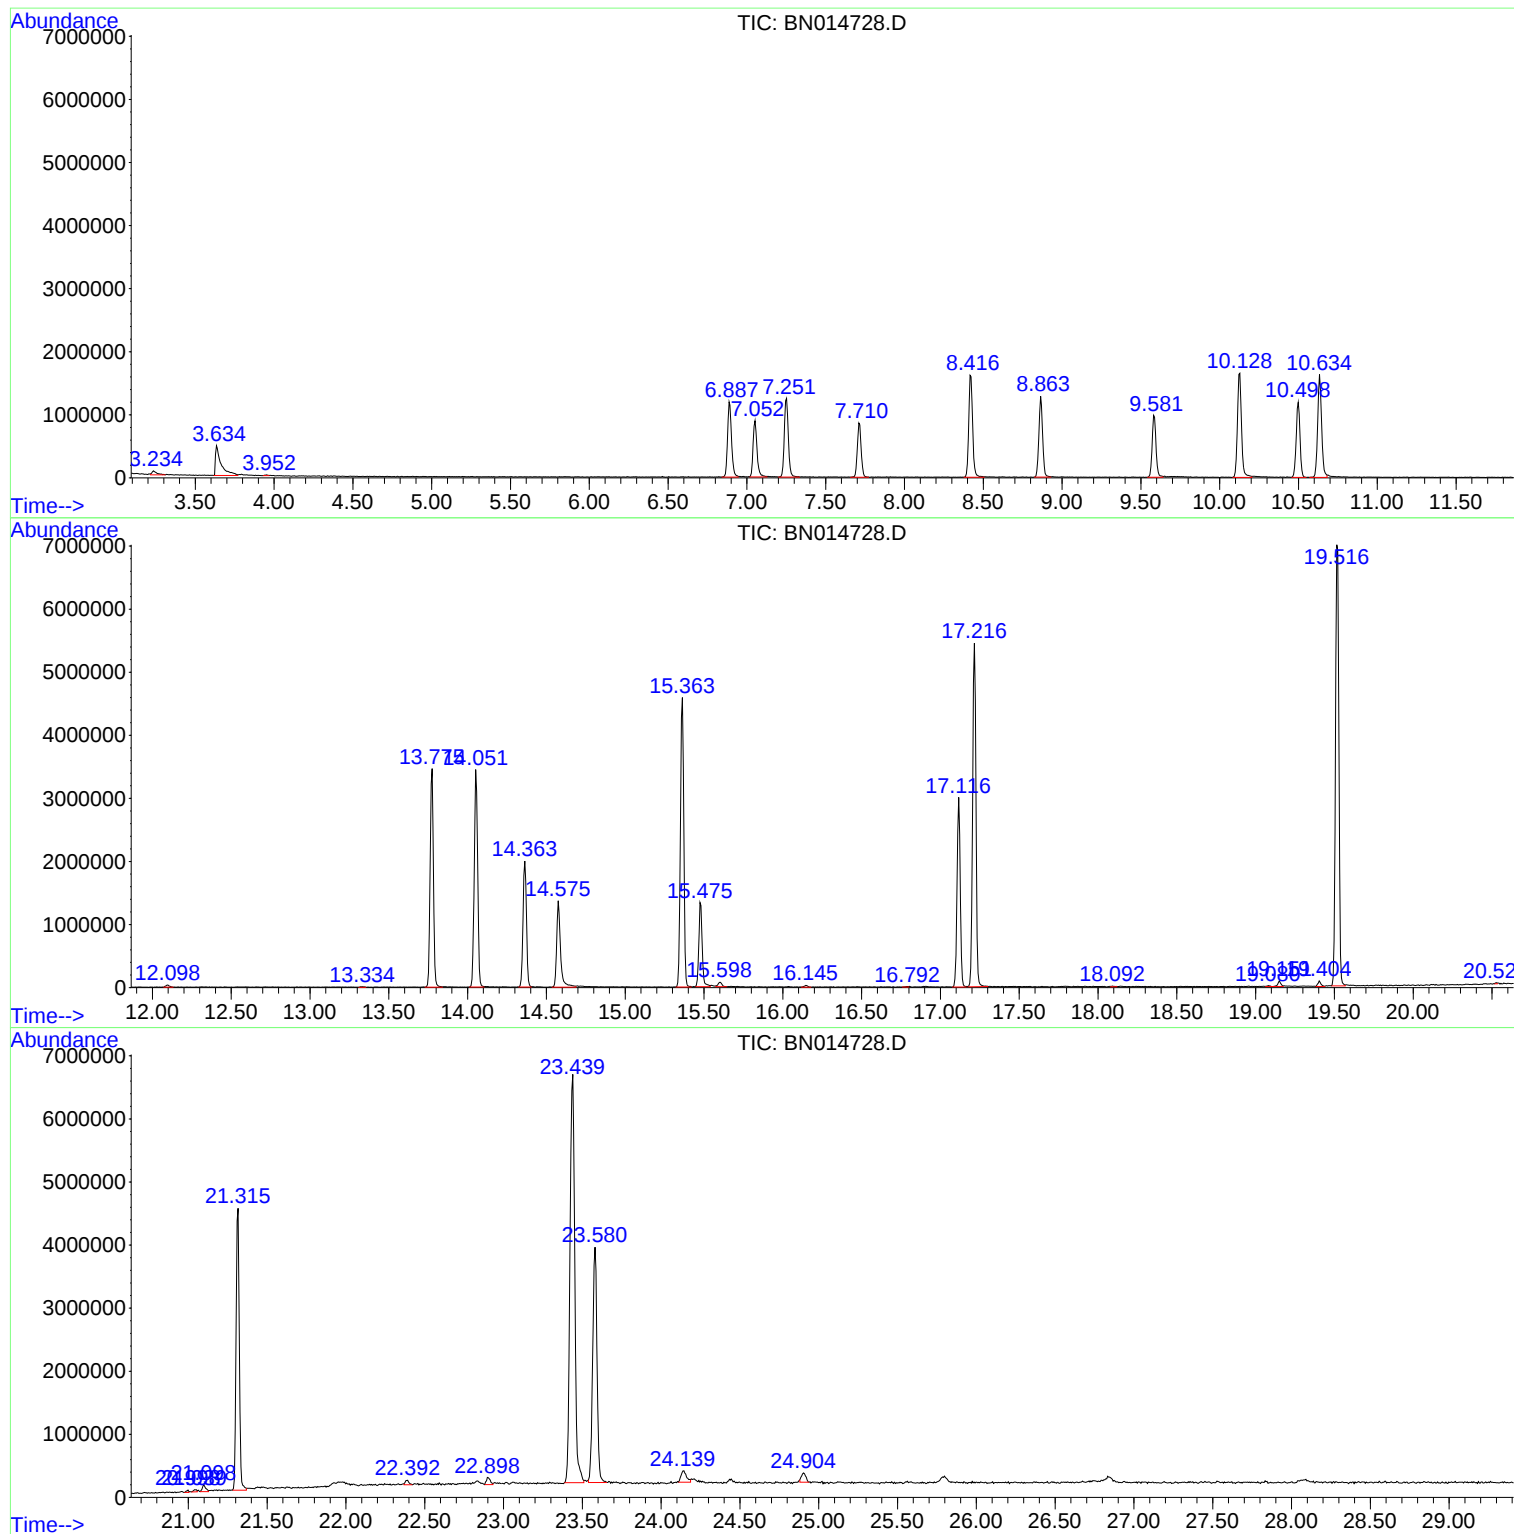

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014728.D
Acq On : 25 May 2021 10:15
Operator : CG/JU
Sample : PB136608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK608

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014728.D
Acq On : 25 May 2021 10:15
Operator : CG/JU
Sample : PB136608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK608

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
