

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014730.D
 Acq On : 25 May 2021 11:43
 Operator : CG/JU
 Sample : M2493-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB428

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014730.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	29	rVB6	20766	31043	0.30%	0.045%
2	3.634	91	93	96	rVB4	12879	12108	0.12%	0.018%
3	3.858	128	131	134	rVV3	15863	18901	0.18%	0.028%
4	4.046	159	163	166	rBV4	13838	22014	0.21%	0.032%
5	4.387	217	221	222	rBV3	8819	10839	0.10%	0.016%
6	4.558	247	250	255	rVB5	7214	12450	0.12%	0.018%
7	6.893	640	647	657	rBV	146037	289334	2.75%	0.422%
8	7.052	668	674	684	rBV	578339	959032	9.13%	1.398%
9	7.252	699	708	716	rBV	649556	1072809	10.21%	1.564%
10	7.716	779	787	796	rBV	755430	1256197	11.96%	1.831%
11	8.422	899	907	920	rBV	500257	849068	8.08%	1.238%
12	8.869	976	983	991	rBV	775513	1311523	12.48%	1.912%
13	9.304	1053	1057	1063	rVB6	16263	23103	0.22%	0.034%
14	9.587	1097	1105	1117	rBV	597228	1016706	9.68%	1.482%
15	9.663	1117	1118	1121	rVV3	12952	10701	0.10%	0.016%
16	10.128	1190	1197	1210	rBV	981602	1760038	16.75%	2.565%
17	10.498	1254	1260	1270	rVV	1007802	1683984	16.03%	2.455%
18	10.646	1278	1285	1292	rBV3	53767	109739	1.04%	0.160%
19	12.093	1527	1531	1538	rBV6	24110	41734	0.40%	0.061%
20	13.775	1811	1817	1822	rBV	2260106	3213160	30.58%	4.684%
21	13.822	1822	1825	1833	rVB	122944	178929	1.70%	0.261%
22	14.057	1856	1865	1874	rBV	2334387	3504844	33.36%	5.109%
23	14.363	1910	1917	1925	rBV	1733964	2591264	24.66%	3.777%
24	14.587	1950	1955	1968	rBV3	115459	248674	2.37%	0.362%
25	15.116	2040	2045	2050	rBV2	75647	114538	1.09%	0.167%
26	15.181	2054	2056	2062	rVV6	12478	20016	0.19%	0.029%
27	15.228	2062	2064	2071	rVB4	12079	18894	0.18%	0.028%
28	15.363	2079	2087	2096	rBV	3386913	4846246	46.12%	7.064%
29	15.481	2100	2107	2123	rVV	900082	1382142	13.15%	2.015%
30	15.604	2123	2128	2133	rVV7	51784	99570	0.95%	0.145%
31	15.639	2133	2134	2140	rVV4	11367	15315	0.15%	0.022%
32	15.734	2148	2150	2153	rVB2	11463	11224	0.11%	0.016%
33	15.933	2179	2184	2186	rBV5	9850	14117	0.13%	0.021%
34	16.045	2200	2203	2207	rBV6	9451	14260	0.14%	0.021%
35	16.151	2217	2221	2225	rVB5	17048	27220	0.26%	0.040%
36	16.363	2254	2257	2261	rVB4	23771	30936	0.29%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014730.D
 Acq On : 25 May 2021 11:43
 Operator : CG/JU
 Sample : M2493-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB428

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	16.798	2328	2331	2335	rBV5	11298	12251	0.12%	0.018%
38	16.898	2345	2348	2354	rBV6	10154	20857	0.20%	0.030%
39	17.116	2378	2385	2394	rBV	2430542	3555960	33.84%	5.183%
40	17.216	2395	2402	2413	rVV2	4271407	6182823	58.84%	9.012%
41	18.028	2535	2540	2545	rBV7	31552	56502	0.54%	0.082%
42	18.669	2646	2649	2651	rVB4	9453	12321	0.12%	0.018%
43	18.875	2682	2684	2688	rVB5	7931	10638	0.10%	0.016%
44	18.916	2688	2691	2693	rBV3	10209	14249	0.14%	0.021%
45	19.092	2716	2721	2722	rVV4	10033	13182	0.13%	0.019%
46	19.151	2727	2731	2736	rVV3	66332	102099	0.97%	0.149%
47	19.186	2736	2737	2741	rVB4	11746	11827	0.11%	0.017%
48	19.333	2756	2762	2764	rBV6	13820	22559	0.21%	0.033%
49	19.410	2770	2775	2780	rVB	54424	77351	0.74%	0.113%
50	19.522	2787	2794	2805	rBV	5772343	8118258	77.26%	11.833%
51	19.863	2849	2852	2854	rBV4	14102	15001	0.14%	0.022%
52	20.051	2882	2884	2886	rBV3	11036	12368	0.12%	0.018%
53	20.116	2892	2895	2896	rBV3	14597	12278	0.12%	0.018%
54	20.357	2933	2936	2941	rBV6	12098	26050	0.25%	0.038%
55	20.539	2964	2967	2971	rBV6	24714	38151	0.36%	0.056%
56	20.574	2971	2973	2975	rVB2	15172	11725	0.11%	0.017%
57	20.721	2996	2998	2999	rBV	19807	11714	0.11%	0.017%
58	20.769	3004	3006	3010	rBV5	15321	16696	0.16%	0.024%
59	20.974	3039	3041	3042	rBV2	18810	11859	0.11%	0.017%
60	21.039	3048	3052	3059	rBV3	195829	303932	2.89%	0.443%
61	21.104	3059	3063	3068	rVB2	93316	131156	1.25%	0.191%
62	21.316	3092	3099	3109	rBV	3762212	5254976	50.01%	7.660%
63	21.445	3117	3121	3124	rBV6	50755	61827	0.59%	0.090%
64	22.245	3255	3257	3258	rBV	30300	22301	0.21%	0.033%
65	22.398	3280	3283	3288	rVB6	83029	97937	0.93%	0.143%
66	22.910	3367	3370	3375	rVB3	122074	170913	1.63%	0.249%
67	23.445	3453	3461	3476	rBV	5115850	10507346	100.00%	15.316%
68	23.586	3478	3485	3496	rVB	3064822	5796818	55.17%	8.449%
69	24.151	3576	3581	3588	rVB7	191244	369451	3.52%	0.539%
70	24.909	3705	3710	3719	rVB7	188751	427724	4.07%	0.623%
71	25.804	3859	3862	3871	rVB8	128672	242931	2.31%	0.354%
72	27.127	4085	4087	4089	rBV3	38147	28862	0.27%	0.042%




Sum of corrected areas: 68605565

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014730.D
Acq On : 25 May 2021 11:43
Operator : CG/JU
Sample : M2493-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB428

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

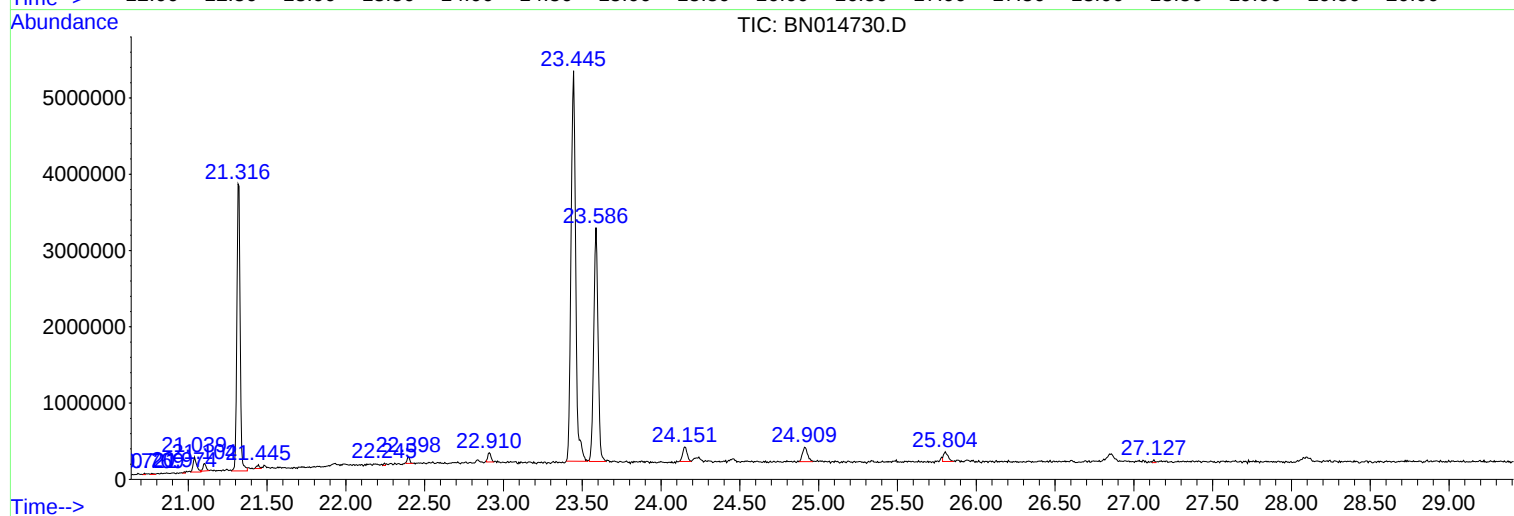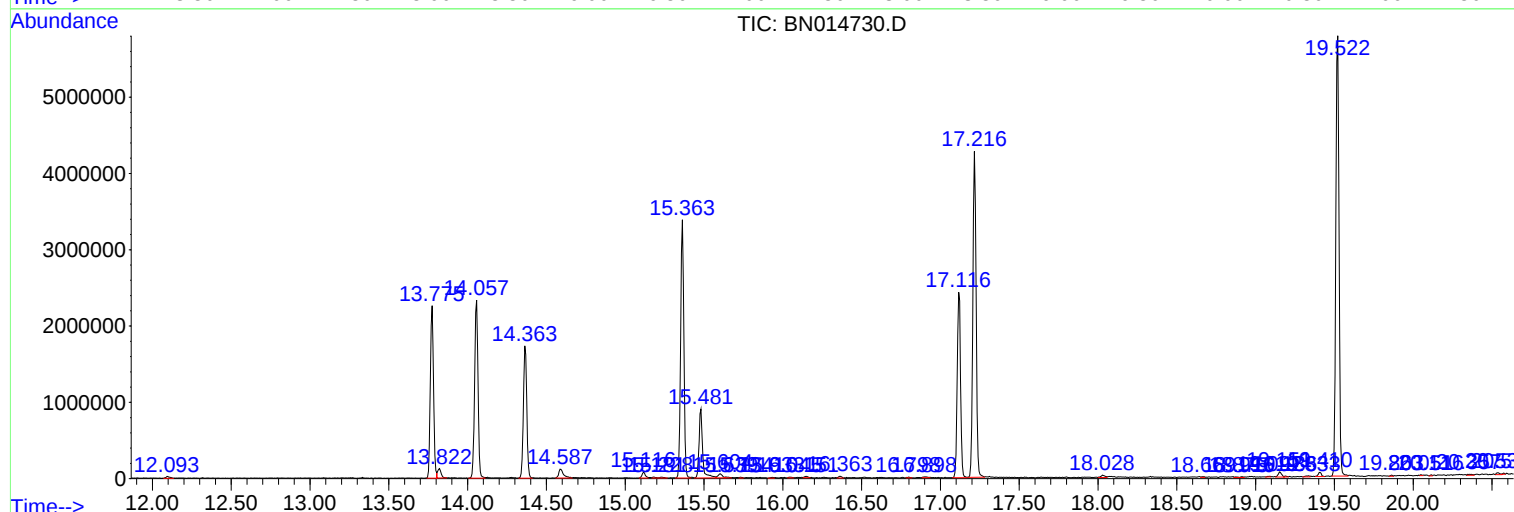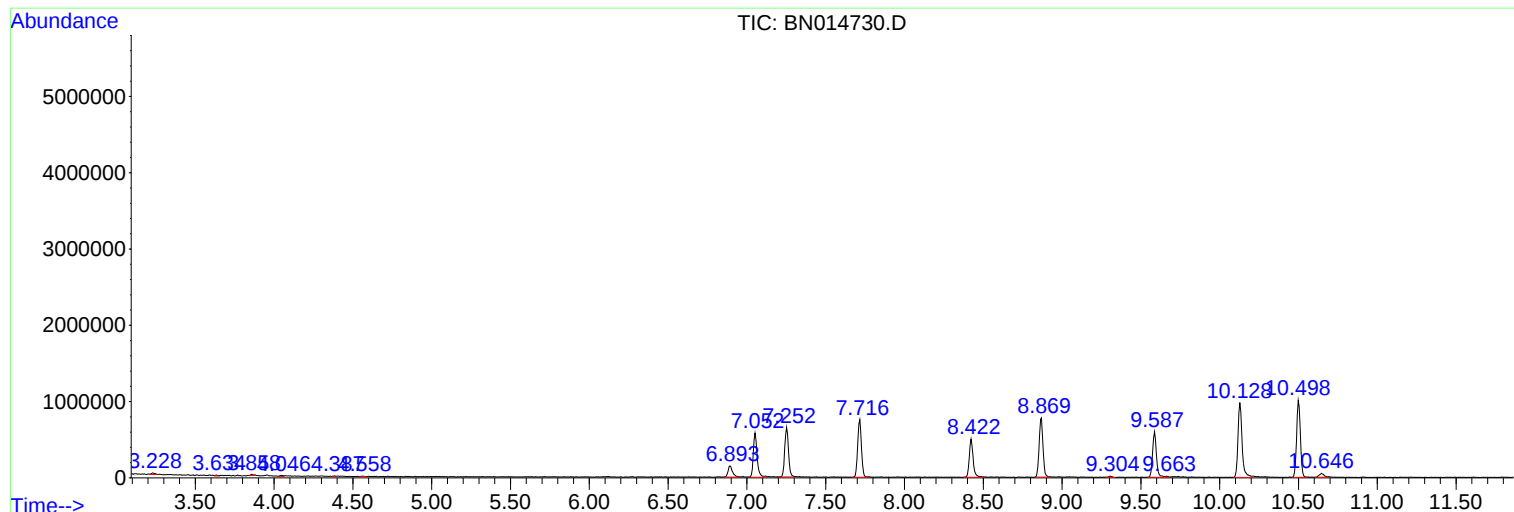

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014730.D
Acq On : 25 May 2021 11:43
Operator : CG/JU
Sample : M2493-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB428

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014730.D
Acq On : 25 May 2021 11:43
Operator : CG/JU
Sample : M2493-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB428

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
