

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014731.D
 Acq On : 25 May 2021 12:18
 Operator : CG/JU
 Sample : M2493-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB432

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014731.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	22	24	31	rVB3	26338	36620	0.31%	0.047%
2	3.858	128	131	136	rBV4	20361	33987	0.28%	0.043%
3	3.952	144	147	156	rVB5	14770	31315	0.26%	0.040%
4	4.046	161	163	169	rVB6	10104	12883	0.11%	0.016%
5	6.116	513	515	519	rVB4	10758	14066	0.12%	0.018%
6	6.893	640	647	658	rBV	194174	351977	2.95%	0.449%
7	7.052	667	674	685	rBV	649937	1113846	9.32%	1.421%
8	7.246	701	707	715	rBV2	761171	1305890	10.93%	1.666%
9	7.710	778	786	795	rBV	867043	1387162	11.61%	1.770%
10	8.416	899	906	919	rBV	626751	1098733	9.19%	1.402%
11	8.863	975	982	990	rBV	930952	1548058	12.95%	1.975%
12	9.581	1096	1104	1113	rBV	725826	1239916	10.37%	1.582%
13	10.122	1190	1196	1206	rBV	1124859	2036139	17.04%	2.598%
14	10.499	1253	1260	1268	rBV	1147694	1913883	16.01%	2.442%
15	10.640	1277	1284	1290	rBV4	64970	130441	1.09%	0.166%
16	12.098	1527	1532	1538	rVV4	23376	39563	0.33%	0.050%
17	12.975	1678	1681	1687	rVB7	7858	13868	0.12%	0.018%
18	13.775	1810	1817	1828	rBV	2728087	3972720	33.24%	5.069%
19	14.051	1856	1864	1876	rBV	2836034	4154059	34.76%	5.300%
20	14.363	1910	1917	1929	rBV	1862320	2830193	23.68%	3.611%
21	14.587	1947	1955	1962	rBV3	186731	357030	2.99%	0.456%
22	14.639	1962	1964	1968	rVV4	17572	24498	0.20%	0.031%
23	15.187	2053	2057	2062	rBV4	14769	22450	0.19%	0.029%
24	15.363	2080	2087	2099	rBV	3857040	5811089	48.62%	7.414%
25	15.475	2101	2106	2116	rBV	1234288	1767277	14.79%	2.255%
26	15.598	2123	2127	2133	rVB3	66720	94611	0.79%	0.121%
27	15.834	2163	2167	2173	rVB6	8187	13547	0.11%	0.017%
28	16.151	2216	2221	2225	rVB6	20823	33760	0.28%	0.043%
29	16.586	2289	2295	2300	rBV7	15196	21103	0.18%	0.027%
30	16.798	2323	2331	2334	rBV7	11642	24378	0.20%	0.031%
31	16.904	2345	2349	2354	rVB6	16043	24199	0.20%	0.031%
32	17.116	2378	2385	2395	rBV	2771150	3914373	32.75%	4.994%
33	17.216	2395	2402	2418	rVV2	5134127	7582855	63.45%	9.675%
34	17.798	2498	2501	2504	rVB4	10053	12557	0.11%	0.016%
35	18.098	2548	2552	2556	rVB4	17265	24029	0.20%	0.031%
36	19.086	2716	2720	2724	rVB7	11898	15735	0.13%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014731.D
 Acq On : 25 May 2021 12:18
 Operator : CG/JU
 Sample : M2493-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB432

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	19.151	2726	2731	2735	rBV2	86075	118004	0.99%	0.151%
38	19.404	2768	2774	2778	rBV2	79416	106257	0.89%	0.136%
39	19.522	2787	2794	2802	rBV2	6551762	9753717	81.61%	12.445%
40	20.080	2887	2889	2891	rBV3	13341	13591	0.11%	0.017%
41	20.445	2950	2951	2954	rBV3	15499	17778	0.15%	0.023%
42	20.533	2963	2966	2969	rBV5	16534	21471	0.18%	0.027%
43	21.051	3050	3054	3058	rBV6	35035	55637	0.47%	0.071%
44	21.104	3060	3063	3068	rVV3	58486	82235	0.69%	0.105%
45	21.221	3079	3083	3084	rBV4	23758	32772	0.27%	0.042%
46	21.316	3093	3099	3108	rBV	4095624	5449286	45.60%	6.953%
47	21.921	3200	3202	3206	rVB5	40569	32019	0.27%	0.041%
48	22.398	3279	3283	3285	rBV5	89370	108330	0.91%	0.138%
49	22.910	3366	3370	3375	rVB4	183749	244443	2.05%	0.312%
50	23.439	3452	3460	3467	rBV2	5933733	11951194	100.00%	15.249%
51	23.586	3477	3485	3493	rBV	3040491	6000526	50.21%	7.656%
52	23.933	3542	3544	3546	rBV3	31968	21192	0.18%	0.027%
53	24.145	3575	3580	3588	rVB4	251877	460834	3.86%	0.588%
54	24.904	3704	3709	3715	rBV6	234247	486249	4.07%	0.620%
55	25.798	3857	3861	3870	rVB9	165629	411130	3.44%	0.525%


Sum of corrected areas: 78375475

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014731.D
Acq On : 25 May 2021 12:18
Operator : CG/JU
Sample : M2493-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB432

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

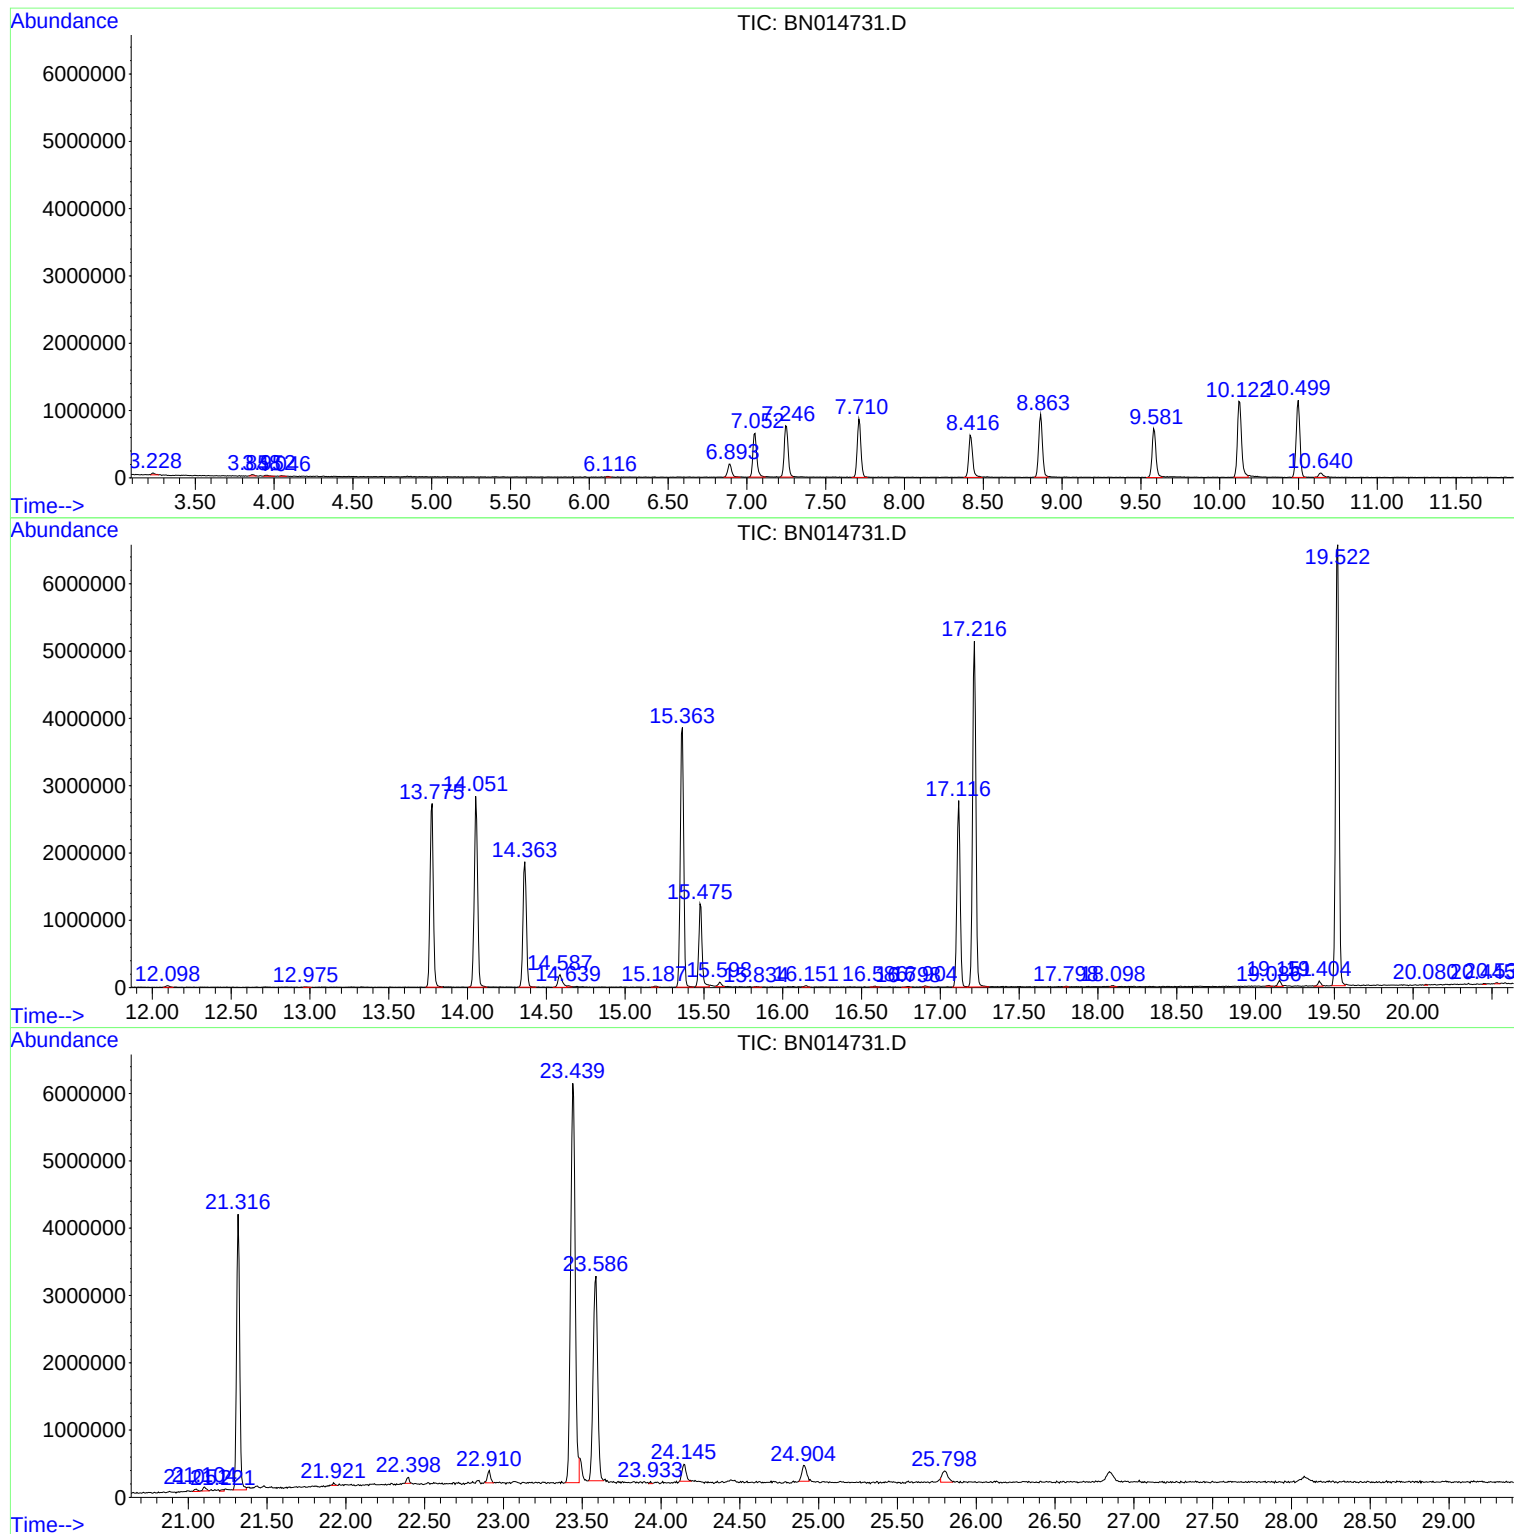

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014731.D
Acq On : 25 May 2021 12:18
Operator : CG/JU
Sample : M2493-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB432

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014731.D
Acq On : 25 May 2021 12:18
Operator : CG/JU
Sample : M2493-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB432

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
